

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022221\
 Data File : PL064910.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Feb 2021 15:45
 Operator : AR\AJ
 Sample : M1452-25
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 17:20:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 09 04:41:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.423	4.099	40567616	32939913	14.419	15.249
28)	SA Decachlor...	8.145	9.258	34525572	26446056	15.353	13.924
Target Compounds							
17)	MA 4,4'-DDT	6.318	0.000	1160885	0	0.515	N.D. #
23)	Chlordane-1	4.295	0.000	2606705	0	22.931	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022221\
Data File : PL064910.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Feb 2021 15:45
Operator : AR\AJ
Sample : M1452-25
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 17:20:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
Quant Title : GC Extractables
QLast Update : Tue Feb 09 04:41:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

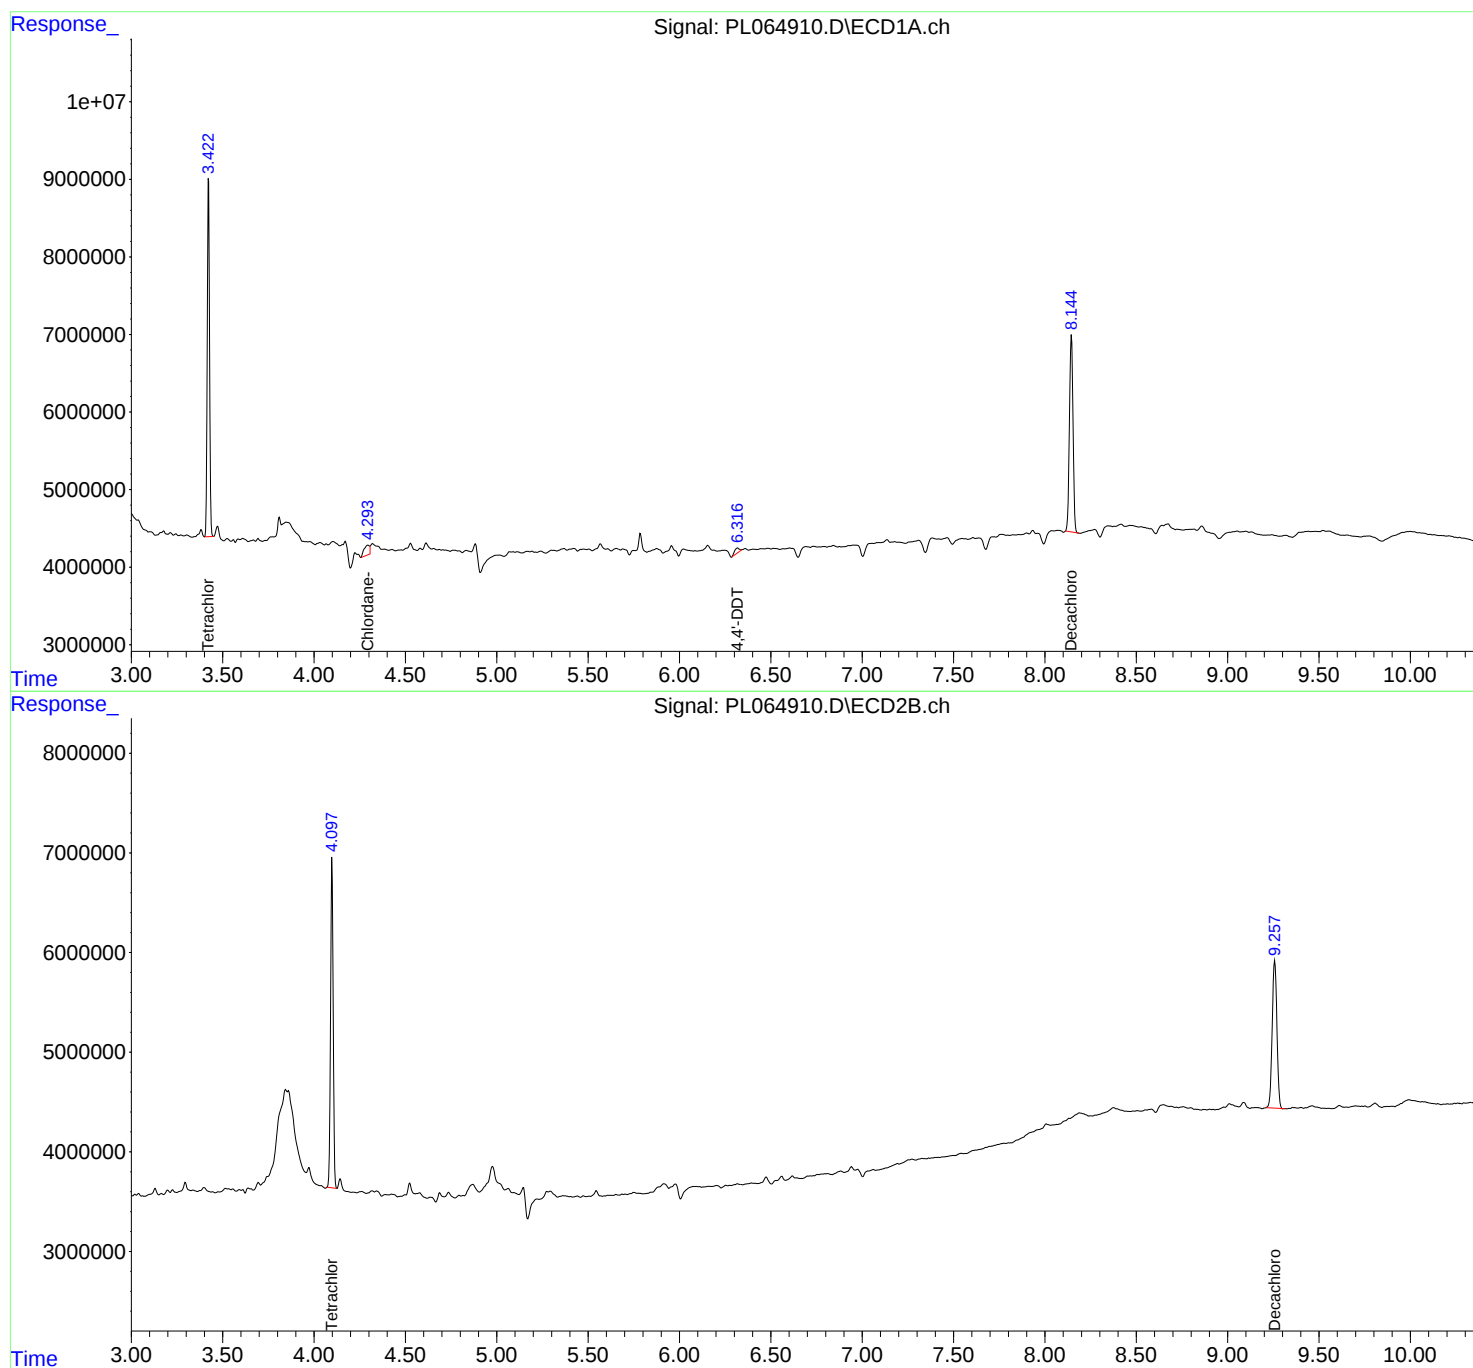


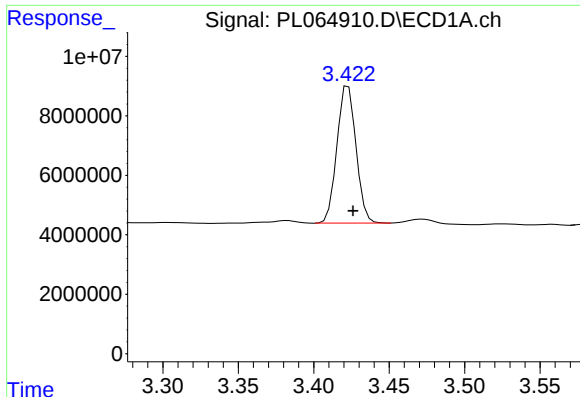

#1 Tetrachloro-m-xylene


R.T.: 3.423 min
Delta R.T.: -0.003 min
Response: 40567616
Conc: 14.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

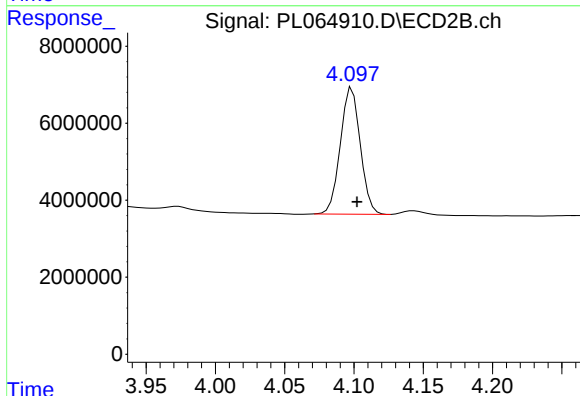


#1 Tetrachloro-m-xylene

R.T.: 4.099 min
Delta R.T.: -0.003 min
Response: 32939913
Conc: 15.25 ng/ml

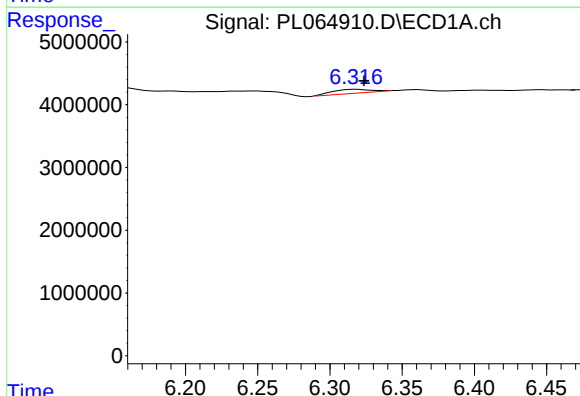


#17 4,4'-DDT

R.T.: 6.318 min
Delta R.T.: -0.006 min
Response: 1160885
Conc: 0.51 ng/ml

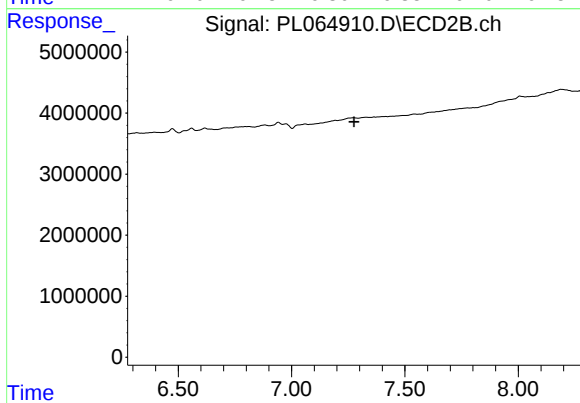

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.276 min
Response: 0
Conc: N.D.

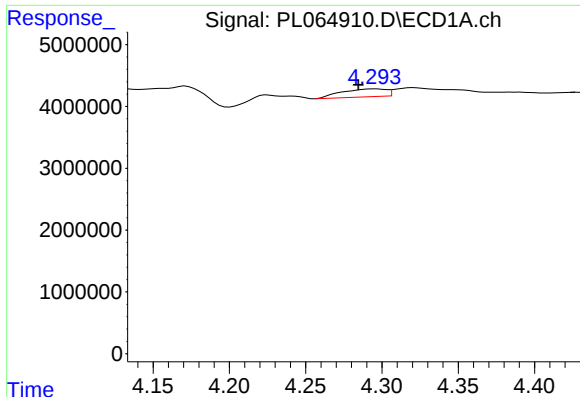

#23 Chlordane-1


R.T.: 4.295 min
Delta R.T.: 0.010 min
Response: 2606705
Conc: 22.93 ng/ml

Instrument :
ECD_L
ClientSampleId :

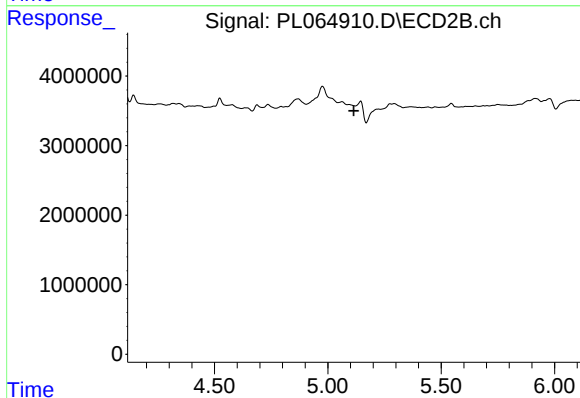


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.114 min
Response: 0
Conc: N.D.

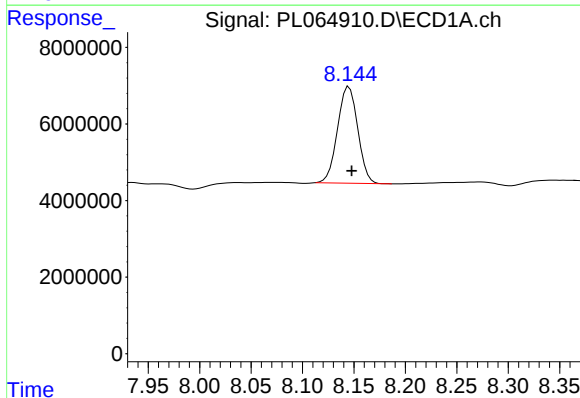

#28 Decachlorobiphenyl

R.T.: 8.145 min
Delta R.T.: -0.003 min
Response: 34525572
Conc: 15.35 ng/ml

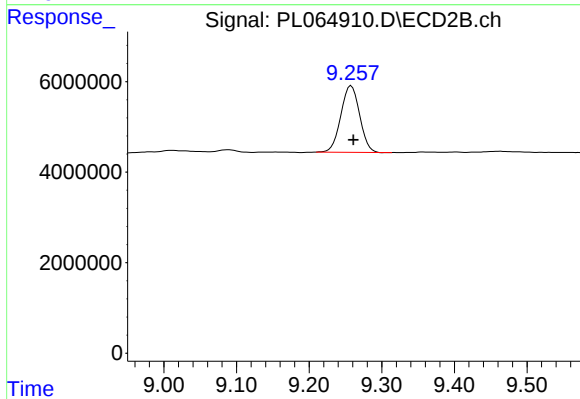

#28 Decachlorobiphenyl

R.T.: 9.258 min
Delta R.T.: -0.003 min
Response: 26446056
Conc: 13.92 ng/ml