

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022221\
 Data File : PL064915.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Feb 2021 17:07
 Operator : AR\AJ
 Sample : PB134765TB
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 17:21:38 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 09 04:41:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.423	4.100	61842498	50553442	21.981	23.402
28)	SA Decachlor...	8.146	9.258	56102110	44551144	24.948	23.456
Target Compounds							
6)	B beta-BHC	0.000	4.974	0	7049774	N.D.	1.778 #
23)	Chlordane-1	4.308f	0.000	3375739	0	29.696	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022221\
Data File : PL064915.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Feb 2021 17:07
Operator : AR\AJ
Sample : PB134765TB
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 17:21:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
Quant Title : GC Extractables
QLast Update : Tue Feb 09 04:41:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

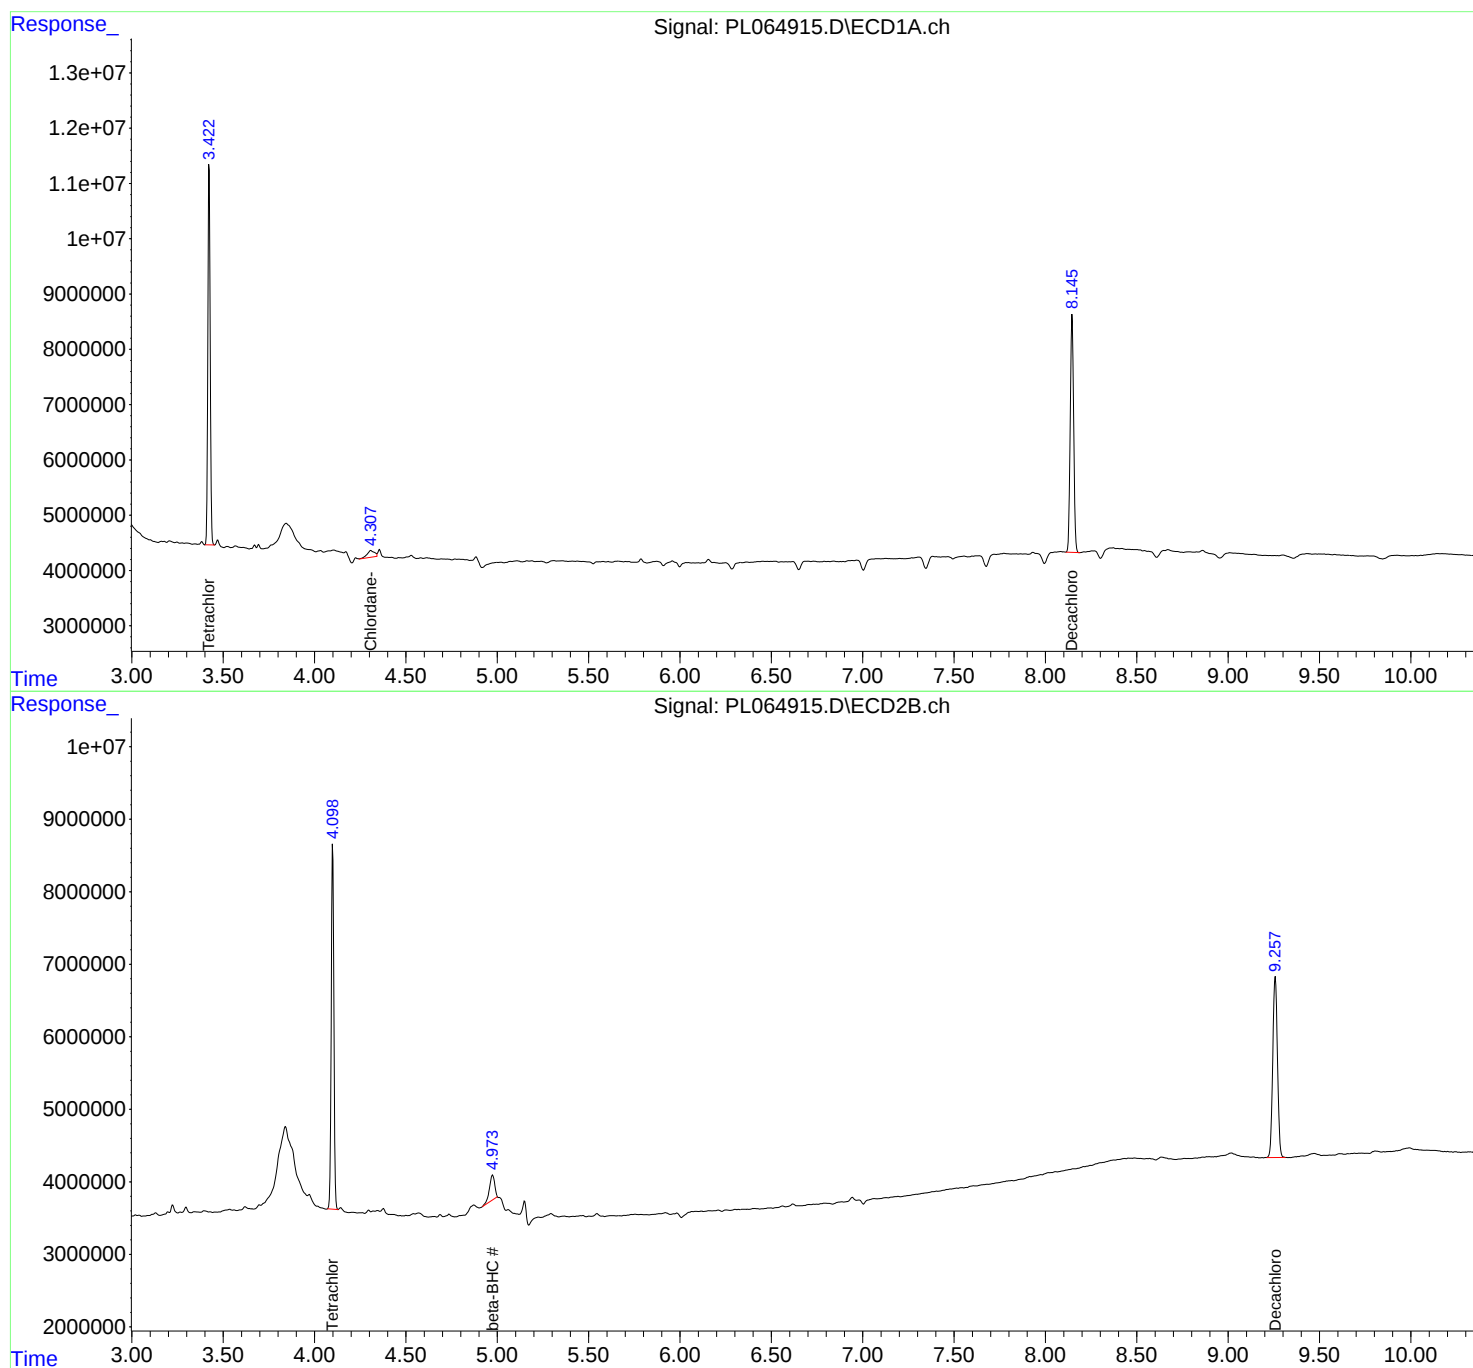


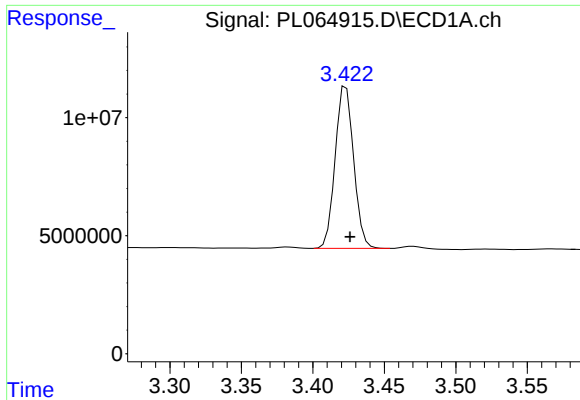

#1 Tetrachloro-m-xylene


R.T.: 3.423 min
Delta R.T.: -0.003 min
Response: 61842498
Conc: 21.98 ng/ml

Instrument :
ECD_L
ClientSampleId :

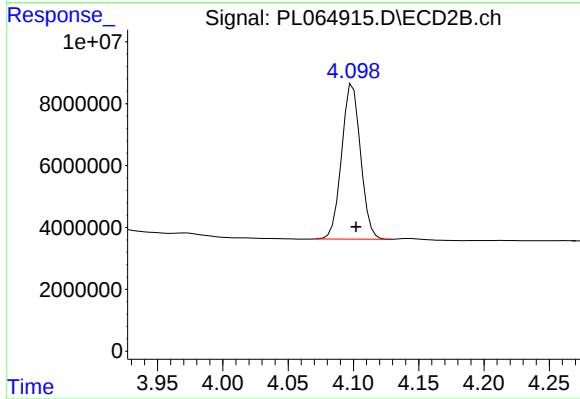


#1 Tetrachloro-m-xylene

R.T.: 4.100 min
Delta R.T.: -0.003 min
Response: 50553442
Conc: 23.40 ng/ml

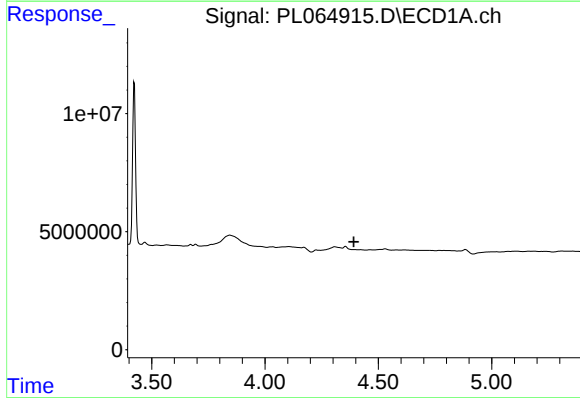


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.391 min
Response: 0
Conc: N.D.

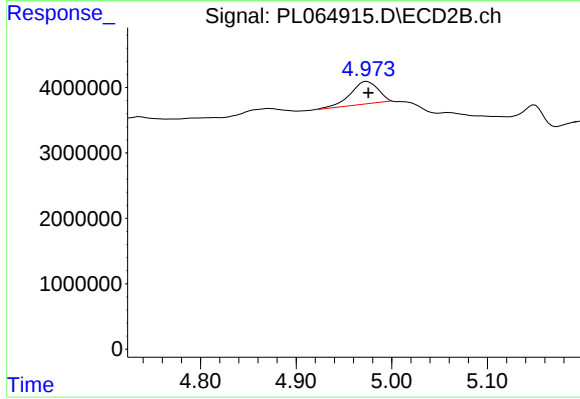

#6 beta-BHC


R.T.: 4.974 min
Delta R.T.: -0.001 min
Response: 7049774
Conc: 1.78 ng/ml

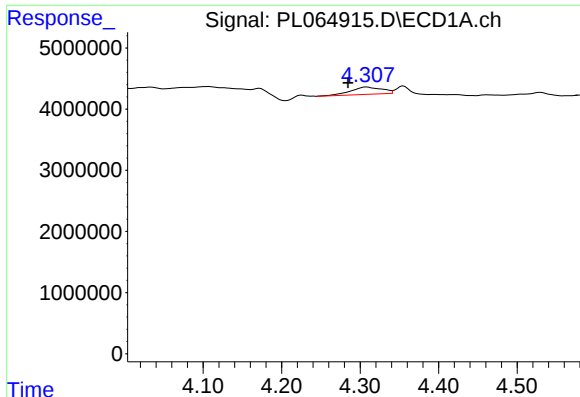

#23 Chlordane-1


R.T.: 4.308 min
Delta R.T.: 0.023 min
Response: 3375739
Conc: 29.70 ng/ml

Instrument :
ECD_L
ClientSampleId :

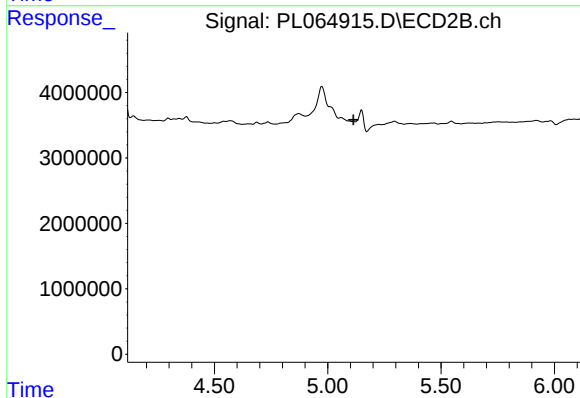


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.114 min
Response: 0
Conc: N.D.

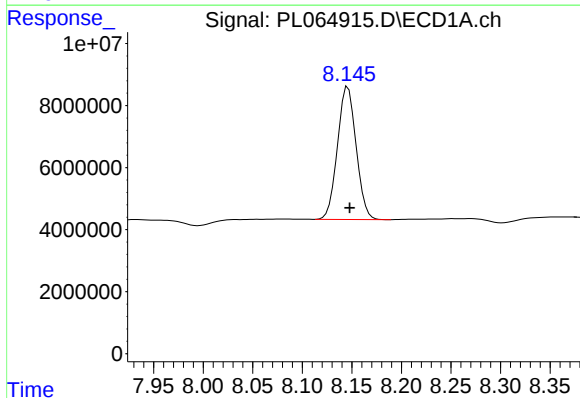

#28 Decachlorobiphenyl

R.T.: 8.146 min
Delta R.T.: -0.002 min
Response: 56102110
Conc: 24.95 ng/ml

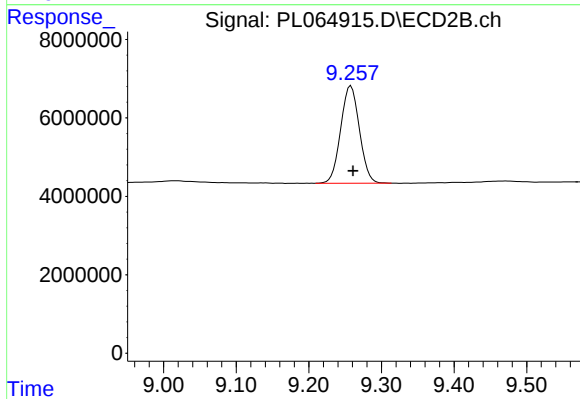

#28 Decachlorobiphenyl

R.T.: 9.258 min
Delta R.T.: -0.003 min
Response: 44551144
Conc: 23.46 ng/ml