

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022221\
 Data File : PL064920.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Feb 2021 18:19
 Operator : AR\AJ
 Sample : M1452-12
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 23 00:38:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 09 04:41:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.424	4.100	55327191	44385505	19.665	20.547
28)	SA Decachlor...	8.147	9.259	46287022	37885929	20.583	19.946
Target Compounds							
9)	A Endosulfan I	5.477f	0.000	1379481	0	0.430	N.D. #
10)	B gamma-Chl...	0.000	6.248	0	1286357	N.D.	0.557 #
16)	A 4,4'-DDD	6.101f	0.000	1117425	0	0.441	N.D. #
23)	Chlordane-1	4.289	0.000	3422273	0	30.105	N.D. #
25)	Chlordane-3	0.000	6.248	0	1286357	N.D.	4.207 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022221\
Data File : PL064920.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Feb 2021 18:19
Operator : AR\AJ
Sample : M1452-12
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
TP-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 23 00:38:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
Quant Title : GC Extractables
QLast Update : Tue Feb 09 04:41:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

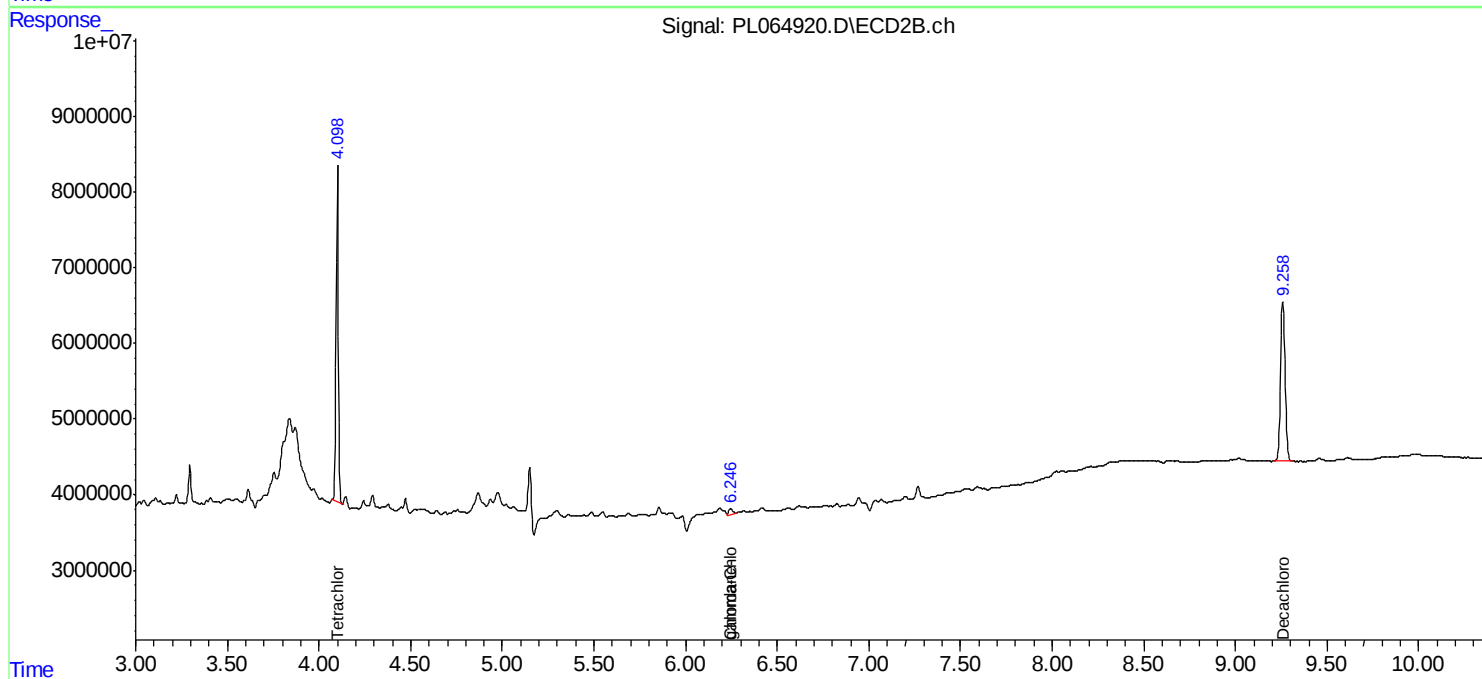


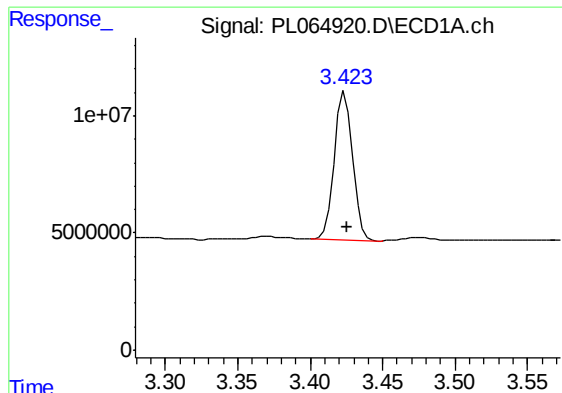

#1 Tetrachloro-m-xylene


R.T.: 3.424 min
Delta R.T.: -0.002 min
Response: 55327191
Conc: 19.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3

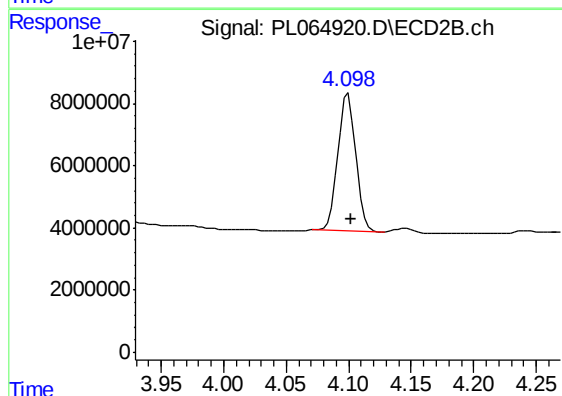


#1 Tetrachloro-m-xylene

R.T.: 4.100 min
Delta R.T.: -0.003 min
Response: 44385505
Conc: 20.55 ng/ml

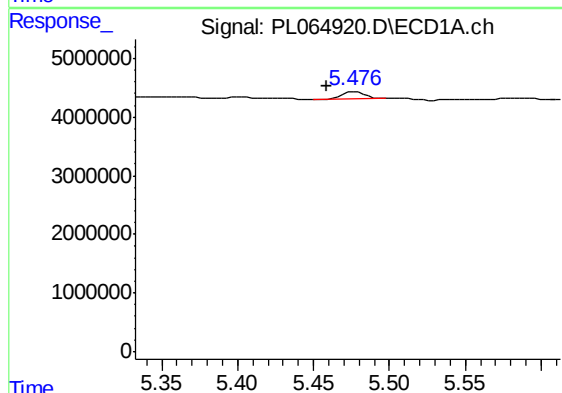


#9 Endosulfan I

R.T.: 5.477 min
Delta R.T.: 0.019 min
Response: 1379481
Conc: 0.43 ng/ml

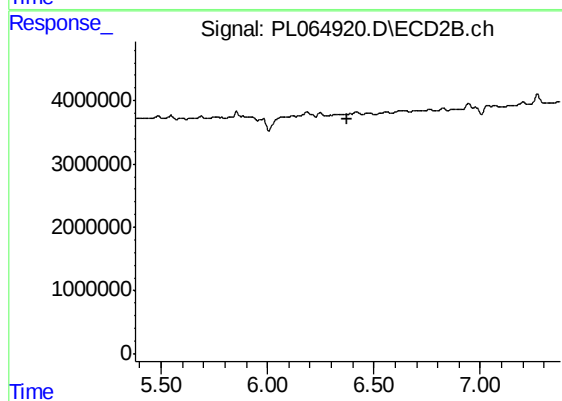

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.376 min
Response: 0
Conc: N.D.

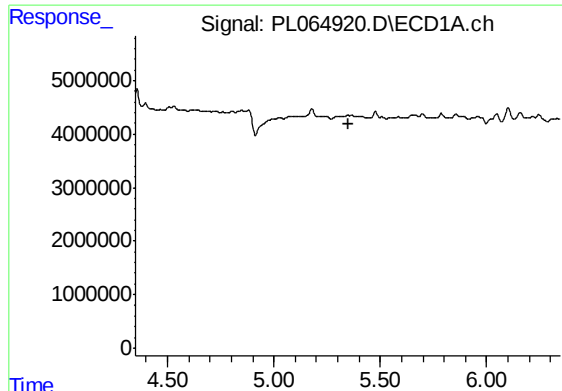

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.349 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-3

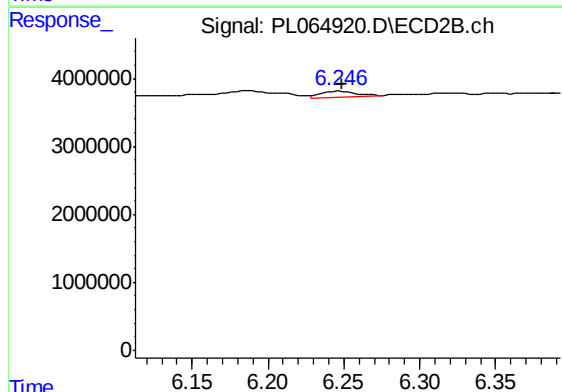


#10 gamma-Chlordane

R.T.: 6.248 min
Delta R.T.: -0.002 min
Response: 1286357
Conc: 0.56 ng/ml

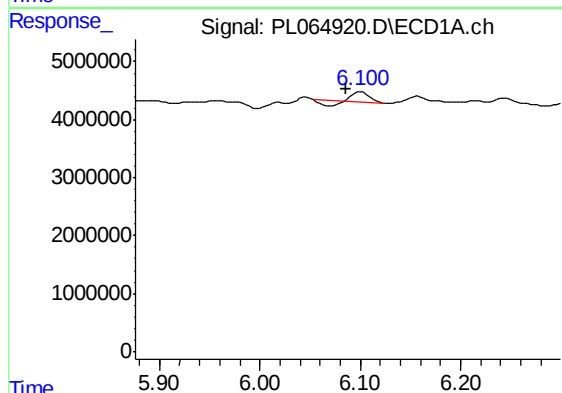


#16 4,4'-DDD

R.T.: 6.101 min
Delta R.T.: 0.016 min
Response: 1117425
Conc: 0.44 ng/ml

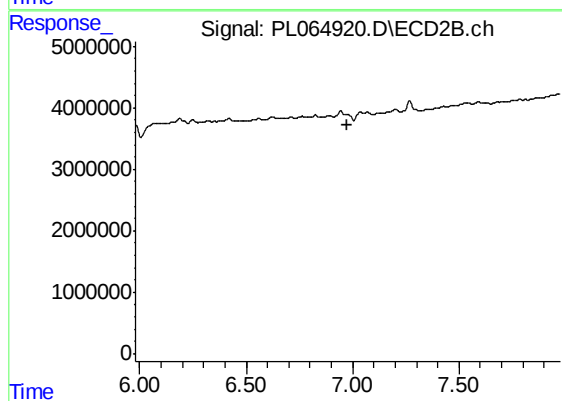

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.977 min
Response: 0
Conc: N.D.

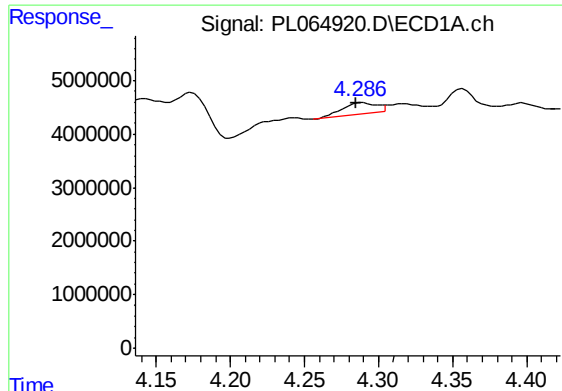

#23 Chlordane-1


R.T.: 4.289 min
Delta R.T.: 0.004 min
Response: 3422273
Conc: 30.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3

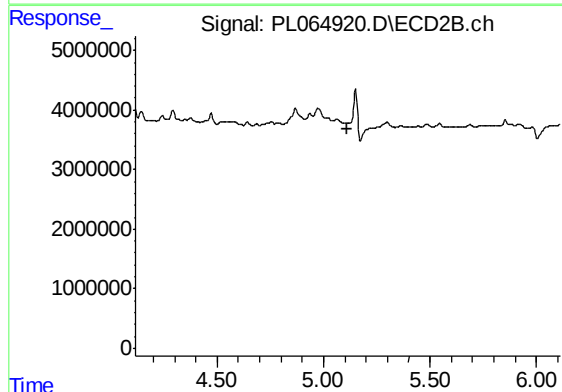


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.114 min
Response: 0
Conc: N.D.

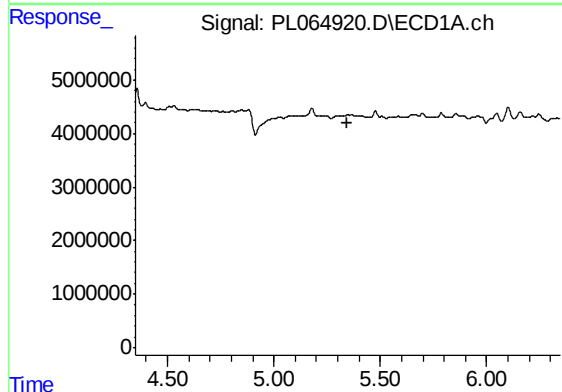


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.347 min
Response: 0
Conc: N.D.

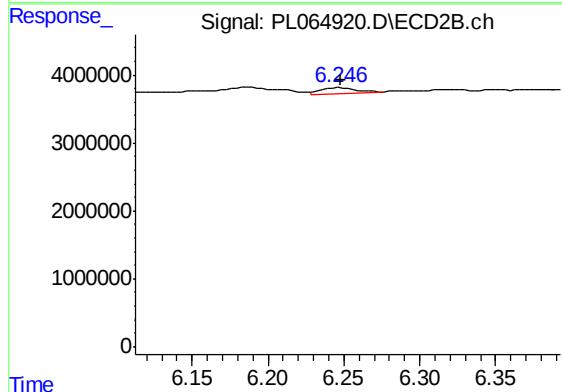

#25 Chlordane-3


R.T.: 6.248 min
Delta R.T.: 0.000 min
Response: 1286357
Conc: 4.21 ng/ml

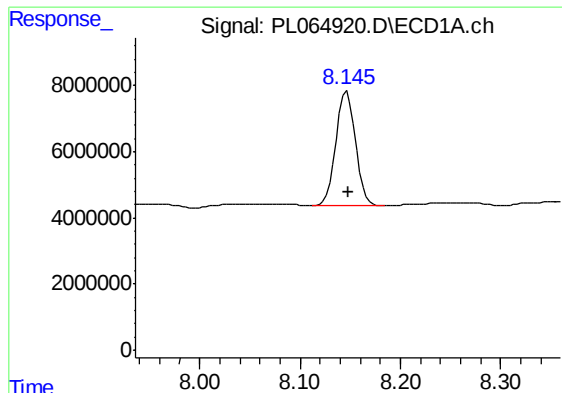

#28 Decachlorobiphenyl

R.T.: 8.147 min
Delta R.T.: -0.001 min
Response: 46287022
Conc: 20.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3

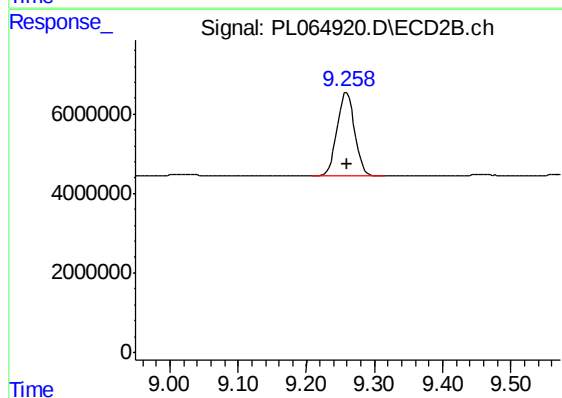

#28 Decachlorobiphenyl

R.T.: 9.259 min
Delta R.T.: -0.002 min
Response: 37885929
Conc: 19.95 ng/ml