

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022221\
 Data File : PL064921.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Feb 2021 18:33
 Operator : AR\AJ
 Sample : M1452-16
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-4

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 23 00:38:56 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 09 04:41:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.424	4.099	60899092	49374035	21.645	22.856
28)	SA Decachlor...	8.146	9.258	54858418	44012684	24.395	23.172
Target Compounds							
7)	B delta-BHC	0.000	5.215f	0	2205001	N.D.	0.816 #
10)	B gamma-Chl...	0.000	6.248	0	888804	N.D.	0.385 #
16)	A 4,4'-DDD	6.101f	0.000	1149448	0	0.454	N.D. #
22)	Mirex	7.268	0.000	14542282	0	6.882	N.D. #
25)	Chlordane-3	0.000	6.248	0	888804	N.D.	2.907 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022221\
Data File : PL064921.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Feb 2021 18:33
Operator : AR\AJ
Sample : M1452-16
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-4

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 23 00:38:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
Quant Title : GC Extractables
QLast Update : Tue Feb 09 04:41:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

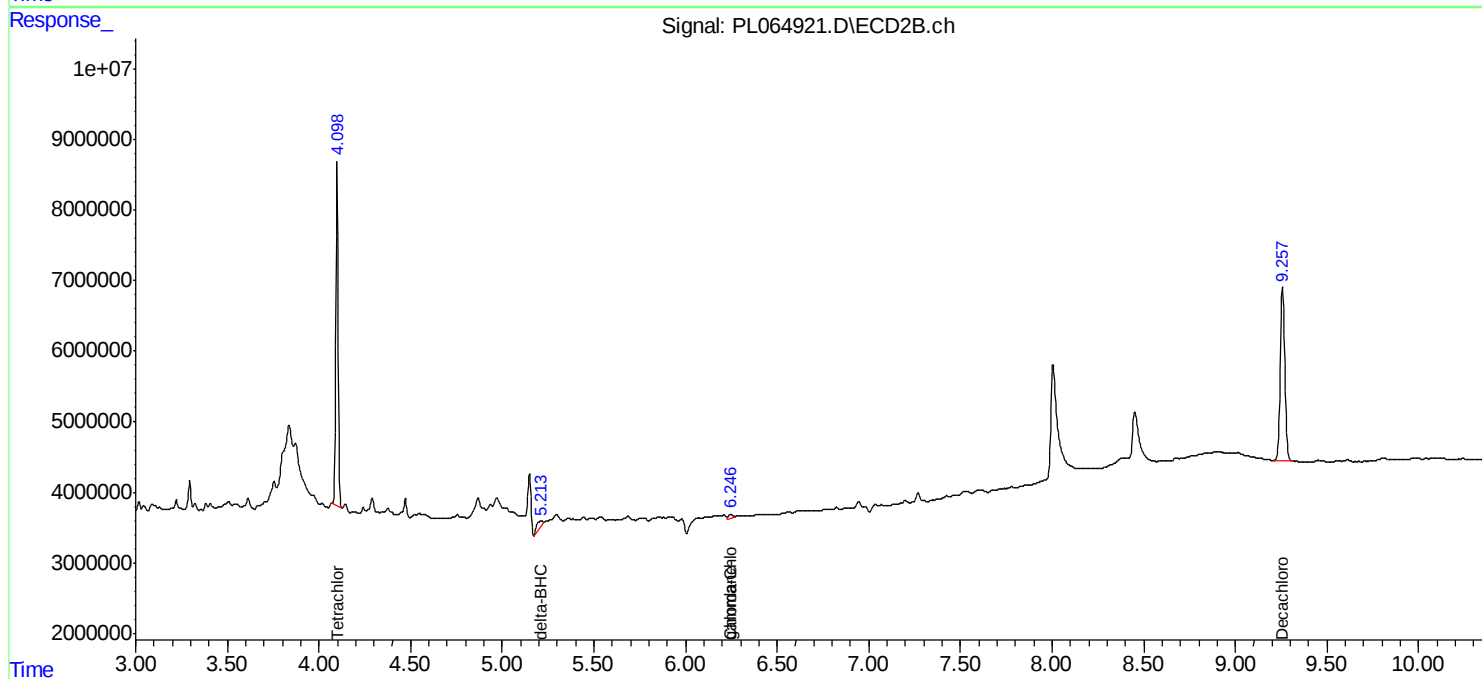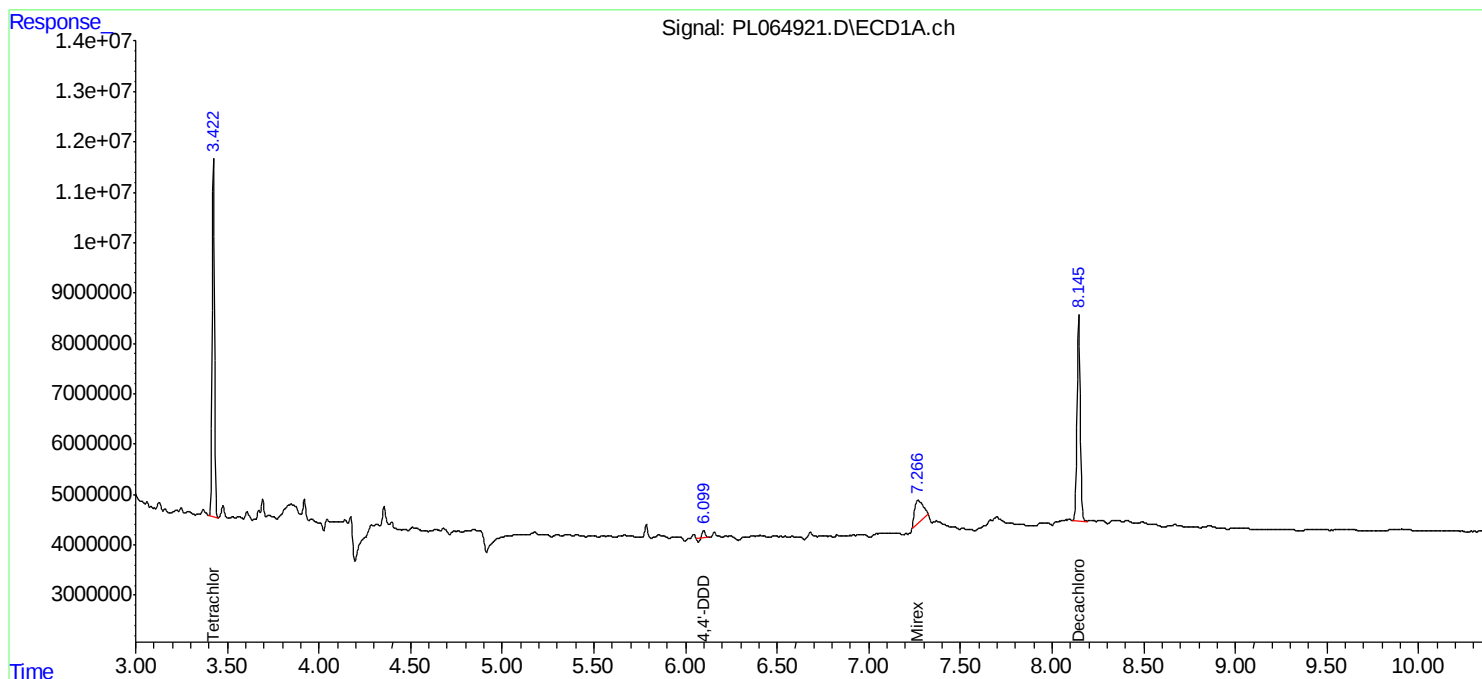


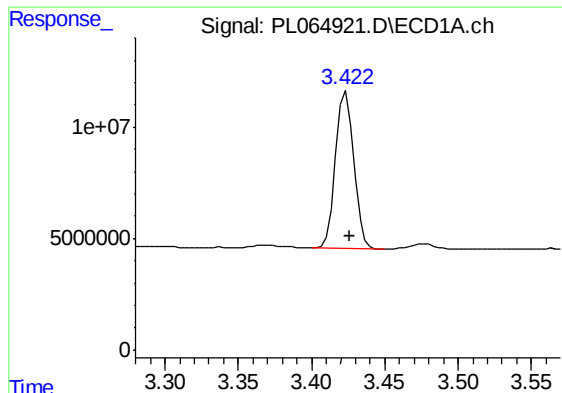

#1 Tetrachloro-m-xylene


R.T.: 3.424 min
Delta R.T.: -0.002 min
Response: 60899092
Conc: 21.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-4

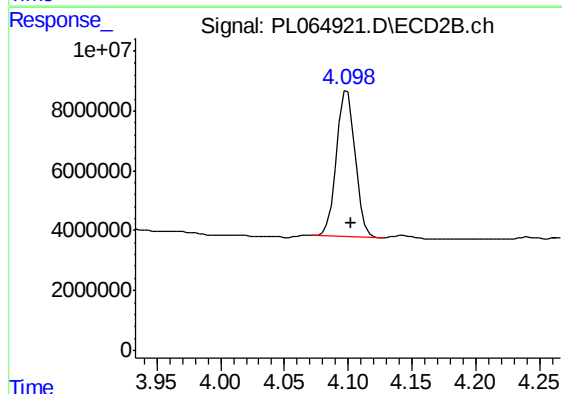


#1 Tetrachloro-m-xylene

R.T.: 4.099 min
Delta R.T.: -0.003 min
Response: 49374035
Conc: 22.86 ng/ml

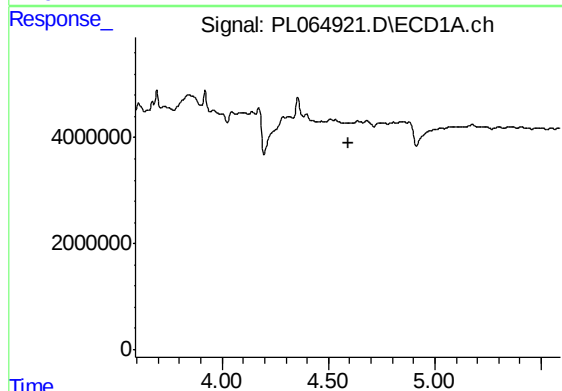


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.593 min
Response: 0
Conc: N.D.

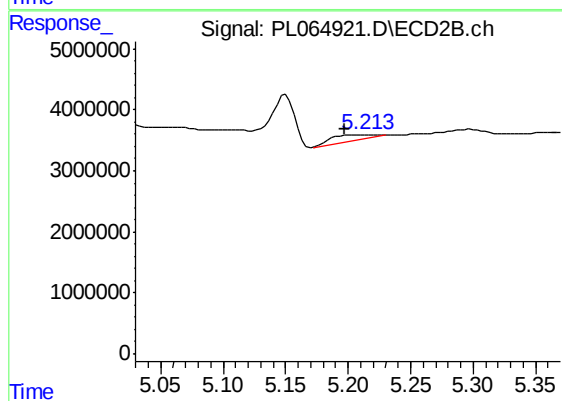

#7 delta-BHC


R.T.: 5.215 min
Delta R.T.: 0.017 min
Response: 2205001
Conc: 0.82 ng/ml

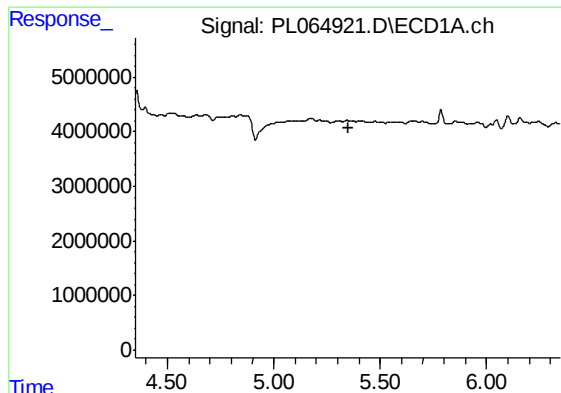

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.349 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-4

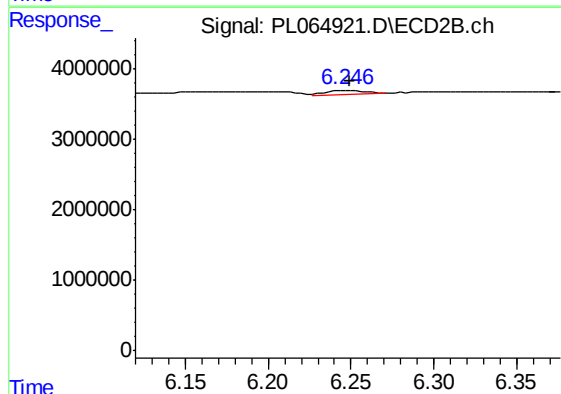


#10 gamma-Chlordane

R.T.: 6.248 min
Delta R.T.: -0.001 min
Response: 888804
Conc: 0.38 ng/ml

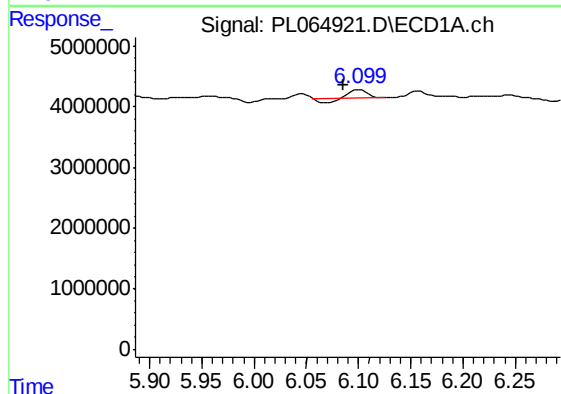


#16 4,4'-DDD

R.T.: 6.101 min
Delta R.T.: 0.015 min
Response: 1149448
Conc: 0.45 ng/ml

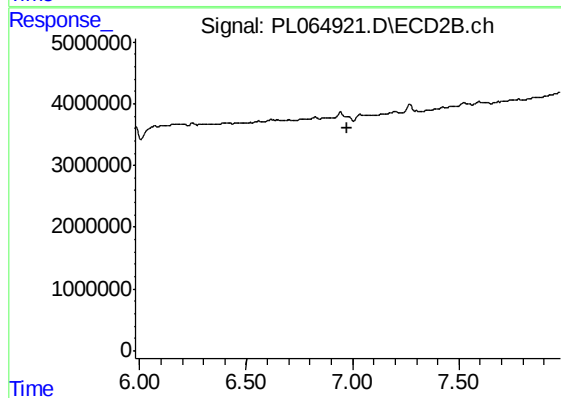

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.977 min
Response: 0
Conc: N.D.

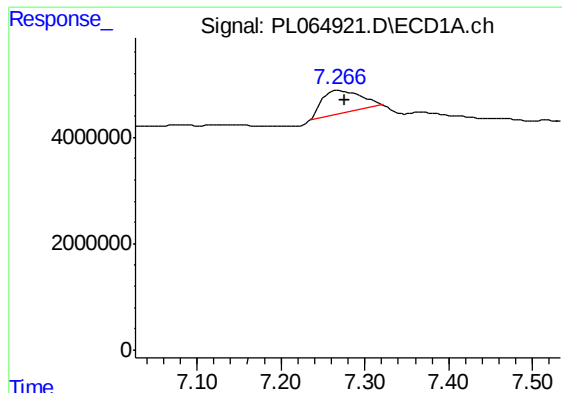

#22 Mirex


R.T.: 7.268 min
Delta R.T.: -0.008 min
Response: 14542282
Conc: 6.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-4

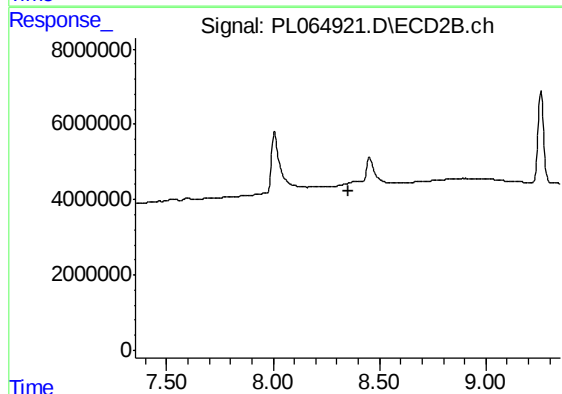


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 8.352 min
Response: 0
Conc: N.D.

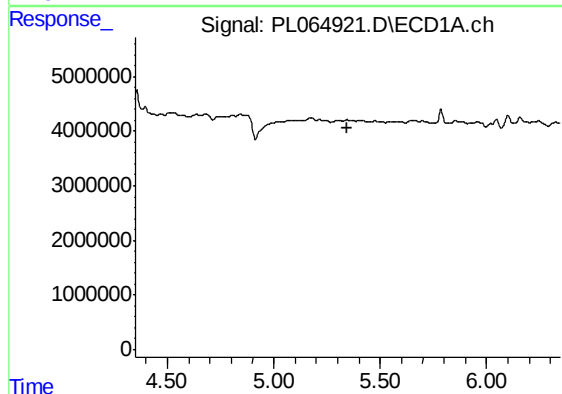


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.347 min
Response: 0
Conc: N.D.

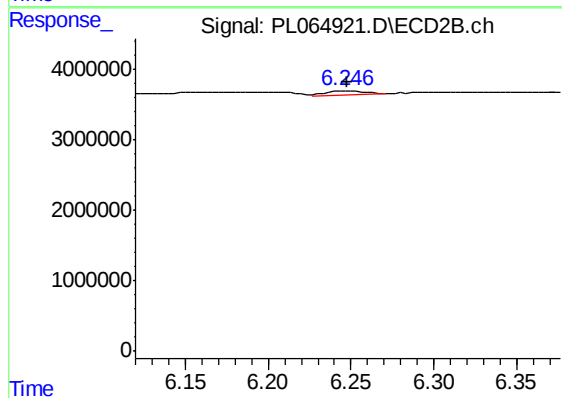

#25 Chlordane-3


R.T.: 6.248 min
Delta R.T.: 0.000 min
Response: 888804
Conc: 2.91 ng/ml

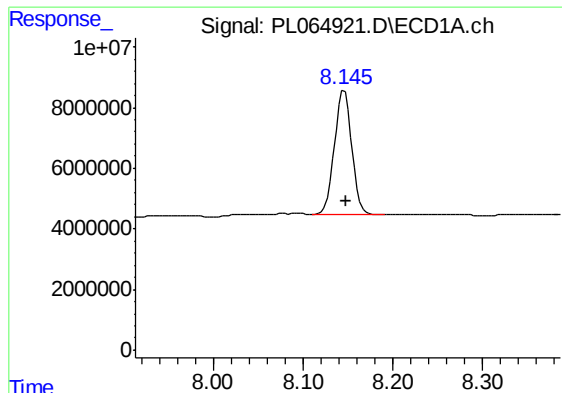

#28 Decachlorobiphenyl

R.T.: 8.146 min
Delta R.T.: -0.002 min
Response: 54858418
Conc: 24.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-4

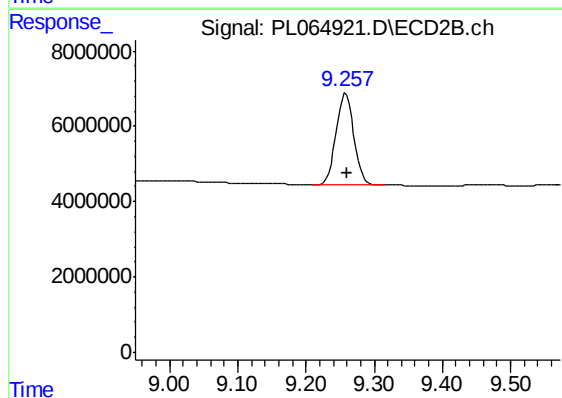

#28 Decachlorobiphenyl

R.T.: 9.258 min
Delta R.T.: -0.002 min
Response: 44012684
Conc: 23.17 ng/ml