

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022221\
 Data File : PL064922.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Feb 2021 18:47
 Operator : AR\AJ
 Sample : M1452-20
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-5

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 23 00:39:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 09 04:41:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.424	4.099	57057222	46180578	20.280	21.378
28)	SA Decachlor...	8.145	9.259	51644689	41735296	22.965	21.973
Target Compounds							
16)	A 4,4'-DDD	6.101f	0.000	1652770	0	0.653	N.D. #
22)	Mirex	7.301f	0.000	1224951	0	0.580	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022221\
Data File : PL064922.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Feb 2021 18:47
Operator : AR\AJ
Sample : M1452-20
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-5

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 23 00:39:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
Quant Title : GC Extractables
QLast Update : Tue Feb 09 04:41:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

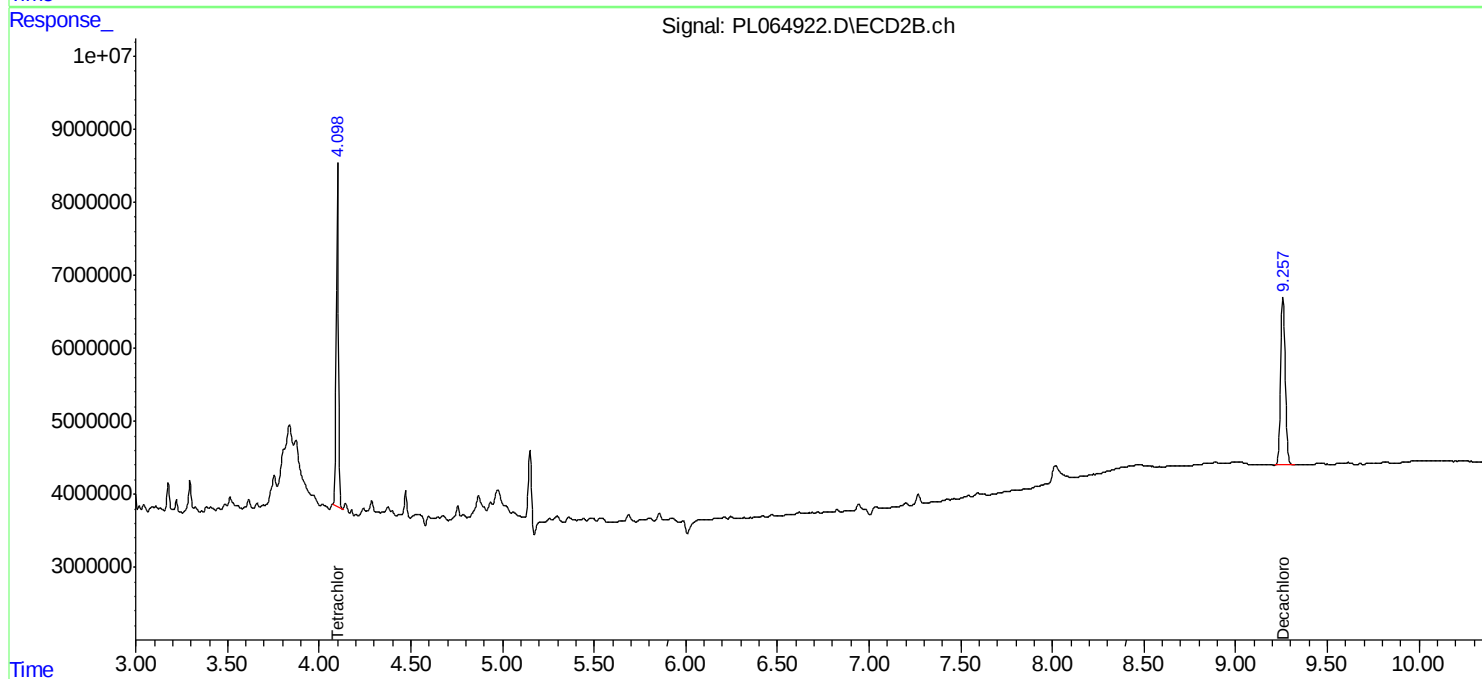


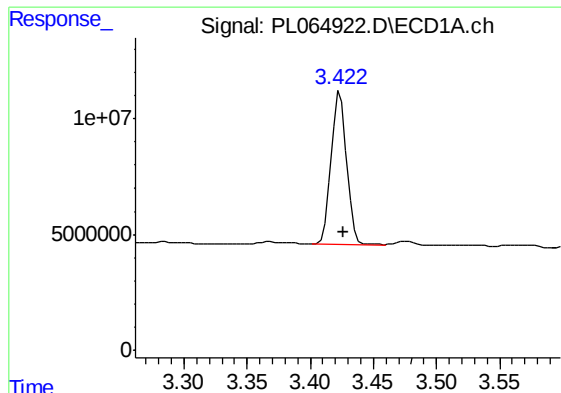

#1 Tetrachloro-m-xylene


R.T.: 3.424 min
Delta R.T.: -0.002 min
Response: 57057222
Conc: 20.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-5

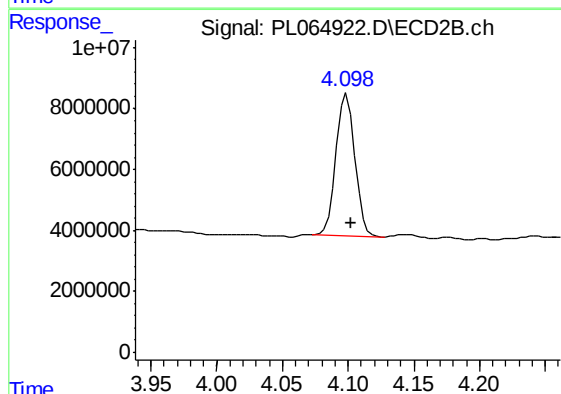


#1 Tetrachloro-m-xylene

R.T.: 4.099 min
Delta R.T.: -0.003 min
Response: 46180578
Conc: 21.38 ng/ml

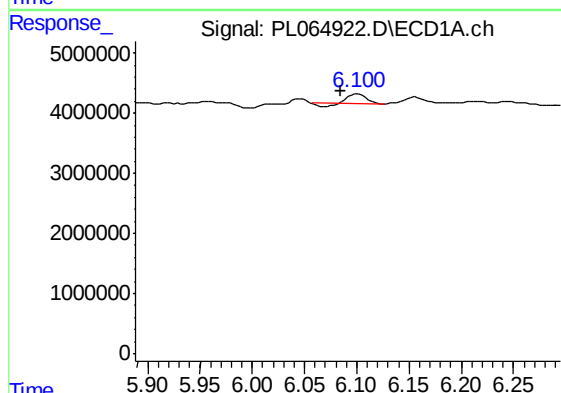


#16 4,4'-DDD

R.T.: 6.101 min
Delta R.T.: 0.016 min
Response: 1652770
Conc: 0.65 ng/ml

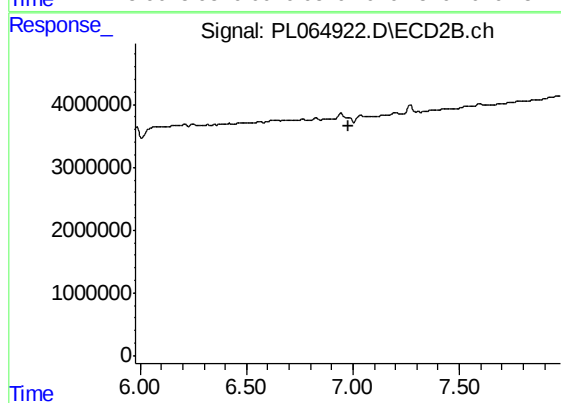

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.977 min
Response: 0
Conc: N.D.

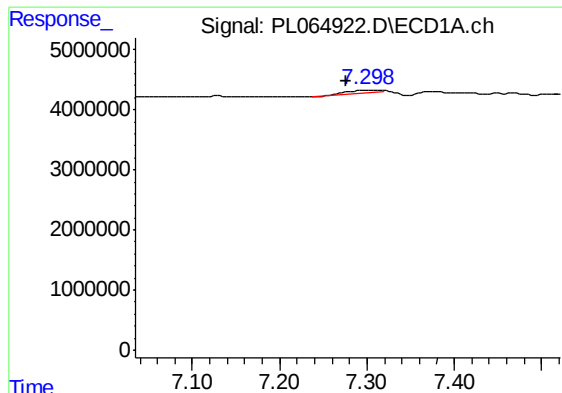

#22 Mirex


R.T.: 7.301 min
Delta R.T.: 0.025 min
Response: 1224951
Conc: 0.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-5

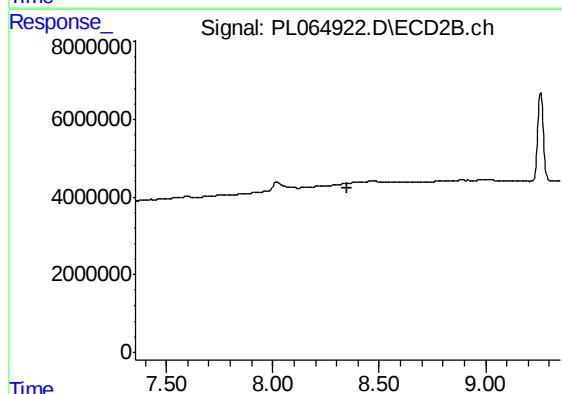


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 8.352 min
Response: 0
Conc: N.D.

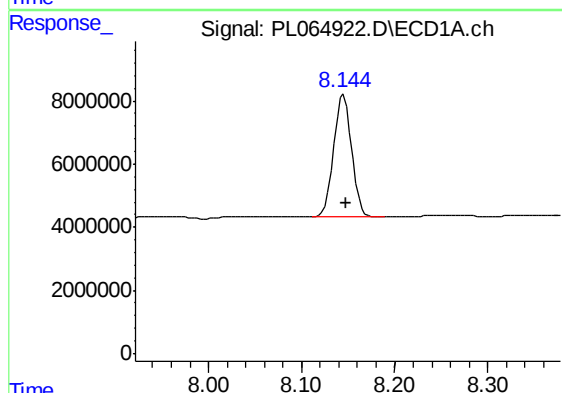

#28 Decachlorobiphenyl

R.T.: 8.145 min
Delta R.T.: -0.002 min
Response: 51644689
Conc: 22.97 ng/ml

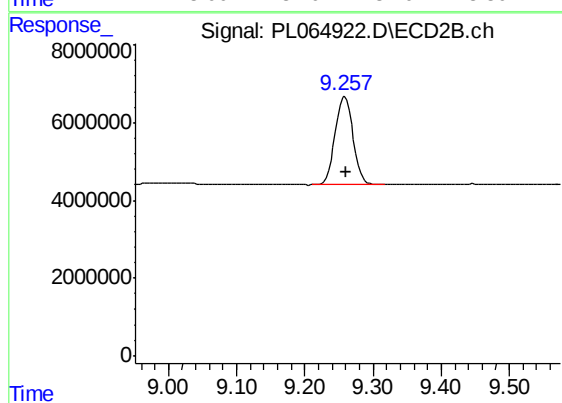

#28 Decachlorobiphenyl

R.T.: 9.259 min
Delta R.T.: -0.002 min
Response: 41735296
Conc: 21.97 ng/ml