

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022221\
 Data File : PL064924.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Feb 2021 19:16
 Operator : AR\AJ
 Sample : M1452-28
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-7

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 23 00:39:38 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 09 04:41:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.424	4.100	58425988	46751592	20.766	21.642
28)	SA Decachlor...	8.146	9.259	51317593	41003982	22.820	21.588
Target Compounds							
10)	B gamma-Chl...	0.000	6.249	0	1267061	N.D.	0.548 #
16)	A 4,4'-DDD	6.101f	0.000	527146	0	0.208	N.D. #
18)	B Endrin a...	6.410	0.000	1085858	0	0.445	N.D. #
24)	Chlordane-2	4.802f	0.000	6836336	0	55.252	N.D. #
25)	Chlordane-3	0.000	6.249	0	1267061	N.D.	4.144 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022221\
Data File : PL064924.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Feb 2021 19:16
Operator : AR\AJ
Sample : M1452-28
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-7

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 23 00:39:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
Quant Title : GC Extractables
QLast Update : Tue Feb 09 04:41:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

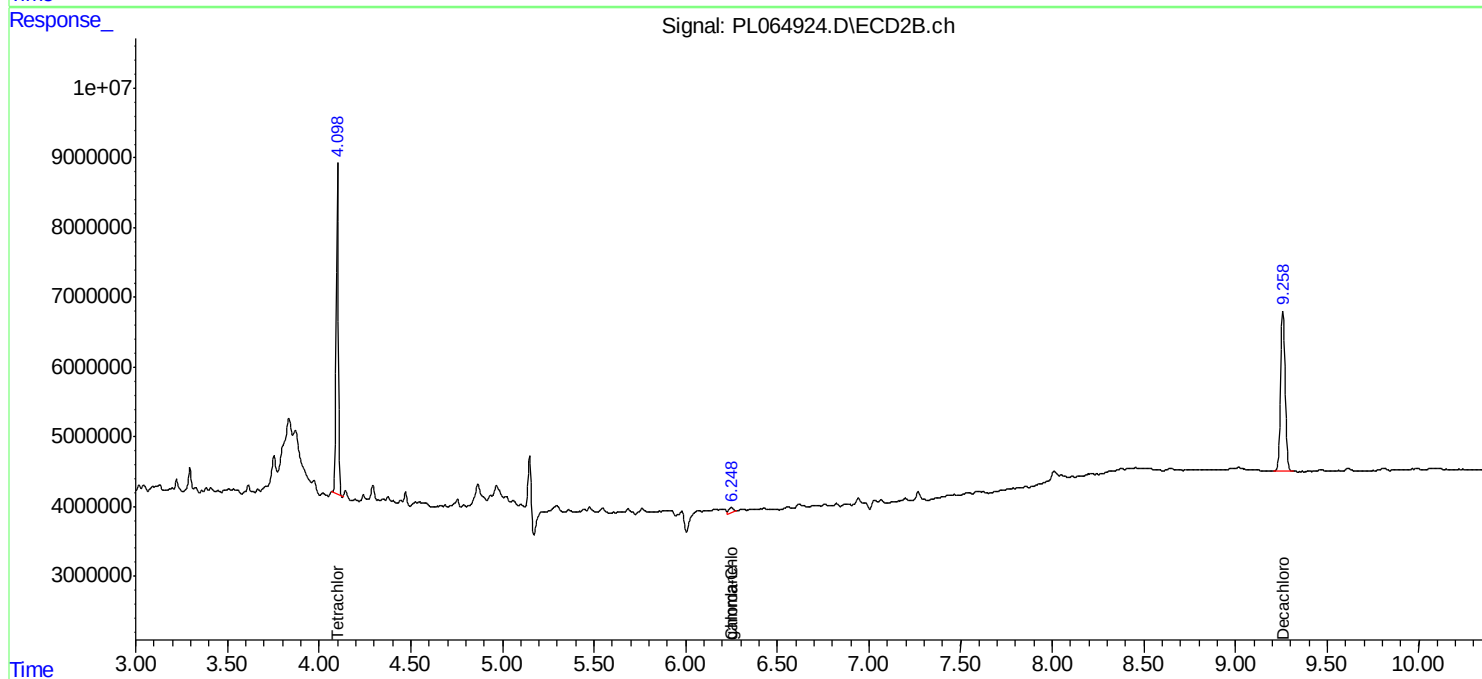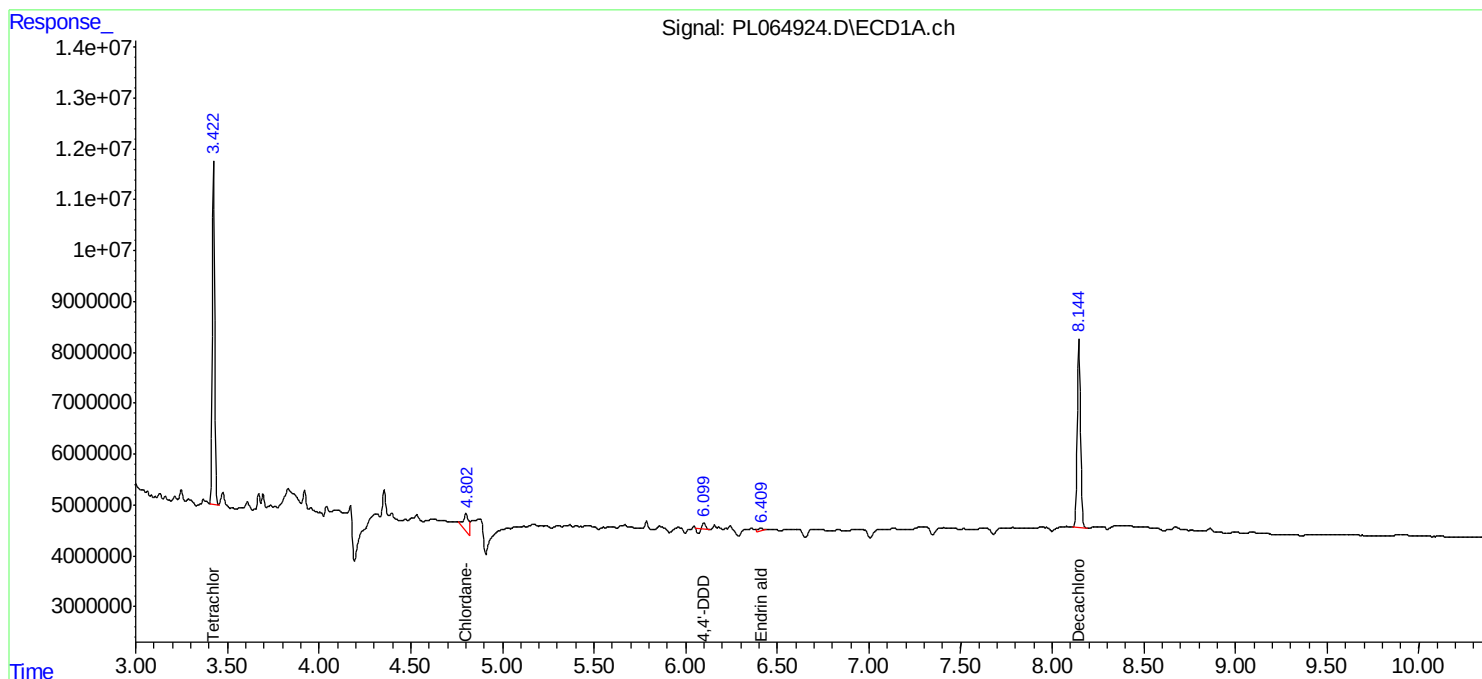


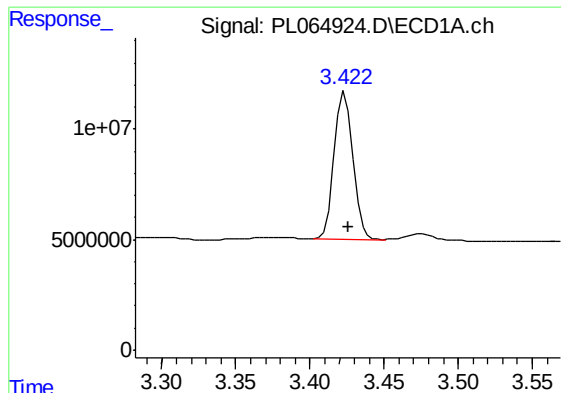

#1 Tetrachloro-m-xylene


R.T.: 3.424 min
Delta R.T.: -0.002 min
Response: 58425988
Conc: 20.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-7

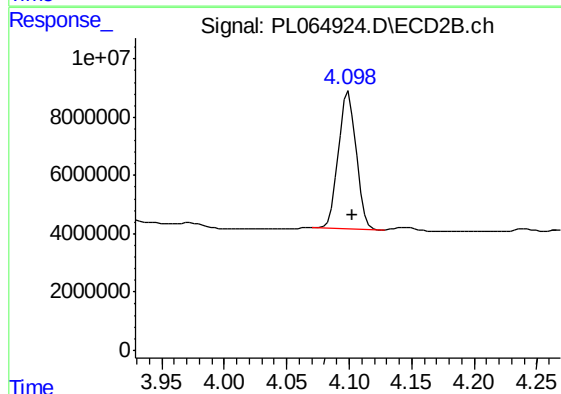


#1 Tetrachloro-m-xylene

R.T.: 4.100 min
Delta R.T.: -0.003 min
Response: 46751592
Conc: 21.64 ng/ml

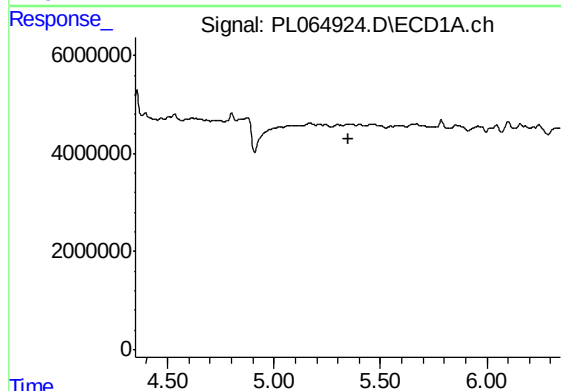


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.349 min
Response: 0
Conc: N.D.

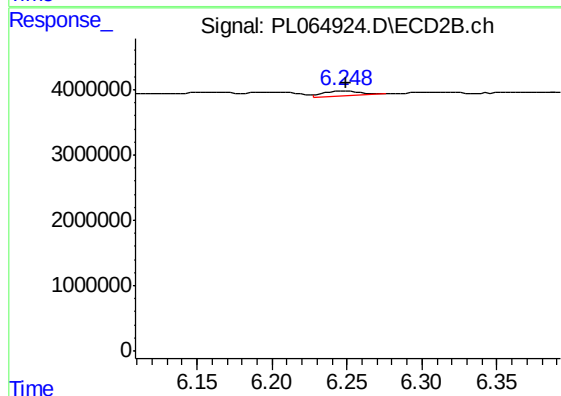

#10 gamma-Chlordane


R.T.: 6.249 min
Delta R.T.: 0.000 min
Response: 1267061
Conc: 0.55 ng/ml

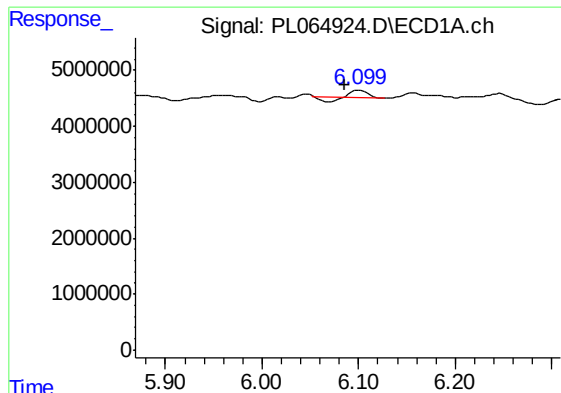

#16 4,4'-DDD


R.T.: 6.101 min
Delta R.T.: 0.015 min
Response: 527146
Conc: 0.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-7

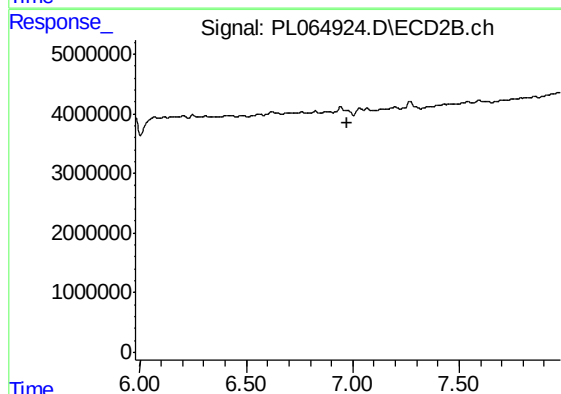


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.977 min
Response: 0
Conc: N.D.

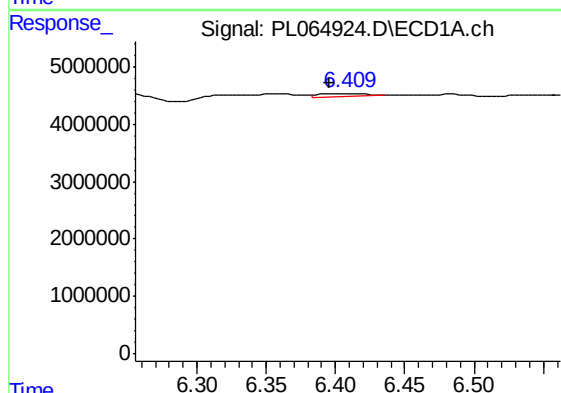


#18 Endrin aldehyde

R.T.: 6.410 min
Delta R.T.: 0.014 min
Response: 1085858
Conc: 0.45 ng/ml

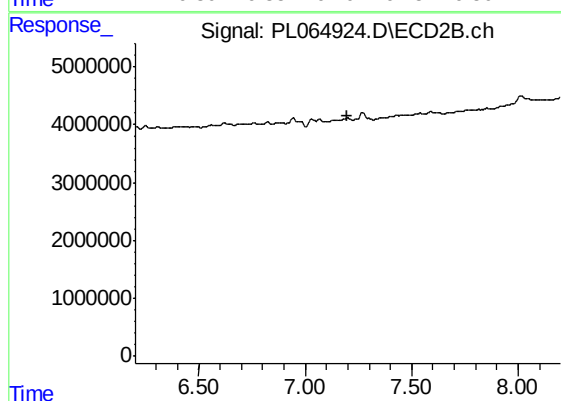

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 7.200 min
Response: 0
Conc: N.D.

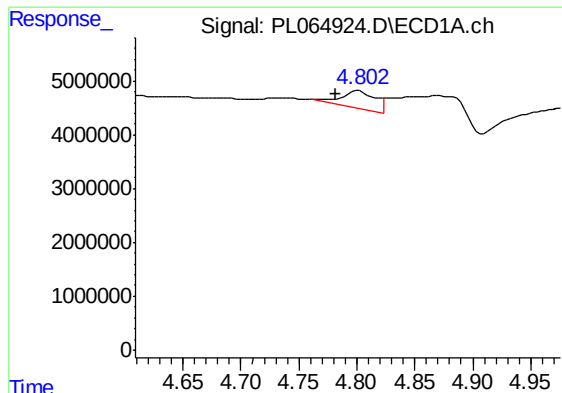

#24 Chlordane-2


R.T.: 4.802 min
Delta R.T.: 0.020 min
Response: 6836336
Conc: 55.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-7

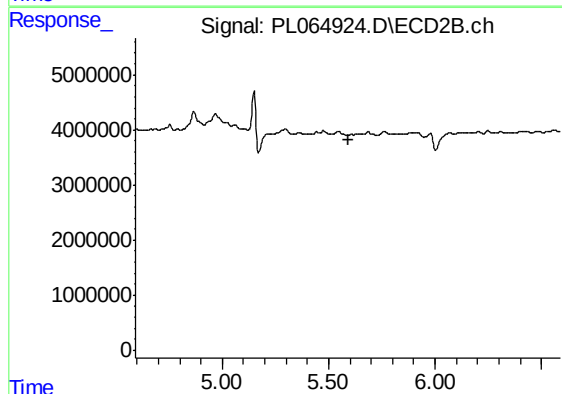


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.592 min
Response: 0
Conc: N.D.

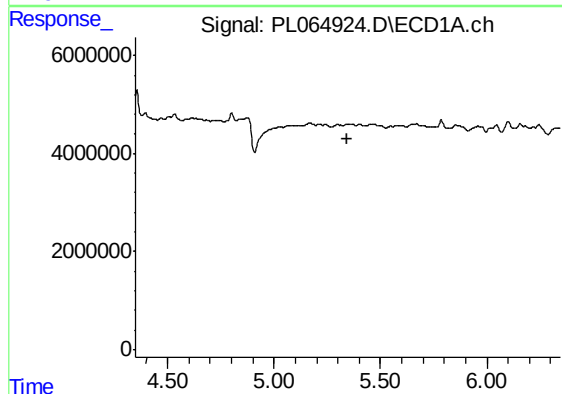


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.347 min
Response: 0
Conc: N.D.

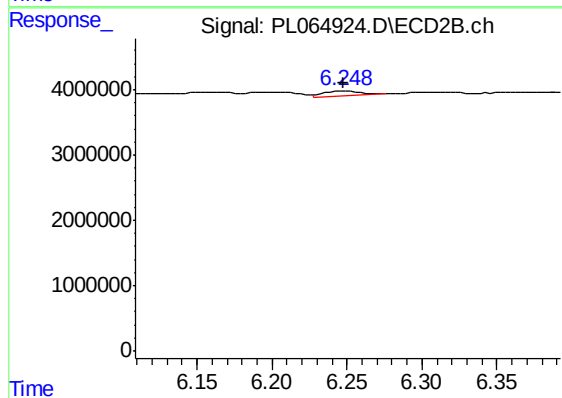

#25 Chlordane-3


R.T.: 6.249 min
Delta R.T.: 0.001 min
Response: 1267061
Conc: 4.14 ng/ml

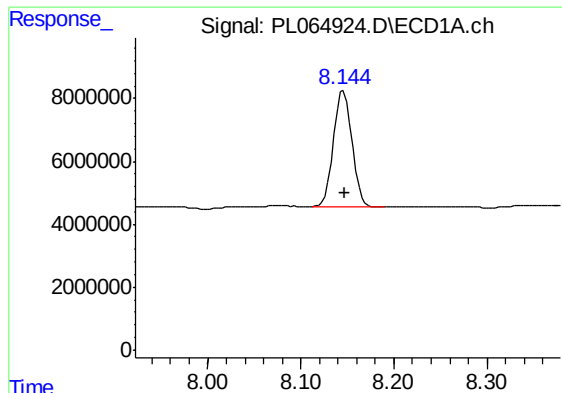

#28 Decachlorobiphenyl

R.T.: 8.146 min
Delta R.T.: -0.002 min
Response: 51317593
Conc: 22.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-7

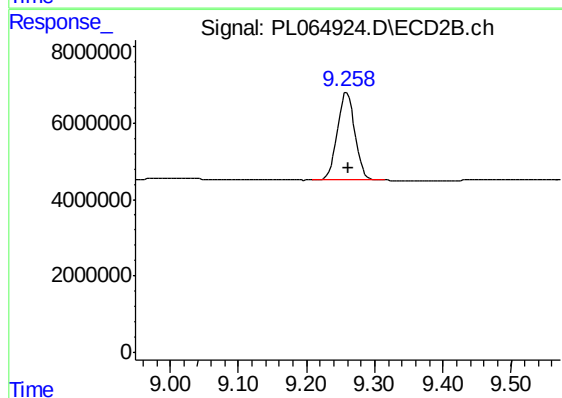

#28 Decachlorobiphenyl

R.T.: 9.259 min
Delta R.T.: -0.001 min
Response: 41003982
Conc: 21.59 ng/ml