

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022221\
 Data File : PL064902.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Feb 2021 13:51
 Operator : AR\AJ
 Sample : M1452-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-1

Manual Integrations
 APPROVED

Ankita
 2/23/2021 3:08:59 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 23 08:03:13 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 09 04:41:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.429	4.101	66658348	53661847	23.692	24.841
28)	SA Decachlor...	8.152	9.261	75441637	51499041	33.548	27.114m
Target Compounds							
17)	MA 4,4'-DDT	6.325	7.271	7434860	6764384	3.297m	4.437m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022221\
Data File : PL064902.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Feb 2021 13:51
Operator : AR\AJ
Sample : M1452-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-1


Manual Integrations
APPROVED

Ankita
2/23/2021 3:08:59 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 23 08:03:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
Quant Title : GC Extractables
QLast Update : Tue Feb 09 04:41:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

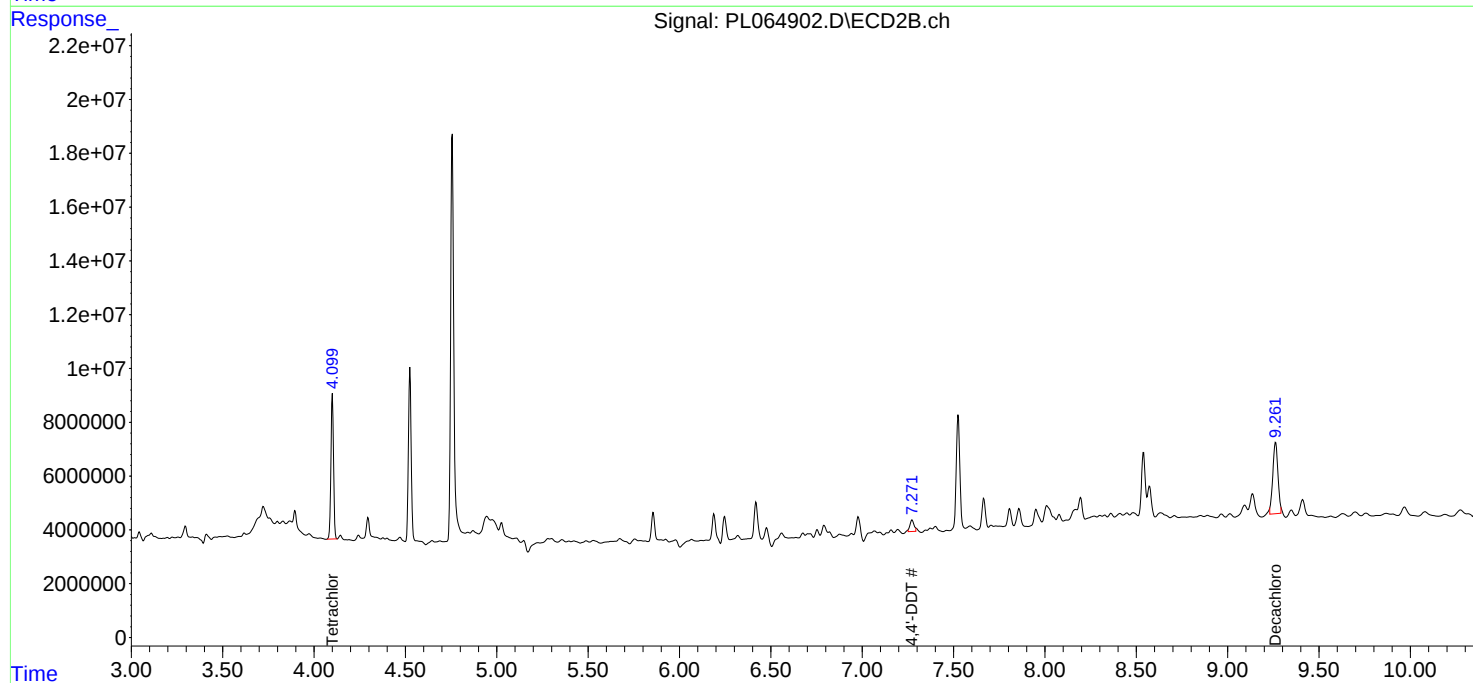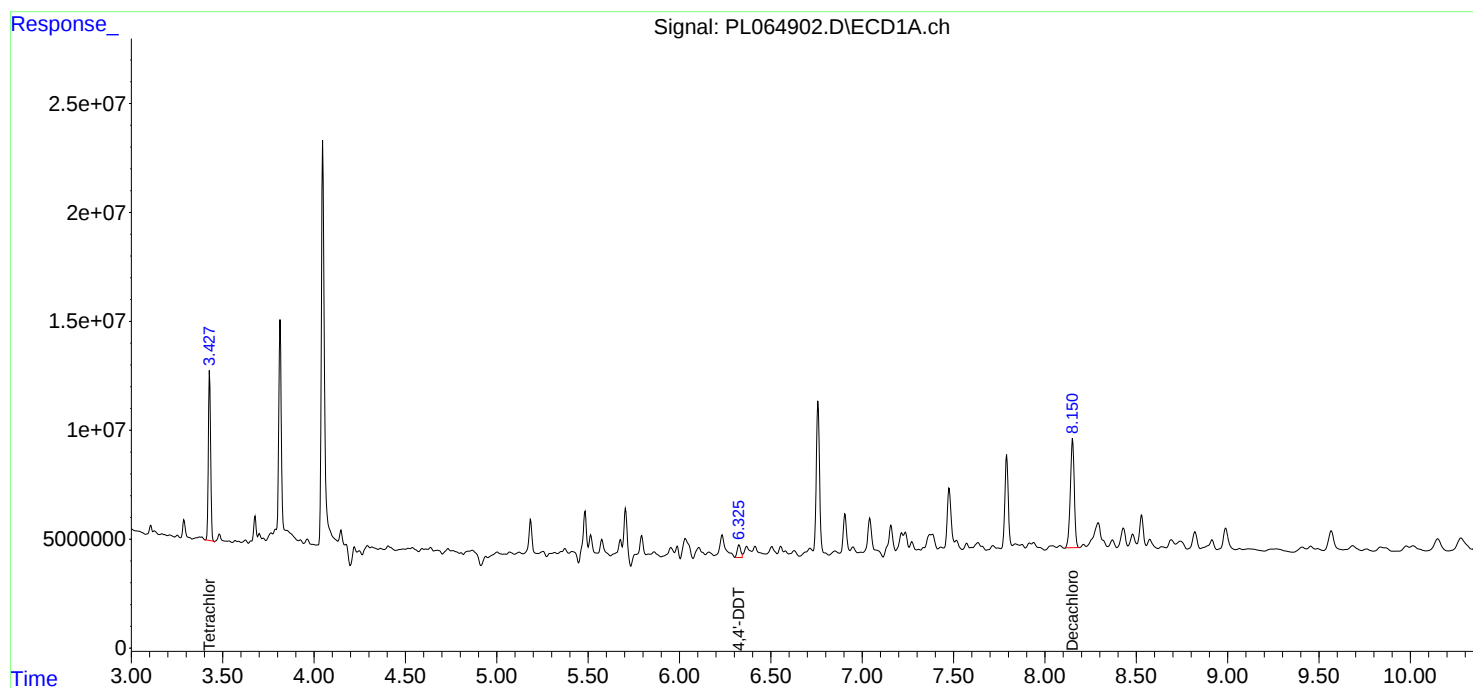

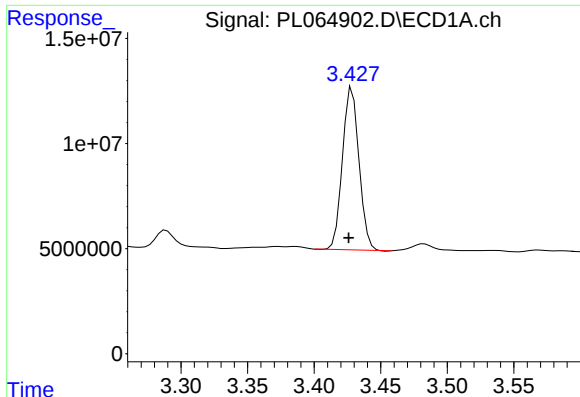


#1 Tetrachloro-m-xylene

R.T.: 3.429 min
Delta R.T.: 0.003 min
Response: 66658348
Conc: 23.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1


Manual Integrations
APPROVED

Ankita
2/23/2021 3:08:59 PM

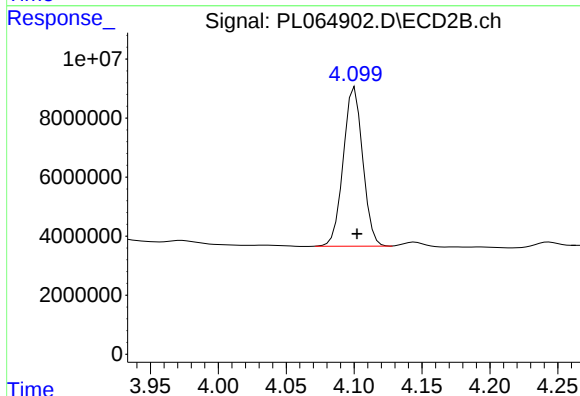


#1 Tetrachloro-m-xylene

R.T.: 4.101 min
Delta R.T.: -0.002 min
Response: 53661847
Conc: 24.84 ng/ml

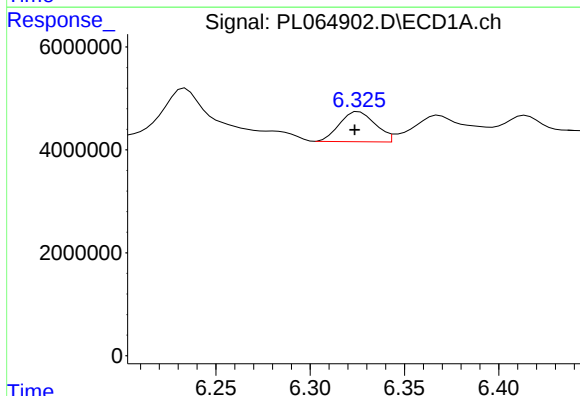


#17 4,4'-DDT

R.T.: 6.325 min
Delta R.T.: 0.000 min
Response: 7434860
Conc: 3.30 ng/ml m

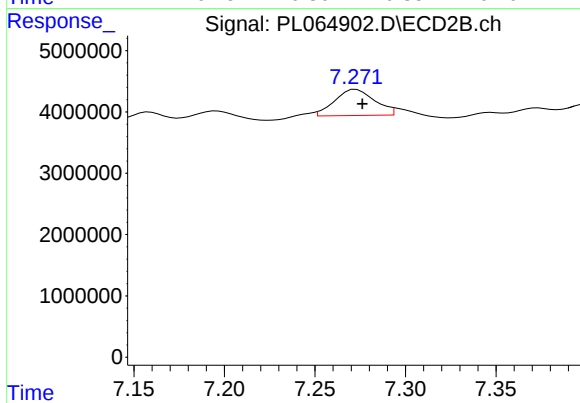

#17 4,4'-DDT

R.T.: 7.271 min
Delta R.T.: -0.005 min
Response: 6764384
Conc: 4.44 ng/ml m

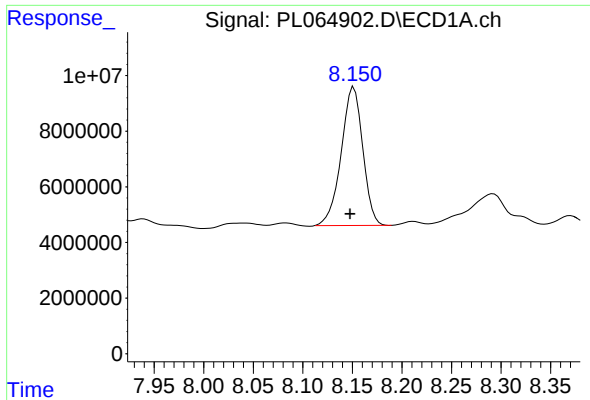


#28 Decachlorobiphenyl

R.T.: 8.152 min
Delta R.T.: 0.004 min
Response: 75441637
Conc: 33.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1

Manual Integrations
APPROVED

Ankita
2/23/2021 3:08:59 PM

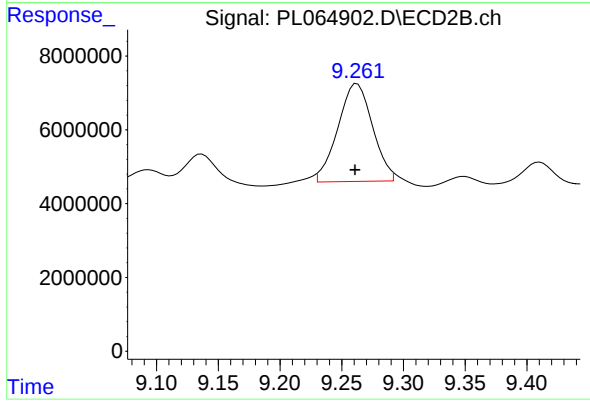

#28 Decachlorobiphenyl

R.T.: 9.261 min
Delta R.T.: 0.000 min
Response: 51499041
Conc: 27.11 ng/ml m