

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022221\
 Data File : PL064909.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Feb 2021 15:31
 Operator : AR\AJ
 Sample : M1452-21
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-6

Manual Integrations
 APPROVED

Ankita
 2/23/2021 10:20:42 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 17:20:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 09 04:41:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.424	4.100	38119711	31861462	13.549	14.749
28)	SA Decachlor...	8.146	9.258	32319394	25187043	14.372	13.261
Target Compounds							
12)	B 4,4'-DDE	5.567	6.474	1910739	1855484	0.611m	0.915m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022221\
Data File : PL064909.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Feb 2021 15:31
Operator : AR\AJ
Sample : M1452-21
Misc :
ALS Vial : 14 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampled :
TP-6


Manual Integrations
APPROVED

Ankita
2/23/2021 10:20:42 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 17:20:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
Quant Title : GC Extractables
QLast Update : Tue Feb 09 04:41:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

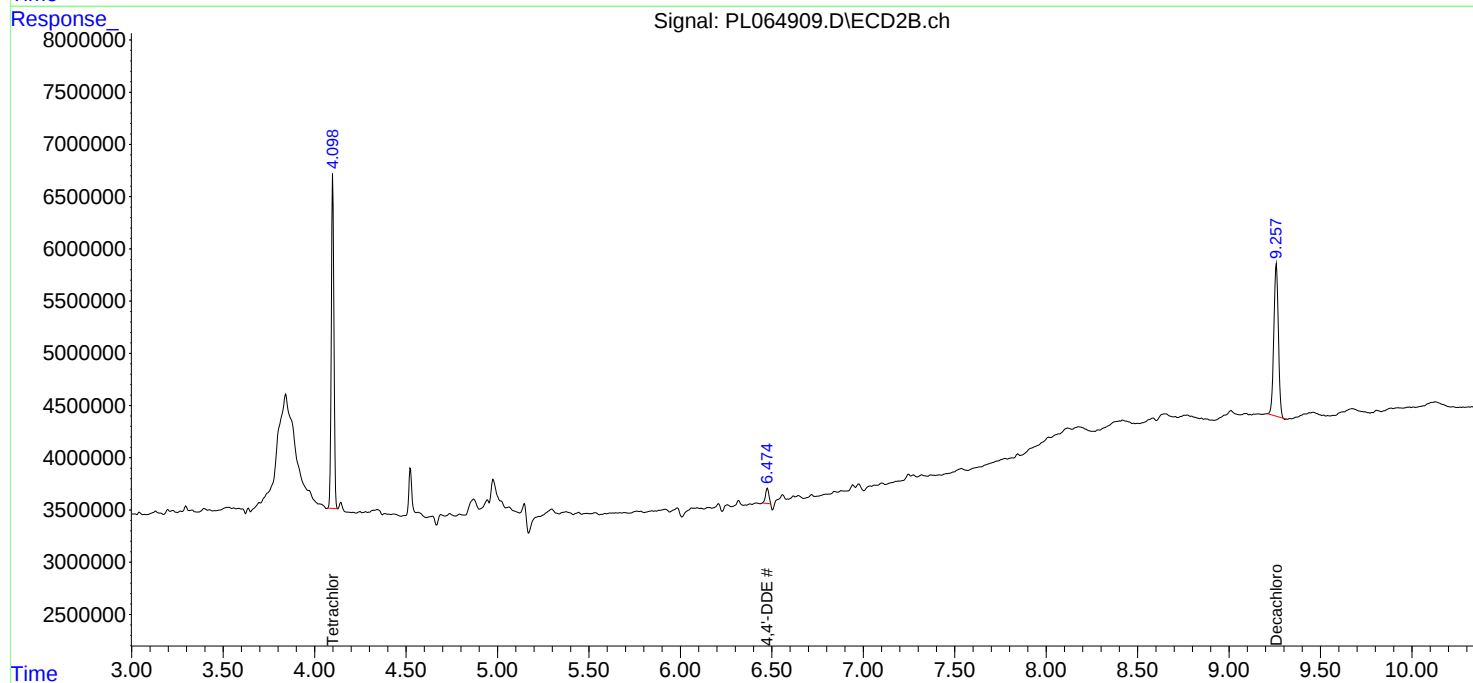

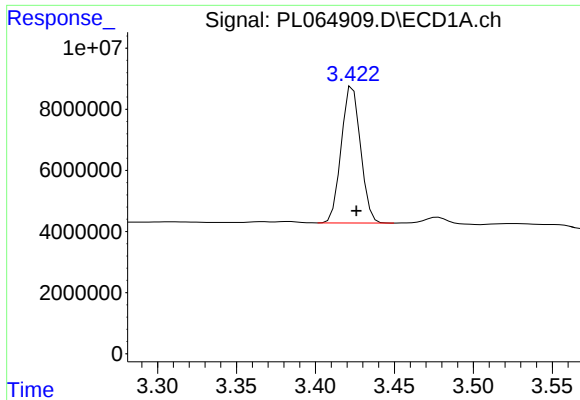


#1 Tetrachloro-m-xylene

R.T.: 3.424 min
Delta R.T.: -0.002 min
Response: 38119711
Conc: 13.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-6


Manual Integrations
APPROVED

Ankita
2/23/2021 10:20:42 AM

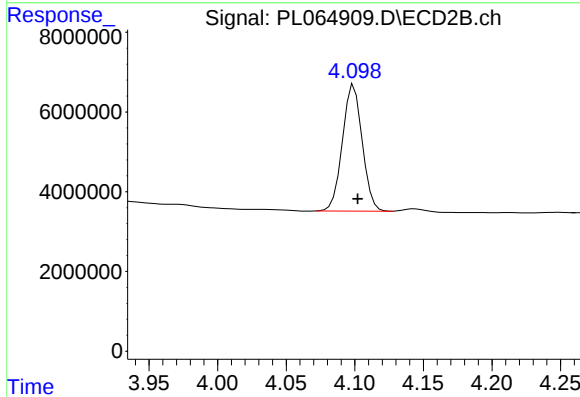


#1 Tetrachloro-m-xylene

R.T.: 4.100 min
Delta R.T.: -0.003 min
Response: 31861462
Conc: 14.75 ng/ml

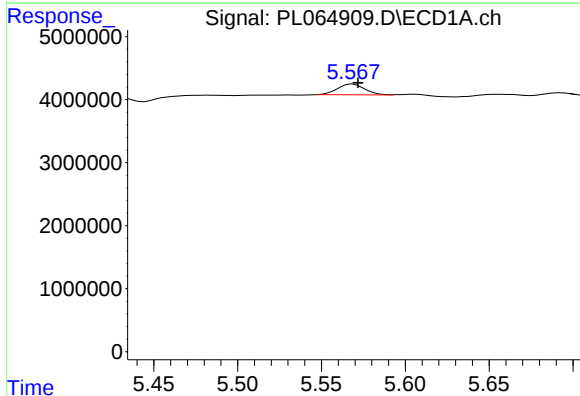


#12 4,4'-DDE

R.T.: 5.567 min
Delta R.T.: -0.004 min
Response: 1910739
Conc: 0.61 ng/ml m

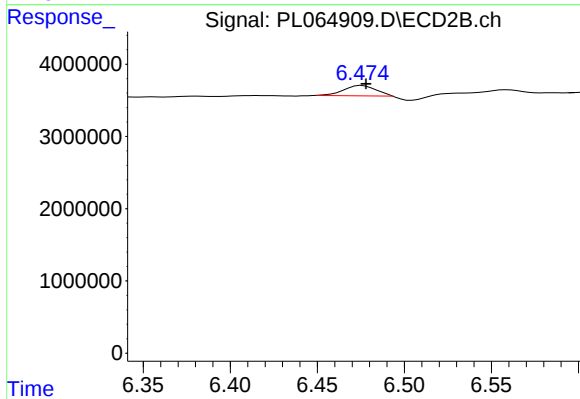

#12 4,4'-DDE

R.T.: 6.474 min
Delta R.T.: -0.004 min
Response: 1855484
Conc: 0.91 ng/ml m

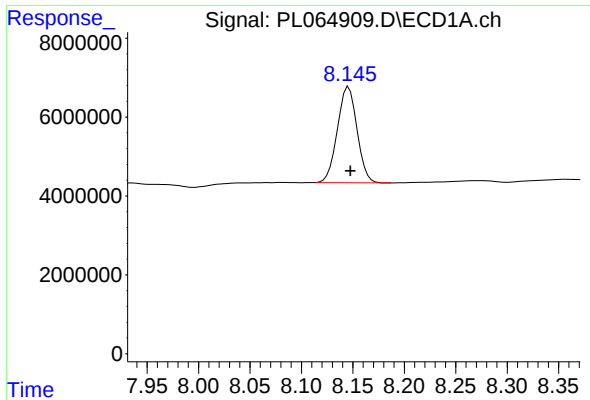


#28 Decachlorobiphenyl

R.T.: 8.146 min
Delta R.T.: -0.002 min
Response: 32319394
Conc: 14.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-6

Manual Integrations
APPROVED

Ankita
2/23/2021 10:20:42 AM

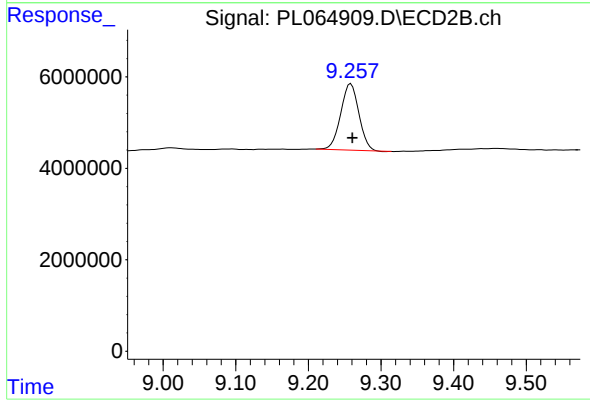

#28 Decachlorobiphenyl

R.T.: 9.258 min
Delta R.T.: -0.002 min
Response: 25187043
Conc: 13.26 ng/ml