

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022222\
 Data File : PL072915.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Feb 2022 02:15
 Operator : AR\AJ
 Sample : N1635-02
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RO-124019

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 03/03/2022
 Supervised By : Ankita Jodhani 03/04/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 23 05:41:25 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020722.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 08 05:14:10 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.550	5.487	5003226	14998727	10.391m	8.683m
2) SA Decachlor...	10.312	11.380	7123042	15309436	9.409	9.654

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022222\
Data File : PL072915.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Feb 2022 02:15
Operator : AR\AJ
Sample : N1635-02
Misc :
ALS Vial : 38 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
RO-124019


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 03/03/2022
Supervised By : Ankita Jodhani 03/04/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 23 05:41:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020722.M
Quant Title : GC Extractables
QLast Update : Tue Feb 08 05:14:10 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

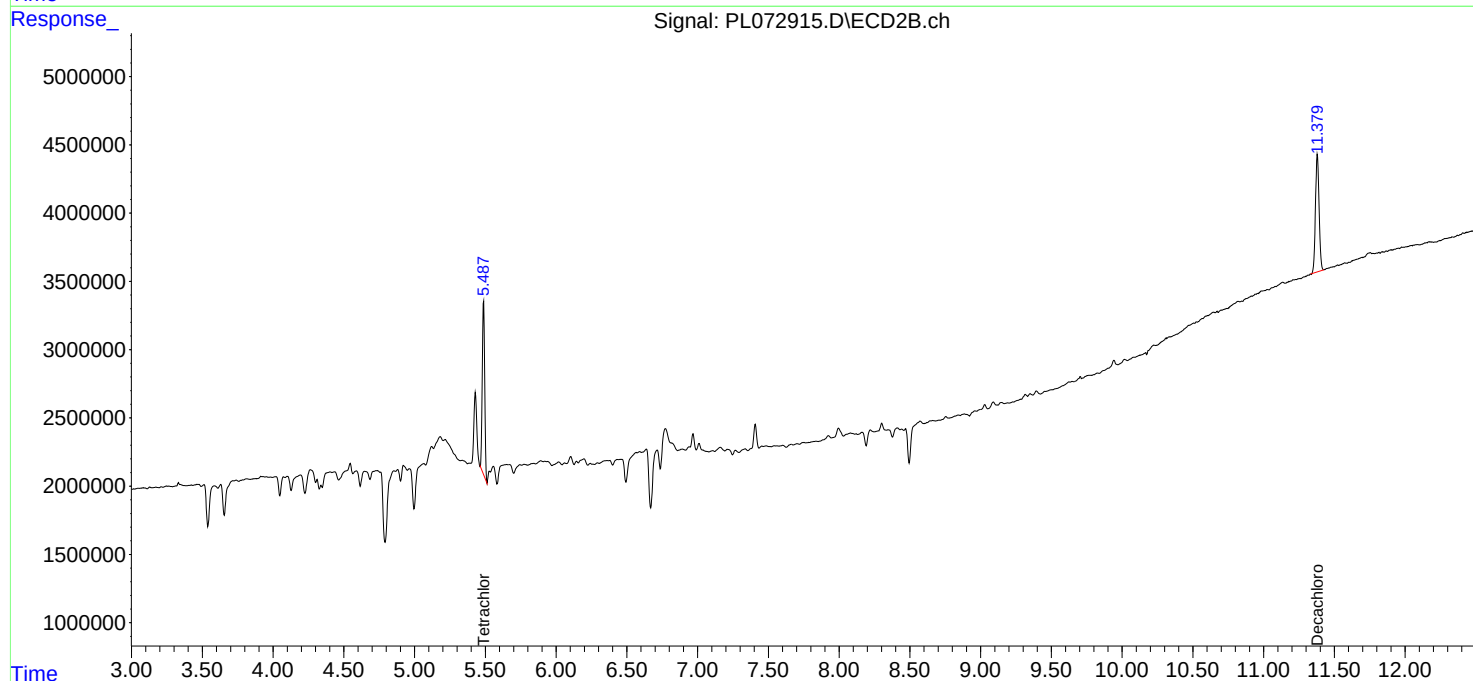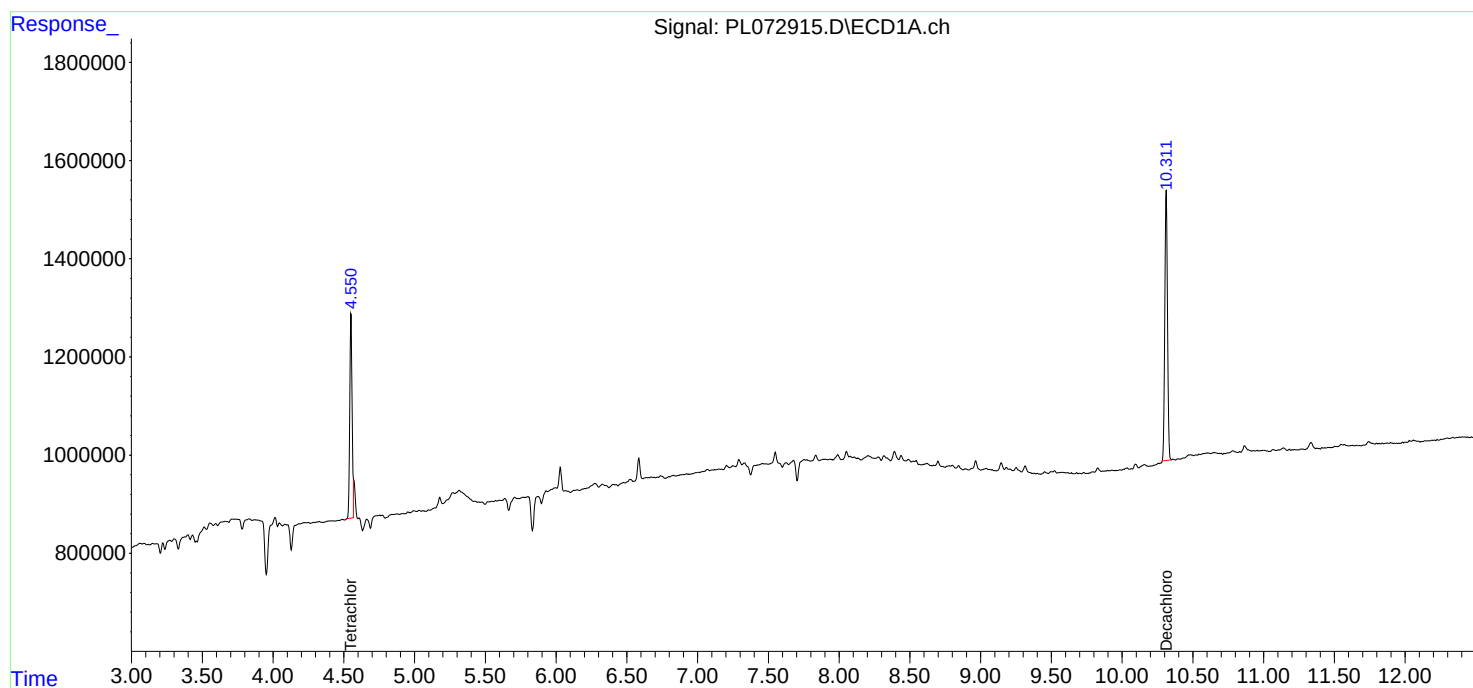

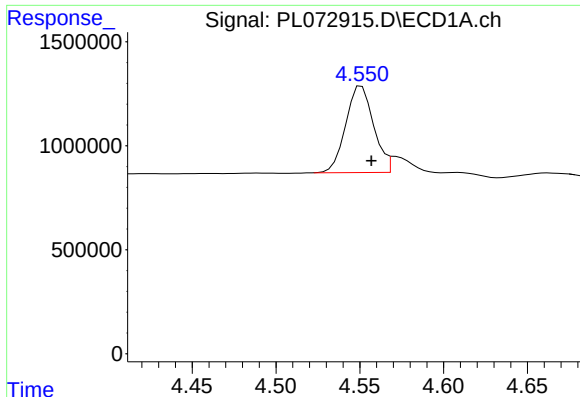


#1 Tetrachloro-m-xylene

R.T.: 4.550 min
Delta R.T.: -0.007 min
Response: 5003226
Conc: 10.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
RO-124019


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/03/2022
Supervised By :Ankita Jodhani 03/04/2022

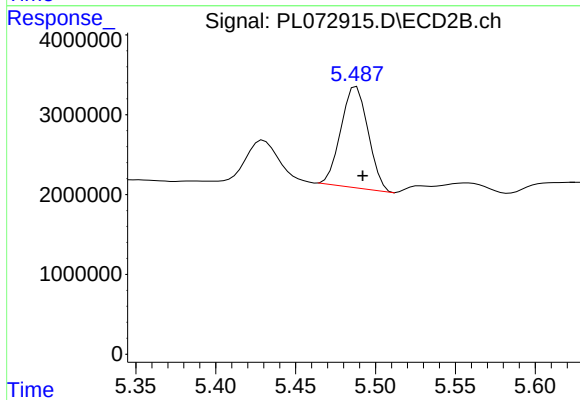


#1 Tetrachloro-m-xylene

R.T.: 5.487 min
Delta R.T.: -0.005 min
Response: 14998727
Conc: 8.68 ng/ml m

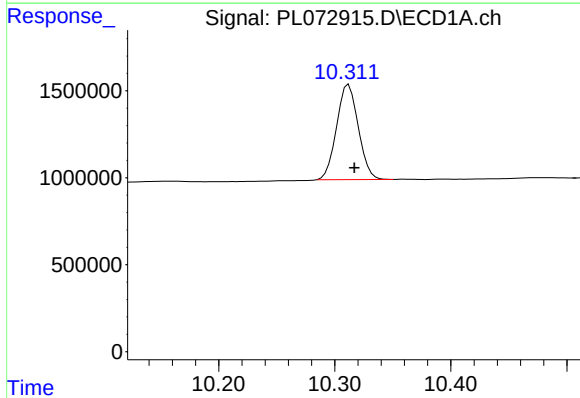

#28 Decachlorobiphenyl

R.T.: 10.312 min
Delta R.T.: -0.005 min
Response: 7123042
Conc: 9.41 ng/ml

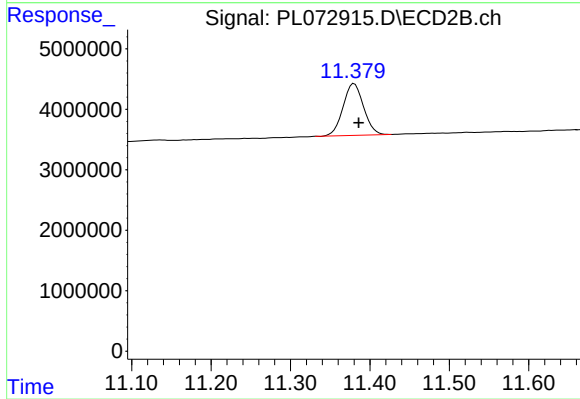

#28 Decachlorobiphenyl

R.T.: 11.380 min
Delta R.T.: -0.006 min
Response: 15309436
Conc: 9.65 ng/ml