

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022223\
 Data File : PL081078.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Feb 2023 13:57
 Operator : AR\AJ
 Sample : 01639-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TR-05-02212023

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 02/23/2023
 Supervised By : Ankita Jodhani 02/23/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 20:16:10 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022023.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 20 18:06:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.352	2.687	19533918	19096261	8.380	8.299
28)	SA Decachlor...	8.789	7.832	19813152	21834654	10.134	9.321
Target Compounds							
12)	B 4,4'-DDE	5.986	5.144	1781260	1723859	0.720m	0.722

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022223\
Data File : PL081078.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Feb 2023 13:57
Operator : AR\AJ
Sample : 01639-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TR-05-02212023


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 02/23/2023
Supervised By : Ankita Jodhani 02/23/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 20:16:10 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022023.M
Quant Title : GC Extractables
QLast Update : Mon Feb 20 18:06:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

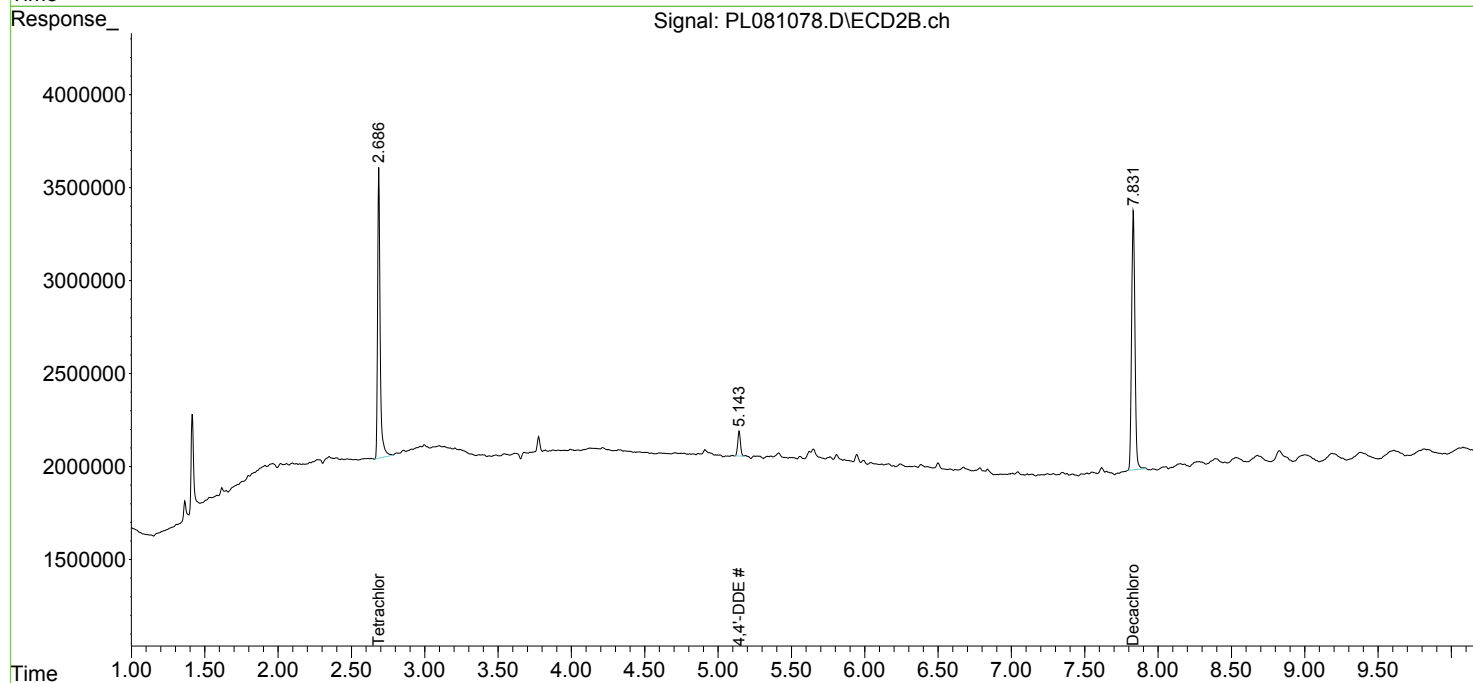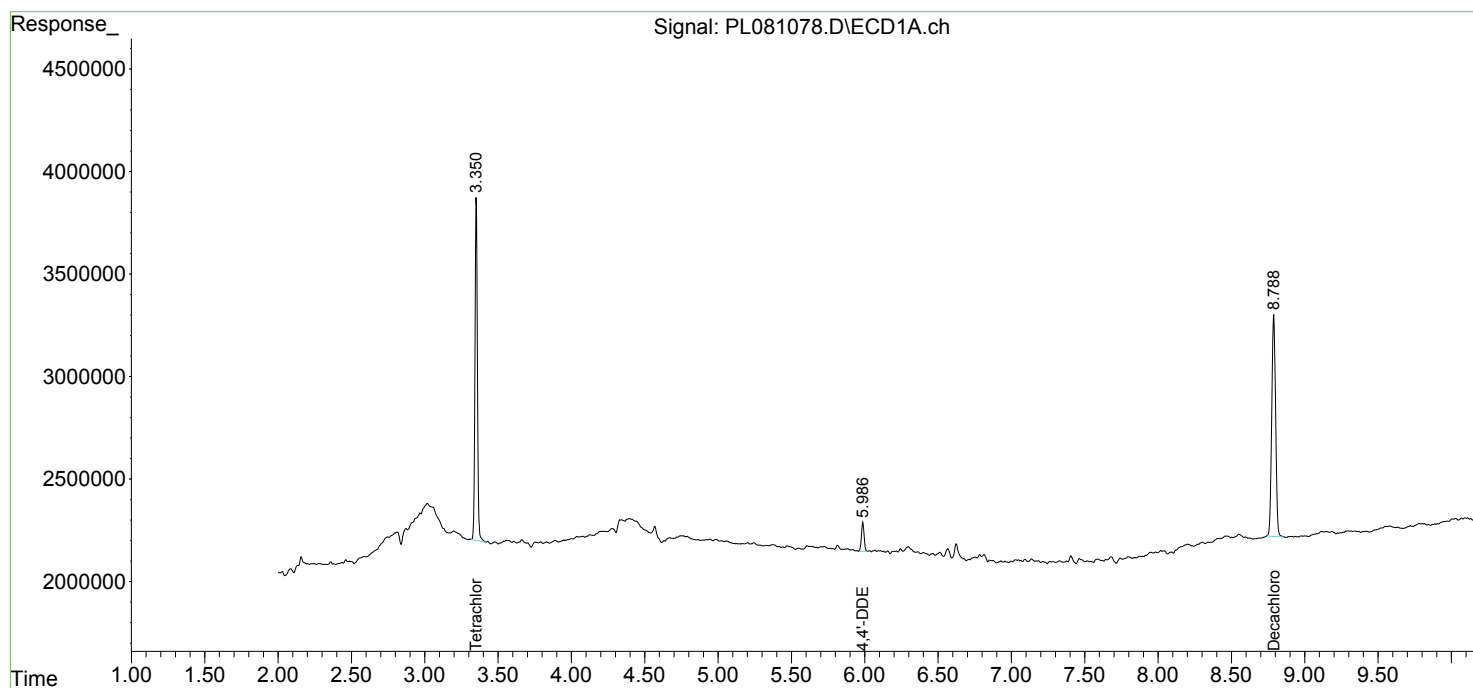

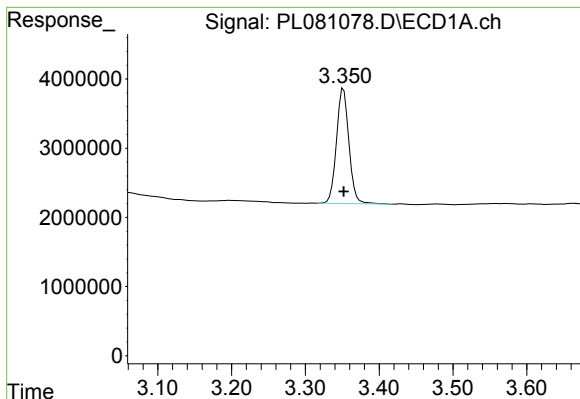


#1 Tetrachloro-m-xylene

R.T.: 3.352 min
Delta R.T.: 0.000 min
Response: 19533918
Conc: 8.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-05-02212023


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/23/2023
Supervised By :Ankita Jodhani 02/23/2023

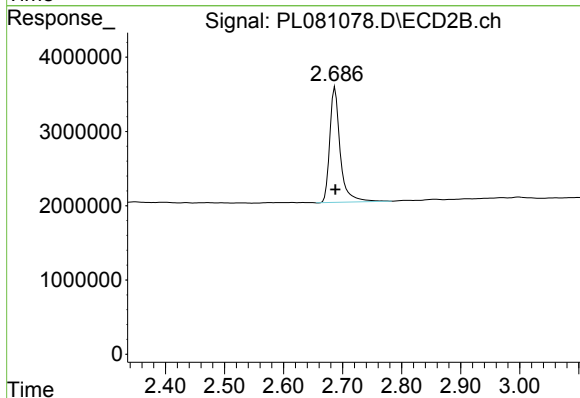


#1 Tetrachloro-m-xylene

R.T.: 2.687 min
Delta R.T.: 0.000 min
Response: 19096261
Conc: 8.30 ng/ml

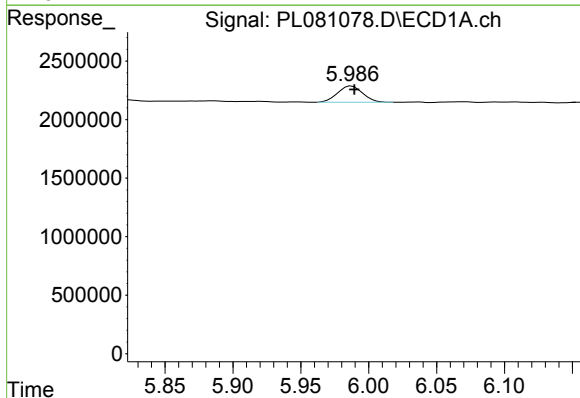


#12 4,4'-DDE

R.T.: 5.986 min
Delta R.T.: -0.003 min
Response: 1781260
Conc: 0.72 ng/ml m

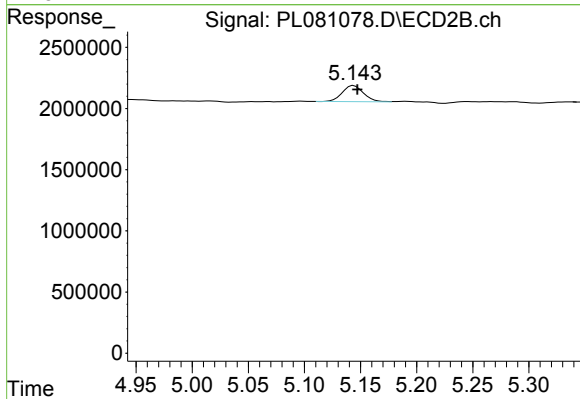

#12 4,4'-DDE

R.T.: 5.144 min
Delta R.T.: -0.003 min
Response: 1723859
Conc: 0.72 ng/ml

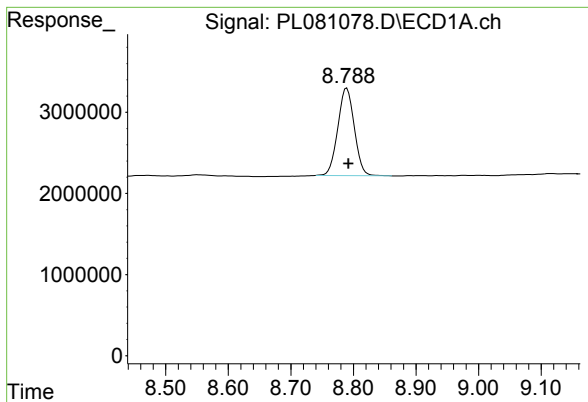


#28 Decachlorobiphenyl

R.T.: 8.789 min
Delta R.T.: -0.003 min
Response: 19813152
Conc: 10.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-05-02212023

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/23/2023
Supervised By :Ankita Jodhani 02/23/2023

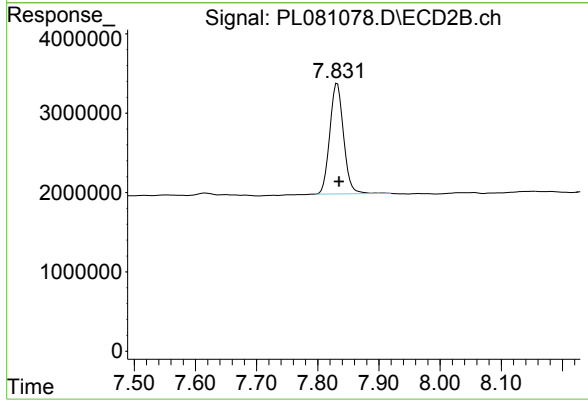

#28 Decachlorobiphenyl

R.T.: 7.832 min
Delta R.T.: -0.003 min
Response: 21834654
Conc: 9.32 ng/ml