

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022224\
 Data File : PL088222.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Feb 2024 16:41
 Operator : AR\AJ
 Sample : P1538-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 20241096-COMPOSITE-35N-N-4-01

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 02/23/2024
 Supervised By :Ankita Jodhani 02/23/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 21:02:21 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021524.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 16 21:46:54 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.634	2.853	38438753	19829763	13.994m	14.139
28) SA Decachlor...	9.305	8.086	15795501	9475343	8.201	7.442

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022224\
Data File : PL088222.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Feb 2024 16:41
Operator : AR\AJ
Sample : P1538-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
20241096-COMPOSITE-35N-N-4-01


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 02/23/2024
Supervised By : Ankita Jodhani 02/23/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 21:02:21 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021524.M
Quant Title : GC Extractables
QLast Update : Fri Feb 16 21:46:54 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

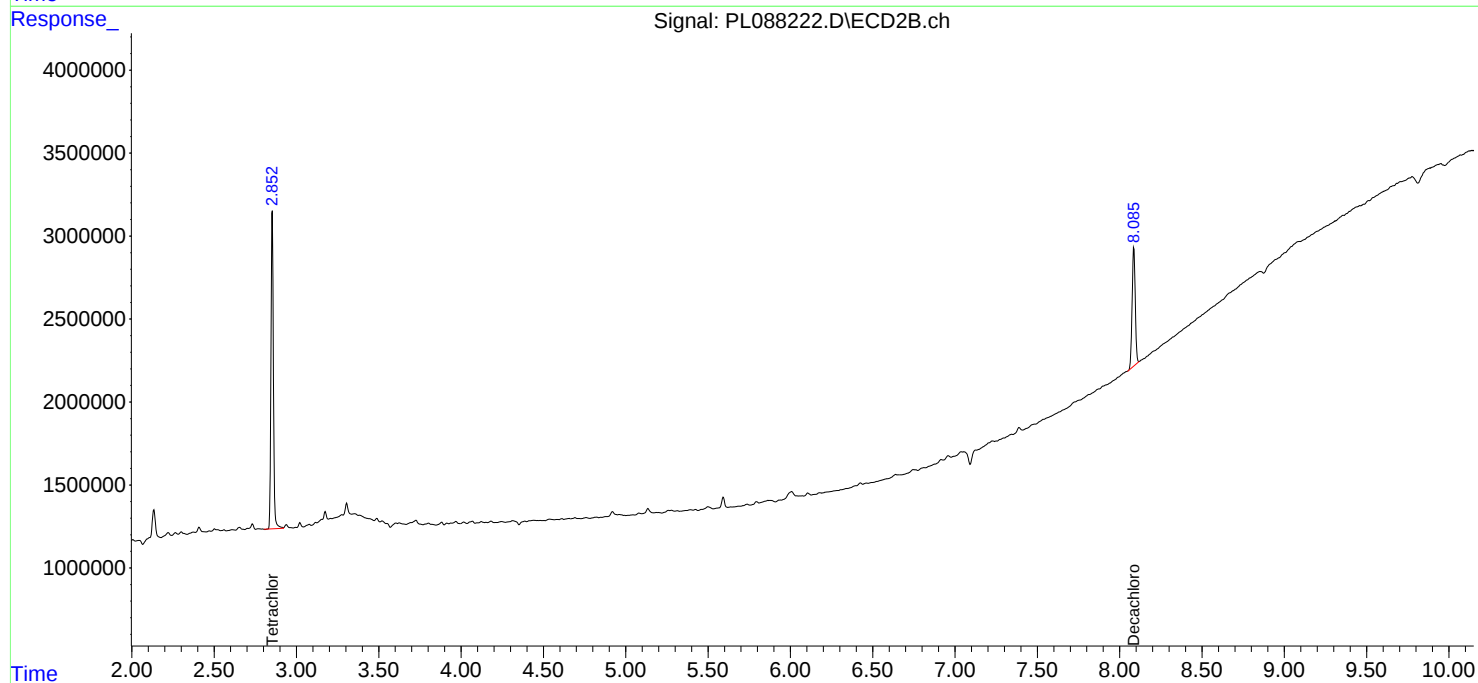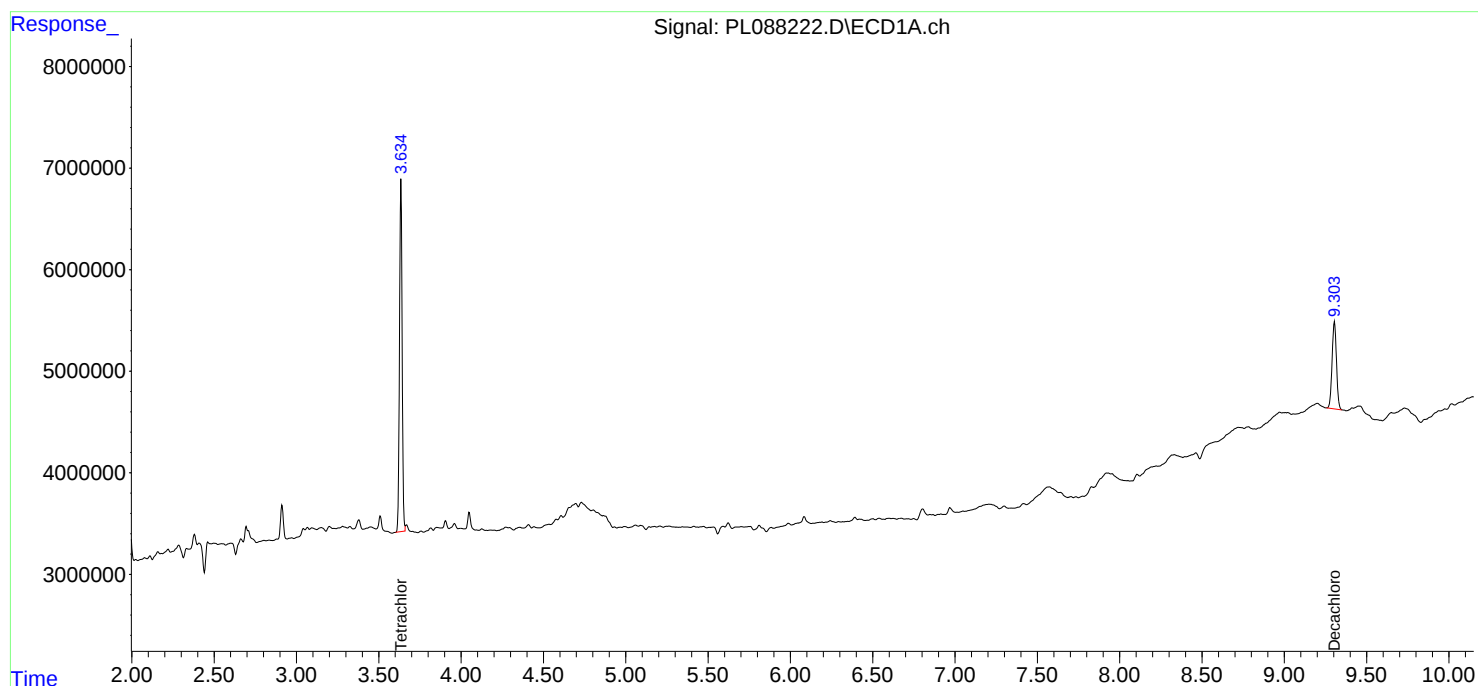

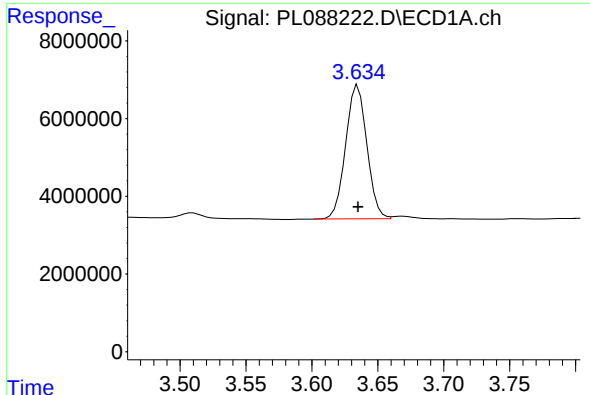


#1 Tetrachloro-m-xylene

R.T.: 3.634 min
Delta R.T.: -0.001 min
Response: 38438753
Conc: 13.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
20241096-COMPOSITE-35N-N-4-01


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/23/2024
Supervised By :Ankita Jodhani 02/23/2024

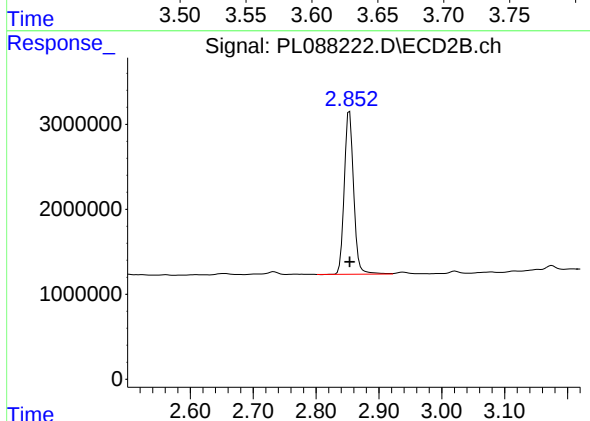


#1 Tetrachloro-m-xylene

R.T.: 2.853 min
Delta R.T.: 0.000 min
Response: 19829763
Conc: 14.14 ng/ml

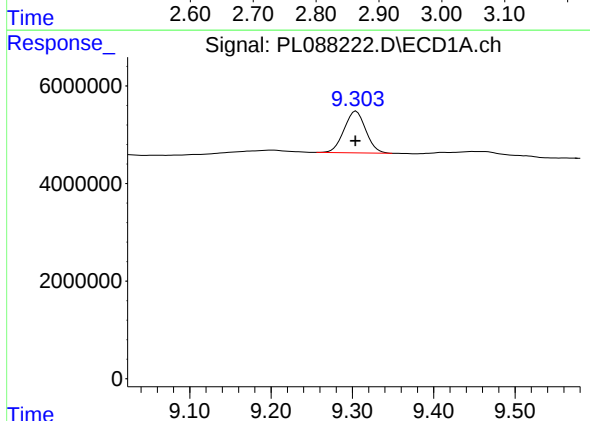

#28 Decachlorobiphenyl

R.T.: 9.305 min
Delta R.T.: 0.000 min
Response: 15795501
Conc: 8.20 ng/ml

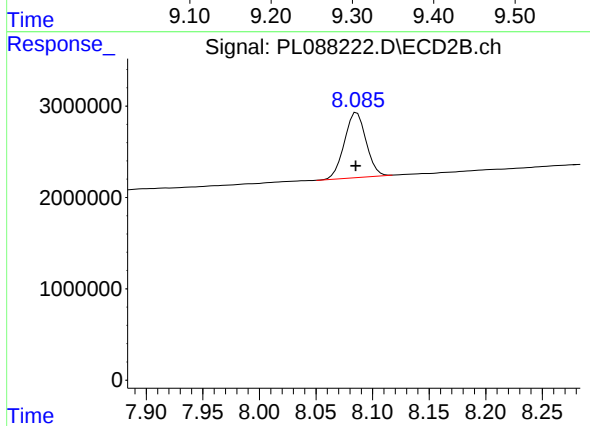

#28 Decachlorobiphenyl

R.T.: 8.086 min
Delta R.T.: 0.000 min
Response: 9475343
Conc: 7.44 ng/ml