

Data Path : P:\HPCHEM1\ECD_L\Data\PL022318\
 Data File : PL033316.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Feb 2018 12:52
 Operator : UA\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 23 13:10:57 2018
 Quant Method : P:\HPCHEM1\ECD_L\methods\PL022318.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 23 13:10:27 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	3.402	3.985	310.1E6	78163434	50.000	50.000
28)	SA Decachlor...	8.102	9.008	362.5E6	73485071	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.259	4.971	145.3E6	38636697	500.000	500.000
24)	Chlordane-2	4.754	5.434	162.2E6	42057979	500.000	500.000
25)	Chlordane-3	5.313	6.074	895.2E6	132.3E6	952.451	500.000 #
26)	Chlordane-4	5.370	6.150	466.8E6	157.2E6	500.000	500.000
27)	Chlordane-5	5.980	6.940	75867373	31212362	500.000	500.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD_L\Data\PL022318\
Data File : PL033316.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Feb 2018 12:52
Operator : UA\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 23 13:10:57 2018
Quant Method : P:\HPCHEM1\ECD_L\methods\PL022318.M
Quant Title : GC Extractables
QLast Update : Fri Feb 23 13:10:27 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

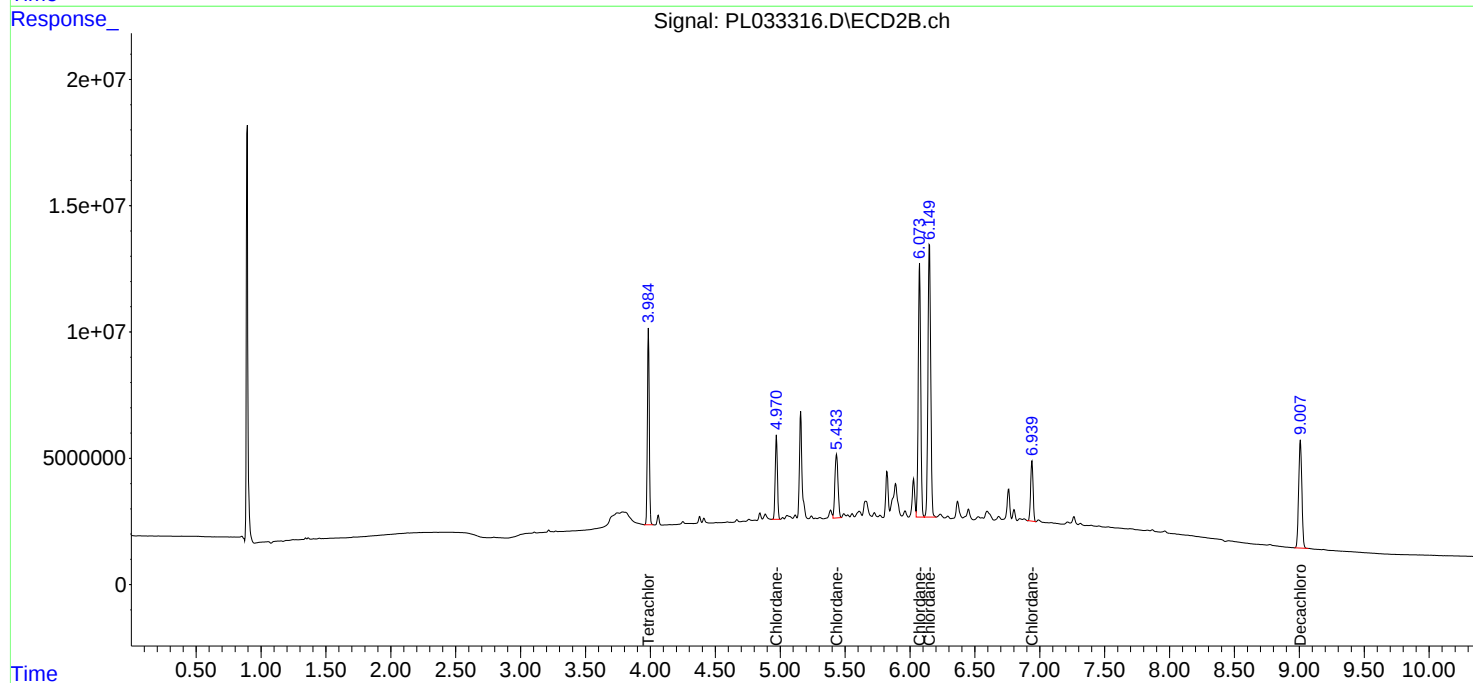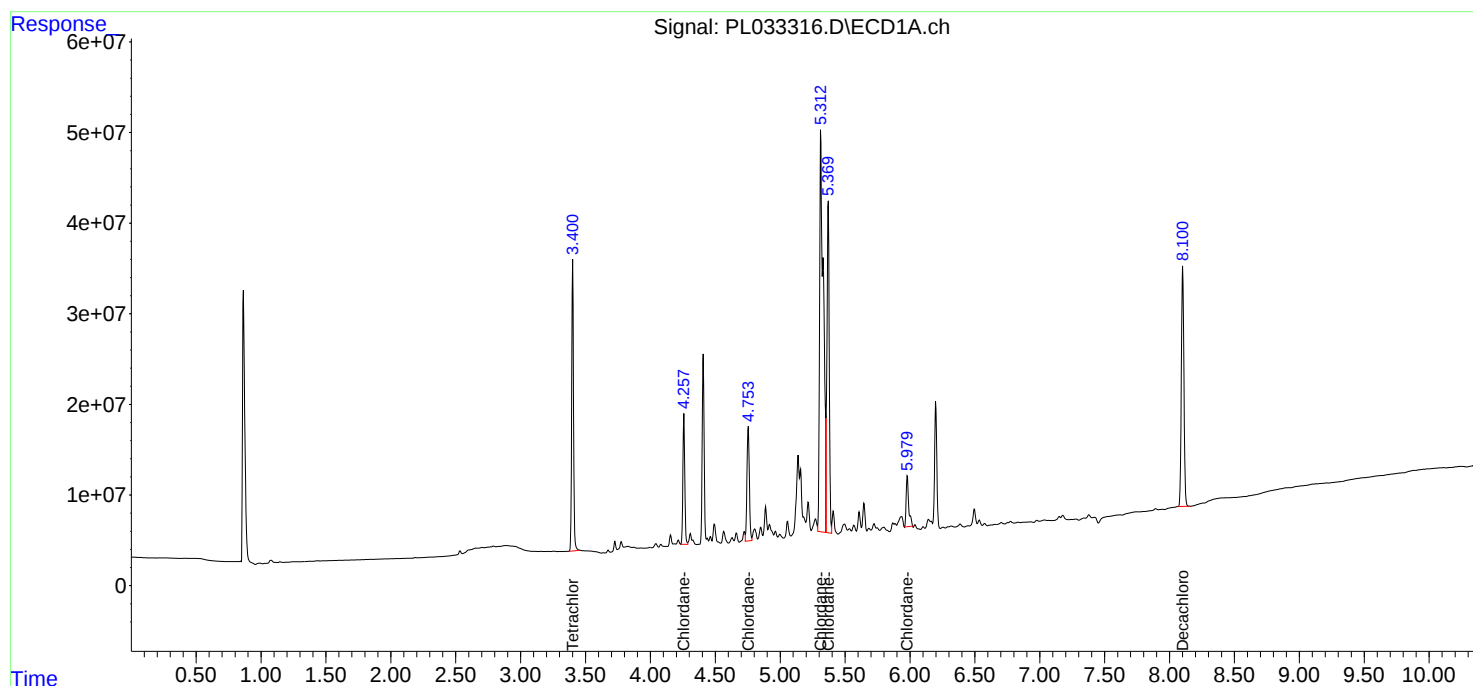

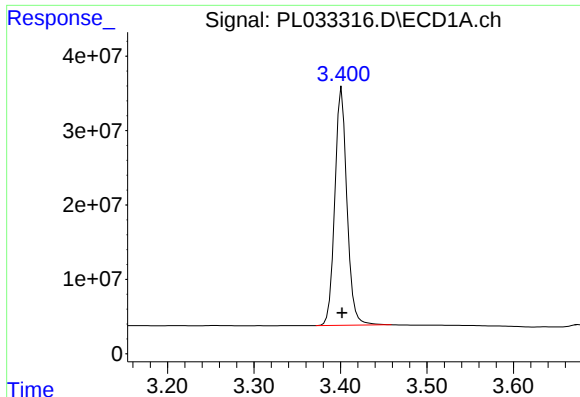


#1 Tetrachloro-m-xylene

R.T.: 3.402 min
Delta R.T.: 0.000 min
Response: 310118099
Conc: 50.00 ng/ml

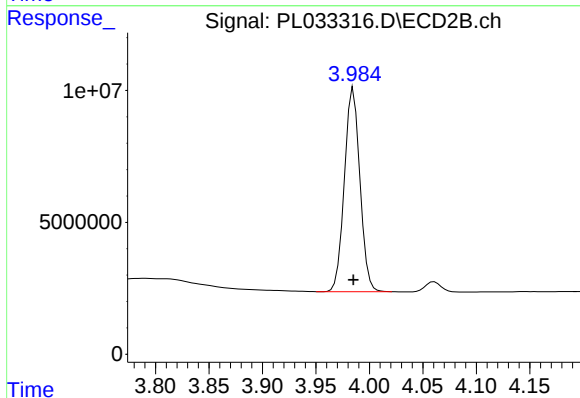


#1 Tetrachloro-m-xylene

R.T.: 3.985 min
Delta R.T.: 0.000 min
Response: 78163434
Conc: 50.00 ng/ml

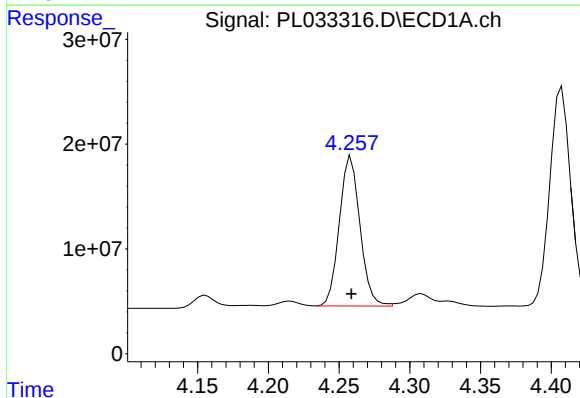


#23 Chlordane-1

R.T.: 4.259 min
Delta R.T.: 0.000 min
Response: 145340201
Conc: 500.00 ng/ml

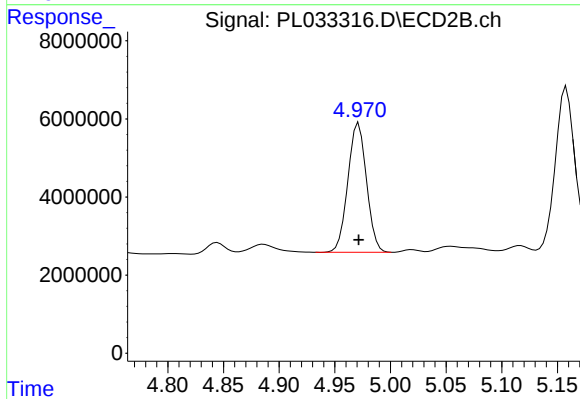


#23 Chlordane-1

R.T.: 4.971 min
Delta R.T.: 0.000 min
Response: 38636697
Conc: 500.00 ng/ml

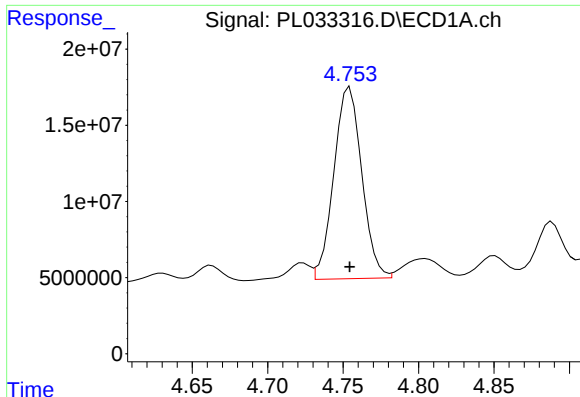


#24 Chlordane-2

R.T.: 4.754 min
Delta R.T.: 0.000 min
Response: 162223042
Conc: 500.00 ng/ml

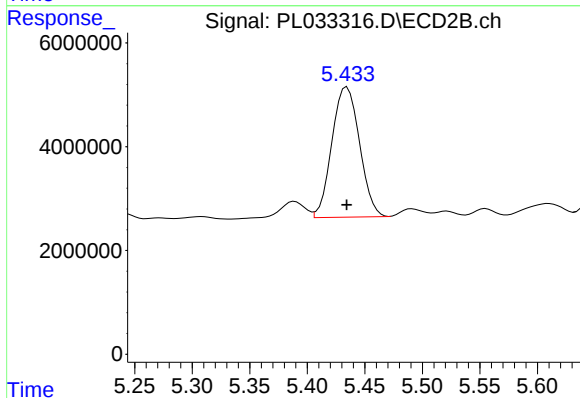


#24 Chlordane-2

R.T.: 5.434 min
Delta R.T.: 0.000 min
Response: 42057979
Conc: 500.00 ng/ml

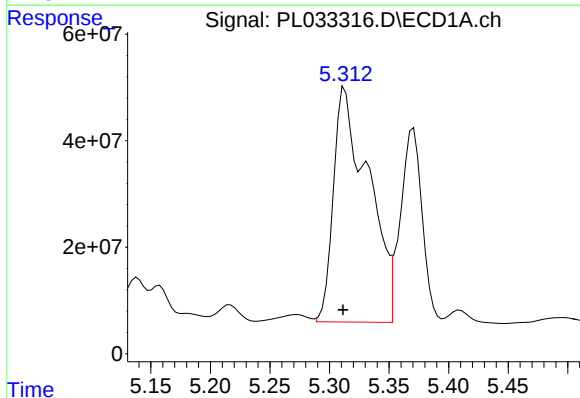


#25 Chlordane-3

R.T.: 5.313 min
Delta R.T.: 0.002 min
Response: 895161153
Conc: 952.45 ng/ml

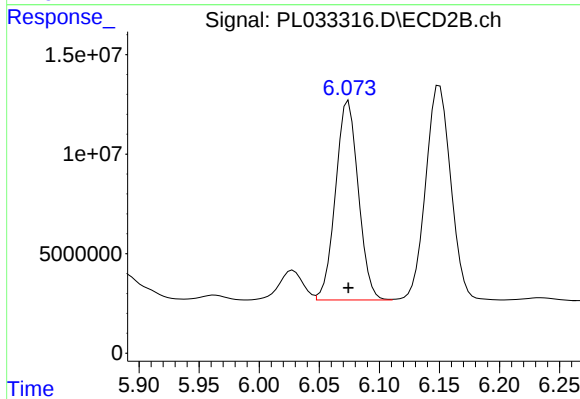


#25 Chlordane-3

R.T.: 6.074 min
Delta R.T.: 0.000 min
Response: 132273322
Conc: 500.00 ng/ml

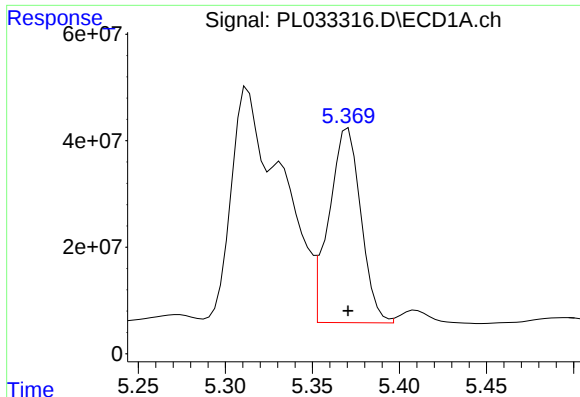


#26 Chlordane-4

R.T.: 5.370 min
Delta R.T.: 0.000 min
Response: 466750788
Conc: 500.00 ng/ml

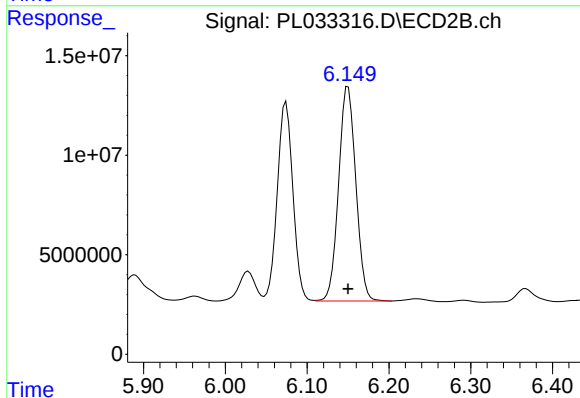


#26 Chlordane-4

R.T.: 6.150 min
Delta R.T.: 0.000 min
Response: 157200975
Conc: 500.00 ng/ml

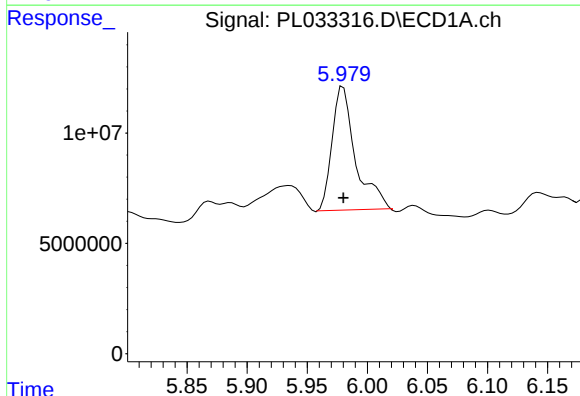


#27 Chlordane-5

R.T.: 5.980 min
Delta R.T.: 0.000 min
Response: 75867373
Conc: 500.00 ng/ml

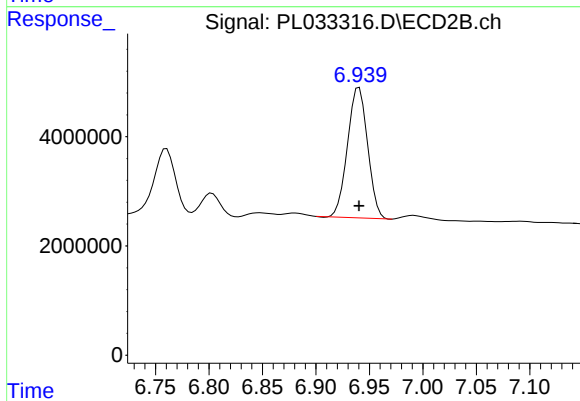


#27 Chlordane-5

R.T.: 6.940 min
Delta R.T.: 0.000 min
Response: 31212362
Conc: 500.00 ng/ml

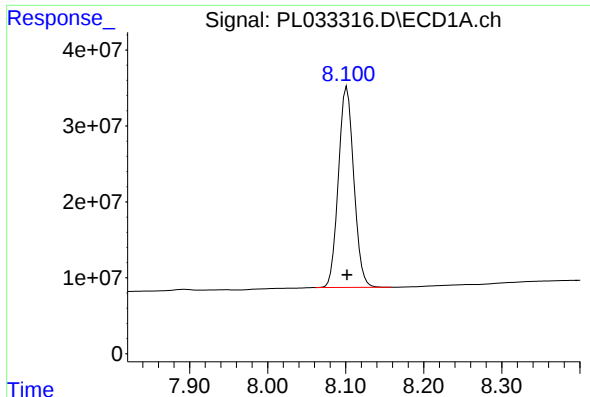

#28 Decachlorobiphenyl

R.T.: 8.102 min
Delta R.T.: 0.000 min
Response: 362495857
Conc: 50.00 ng/ml

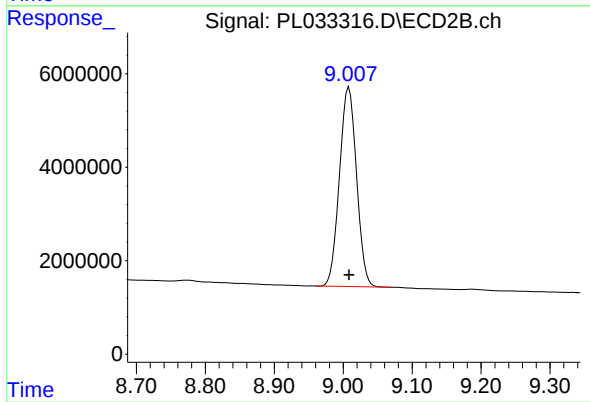

#28 Decachlorobiphenyl

R.T.: 9.008 min
Delta R.T.: 0.000 min
Response: 73485071
Conc: 50.00 ng/ml