

Data Path : P:\HPCHEM1\ECD_L\Data\PL022318\
 Data File : PL033383.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Feb 2018 05:39
 Operator : UA\AJ
 Sample : J1640-01
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 26 03:56:04 2018
 Quant Method : P:\HPCHEM1\ECD_L\methods\PL022318.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 23 13:36:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	3.402	3.985	133.4E6	31784382	22.635	19.662
28)	SA Decachlor...	8.104	9.010	125.3E6	30235229	16.105	19.601
Target Compounds							
2)	A alpha-BHC	3.792f	0.000	647589	0	0.070	N.D. #
4)	MA Heptachlor	4.403	0.000	3105729	0	0.354	N.D. #
5)	MB Aldrin	4.662	5.450	82049624	21884448	9.909	11.794
6)	B beta-BHC	4.403f	0.000	3105729	0	0.828	N.D. #
9)	A Endosulfan I	5.371f	0.000	3687368	0	0.488	N.D. #
10)	B gamma-Chl...	5.314	0.000	13147151	0	1.561	N.D. #
11)	B alpha-Chl...	5.371	0.000	3687368	0	0.446	N.D. #
13)	MA Dieldrin	5.732f	0.000	11506987	0	1.372	N.D. #
24)	Chlordane-2	4.728	5.450	78753115	21884448	245.543	264.410
25)	Chlordane-3	5.314	0.000	13147151	0	13.164	N.D. #
26)	Chlordane-4	5.371	0.000	3687368	0	4.097	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD_L\Data\PL022318\
Data File : PL033383.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Feb 2018 05:39
Operator : UA\AJ
Sample : J1640-01
Misc :
ALS Vial : 54 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 26 03:56:04 2018
Quant Method : P:\HPCHEM1\ECD_L\methods\PL022318.M
Quant Title : GC Extractables
QLast Update : Fri Feb 23 13:36:10 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

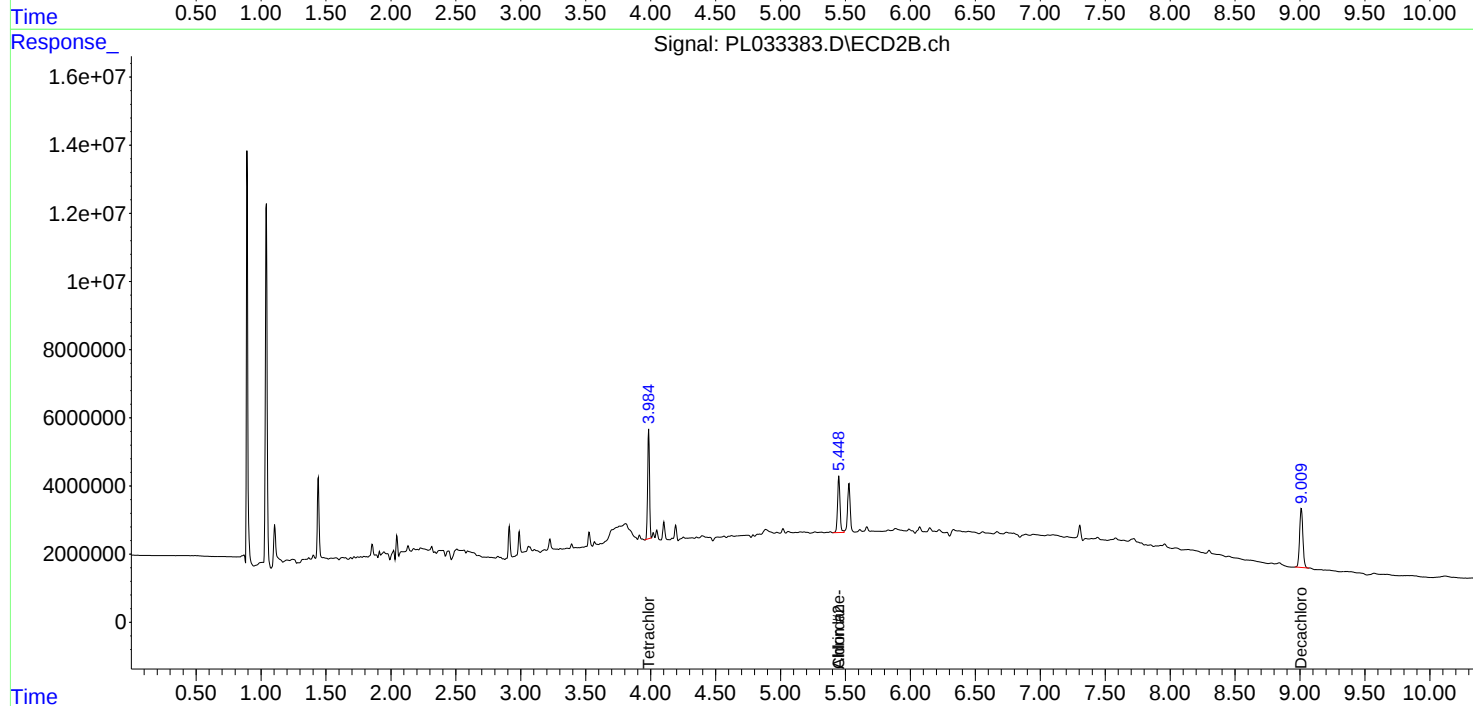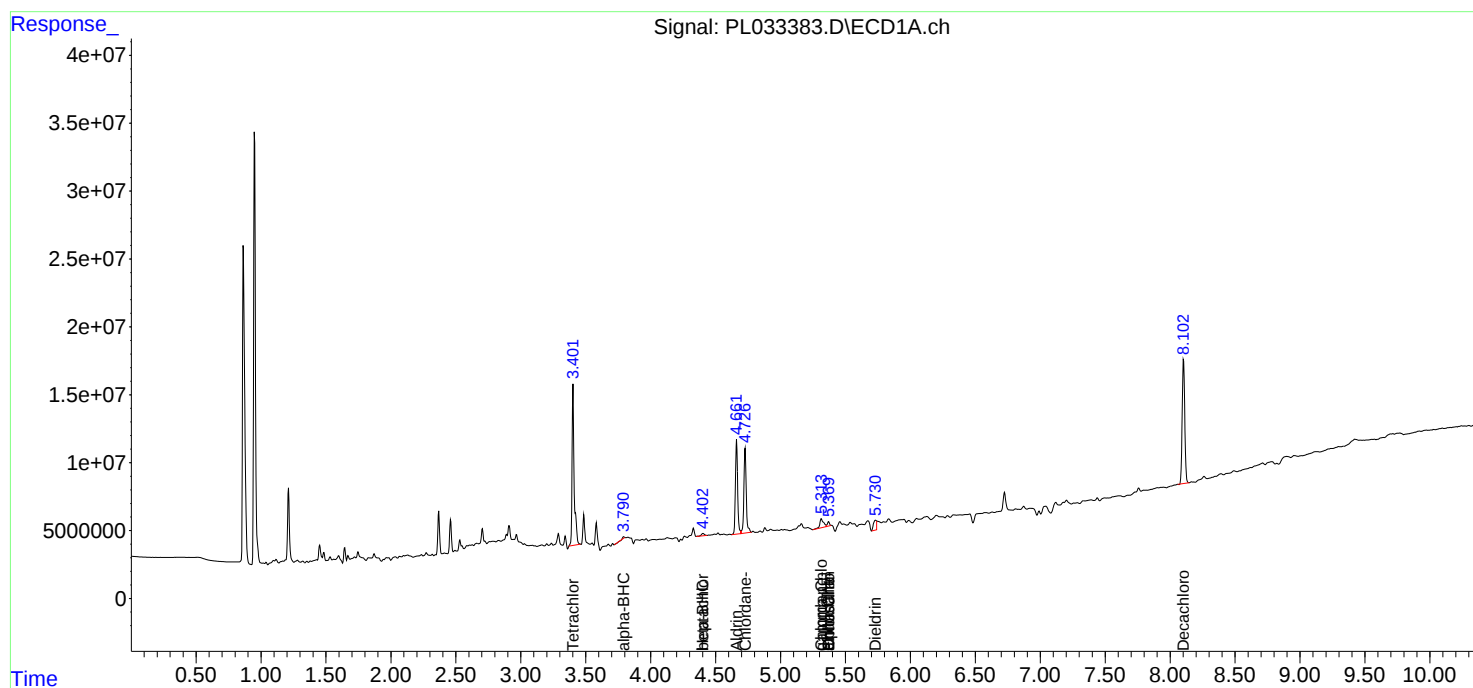

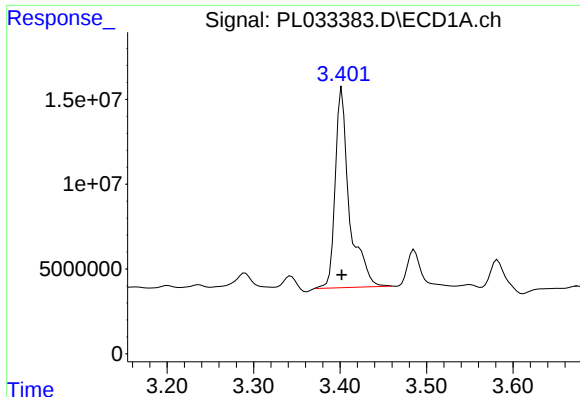


#1 Tetrachloro-m-xylene

R.T.: 3.402 min
Delta R.T.: 0.000 min
Response: 133363022
Conc: 22.63 ng/ml

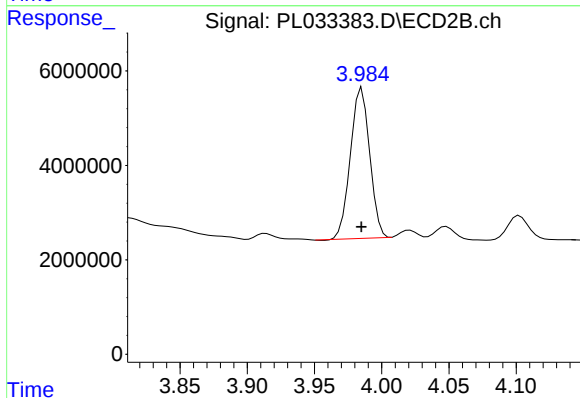


#1 Tetrachloro-m-xylene

R.T.: 3.985 min
Delta R.T.: 0.000 min
Response: 31784382
Conc: 19.66 ng/ml

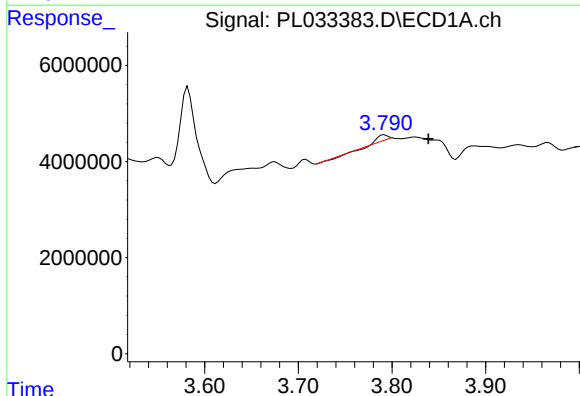


#2 alpha-BHC

R.T.: 3.792 min
Delta R.T.: -0.047 min
Response: 647589
Conc: 0.07 ng/ml

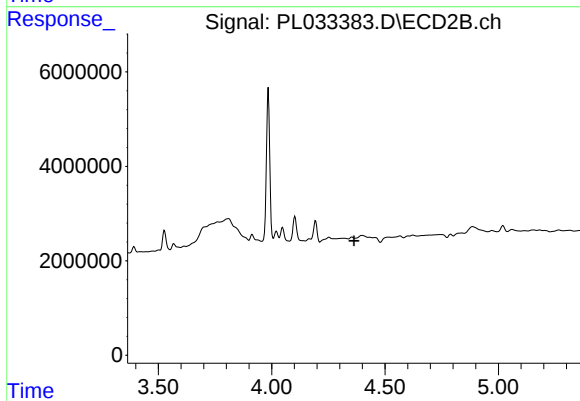


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T.: 4.364 min
Response: 0
Conc: N.D.

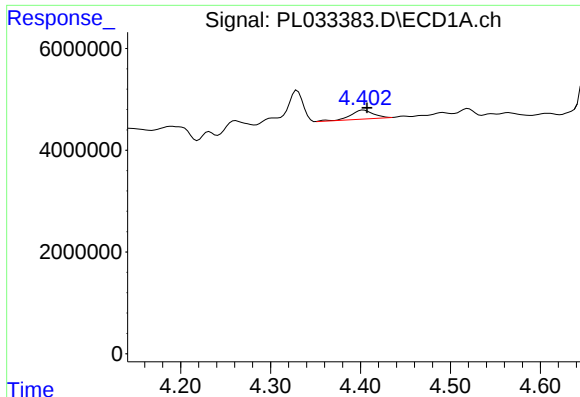


#4 Heptachlor

R.T.: 4.403 min
Delta R.T.: -0.004 min
Response: 3105729
Conc: 0.35 ng/ml

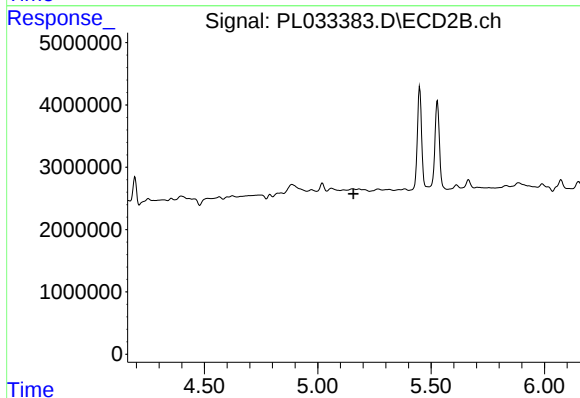


#4 Heptachlor

R.T.: 0.000 min
Exp R.T.: 5.158 min
Response: 0
Conc: N.D.

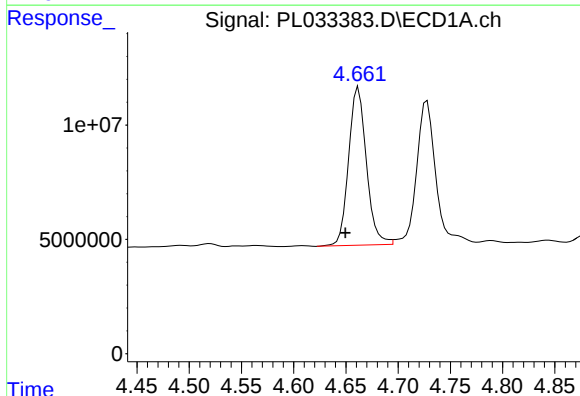


#5 Aldrin

R.T.: 4.662 min
Delta R.T.: 0.012 min
Response: 82049624
Conc: 9.91 ng/ml

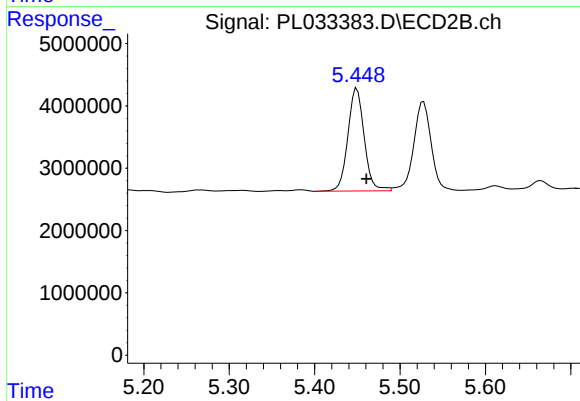


#5 Aldrin

R.T.: 5.450 min
Delta R.T.: -0.011 min
Response: 21884448
Conc: 11.79 ng/ml

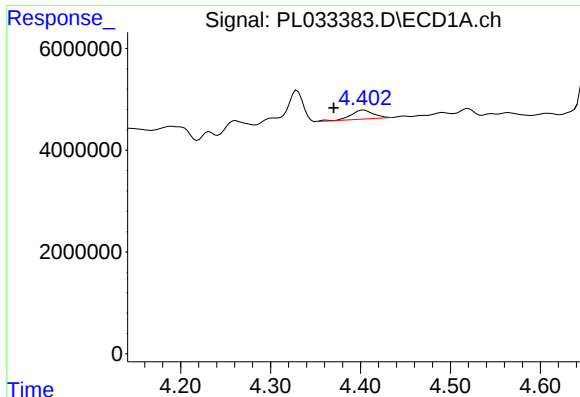


#6 beta-BHC

R.T.: 4.403 min
Delta R.T.: 0.033 min
Response: 3105729
Conc: 0.83 ng/ml

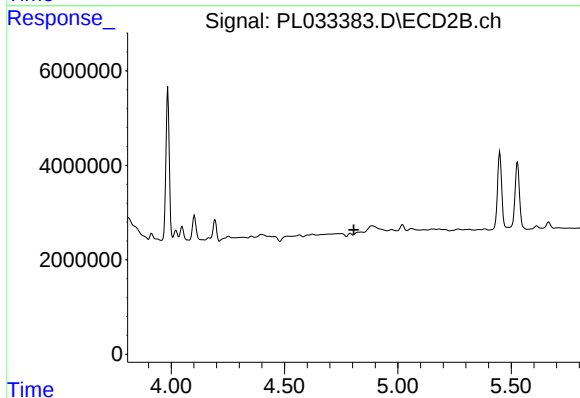


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.805 min
Response: 0
Conc: N.D.

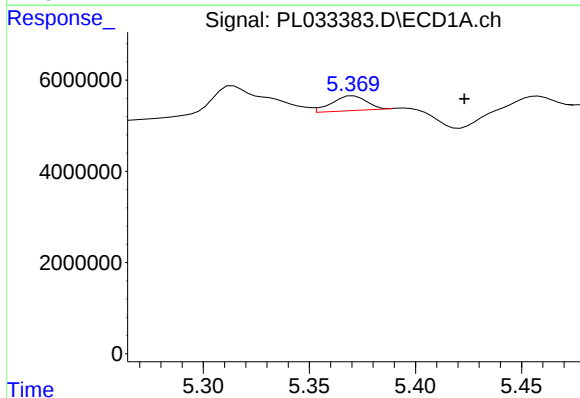


#9 Endosulfan I

R.T.: 5.371 min
Delta R.T.: -0.052 min
Response: 3687368
Conc: 0.49 ng/ml

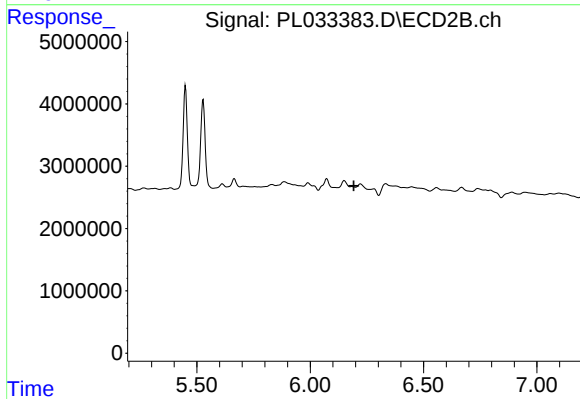


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 6.192 min
Response: 0
Conc: N.D.

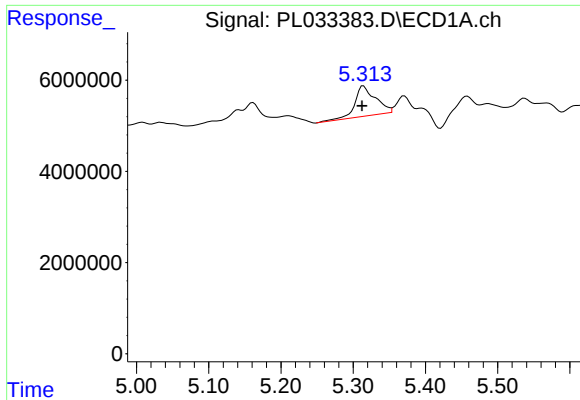


#10 gamma-Chlordane

R.T.: 5.314 min
Delta R.T.: 0.002 min
Response: 13147151
Conc: 1.56 ng/ml

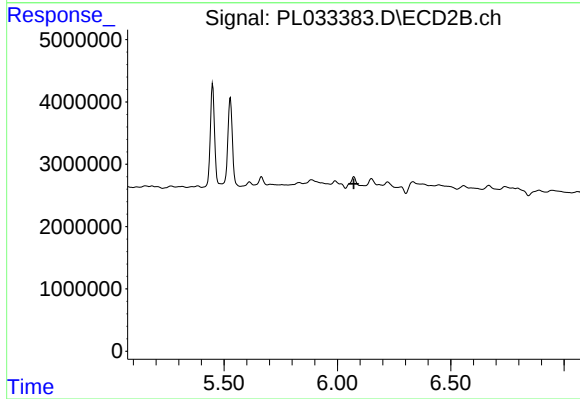


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.073 min
Response: 0
Conc: N.D.

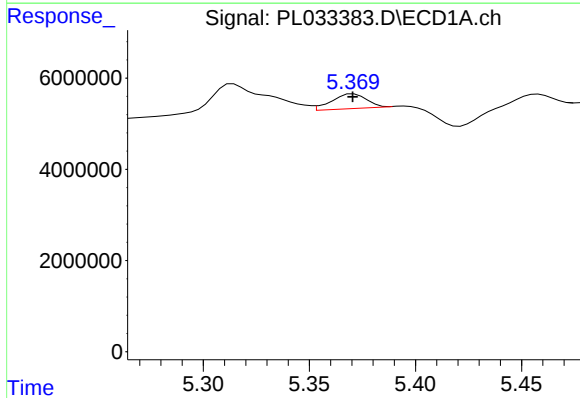


#11 alpha-Chlordane

R.T.: 5.371 min
Delta R.T.: 0.000 min
Response: 3687368
Conc: 0.45 ng/ml

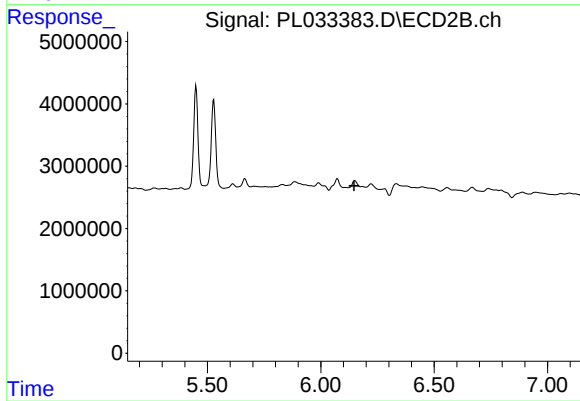


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.147 min
Response: 0
Conc: N.D.

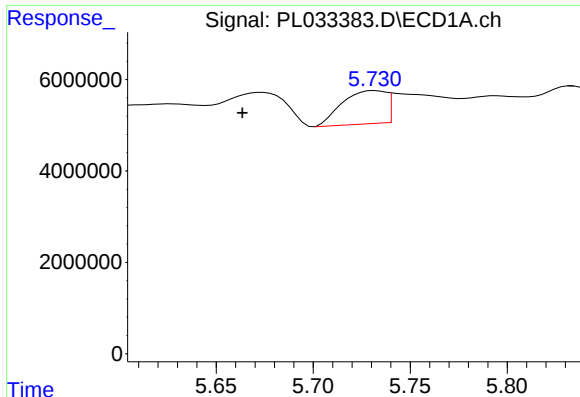


#13 Dieldrin

R.T.: 5.732 min
Delta R.T.: 0.068 min
Response: 11506987
Conc: 1.37 ng/ml

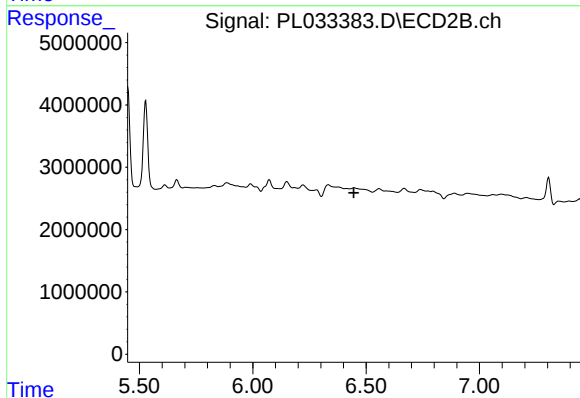


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 6.446 min
Response: 0
Conc: N.D.

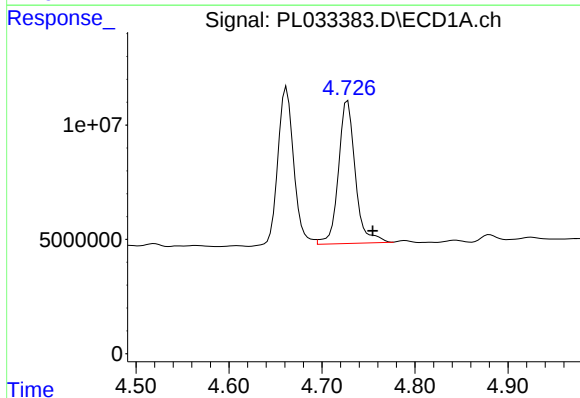


#24 Chlordane-2

R.T.: 4.728 min
Delta R.T.: -0.027 min
Response: 78753115
Conc: 245.54 ng/ml

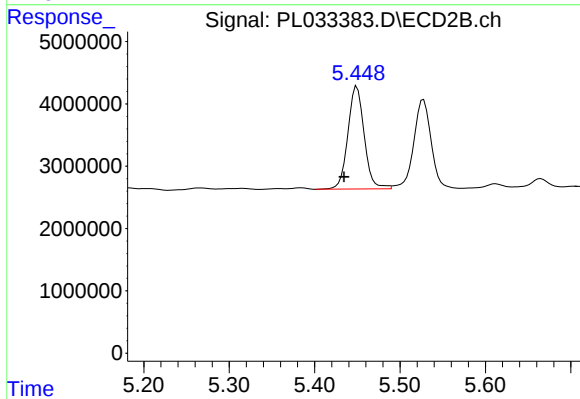


#24 Chlordane-2

R.T.: 5.450 min
Delta R.T.: 0.015 min
Response: 21884448
Conc: 264.41 ng/ml

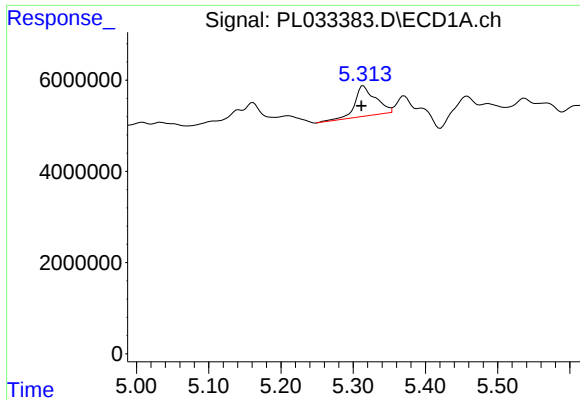


#25 Chlordane-3

R.T.: 5.314 min
Delta R.T.: 0.003 min
Response: 13147151
Conc: 13.16 ng/ml

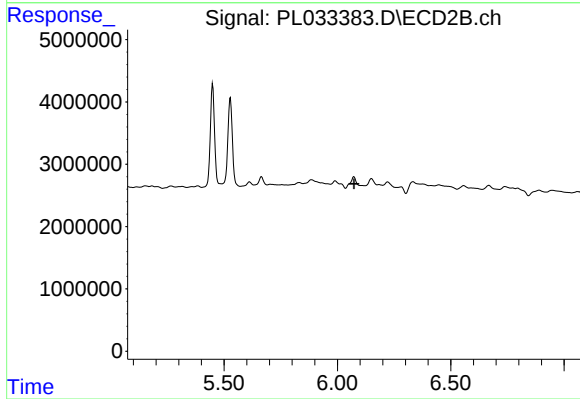


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 6.074 min
Response: 0
Conc: N.D.

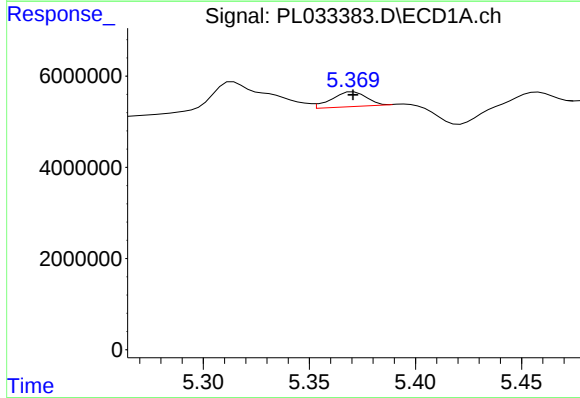


#26 Chlordane-4

R.T.: 5.371 min
Delta R.T.: 0.000 min
Response: 3687368
Conc: 4.10 ng/ml

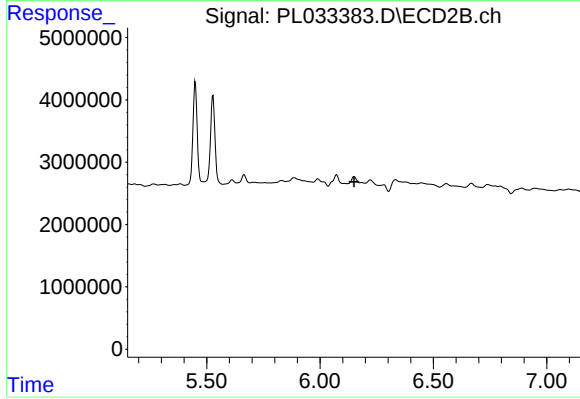


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 6.150 min
Response: 0
Conc: N.D.

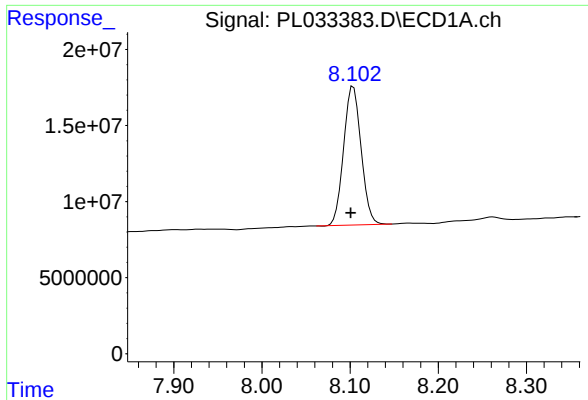

#28 Decachlorobiphenyl

R.T.: 8.104 min
Delta R.T.: 0.003 min
Response: 125302386
Conc: 16.10 ng/ml

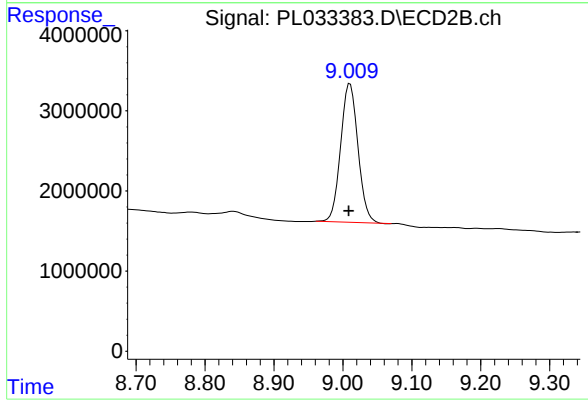

#28 Decachlorobiphenyl

R.T.: 9.010 min
Delta R.T.: 0.002 min
Response: 30235229
Conc: 19.60 ng/ml