

Data Path : P:\HPCHEM1\ECD_L\Data\PL022318\
 Data File : PL033387.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Feb 2018 06:39
 Operator : UA\AJ
 Sample : J1652-04
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 26 03:57:14 2018
 Quant Method : P:\HPCHEM1\ECD_L\methods\PL022318.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 23 13:36:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	3.403	3.985	74716069	22571216	12.681	13.962
28)	SA Decachlor...	8.104	9.012	100.7E6	24016976	12.949	15.569
Target Compounds							
2)	A alpha-BHC	3.792f	0.000	4870980	0	0.528	N.D. #
6)	B beta-BHC	4.329f	0.000	6740468	0	1.797	N.D. #
12)	B 4,4'-DDE	5.538	0.000	4387370	0	0.525	N.D. #
13)	MA Dieldrin	5.729f	0.000	8418091	0	1.004	N.D. #
14)	MA Endrin	5.979f	0.000	11675594	0	1.456	N.D. #
16)	A 4,4'-DDD	6.113f	0.000	10668219	0	1.571	N.D. #
17)	MA 4,4'-DDT	6.284	0.000	19468594	0	2.677	N.D. #
18)	B Endrin al...	6.375	0.000	4713143	0	0.741	N.D. #
19)	B Endosulfa...	6.567	0.000	6674123	0	0.918	N.D. #
20)	A Methoxychlor	6.813	0.000	13350136	0	3.342	N.D. #
21)	B Endrin ke...	7.084	0.000	3169157	0	0.396	N.D. #
27)	Chlordane-5	5.979	0.000	11675594	0	75.036	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD_L\Data\PL022318\
Data File : PL033387.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Feb 2018 06:39
Operator : UA\AJ
Sample : J1652-04
Misc :
ALS Vial : 58 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 26 03:57:14 2018
Quant Method : P:\HPCHEM1\ECD_L\methods\PL022318.M
Quant Title : GC Extractables
QLast Update : Fri Feb 23 13:36:10 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

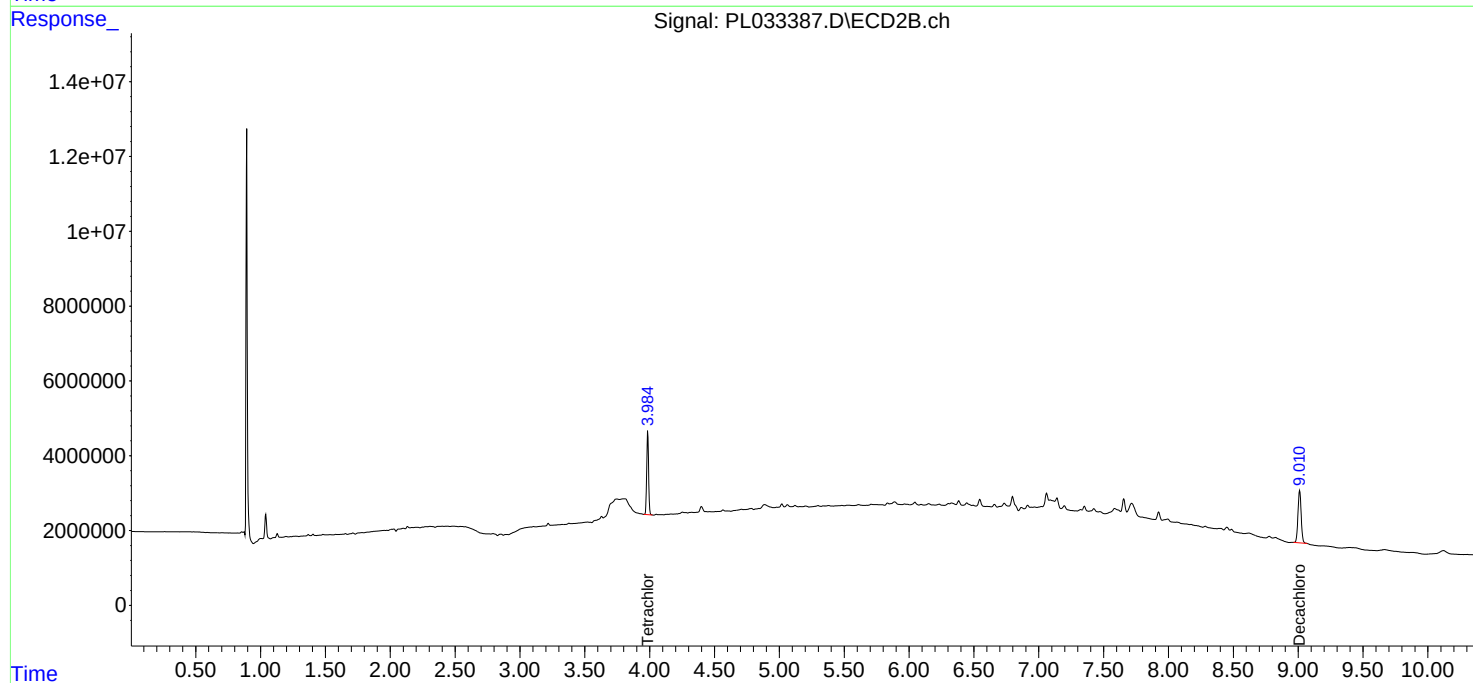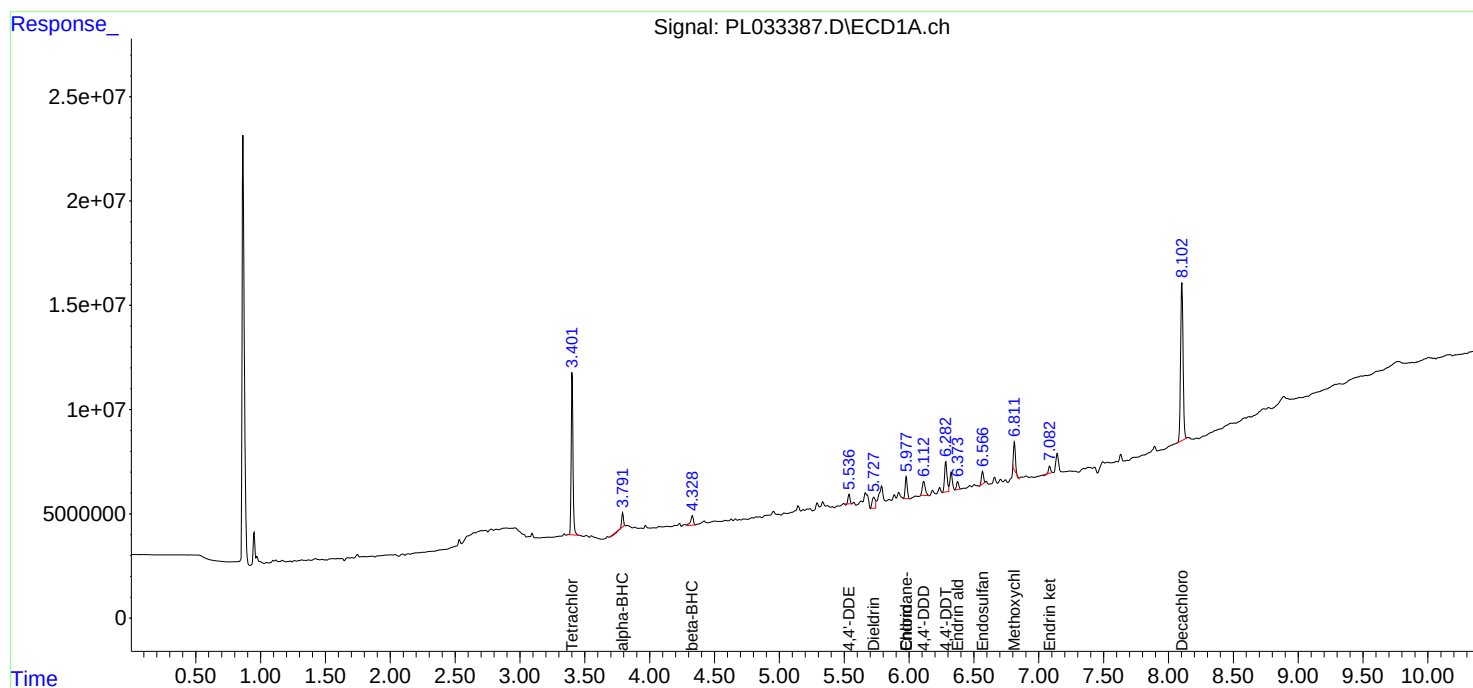

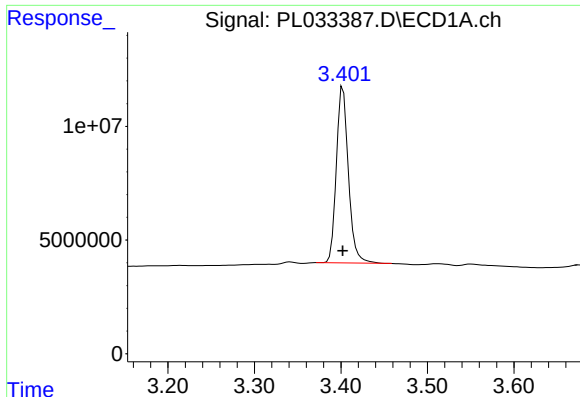


#1 Tetrachloro-m-xylene

R.T.: 3.403 min
Delta R.T.: 0.000 min
Response: 74716069
Conc: 12.68 ng/ml

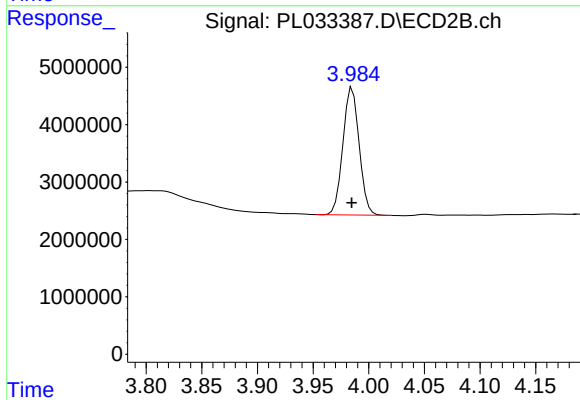


#1 Tetrachloro-m-xylene

R.T.: 3.985 min
Delta R.T.: 0.000 min
Response: 22571216
Conc: 13.96 ng/ml

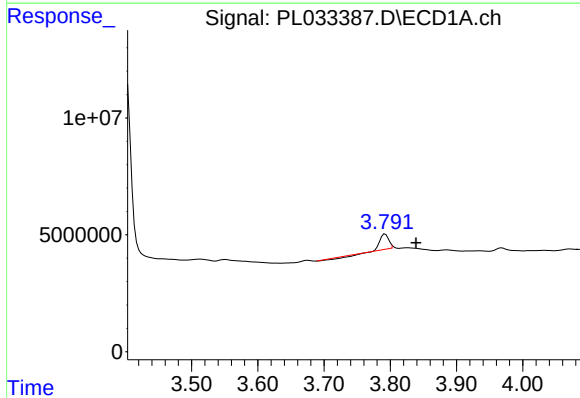


#2 alpha-BHC

R.T.: 3.792 min
Delta R.T.: -0.047 min
Response: 4870980
Conc: 0.53 ng/ml

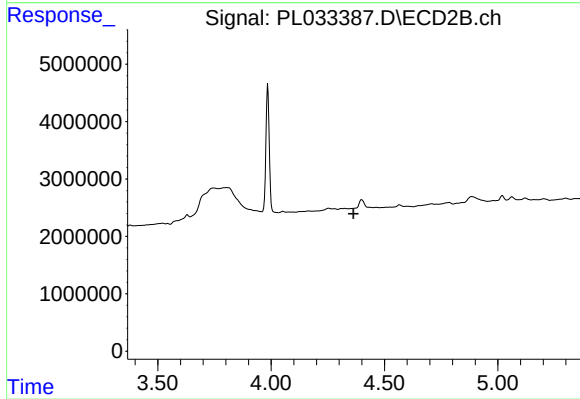


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T.: 4.364 min
Response: 0
Conc: N.D.

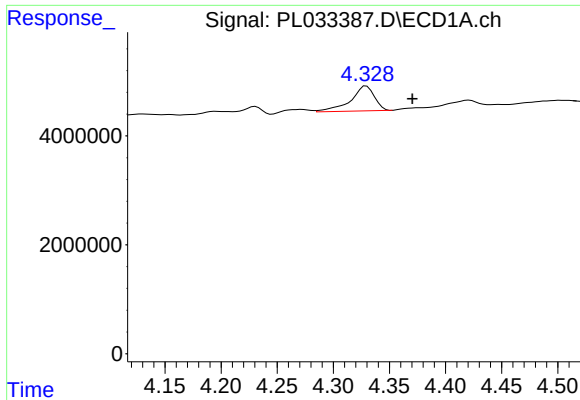


#6 beta-BHC

R.T.: 4.329 min
Delta R.T.: -0.041 min
Response: 6740468
Conc: 1.80 ng/ml

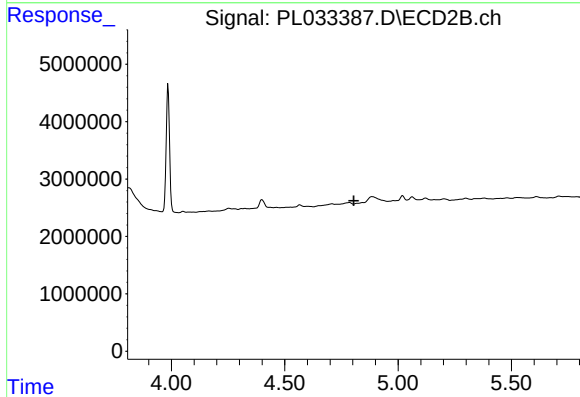


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.805 min
Response: 0
Conc: N.D.

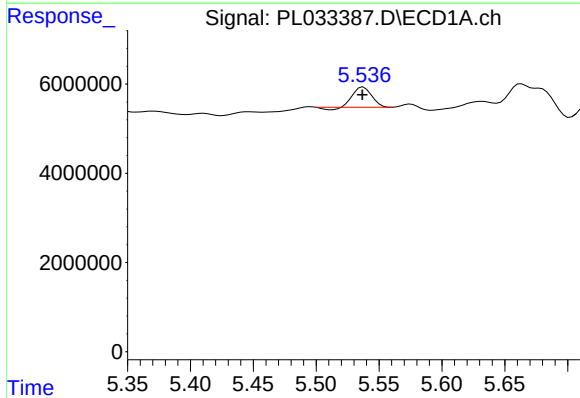


#12 4,4'-DDE

R.T.: 5.538 min
Delta R.T.: 0.000 min
Response: 4387370
Conc: 0.52 ng/ml

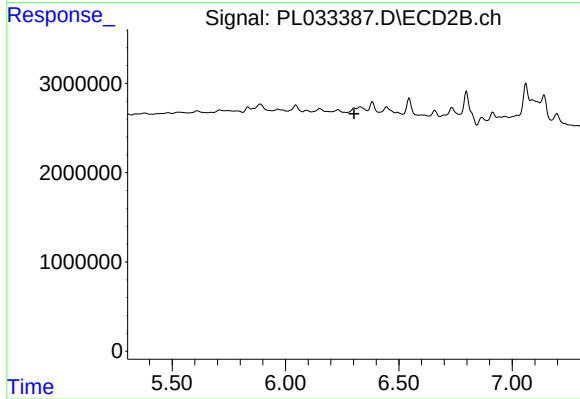


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 6.302 min
Response: 0
Conc: N.D.

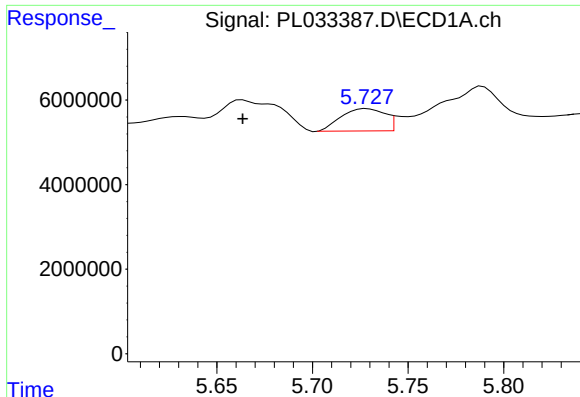


#13 Dieldrin

R.T.: 5.729 min
Delta R.T.: 0.065 min
Response: 8418091
Conc: 1.00 ng/ml

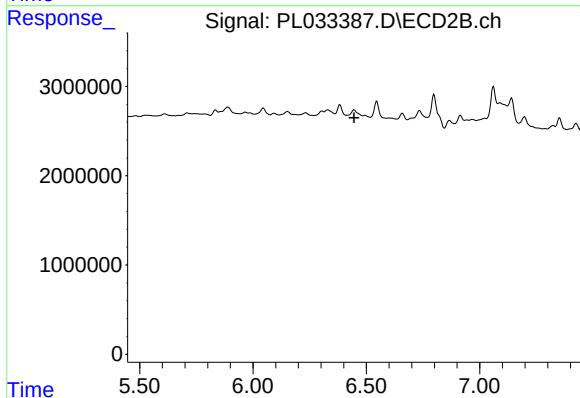


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.446 min
Response: 0
Conc: N.D.

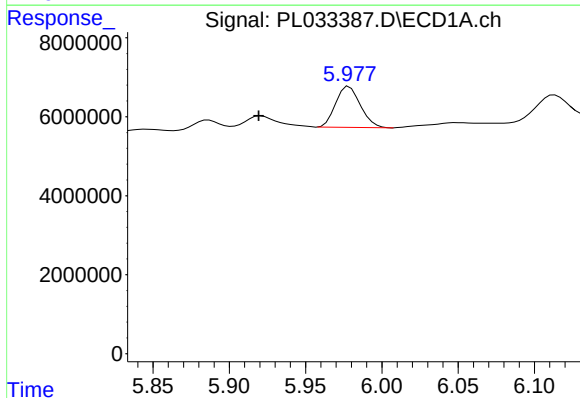


#14 Endrin

R.T.: 5.979 min
Delta R.T.: 0.059 min
Response: 11675594
Conc: 1.46 ng/ml

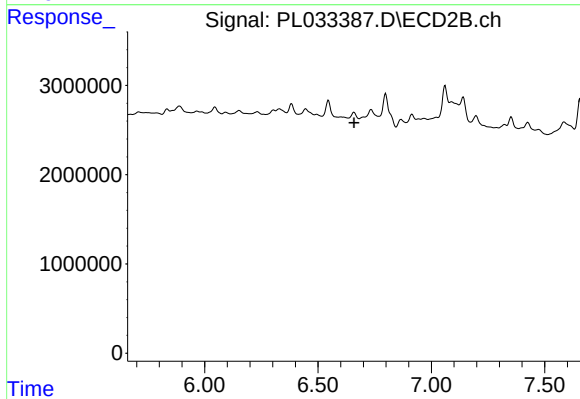


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.660 min
Response: 0
Conc: N.D.

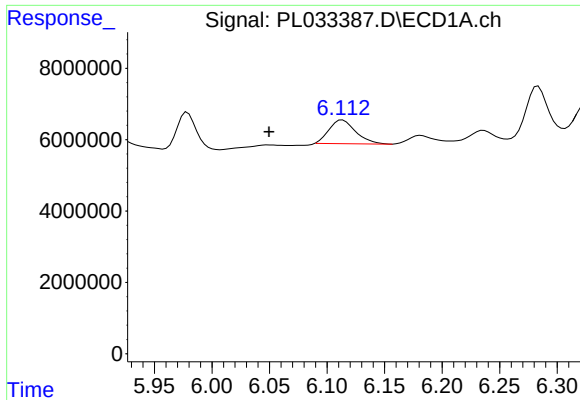


#16 4,4'-DDD

R.T.: 6.113 min
Delta R.T.: 0.064 min
Response: 10668219
Conc: 1.57 ng/ml

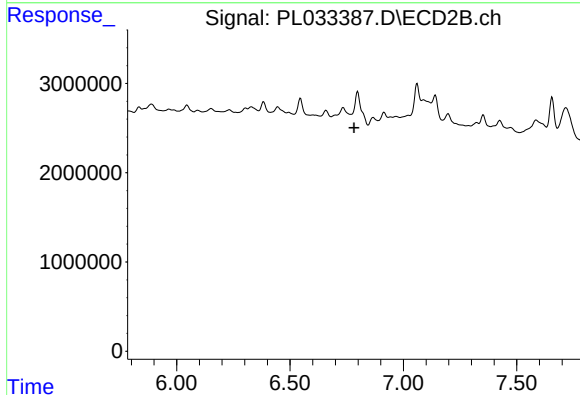


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.783 min
Response: 0
Conc: N.D.

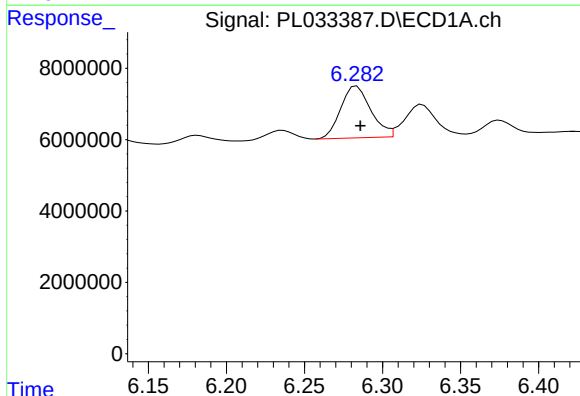


#17 4,4'-DDT

R.T.: 6.284 min
Delta R.T.: -0.002 min
Response: 19468594
Conc: 2.68 ng/ml

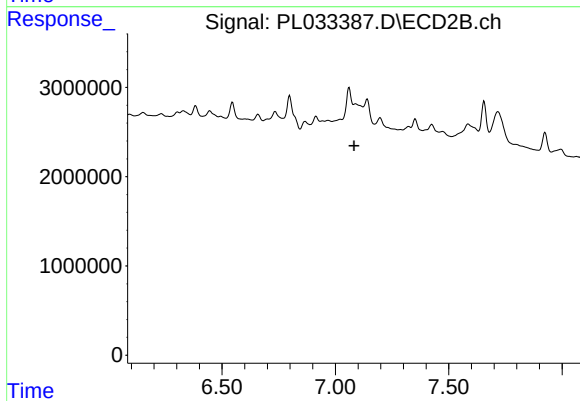


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 7.082 min
Response: 0
Conc: N.D.

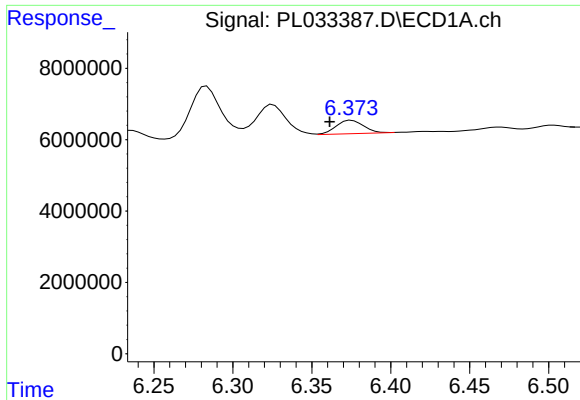


#18 Endrin aldehyde

R.T.: 6.375 min
Delta R.T.: 0.014 min
Response: 4713143
Conc: 0.74 ng/ml

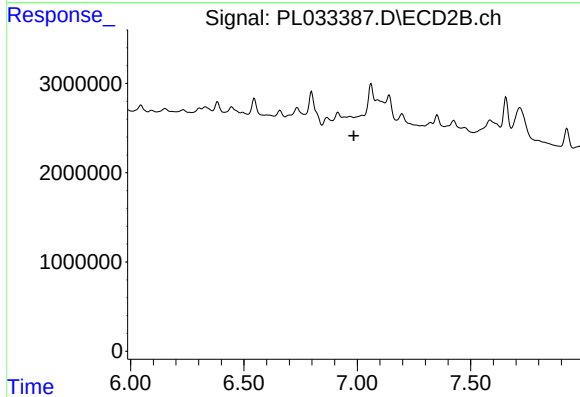


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.985 min
Response: 0
Conc: N.D.

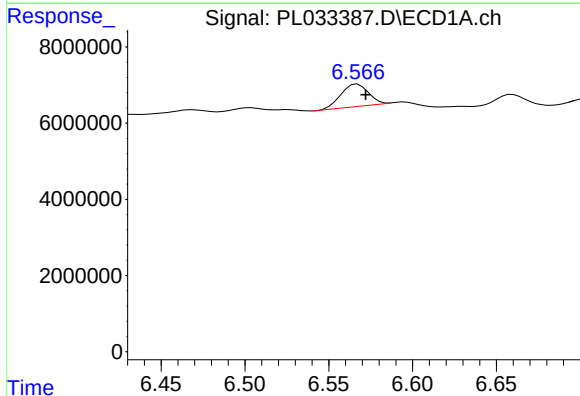


#19 Endosulfan Sulfate

R.T.: 6.567 min
Delta R.T.: -0.005 min
Response: 6674123
Conc: 0.92 ng/ml

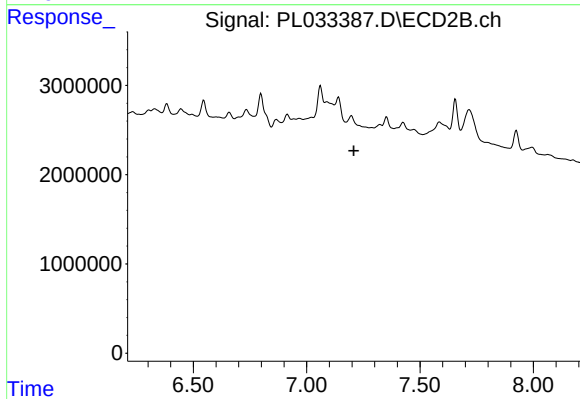


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 7.208 min
Response: 0
Conc: N.D.

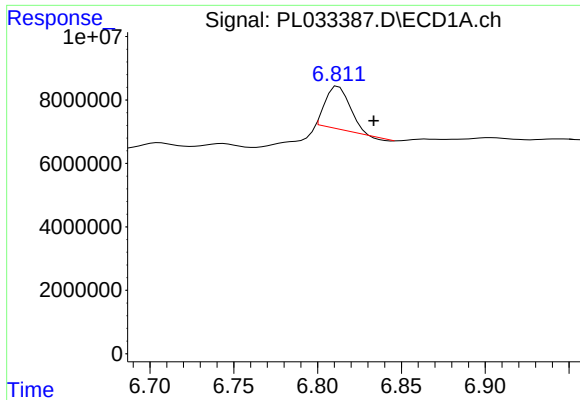


#20 Methoxychlor

R.T.: 6.813 min
Delta R.T.: -0.021 min
Response: 13350136
Conc: 3.34 ng/ml

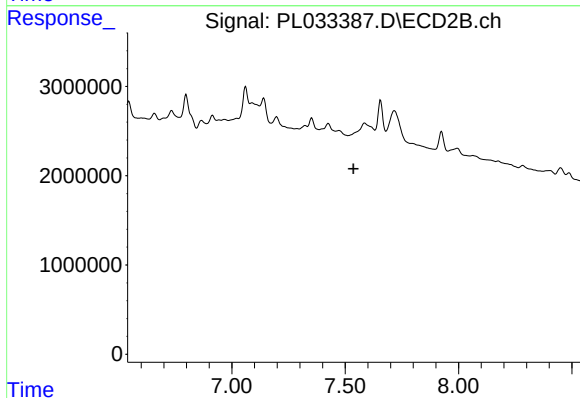


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 7.537 min
Response: 0
Conc: N.D.

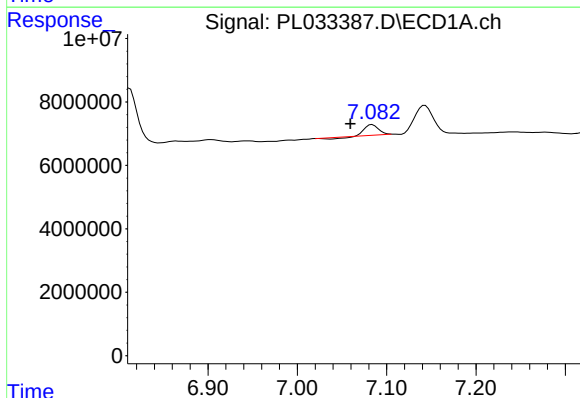


#21 Endrin ketone

R.T.: 7.084 min
Delta R.T.: 0.024 min
Response: 3169157
Conc: 0.40 ng/ml

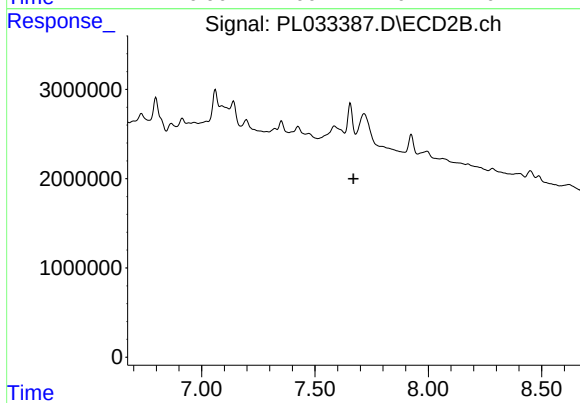


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 7.670 min
Response: 0
Conc: N.D.

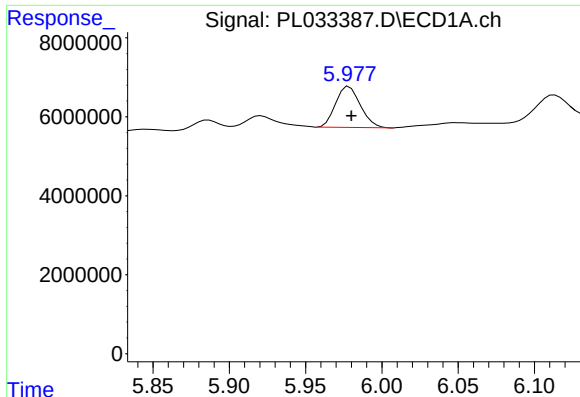


#27 Chlordane-5

R.T.: 5.979 min
Delta R.T.: -0.001 min
Response: 11675594
Conc: 75.04 ng/ml

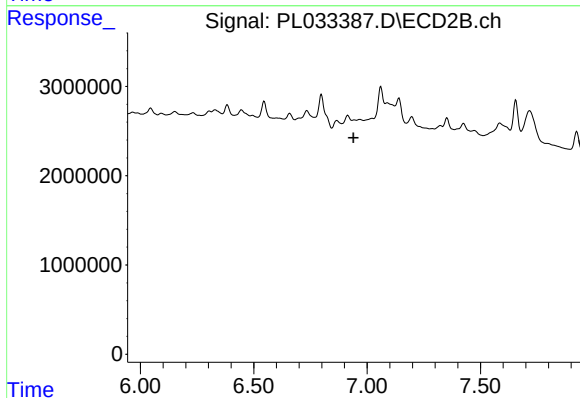


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.940 min
Response: 0
Conc: N.D.

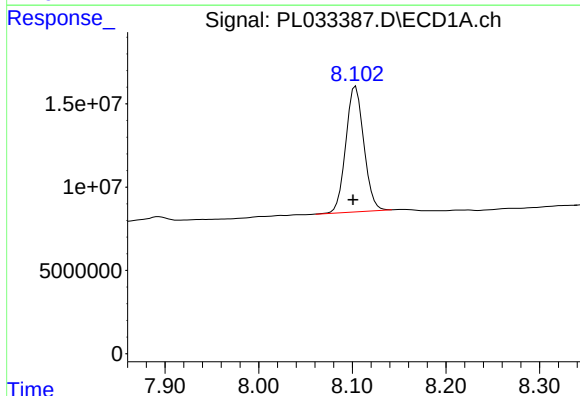

#28 Decachlorobiphenyl

R.T.: 8.104 min
Delta R.T.: 0.003 min
Response: 100748079
Conc: 12.95 ng/ml

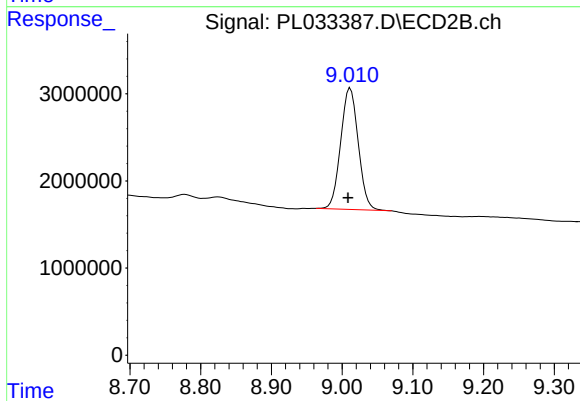

#28 Decachlorobiphenyl

R.T.: 9.012 min
Delta R.T.: 0.003 min
Response: 24016976
Conc: 15.57 ng/ml