

Data Path : P:\HPCHEM1\ECD_L\Data\PL022318\
 Data File : PL033318.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Feb 2018 13:22
 Operator : UA\AJ
 Sample : PCHLORIC050
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 23 13:33:49 2018
 Quant Method : P:\HPCHEM1\ECD_L\methods\PL022318.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 23 13:28:48 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	3.401	3.984	29877973	8024699	4.911	5.237
28)	SA Decachlor...	8.102	9.008	39406877	8184649	5.561	5.687
Target Compounds							
23)	Chlordane-1	4.259	4.969	13344865	3975386	46.778	52.481m
24)	Chlordane-2	4.754	5.432	16580782	4263349	52.139	51.902m
25)	Chlordane-3	5.313	6.073	46668146	13413814	45.975	51.477
26)	Chlordane-4	5.370	6.149	42366382	16364528	46.391	52.759
27)	Chlordane-5	5.980	6.938	8530290	3032597	56.176	49.506m


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD_L\Data\PL022318\
Data File : PL033318.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Feb 2018 13:22
Operator : UA\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 23 13:33:49 2018
Quant Method : P:\HPCHEM1\ECD_L\methods\PL022318.M
Quant Title : GC Extractables
QLast Update : Fri Feb 23 13:28:48 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

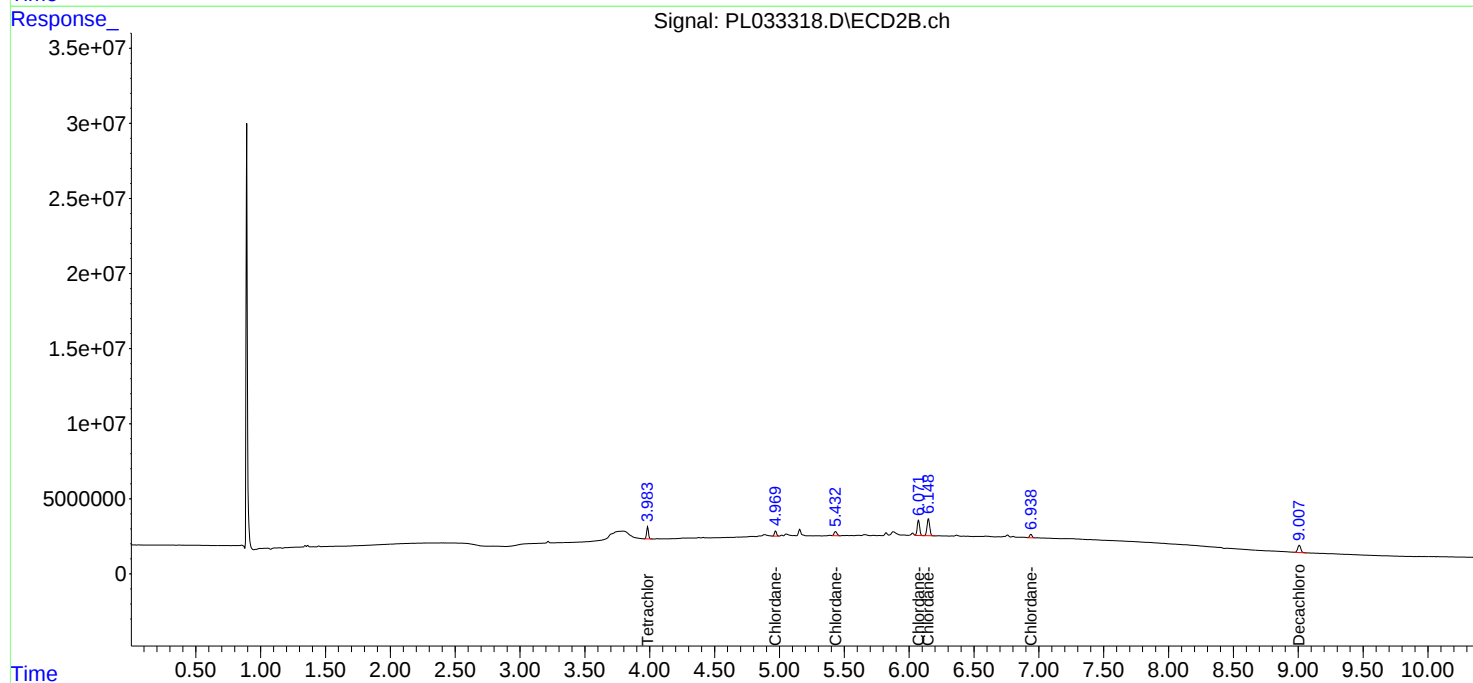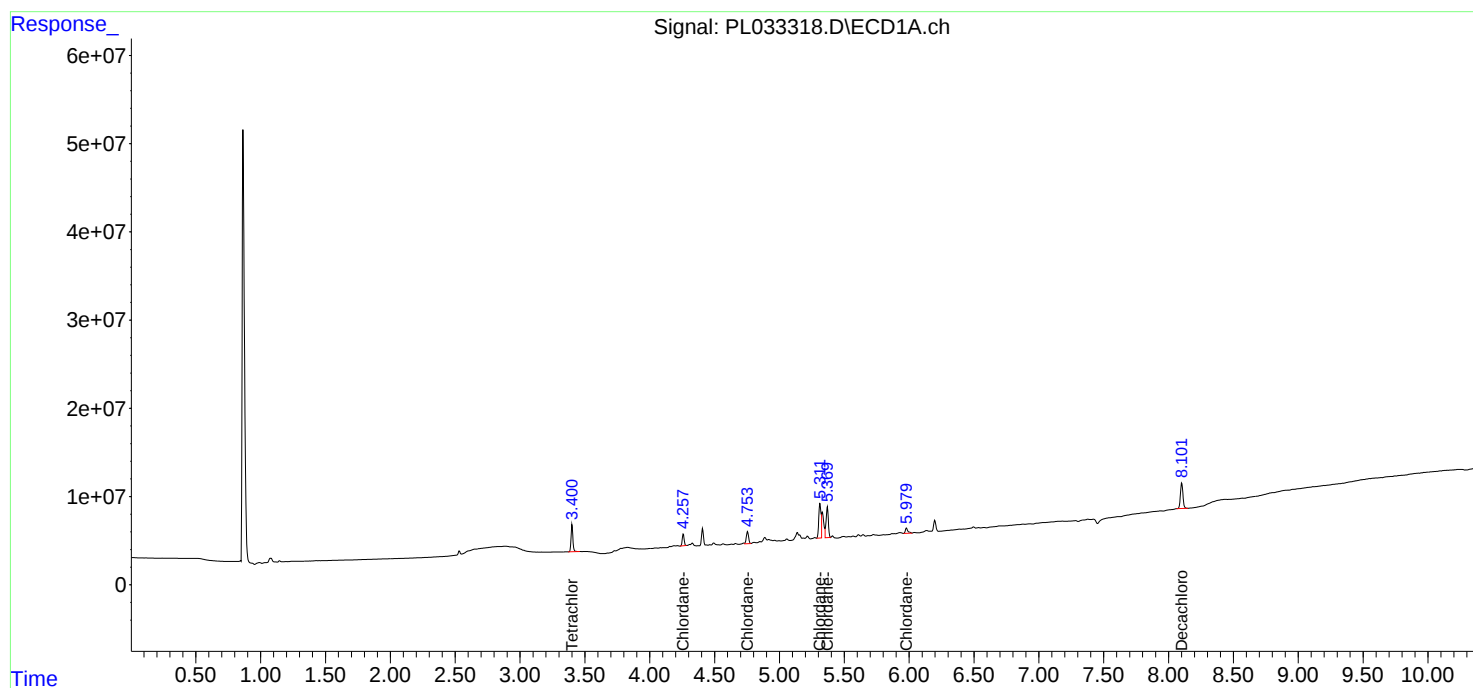

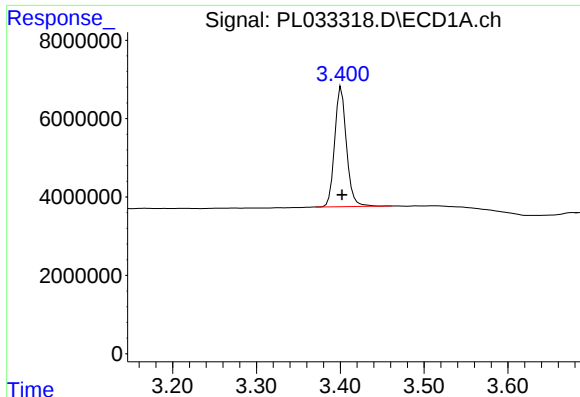


#1 Tetrachloro-m-xylene

R.T.: 3.401 min
Delta R.T.: 0.000 min
Response: 29877973
Conc: 4.91 ng/ml

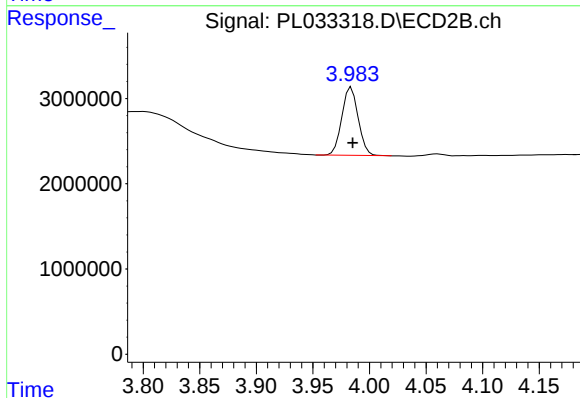


#1 Tetrachloro-m-xylene

R.T.: 3.984 min
Delta R.T.: -0.001 min
Response: 8024699
Conc: 5.24 ng/ml

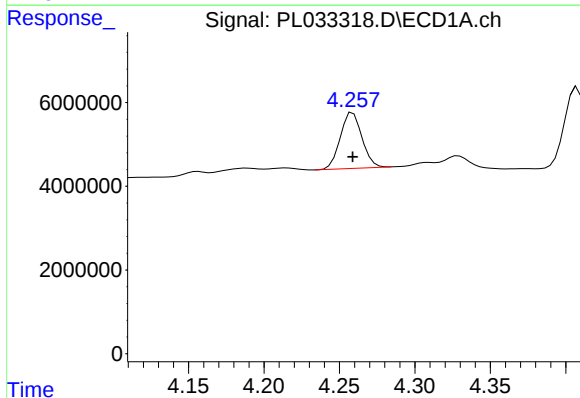


#23 Chlordane-1

R.T.: 4.259 min
Delta R.T.: 0.000 min
Response: 13344865
Conc: 46.78 ng/ml

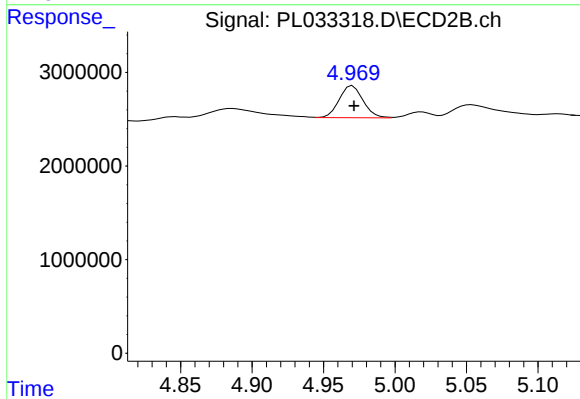


#23 Chlordane-1

R.T.: 4.969 min
Delta R.T.: -0.002 min
Response: 3975386
Conc: 52.48 ng/ml m

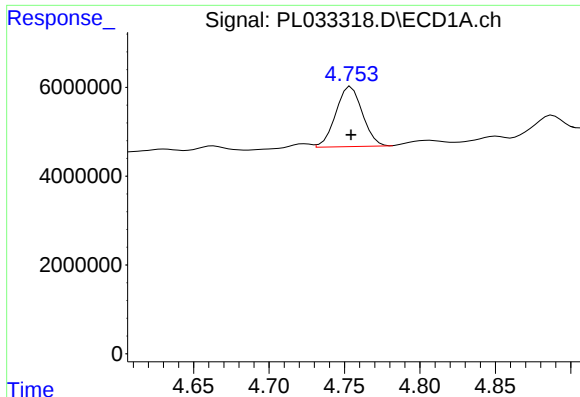


#24 Chlordane-2

R.T.: 4.754 min
Delta R.T.: 0.000 min
Response: 16580782
Conc: 52.14 ng/ml

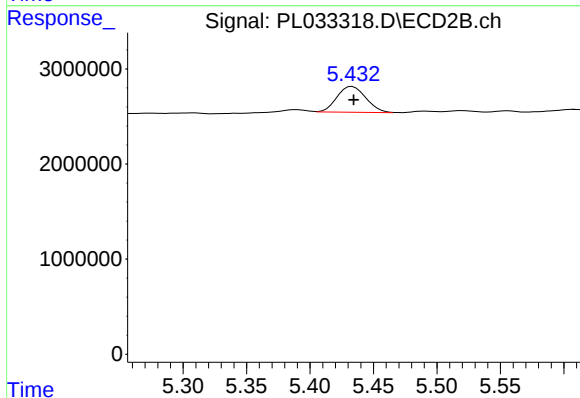


#24 Chlordane-2

R.T.: 5.432 min
Delta R.T.: -0.002 min
Response: 4263349
Conc: 51.90 ng/ml m

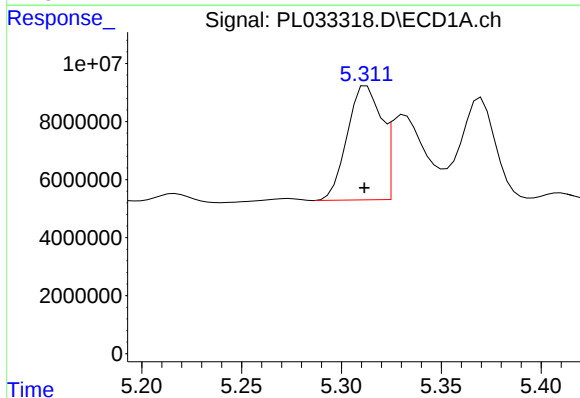


#25 Chlordane-3

R.T.: 5.313 min
Delta R.T.: 0.001 min
Response: 46668146
Conc: 45.97 ng/ml

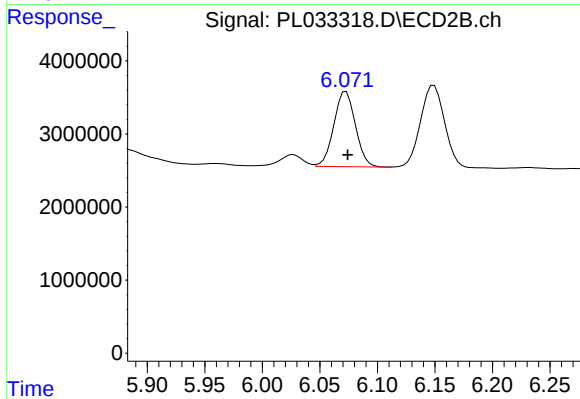


#25 Chlordane-3

R.T.: 6.073 min
Delta R.T.: -0.002 min
Response: 13413814
Conc: 51.48 ng/ml

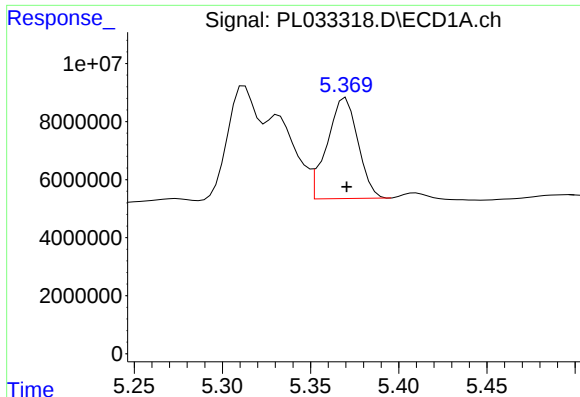


#26 Chlordane-4

R.T.: 5.370 min
Delta R.T.: 0.000 min
Response: 42366382
Conc: 46.39 ng/ml

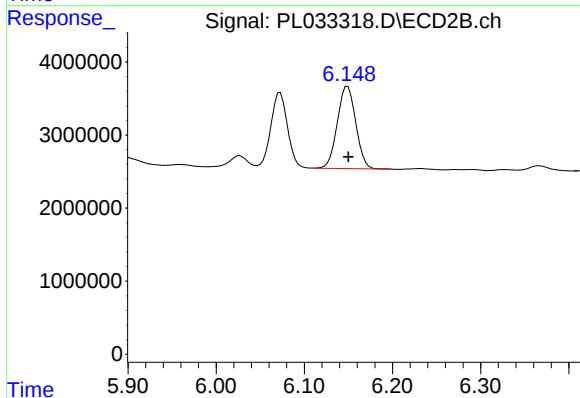


#26 Chlordane-4

R.T.: 6.149 min
Delta R.T.: 0.000 min
Response: 16364528
Conc: 52.76 ng/ml

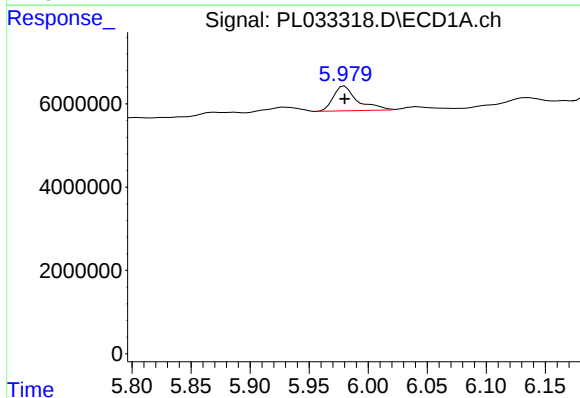


#27 Chlordane-5

R.T.: 5.980 min
Delta R.T.: 0.000 min
Response: 8530290
Conc: 56.18 ng/ml

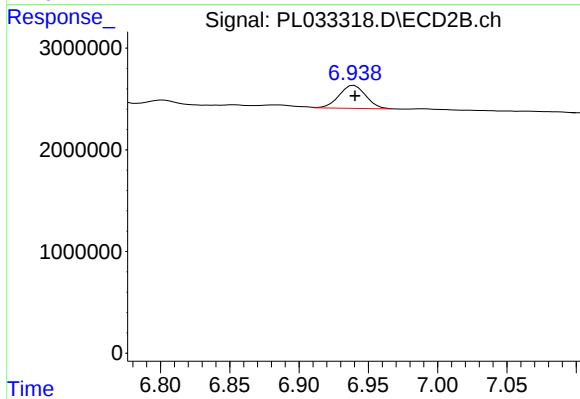

#27 Chlordane-5

R.T.: 6.938 min
Delta R.T.: -0.002 min
Response: 3032597
Conc: 49.51 ng/ml m

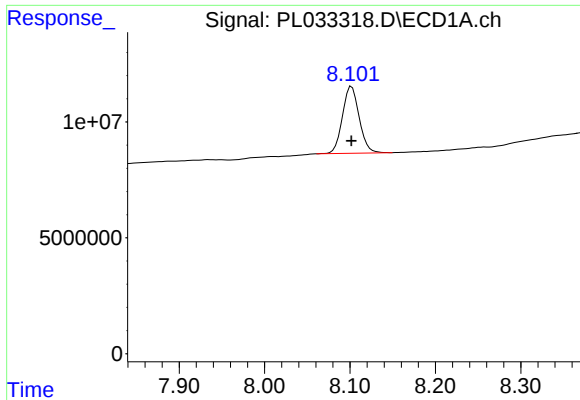


#28 Decachlorobiphenyl

R.T.: 8.102 min

Delta R.T.: 0.000 min

Response: 39406877

Conc: 5.56 ng/ml

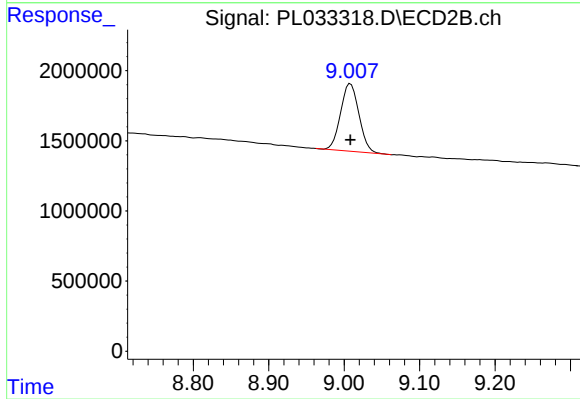

#28 Decachlorobiphenyl

R.T.: 9.008 min

Delta R.T.: 0.000 min

Response: 8184649

Conc: 5.69 ng/ml