

Data Path : P:\HPCHEM1\ECD_L\Data\PL022318\
 Data File : PL033321.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Feb 2018 14:07
 Operator : UA\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 23 23:03:15 2018
 Quant Method : P:\HPCHEM1\ECD_L\methods\PL022318.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 23 13:36:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	3.402	3.985	297.8E6	76215259	50.545	47.146
28)	SA Decachlor...	8.103	9.009	354.8E6	72480919	45.599	46.987
Target Compounds							
23)	Chlordane-1	4.259	4.971	139.9E6	37566403	496.877	491.057
24)	Chlordane-2	4.755	5.434	157.2E6	41122435	490.111	496.846
25)	Chlordane-3	5.313	6.074	503.6E6	128.4E6	504.223	489.874
26)	Chlordane-4	5.371	6.150	445.6E6	153.4E6	495.087	489.134
27)	Chlordane-5	5.981	6.940	72470430	30177552	465.748	493.612


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD_L\Data\PL022318\
Data File : PL033321.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Feb 2018 14:07
Operator : UA\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 23 23:03:15 2018
Quant Method : P:\HPCHEM1\ECD_L\methods\PL022318.M
Quant Title : GC Extractables
QLast Update : Fri Feb 23 13:36:10 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

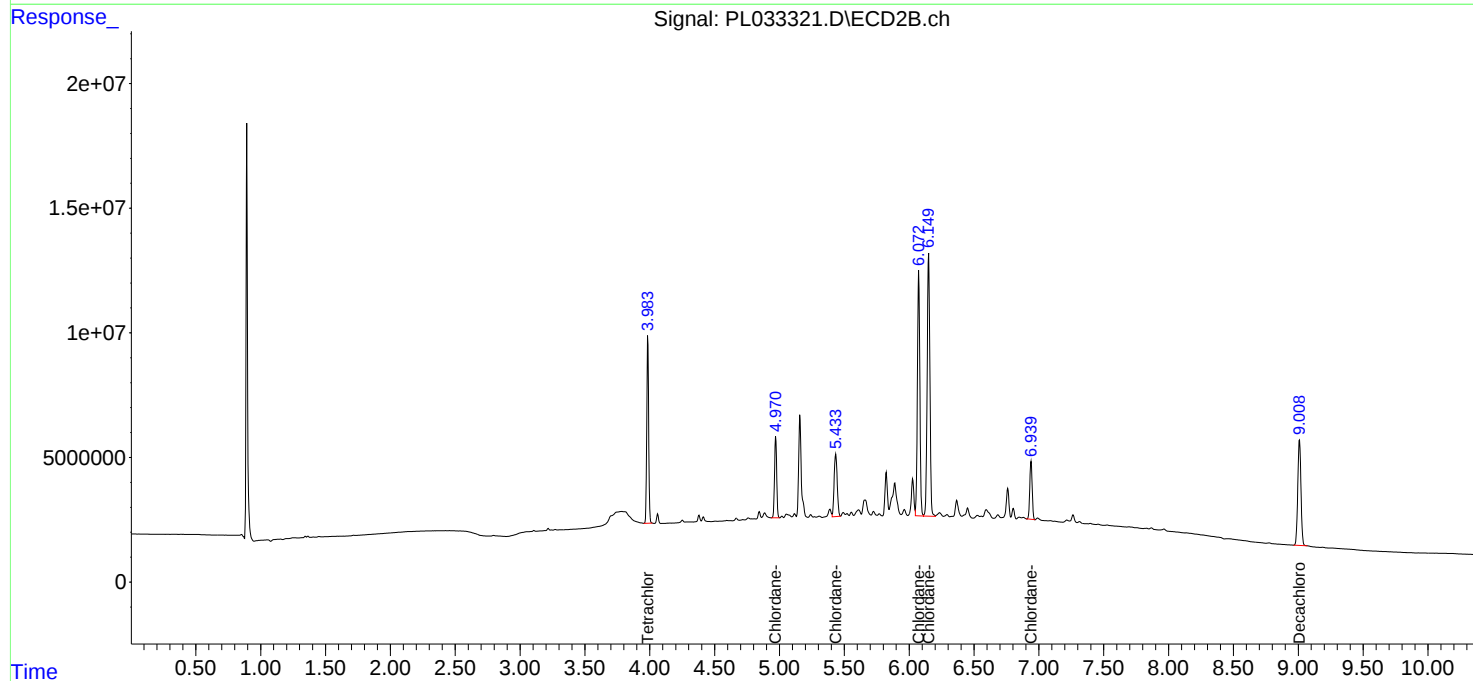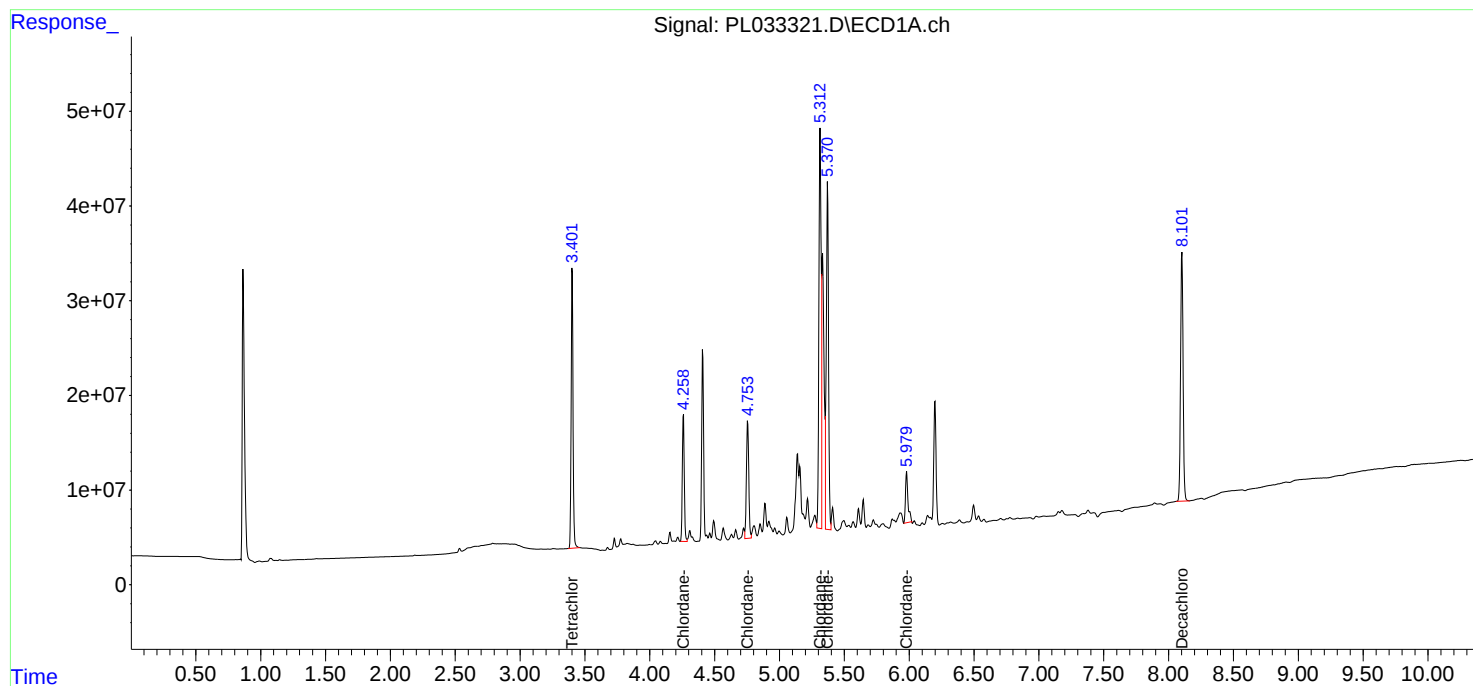

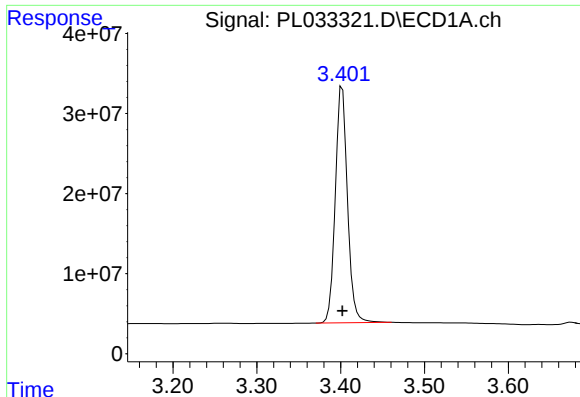


#1 Tetrachloro-m-xylene

R.T.: 3.402 min
Delta R.T.: 0.000 min
Response: 297807771
Conc: 50.54 ng/ml

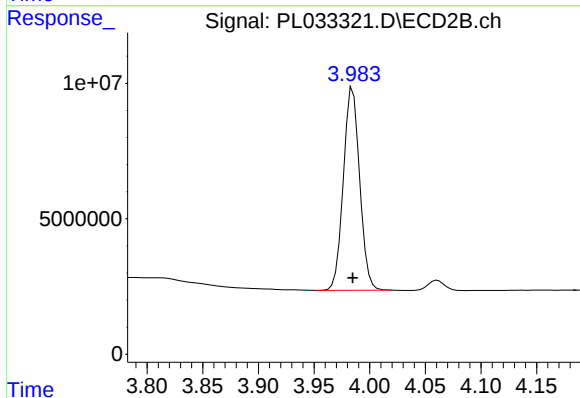


#1 Tetrachloro-m-xylene

R.T.: 3.985 min
Delta R.T.: 0.000 min
Response: 76215259
Conc: 47.15 ng/ml

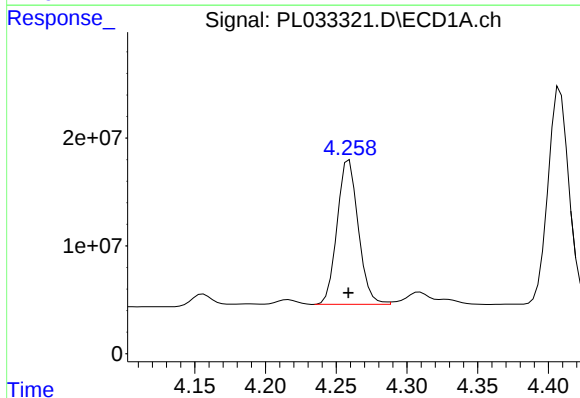


#23 Chlordane-1

R.T.: 4.259 min
Delta R.T.: 0.000 min
Response: 139922124
Conc: 496.88 ng/ml

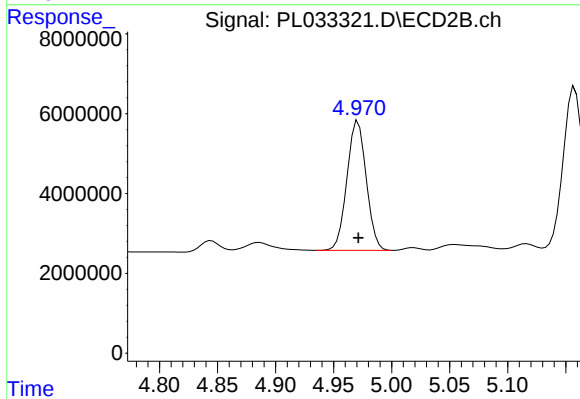


#23 Chlordane-1

R.T.: 4.971 min
Delta R.T.: 0.000 min
Response: 37566403
Conc: 491.06 ng/ml

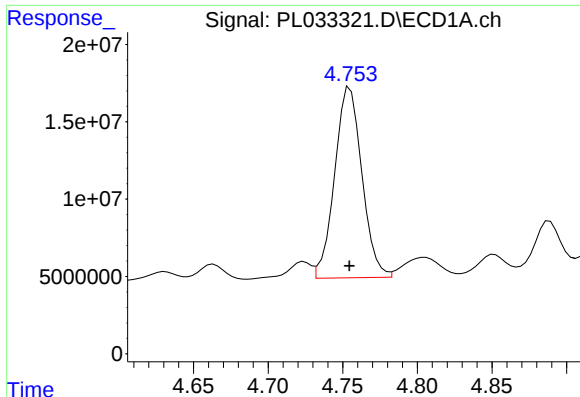


#24 Chlordane-2

R.T.: 4.755 min
Delta R.T.: 0.000 min
Response: 157193310
Conc: 490.11 ng/ml

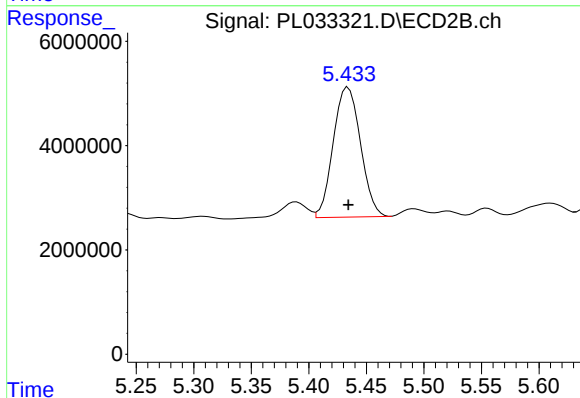


#24 Chlordane-2

R.T.: 5.434 min
Delta R.T.: 0.000 min
Response: 41122435
Conc: 496.85 ng/ml

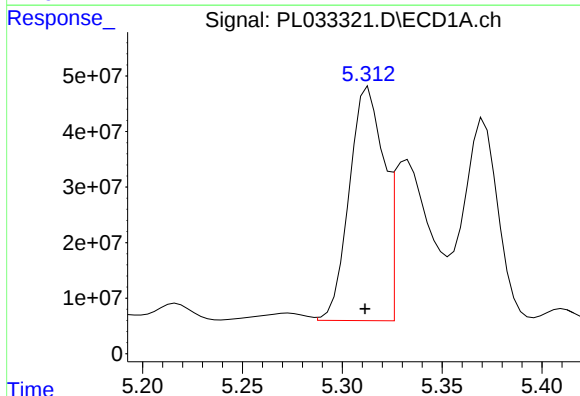


#25 Chlordane-3

R.T.: 5.313 min
Delta R.T.: 0.002 min
Response: 503587686
Conc: 504.22 ng/ml

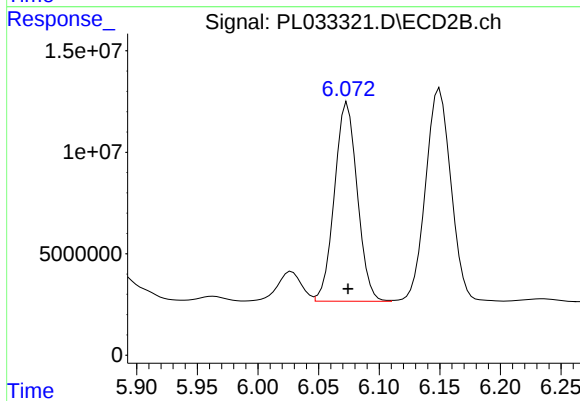


#25 Chlordane-3

R.T.: 6.074 min
Delta R.T.: 0.000 min
Response: 128404694
Conc: 489.87 ng/ml

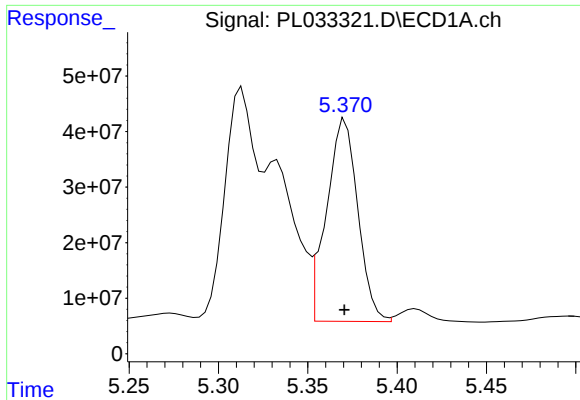


#26 Chlordane-4

R.T.: 5.371 min
Delta R.T.: 0.000 min
Response: 445609402
Conc: 495.09 ng/ml

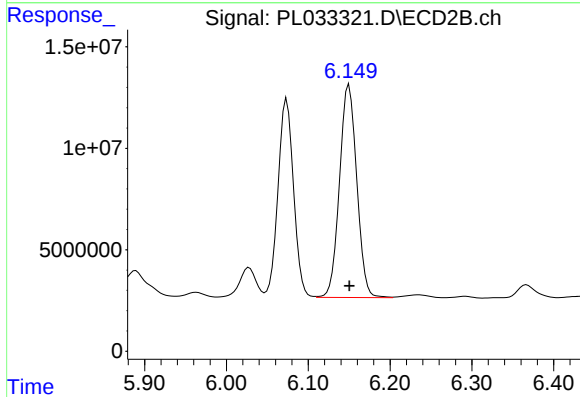


#26 Chlordane-4

R.T.: 6.150 min
Delta R.T.: 0.000 min
Response: 153391356
Conc: 489.13 ng/ml

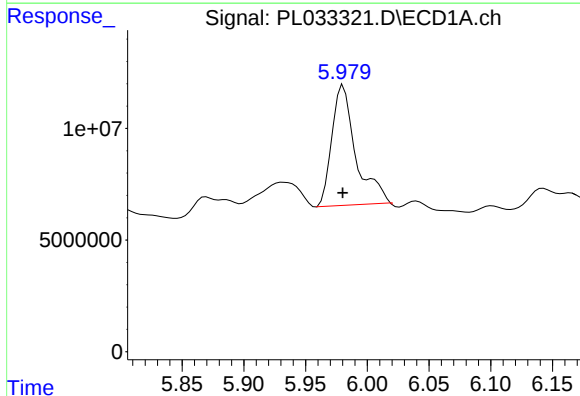


#27 Chlordane-5

R.T.: 5.981 min
Delta R.T.: 0.000 min
Response: 72470430
Conc: 465.75 ng/ml

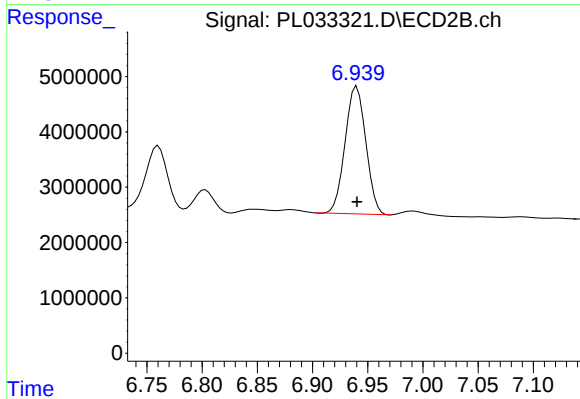


#27 Chlordane-5

R.T.: 6.940 min
Delta R.T.: 0.000 min
Response: 30177552
Conc: 493.61 ng/ml

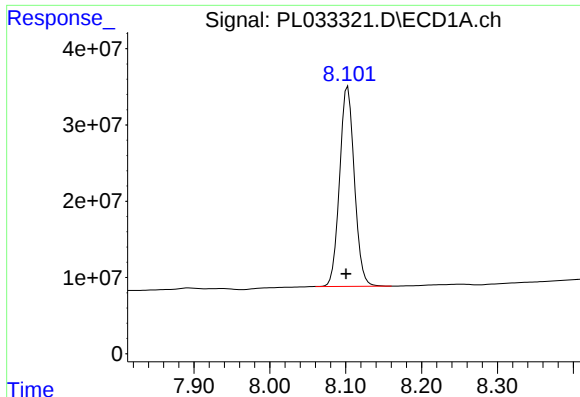

#28 Decachlorobiphenyl

R.T.: 8.103 min
Delta R.T.: 0.002 min
Response: 354774420
Conc: 45.60 ng/ml

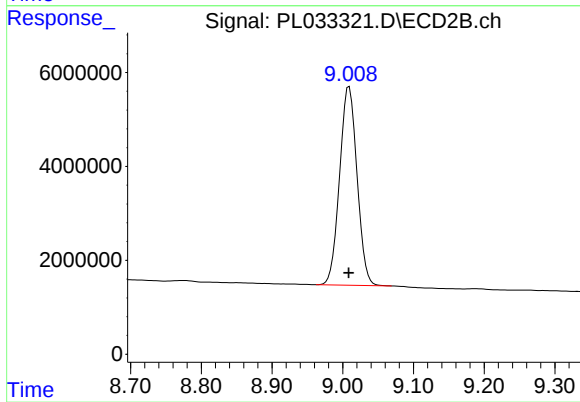

#28 Decachlorobiphenyl

R.T.: 9.009 min
Delta R.T.: 0.000 min
Response: 72480919
Conc: 46.99 ng/ml