

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022323\
 Data File : PL081103.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Feb 2023 14:40
 Operator : AR\AJ
 Sample : 01654-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 UGT

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 02/24/2023
 Supervised By : Ankita Jodhani 02/24/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 23 19:09:53 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022023.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 20 18:06:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.350	2.687	20161283	19516954	8.649	8.481
28) SA Decachlor...	8.785	7.830	16428933	19557332	8.403	8.348
Target Compounds						
17) MA 4,4'-DDT	6.810	5.946	5110041	6960002	2.262m	3.210 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022323\
Data File : PL081103.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Feb 2023 14:40
Operator : AR\AJ
Sample : 01654-01
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
UGT


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 02/24/2023
Supervised By : Ankita Jodhani 02/24/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 23 19:09:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022023.M
Quant Title : GC Extractables
QLast Update : Mon Feb 20 18:06:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

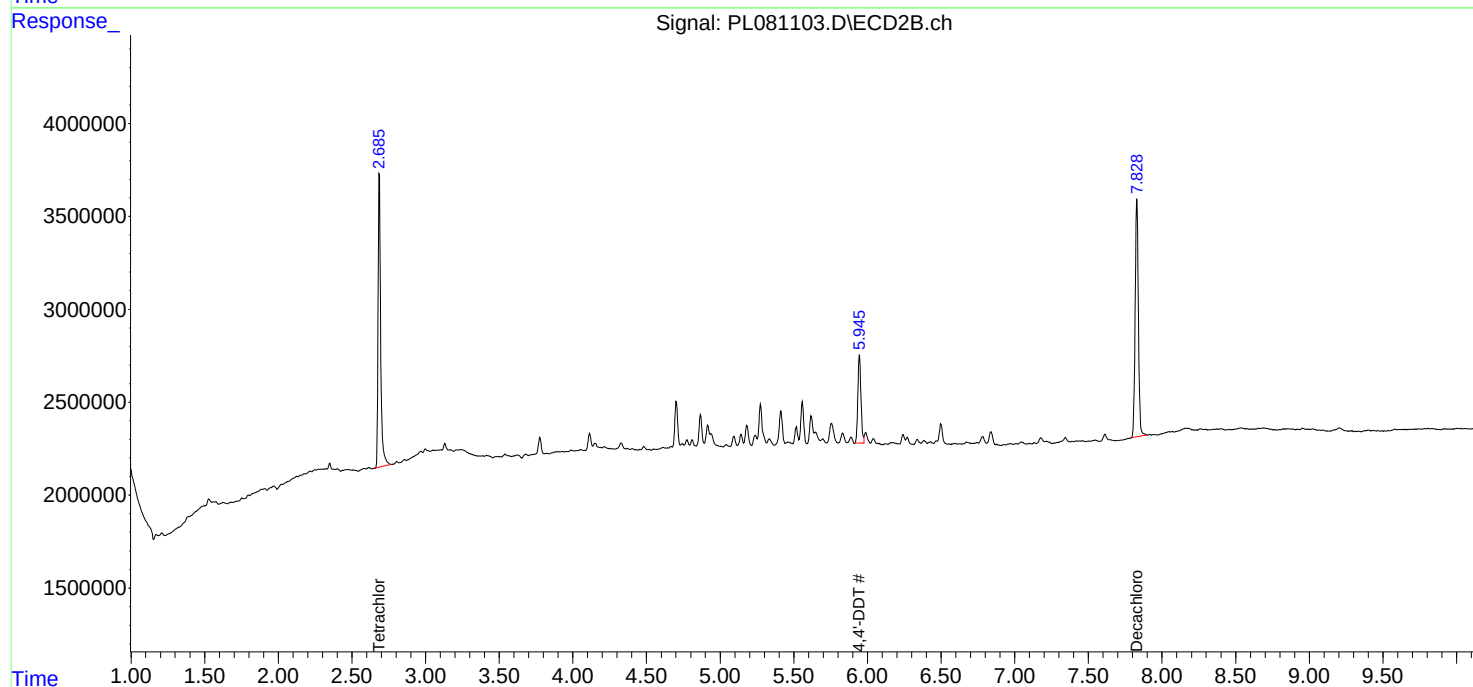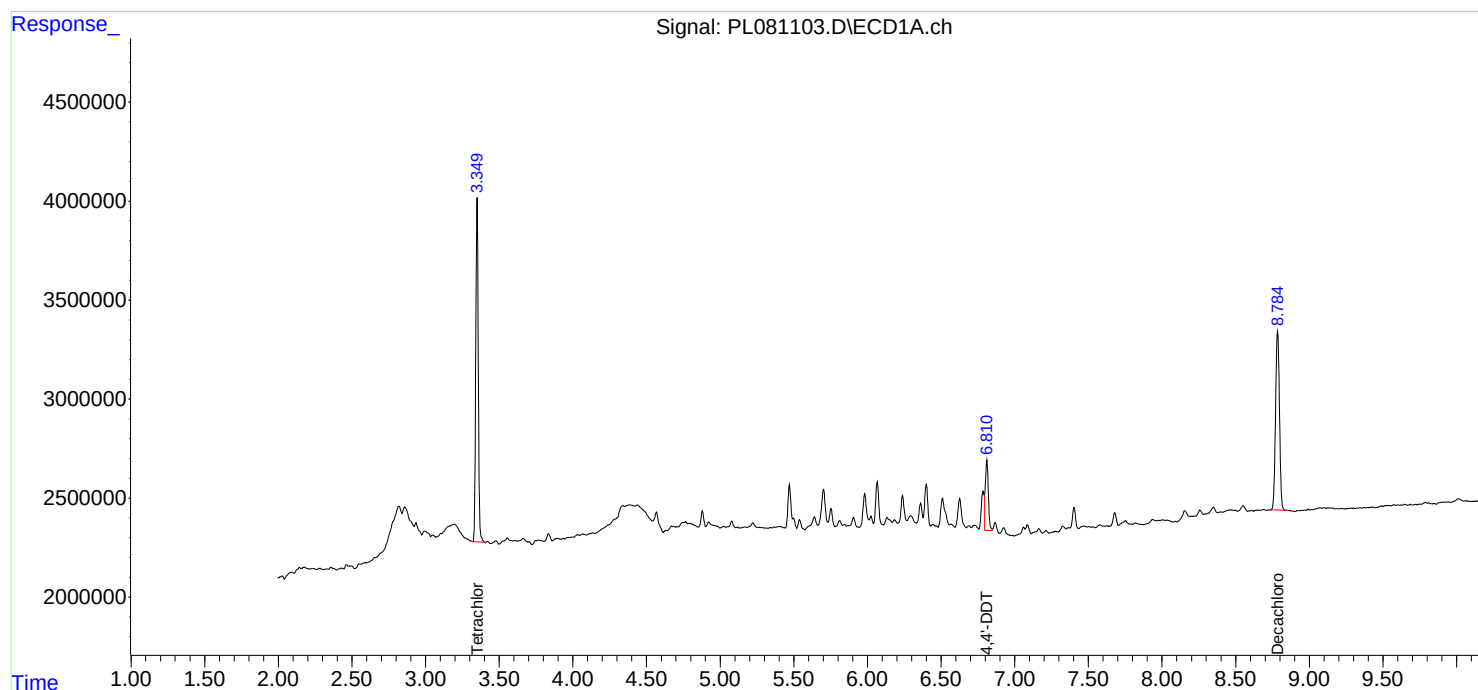

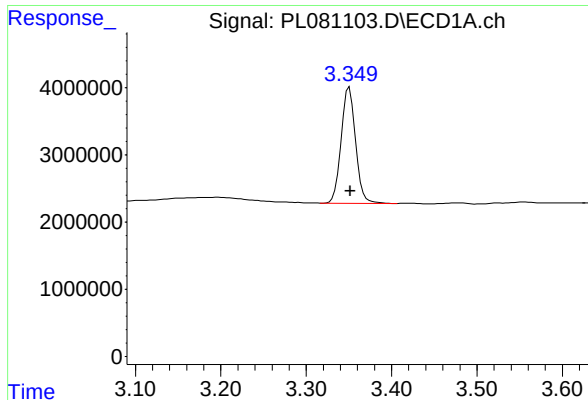


#1 Tetrachloro-m-xylene

R.T.: 3.350 min
Delta R.T.: -0.002 min
Response: 20161283
Conc: 8.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
UGT


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/24/2023
Supervised By :Ankita Jodhani 02/24/2023

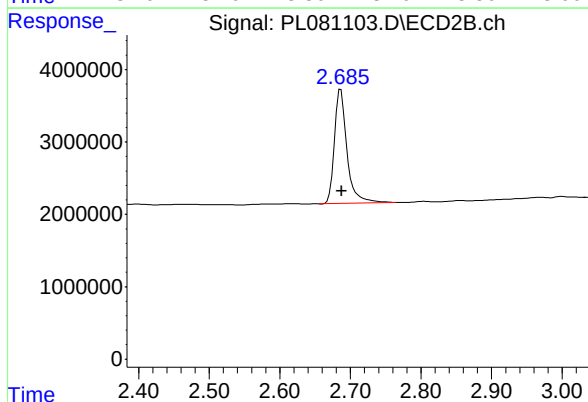


#1 Tetrachloro-m-xylene

R.T.: 2.687 min
Delta R.T.: -0.001 min
Response: 19516954
Conc: 8.48 ng/ml

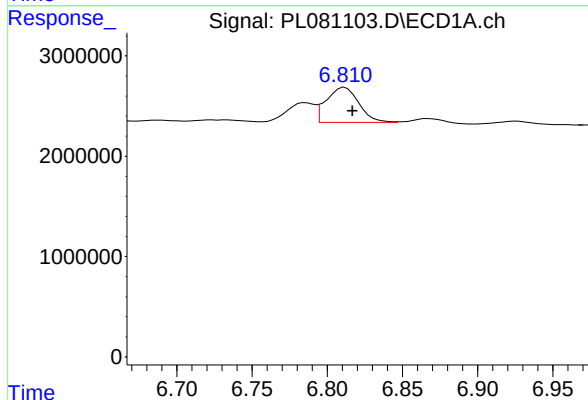


#17 4,4'-DDT

R.T.: 6.810 min
Delta R.T.: -0.007 min
Response: 5110041
Conc: 2.26 ng/ml m

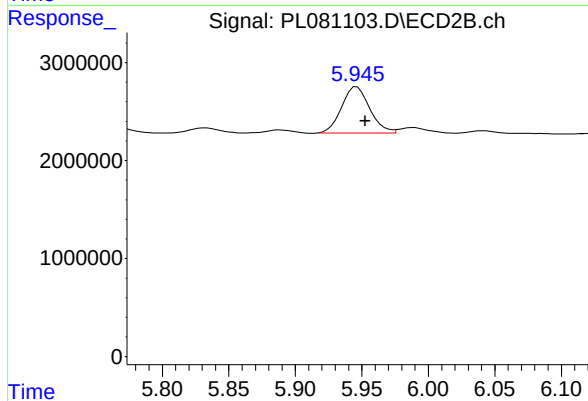

#17 4,4'-DDT

R.T.: 5.946 min
Delta R.T.: -0.006 min
Response: 6960002
Conc: 3.21 ng/ml

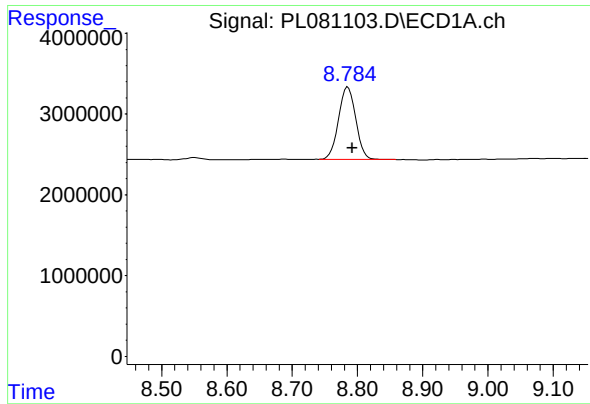


#28 Decachlorobiphenyl

R.T.: 8.785 min
Delta R.T.: -0.007 min
Response: 16428933
Conc: 8.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
UGT

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/24/2023
Supervised By :Ankita Jodhani 02/24/2023

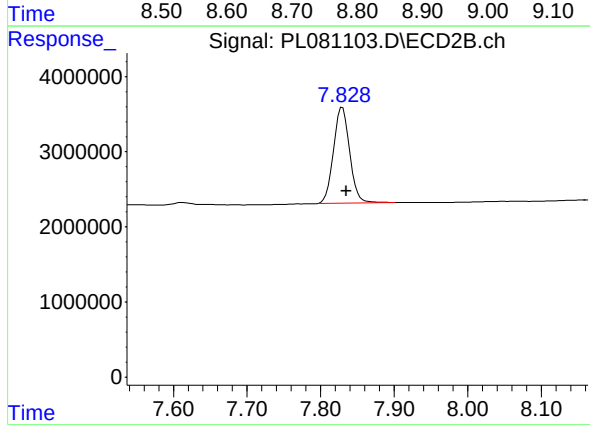

#28 Decachlorobiphenyl

R.T.: 7.830 min
Delta R.T.: -0.005 min
Response: 19557332
Conc: 8.35 ng/ml