

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022324\
 Data File : PL088271.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Feb 2024 19:26
 Operator : AR\AJ
 Sample : P1564-17
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 LKWD-BACKFILL-17

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 24 00:26:05 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021524.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 16 21:46:54 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.635	2.853	59979233	31109298	21.837	22.181
28) SA Decachlor...	9.306	8.087	42595087	26611313	22.117	20.900

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022324\
Data File : PL088271.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Feb 2024 19:26
Operator : AR\AJ
Sample : P1564-17
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
LKWD-BACKFILL-17

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 24 00:26:05 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021524.M
Quant Title : GC Extractables
QLast Update : Fri Feb 16 21:46:54 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

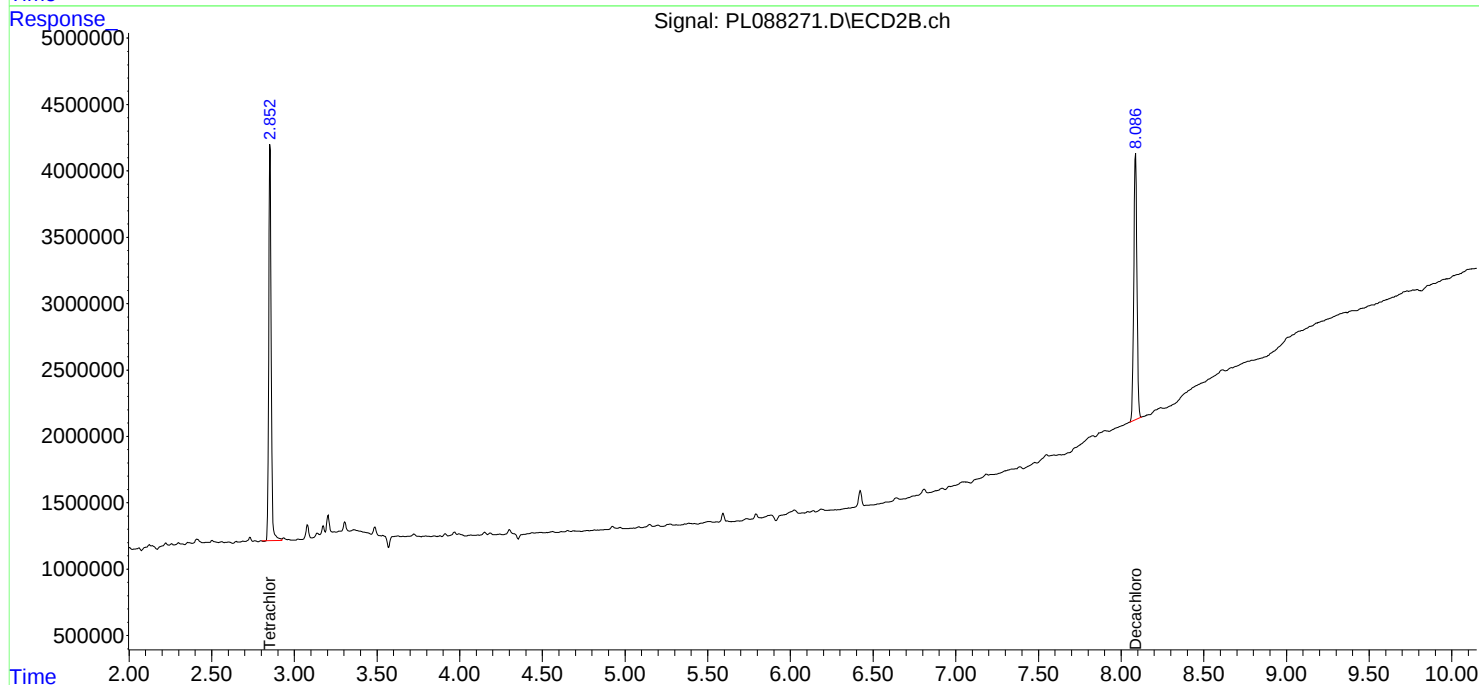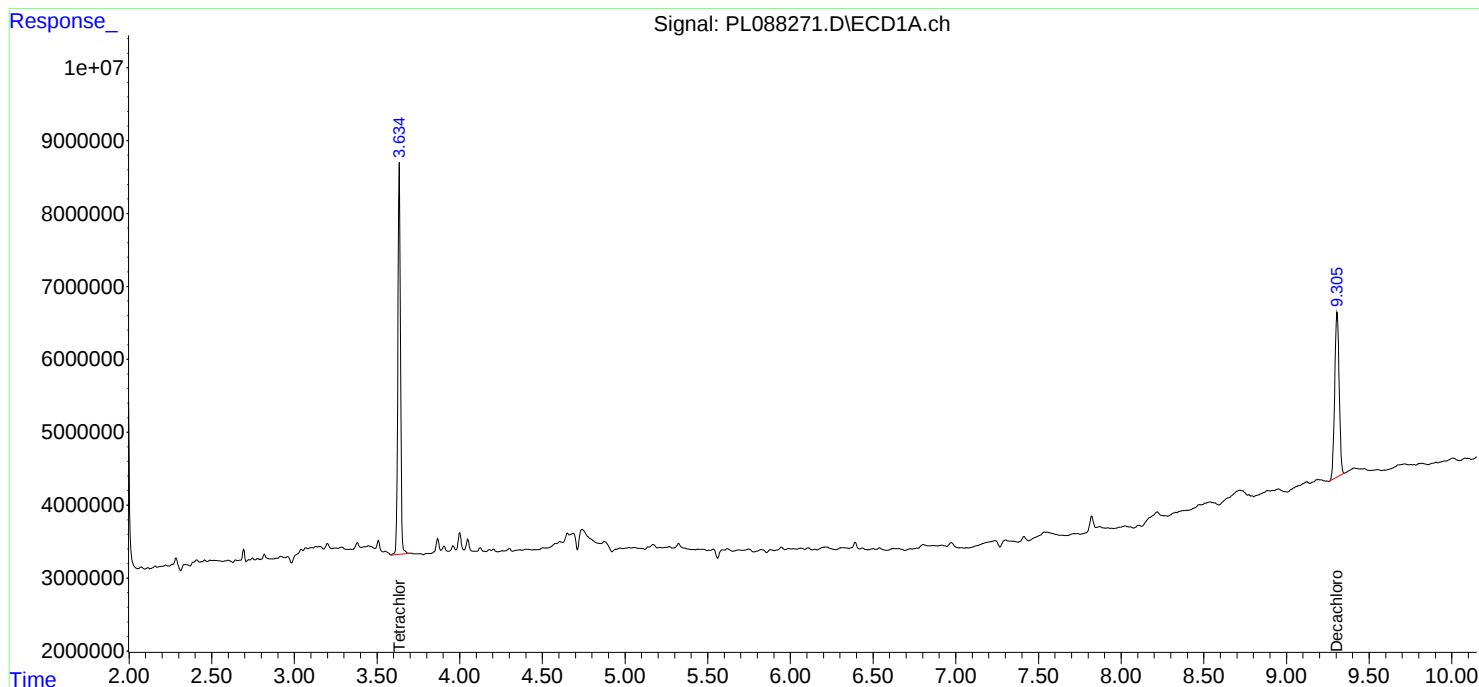


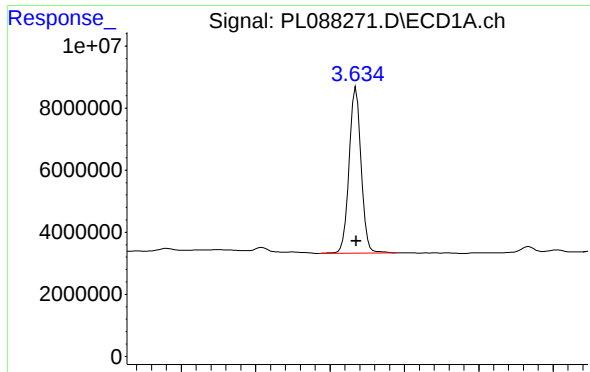

#1 Tetrachloro-m-xylene


R.T.: 3.635 min
Delta R.T.: 0.000 min
Response: 59979233
Conc: 21.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
LKWD-BACKFILL-17

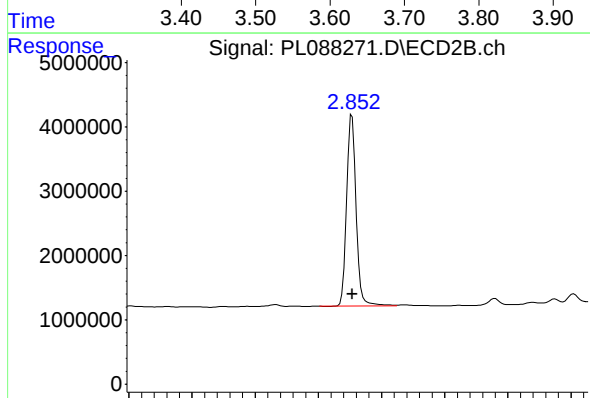


#1 Tetrachloro-m-xylene

R.T.: 2.853 min
Delta R.T.: 0.000 min
Response: 31109298
Conc: 22.18 ng/ml

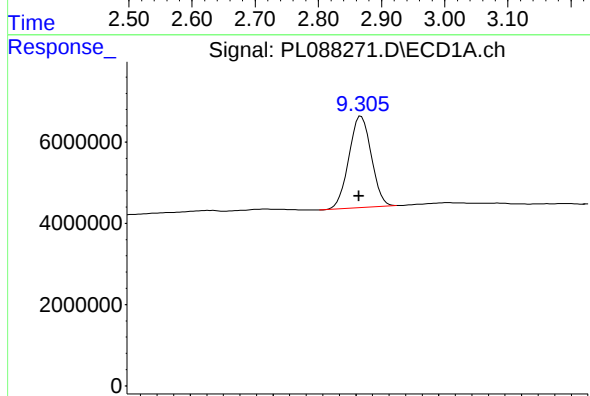

#28 Decachlorobiphenyl

R.T.: 9.306 min
Delta R.T.: 0.003 min
Response: 42595087
Conc: 22.12 ng/ml

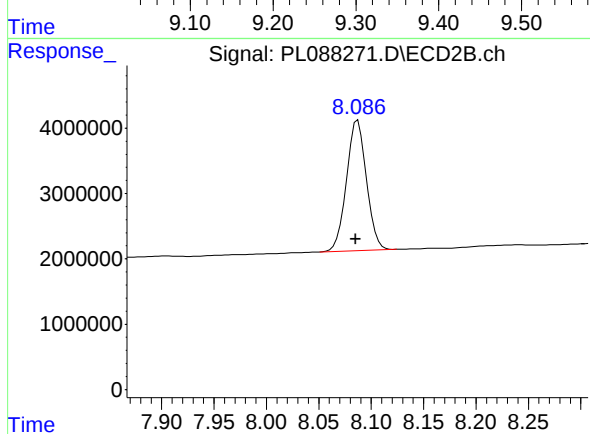

#28 Decachlorobiphenyl

R.T.: 8.087 min
Delta R.T.: 0.002 min
Response: 26611313
Conc: 20.90 ng/ml