

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022420\
 Data File : PL056787.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Feb 2020 13:11
 Operator : AJ\MA
 Sample : PB127023BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB127023BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 25 02:35:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021920.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 20 02:32:45 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.504	4.019	180.8E6	47905829	20.903	19.232
28)	SA Decachlor...	8.260	9.098	242.5E6	46462748	20.384	22.111
Target Compounds							
11)	B alpha-Chl...	5.499	0.000	31128331	0	2.156	N.D. #
13)	MA Dieldrin	5.785	0.000	31886902	0	2.139	N.D. #
14)	MA Endrin	6.076f	0.000	16043977	0	1.189	N.D. #
15)	B Endosulfa...	6.303f	0.000	22522727	0	1.814	N.D. #
16)	A 4,4'-DDD	6.182	0.000	25378263	0	2.269	N.D. #
17)	MA 4,4'-DDT	6.421	0.000	37591684	0	3.452	N.D. #
18)	B Endrin al...	6.490	0.000	18462836	0	1.706	N.D. #
26)	Chlordane-4	5.499	0.000	31128331	0	28.978	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022420\
Data File : PL056787.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Feb 2020 13:11
Operator : AJ\MA
Sample : PB127023BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB127023BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 25 02:35:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021920.M
Quant Title : GC Extractables
QLast Update : Thu Feb 20 02:32:45 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

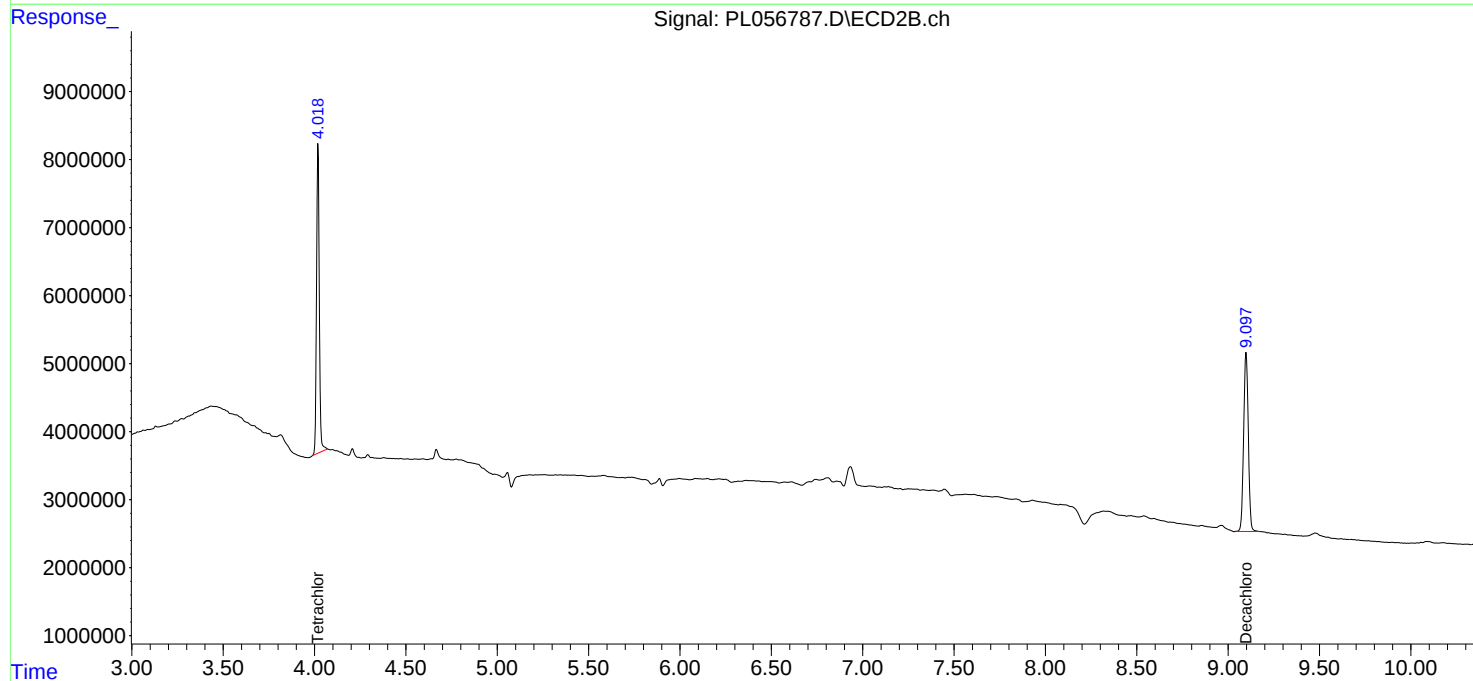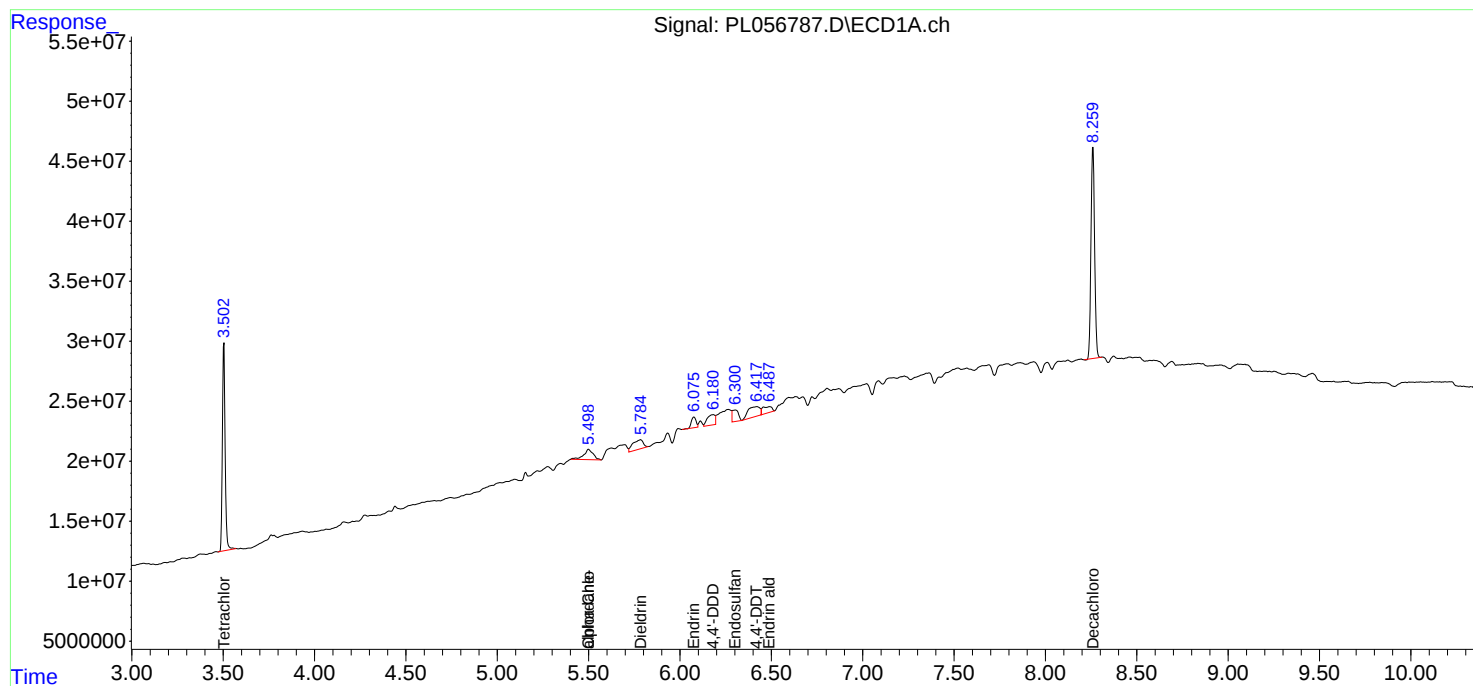


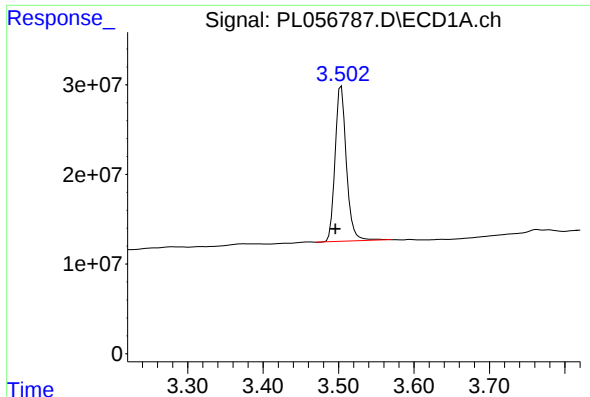

#1 Tetrachloro-m-xylene


R.T.: 3.504 min
Delta R.T.: 0.008 min
Response: 180764730
Conc: 20.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB127023BL

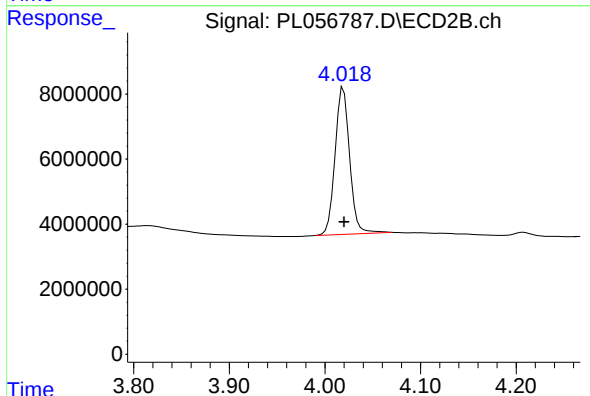


#1 Tetrachloro-m-xylene

R.T.: 4.019 min
Delta R.T.: 0.000 min
Response: 47905829
Conc: 19.23 ng/ml

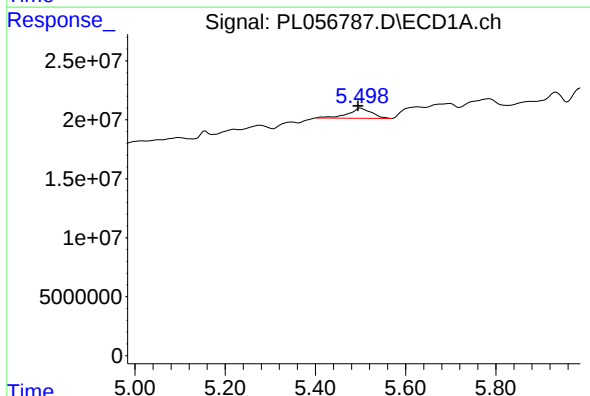


#11 alpha-Chlordane

R.T.: 5.499 min
Delta R.T.: 0.004 min
Response: 31128331
Conc: 2.16 ng/ml

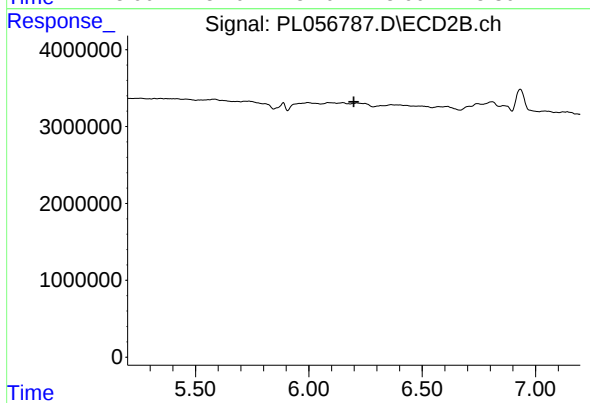

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.199 min
Response: 0
Conc: N.D.

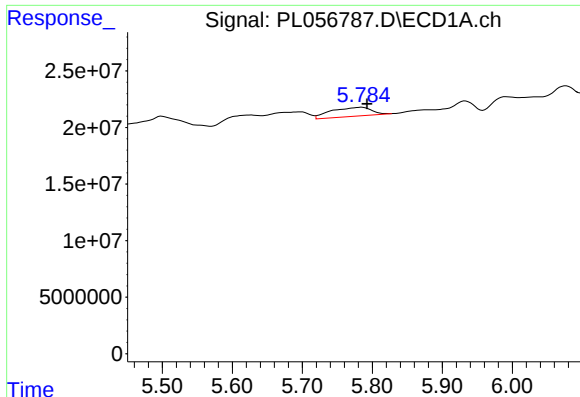

#13 Dieldrin


R.T.: 5.785 min
Delta R.T.: -0.007 min
Response: 31886902
Conc: 2.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB127023BL

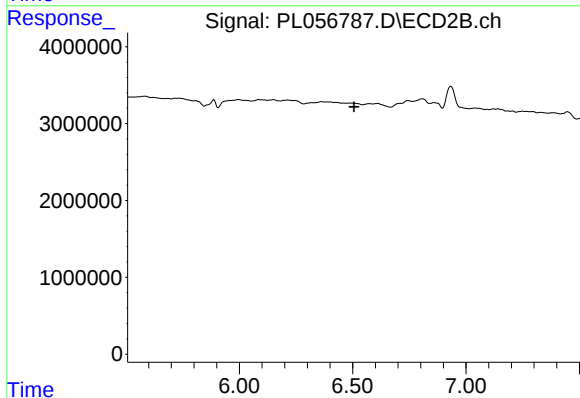


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.506 min
Response: 0
Conc: N.D.

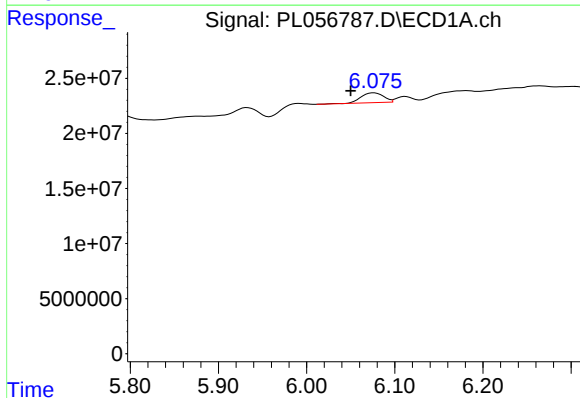


#14 Endrin

R.T.: 6.076 min
Delta R.T.: 0.026 min
Response: 16043977
Conc: 1.19 ng/ml

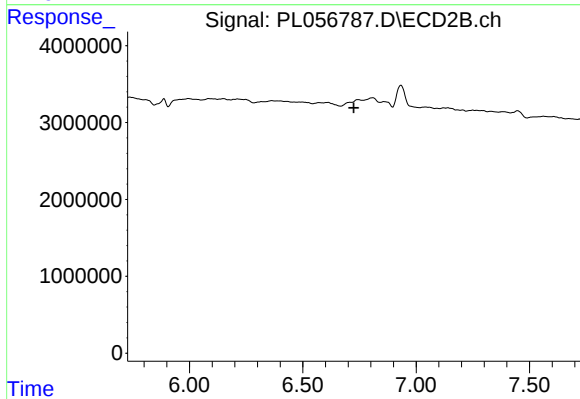

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.725 min
Response: 0
Conc: N.D.

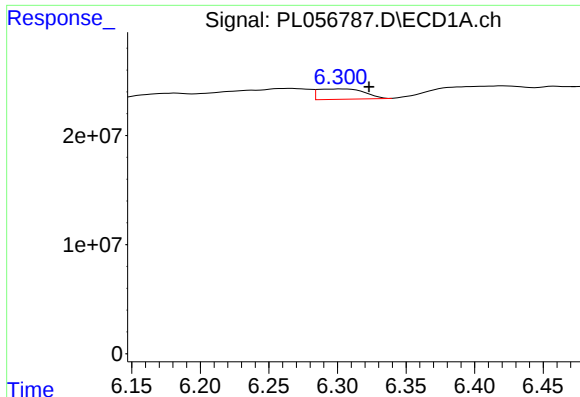

#15 Endosulfan II


R.T.: 6.303 min
Delta R.T.: -0.020 min
Response: 22522727
Conc: 1.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB127023BL

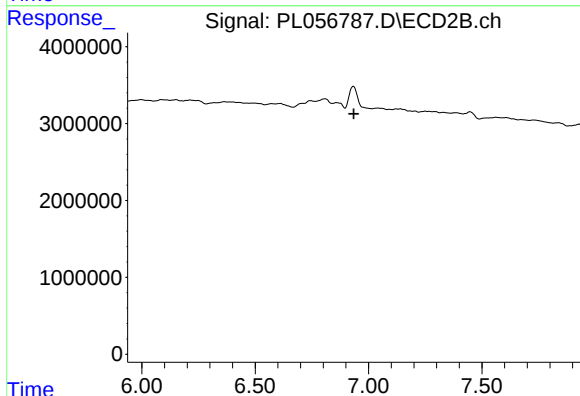


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.936 min
Response: 0
Conc: N.D.

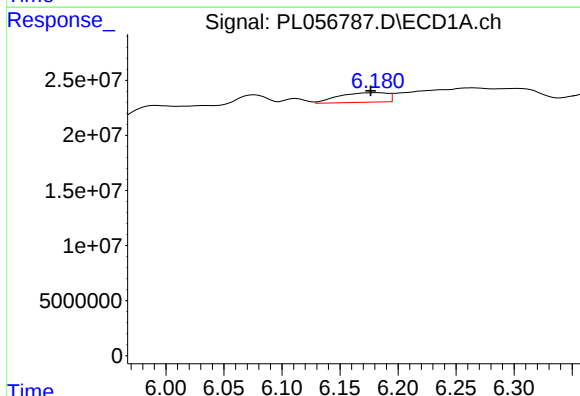


#16 4,4'-DDD

R.T.: 6.182 min
Delta R.T.: 0.006 min
Response: 25378263
Conc: 2.27 ng/ml

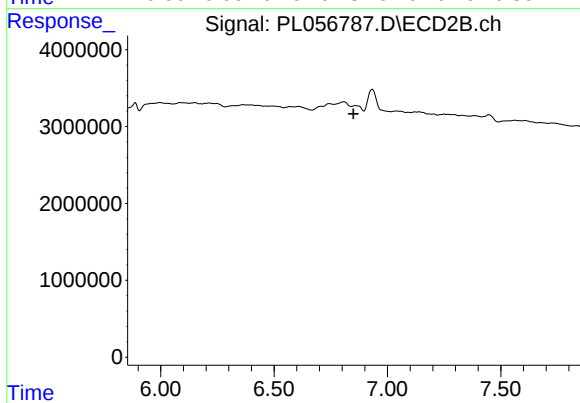

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.850 min
Response: 0
Conc: N.D.

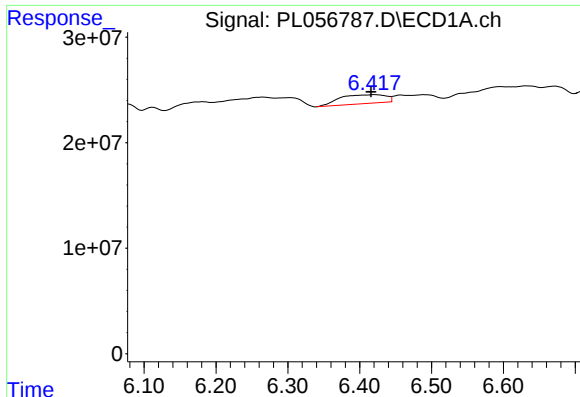

#17 4,4'-DDT


R.T.: 6.421 min
Delta R.T.: 0.005 min
Response: 37591684
Conc: 3.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB127023BL

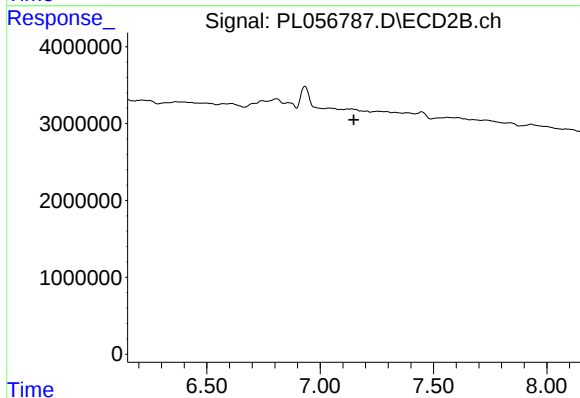


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.148 min
Response: 0
Conc: N.D.

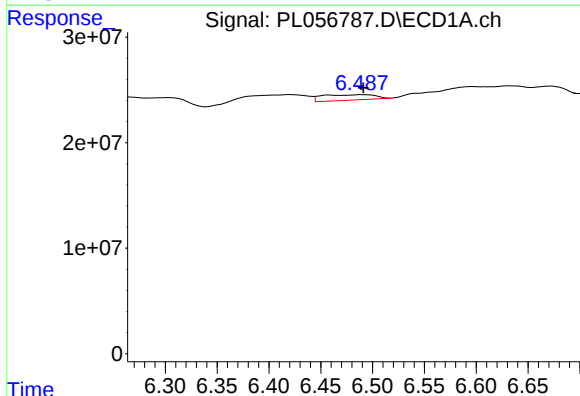


#18 Endrin aldehyde

R.T.: 6.490 min
Delta R.T.: -0.001 min
Response: 18462836
Conc: 1.71 ng/ml

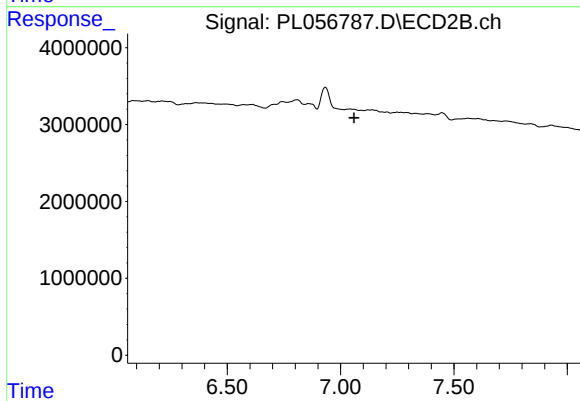

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 7.060 min
Response: 0
Conc: N.D.

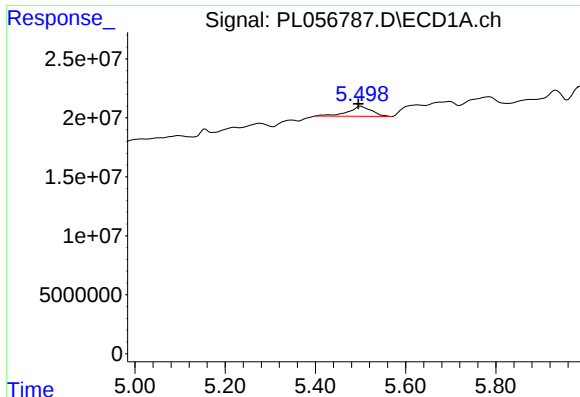

#26 Chlordane-4


R.T.: 5.499 min
Delta R.T.: 0.004 min
Response: 31128331
Conc: 28.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB127023BL

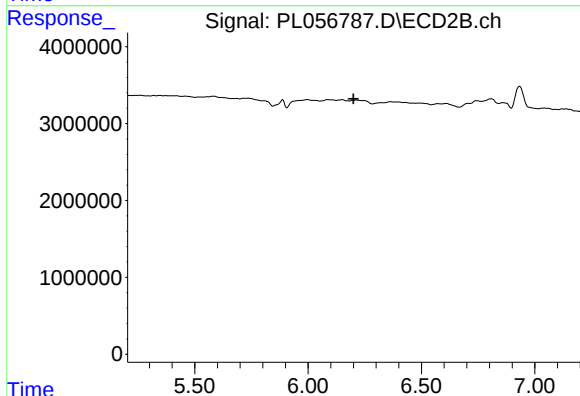


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.200 min
Response: 0
Conc: N.D.

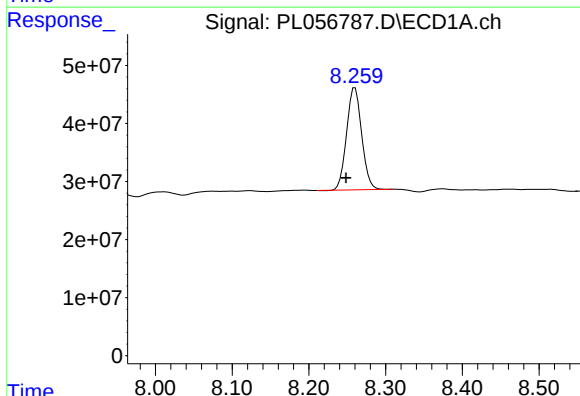

#28 Decachlorobiphenyl

R.T.: 8.260 min
Delta R.T.: 0.012 min
Response: 242469097
Conc: 20.38 ng/ml

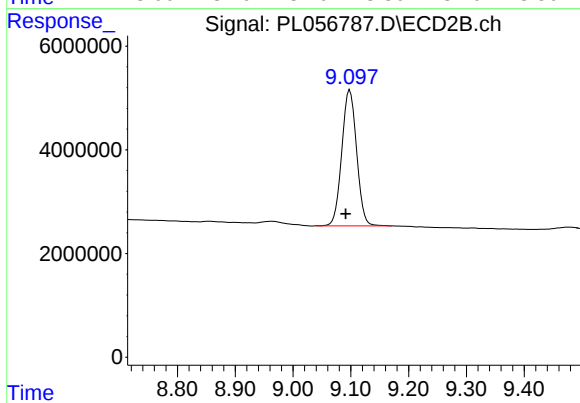

#28 Decachlorobiphenyl

R.T.: 9.098 min
Delta R.T.: 0.007 min
Response: 46462748
Conc: 22.11 ng/ml