

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022420\
 Data File : PL056789.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Feb 2020 13:54
 Operator : AJ\MA
 Sample : L1655-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FK-BPM-01-AA1-BB1-AA1A-BB1A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 25 02:36:09 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021920.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 20 02:32:45 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.497	4.020	214.2E6	62874286	24.766	25.241
28)	SA Decachlor...	8.252	9.094	240.4E6	48185974	20.209	22.931
Target Compounds							
15)	B Endosulfa...	6.300f	0.000	8296482	0	0.668	N.D. #
17)	MA 4,4'-DDT	6.415	0.000	11119840	0	1.021	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022420\
Data File : PL056789.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Feb 2020 13:54
Operator : AJ\MA
Sample : L1655-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
FK-BPM-01-AA1-BB1-AA1A-BB1A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 25 02:36:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021920.M
Quant Title : GC Extractables
QLast Update : Thu Feb 20 02:32:45 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

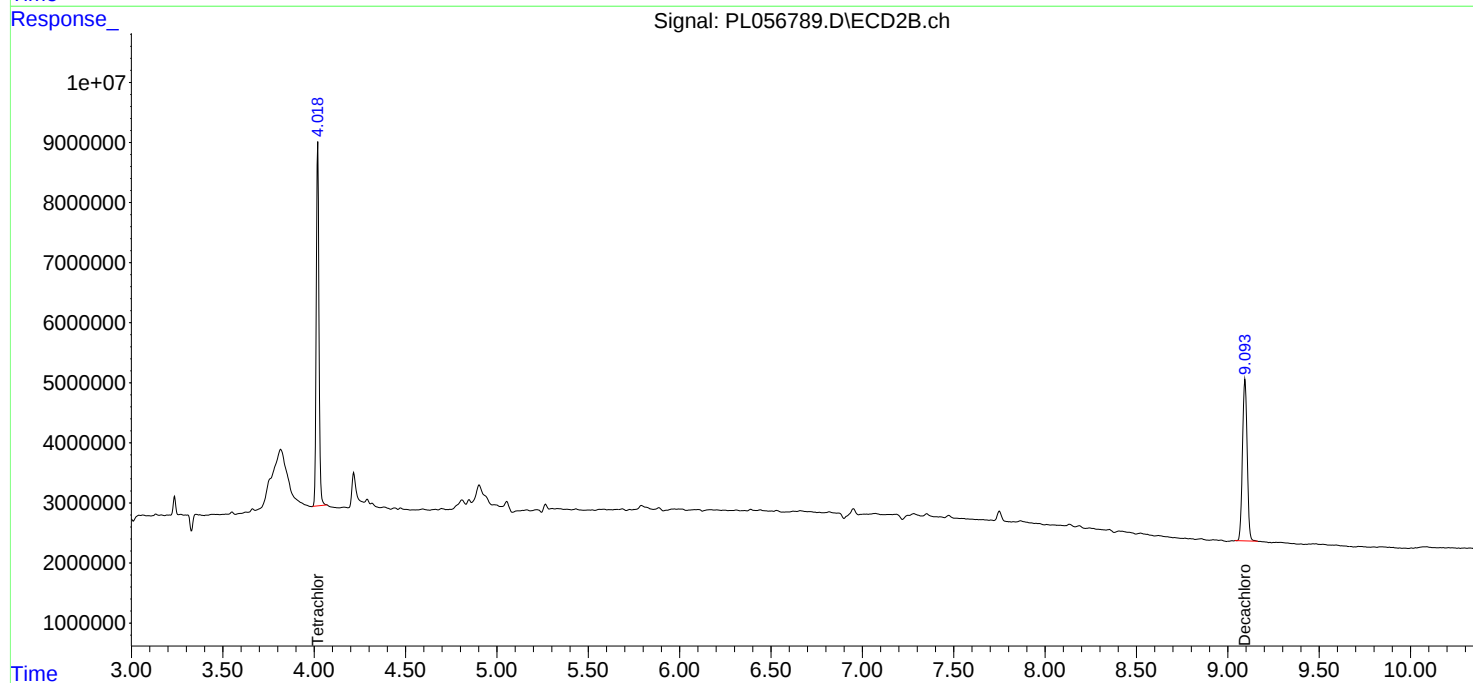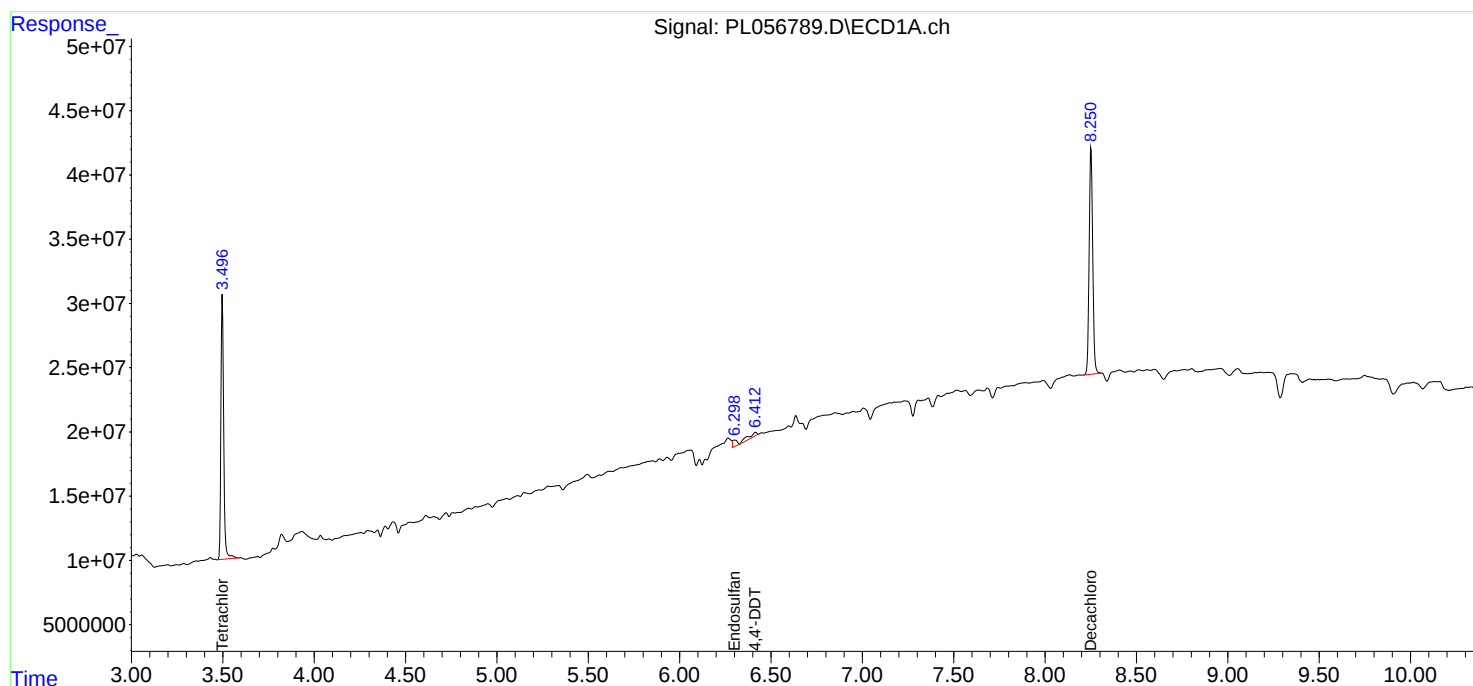


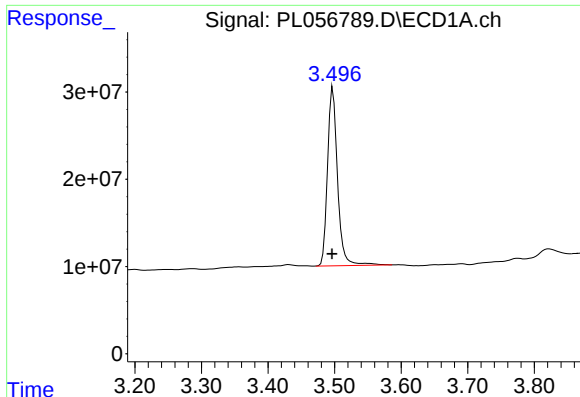

#1 Tetrachloro-m-xylene


R.T.: 3.497 min
Delta R.T.: 0.001 min
Response: 214164670
Conc: 24.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-BPM-01-AA1-BB1-AA1A-BB1A

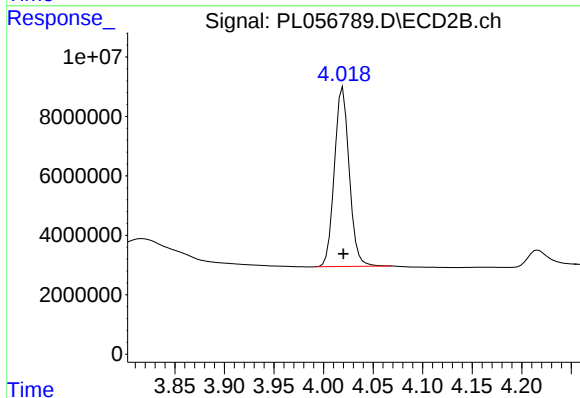


#1 Tetrachloro-m-xylene

R.T.: 4.020 min
Delta R.T.: 0.000 min
Response: 62874286
Conc: 25.24 ng/ml

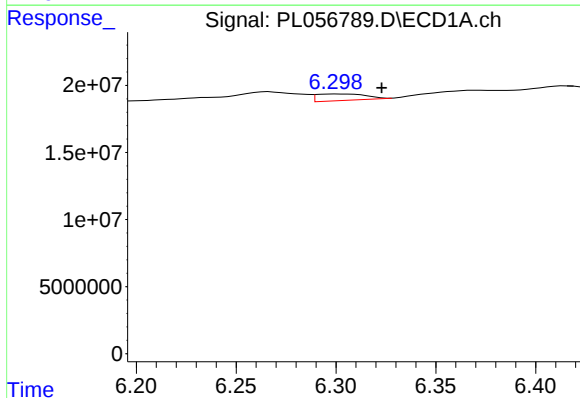


#15 Endosulfan II

R.T.: 6.300 min
Delta R.T.: -0.023 min
Response: 8296482
Conc: 0.67 ng/ml

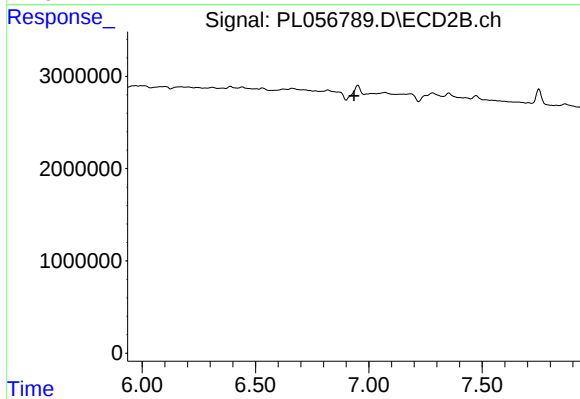

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.936 min
Response: 0
Conc: N.D.

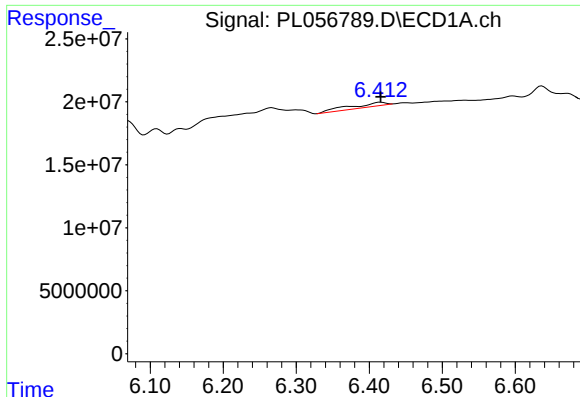

#17 4,4'-DDT


R.T.: 6.415 min
Delta R.T.: 0.000 min
Response: 11119840
Conc: 1.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-BPM-01-AA1-BB1-AA1A-BB1A

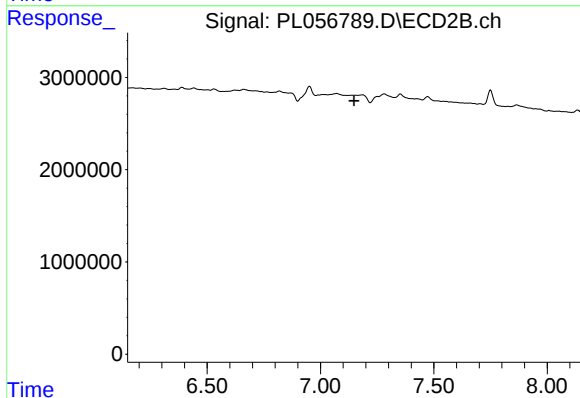


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 7.148 min
Response: 0
Conc: N.D.

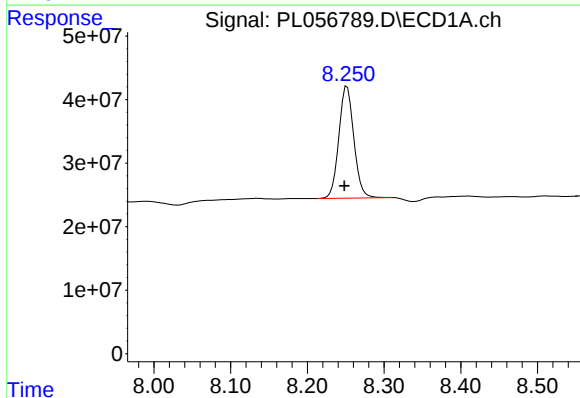

#28 Decachlorobiphenyl

R.T.: 8.252 min
Delta R.T.: 0.003 min
Response: 240389969
Conc: 20.21 ng/ml

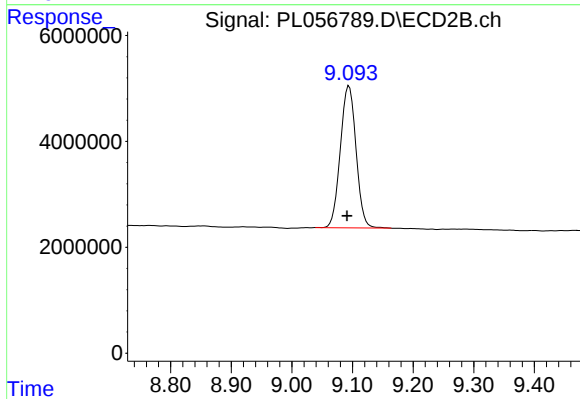

#28 Decachlorobiphenyl

R.T.: 9.094 min
Delta R.T.: 0.003 min
Response: 48185974
Conc: 22.93 ng/ml