

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022420\
 Data File : PL056790.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Feb 2020 14:08
 Operator : AJ\MA
 Sample : L1656-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FK-BPM-04-006-ABCD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 25 02:36:20 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021920.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 20 02:32:45 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.497	4.019	215.9E6	64840476	24.969	26.030
28)	SA Decachlor...	8.252	9.093	237.9E6	49410932	20.002	23.514
Target Compounds							
23)	Chlordane-1	4.391f	0.000	10603246	0	29.106	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022420\
Data File : PL056790.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Feb 2020 14:08
Operator : AJ\MA
Sample : L1656-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
FK-BPM-04-006-ABCD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 25 02:36:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021920.M
Quant Title : GC Extractables
QLast Update : Thu Feb 20 02:32:45 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

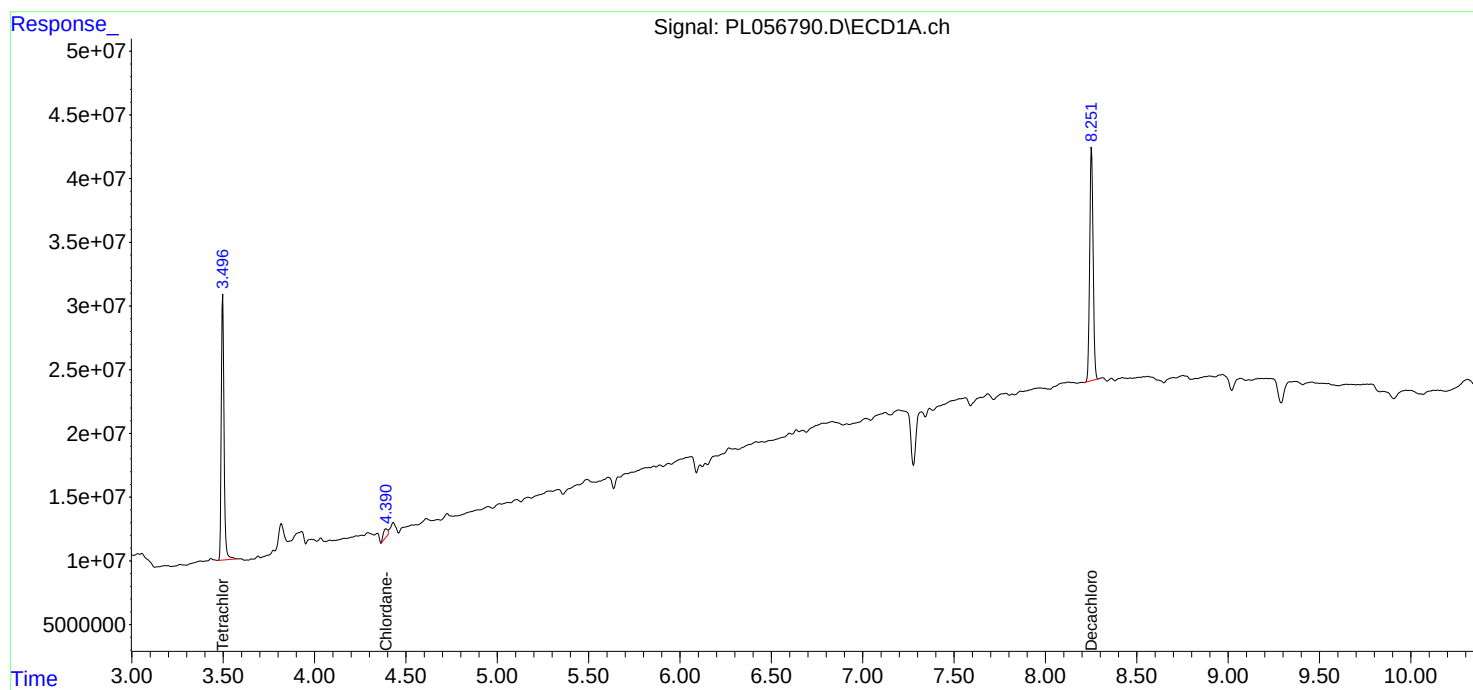


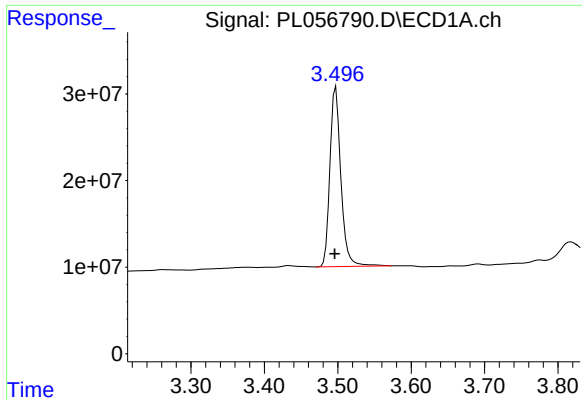

#1 Tetrachloro-m-xylene


R.T.: 3.497 min
Delta R.T.: 0.001 min
Response: 215924412
Conc: 24.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-BPM-04-006-ABCD

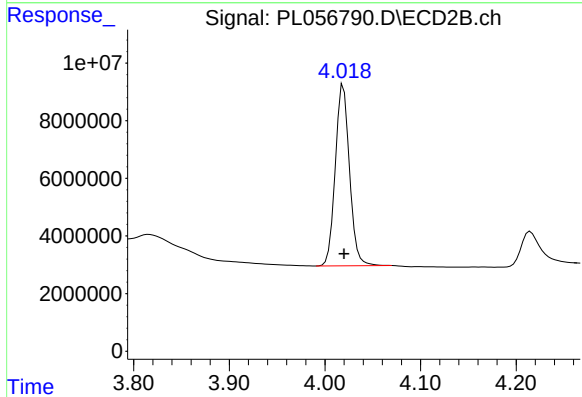


#1 Tetrachloro-m-xylene

R.T.: 4.019 min
Delta R.T.: 0.000 min
Response: 64840476
Conc: 26.03 ng/ml

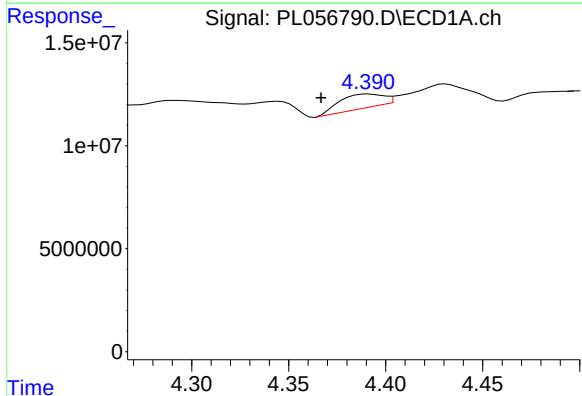


#23 Chlordane-1

R.T.: 4.391 min
Delta R.T.: 0.024 min
Response: 10603246
Conc: 29.11 ng/ml

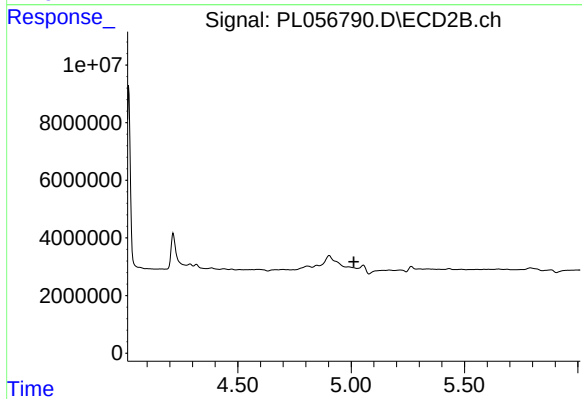

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.012 min
Response: 0
Conc: N.D.

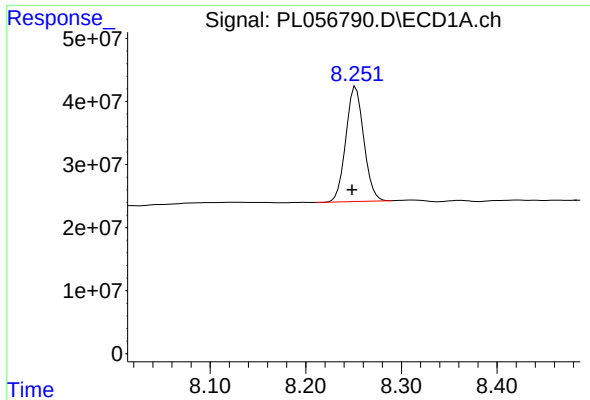

#28 Decachlorobiphenyl

R.T.: 8.252 min
Delta R.T.: 0.004 min
Response: 237930443
Conc: 20.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-BPM-04-006-ABCD

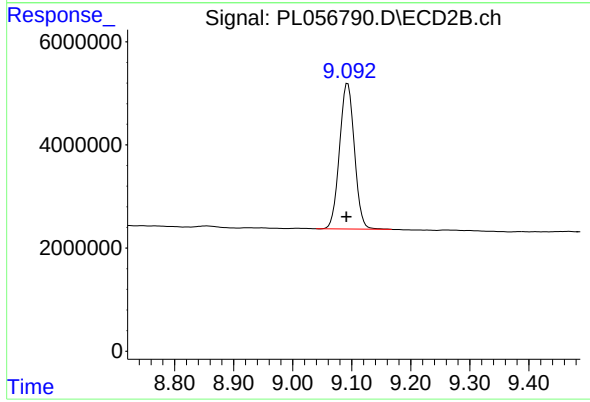

#28 Decachlorobiphenyl

R.T.: 9.093 min
Delta R.T.: 0.002 min
Response: 49410932
Conc: 23.51 ng/ml