

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022420\
 Data File : PL056796.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Feb 2020 15:33
 Operator : AJ\MA
 Sample : L1654-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 25 02:37:34 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021920.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 20 02:32:45 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.498	4.020	217.5E6	66852529	25.154	26.838
28)	SA Decachlor...	8.253	9.093	261.2E6	53399387	21.956	25.412
Target Compounds							
11)	B alpha-Chl...	5.492	0.000	15549770	0	1.077	N.D. #
12)	B 4,4'-DDE	5.678f	0.000	10798329	0	0.768	N.D. #
17)	MA 4,4'-DDT	6.418	0.000	7133767	0	0.655	N.D. #
26)	Chlordane-4	5.492	0.000	15549770	0	14.475	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022420\
Data File : PL056796.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Feb 2020 15:33
Operator : AJ\MA
Sample : L1654-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 25 02:37:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021920.M
Quant Title : GC Extractables
QLast Update : Thu Feb 20 02:32:45 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

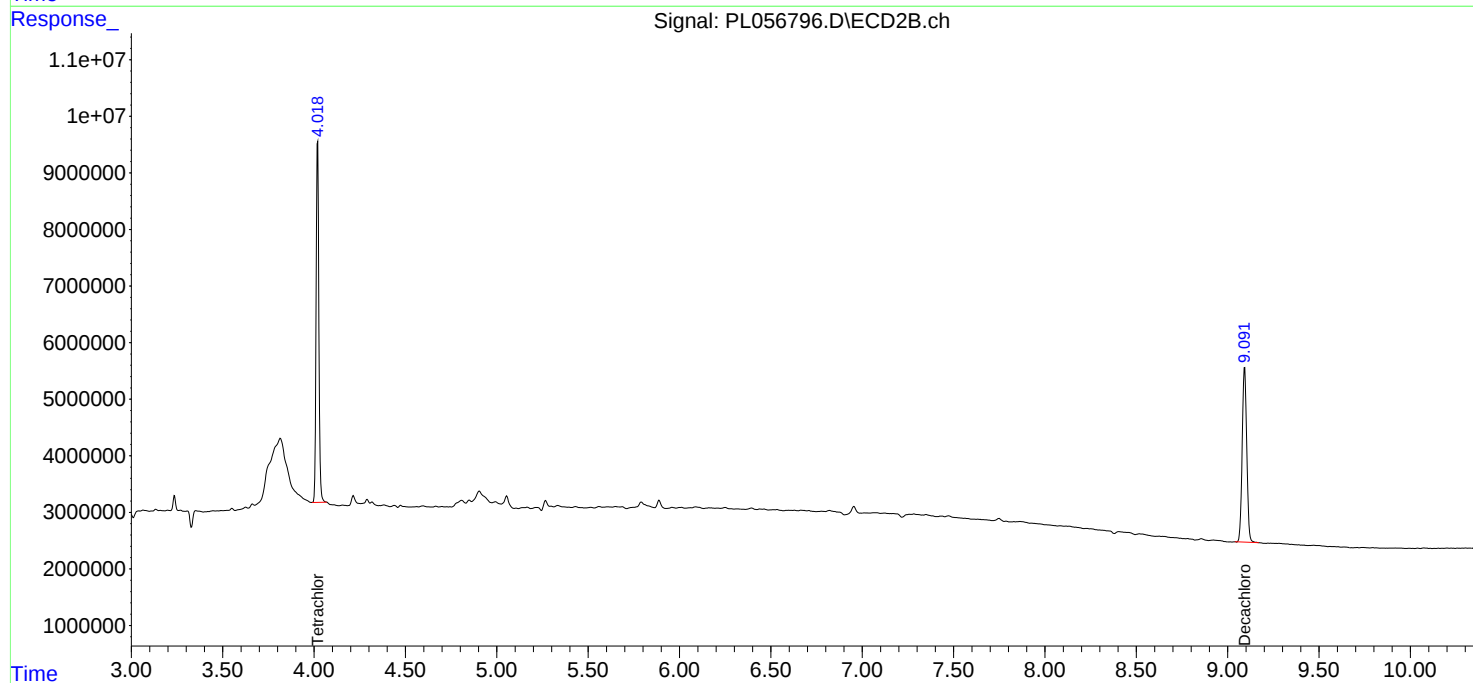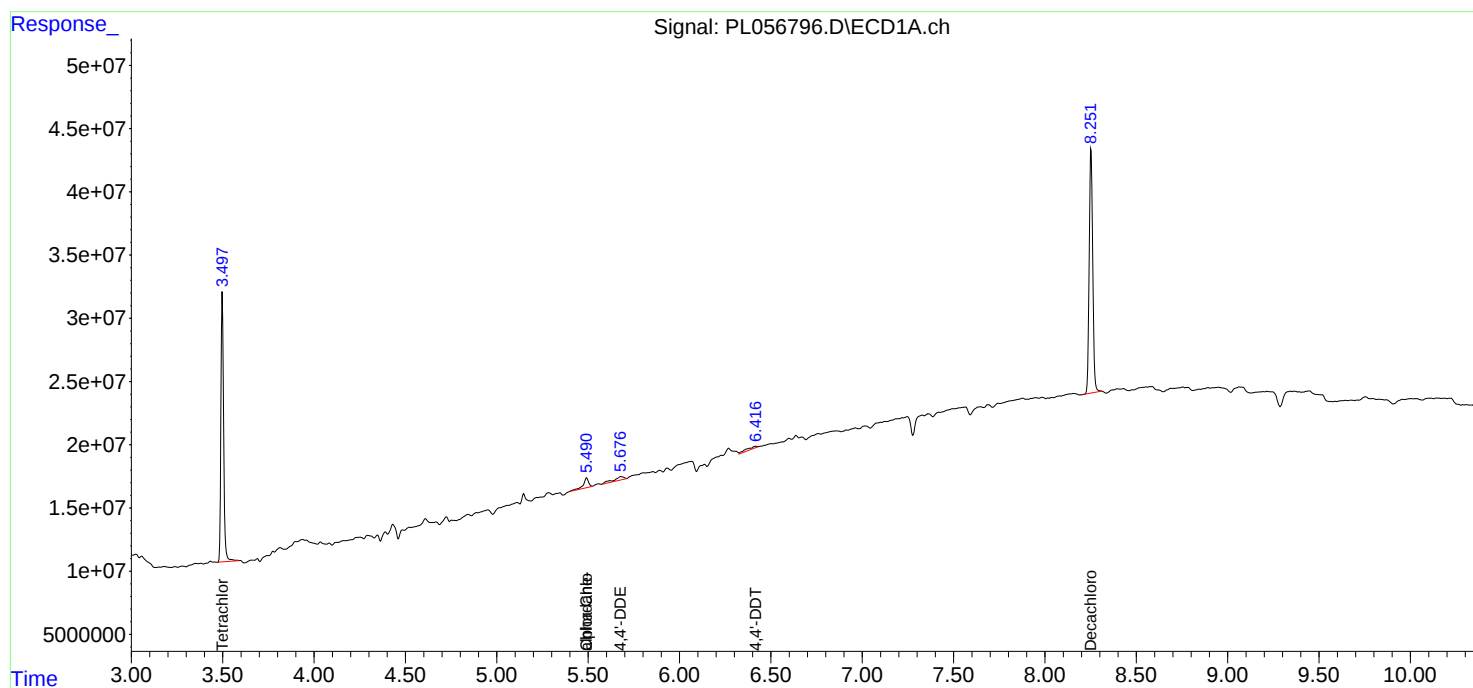


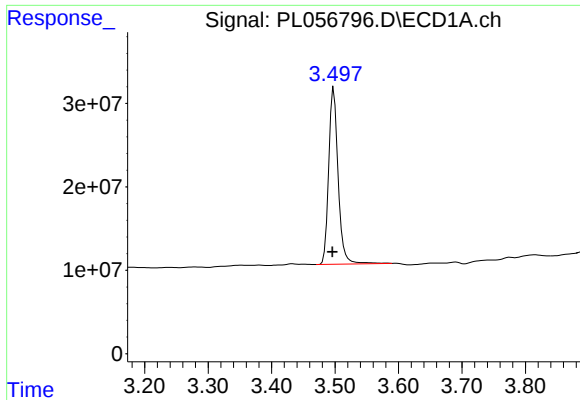

#1 Tetrachloro-m-xylene


R.T.: 3.498 min
Delta R.T.: 0.002 min
Response: 217525909
Conc: 25.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

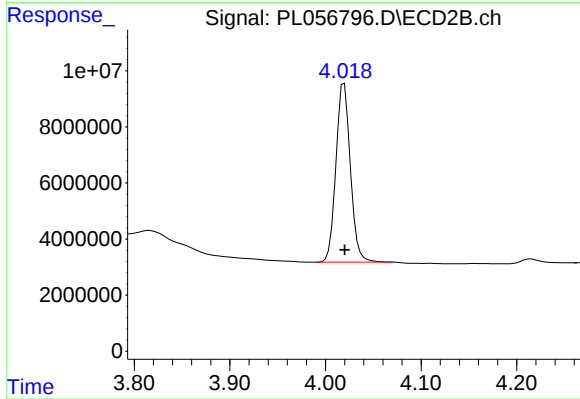


#1 Tetrachloro-m-xylene

R.T.: 4.020 min
Delta R.T.: 0.000 min
Response: 66852529
Conc: 26.84 ng/ml

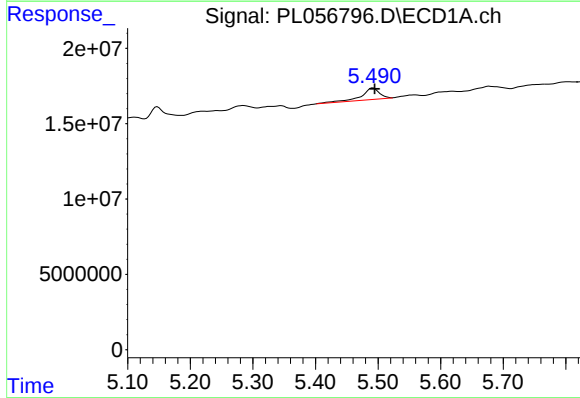


#11 alpha-Chlordane

R.T.: 5.492 min
Delta R.T.: -0.003 min
Response: 15549770
Conc: 1.08 ng/ml

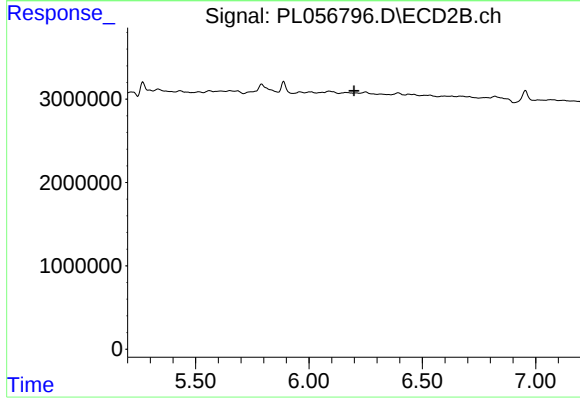

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.199 min
Response: 0
Conc: N.D.

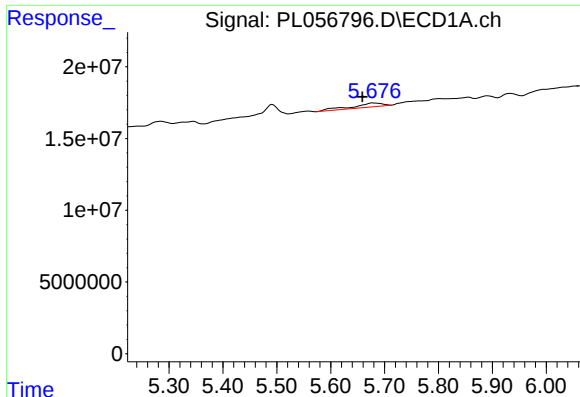

#12 4,4'-DDE


R.T.: 5.678 min
Delta R.T.: 0.019 min
Response: 10798329
Conc: 0.77 ng/ml

Instrument :
ECD_L
ClientSampleId :

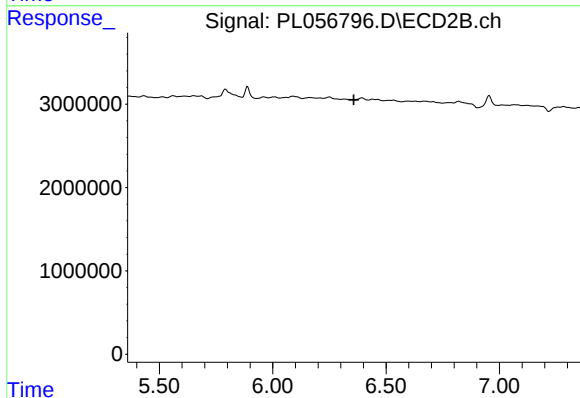


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.358 min
Response: 0
Conc: N.D.

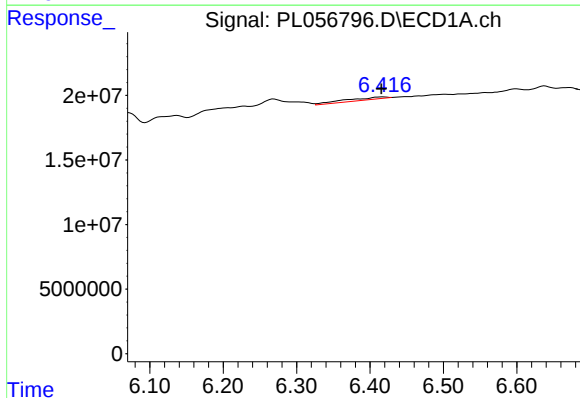


#17 4,4'-DDT

R.T.: 6.418 min
Delta R.T.: 0.002 min
Response: 7133767
Conc: 0.66 ng/ml

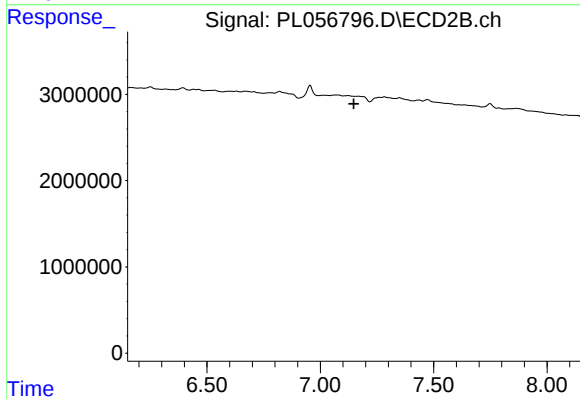

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 7.148 min
Response: 0
Conc: N.D.

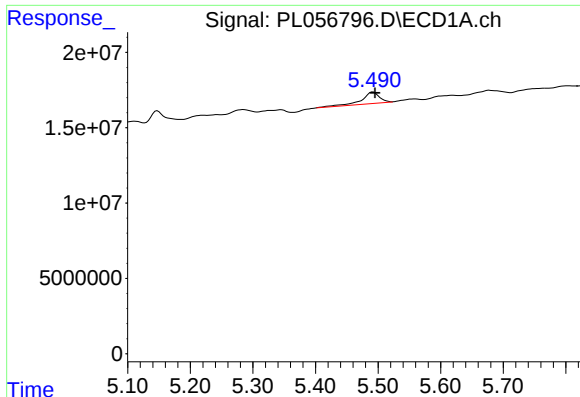

#26 Chlordane-4


R.T.: 5.492 min
Delta R.T.: -0.003 min
Response: 15549770
Conc: 14.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

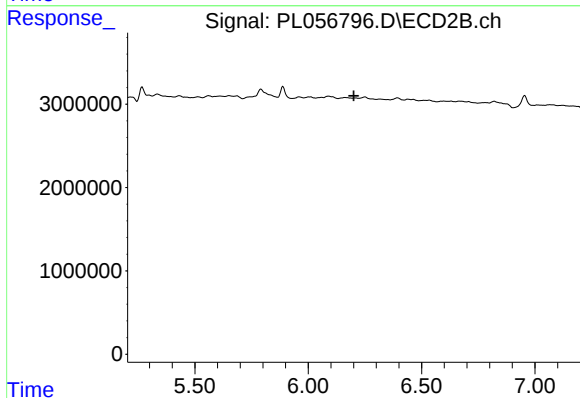


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.200 min
Response: 0
Conc: N.D.

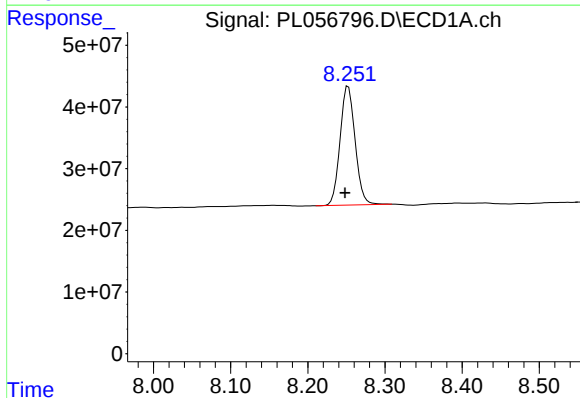

#28 Decachlorobiphenyl

R.T.: 8.253 min
Delta R.T.: 0.004 min
Response: 261168295
Conc: 21.96 ng/ml

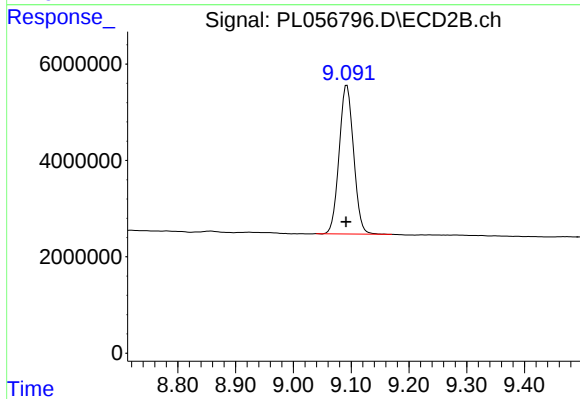

#28 Decachlorobiphenyl

R.T.: 9.093 min
Delta R.T.: 0.002 min
Response: 53399387
Conc: 25.41 ng/ml