

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022420\
 Data File : PL056799.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Feb 2020 16:15
 Operator : AJ\MA
 Sample : L1593-02
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 STOCKPILE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 25 02:38:22 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021920.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 20 02:32:45 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.499	4.019	220.9E6	36495896	25.540	14.651 #
28)	SA Decachlor...	8.252	9.093	183.0E6	42704400	15.388	20.323 #
Target Compounds							
3)	MA gamma-BHC...	0.000	4.704	0	4081340	N.D.	1.185 #
9)	A Endosulfan I	5.559	0.000	38958236	0	2.914	N.D. #
12)	B 4,4'-DDE	5.684f	0.000	36330335	0	2.583	N.D. #
15)	B Endosulfa...	6.314	0.000	23852611	0	1.921	N.D. #
16)	A 4,4'-DDD	6.180	0.000	27560774	0	2.464	N.D. #
17)	MA 4,4'-DDT	6.395f	0.000	33381676	0	3.065	N.D. #
18)	B Endrin al...	6.469f	0.000	19948315	0	1.843	N.D. #
27)	Chlordane-5	6.314f	0.000	23852611	0	72.846	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022420\
Data File : PL056799.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Feb 2020 16:15
Operator : AJ\MA
Sample : L1593-02
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
STOCKPILE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 25 02:38:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021920.M
Quant Title : GC Extractables
QLast Update : Thu Feb 20 02:32:45 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

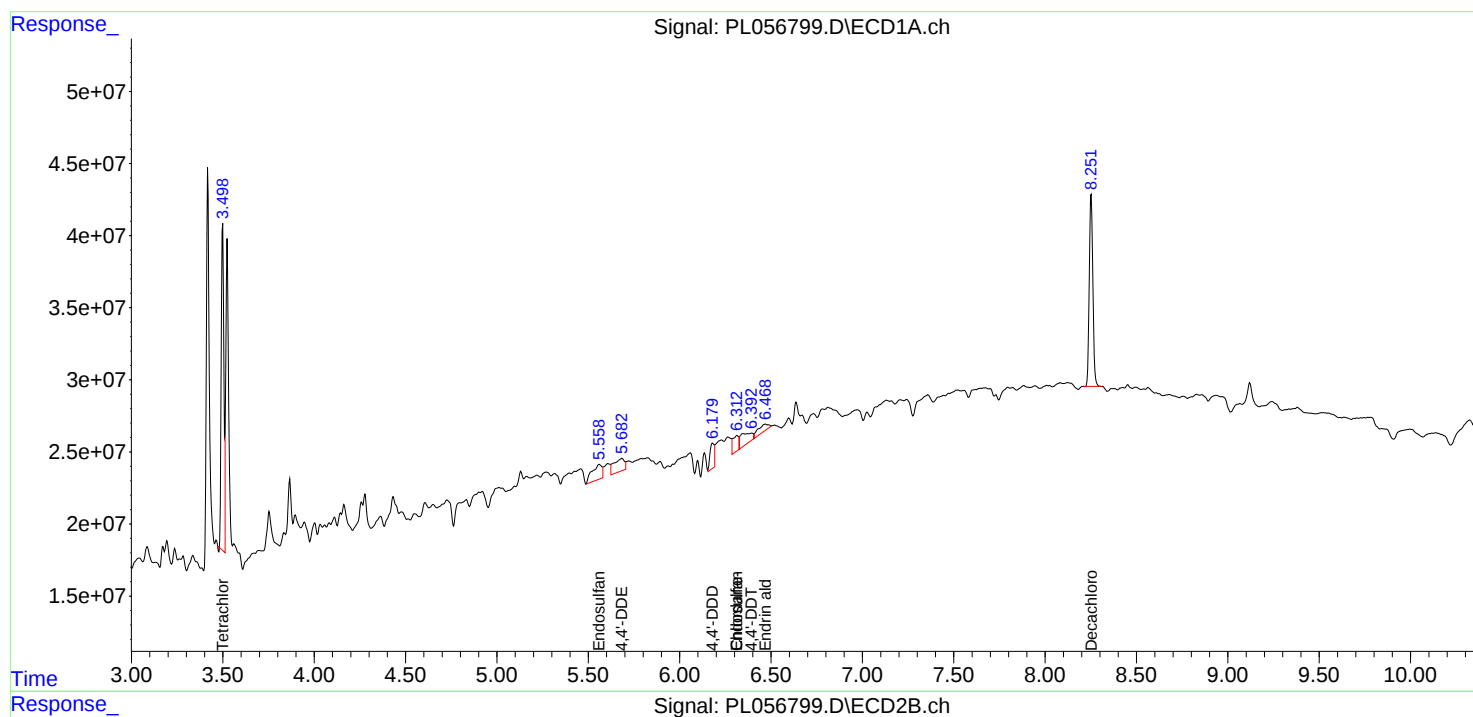


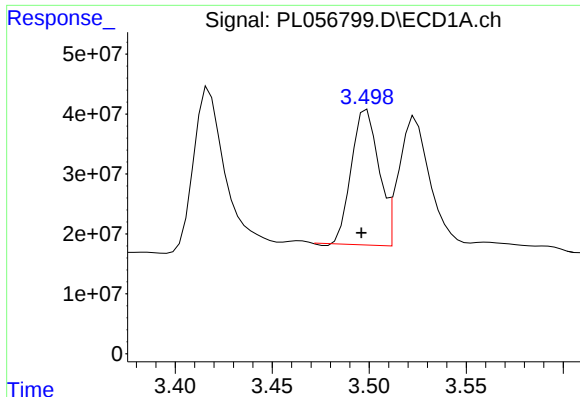

#1 Tetrachloro-m-xylene


R.T.: 3.499 min
Delta R.T.: 0.003 min
Response: 220857261
Conc: 25.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
STOCKPILE

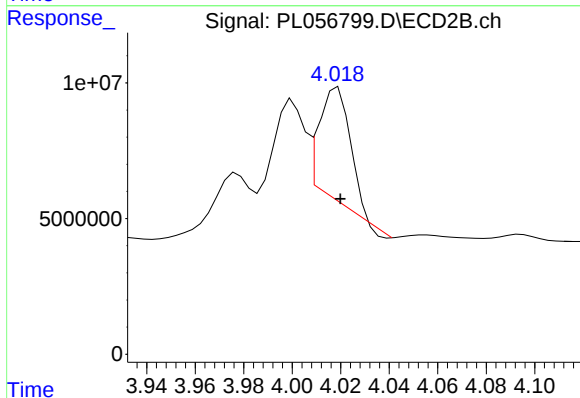


#1 Tetrachloro-m-xylene

R.T.: 4.019 min
Delta R.T.: 0.000 min
Response: 36495896
Conc: 14.65 ng/ml

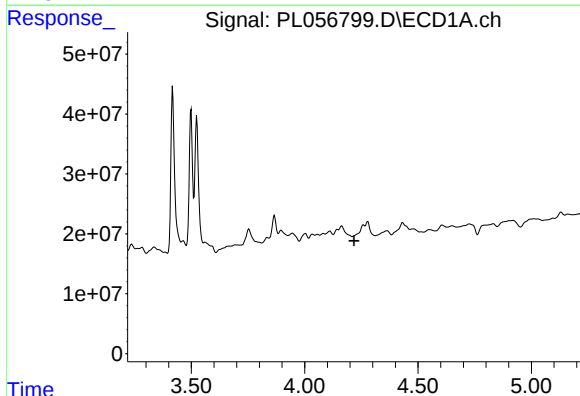


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.218 min
Response: 0
Conc: N.D.

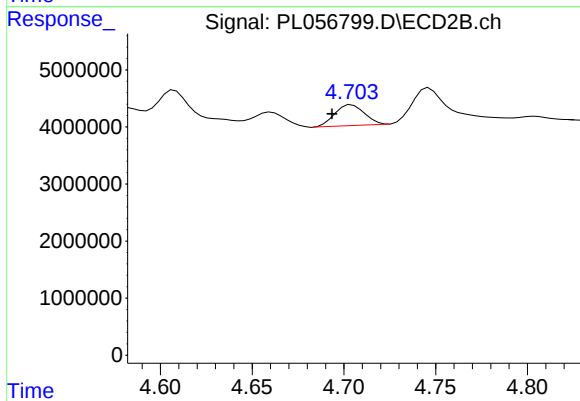

#3 gamma-BHC (Lindane)


R.T.: 4.704 min
Delta R.T.: 0.011 min
Response: 4081340
Conc: 1.19 ng/ml

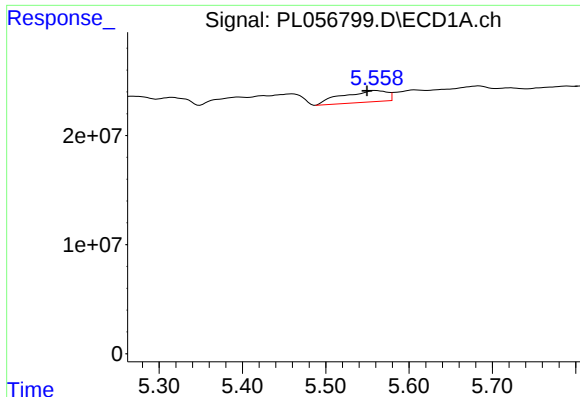

#9 Endosulfan I


R.T.: 5.559 min
Delta R.T.: 0.010 min
Response: 38958236
Conc: 2.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
STOCKPILE

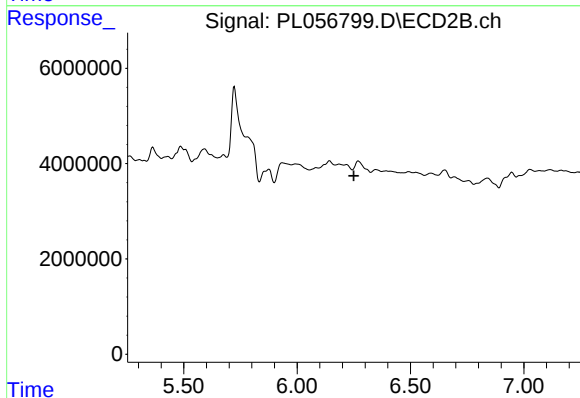


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.250 min
Response: 0
Conc: N.D.

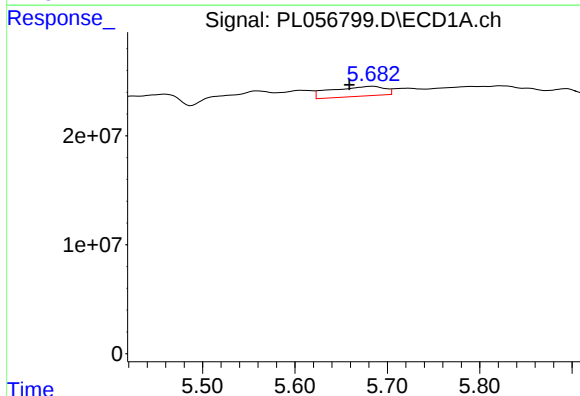


#12 4,4'-DDE

R.T.: 5.684 min
Delta R.T.: 0.025 min
Response: 36330335
Conc: 2.58 ng/ml

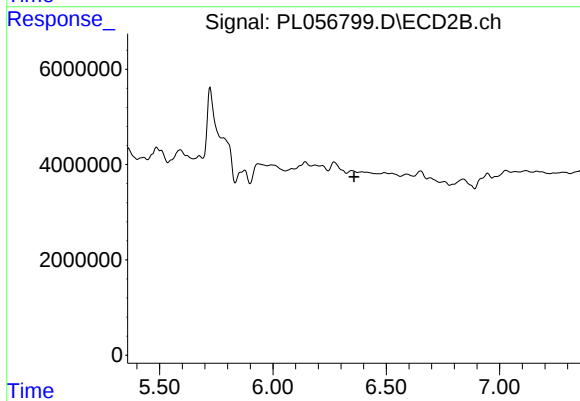

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T. : 6.358 min
Response: 0
Conc: N.D.

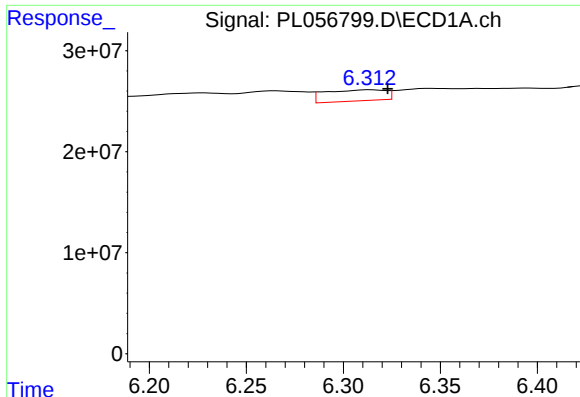

#15 Endosulfan II


R.T.: 6.314 min
Delta R.T.: -0.009 min
Response: 23852611
Conc: 1.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
STOCKPILE

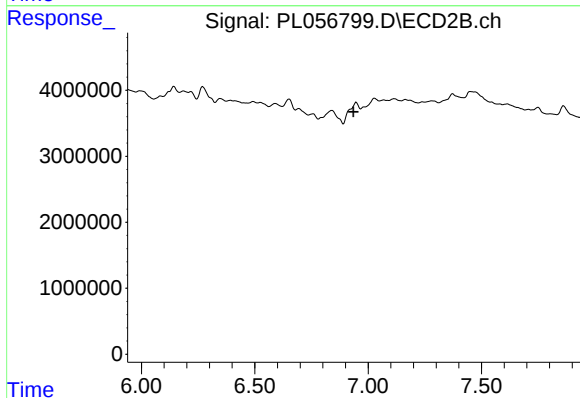


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.936 min
Response: 0
Conc: N.D.

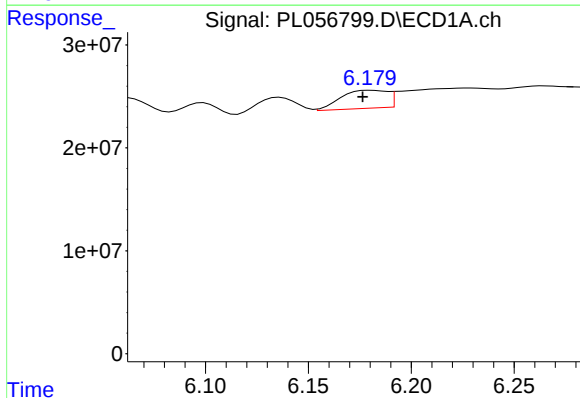


#16 4,4'-DDD

R.T.: 6.180 min
Delta R.T.: 0.004 min
Response: 27560774
Conc: 2.46 ng/ml

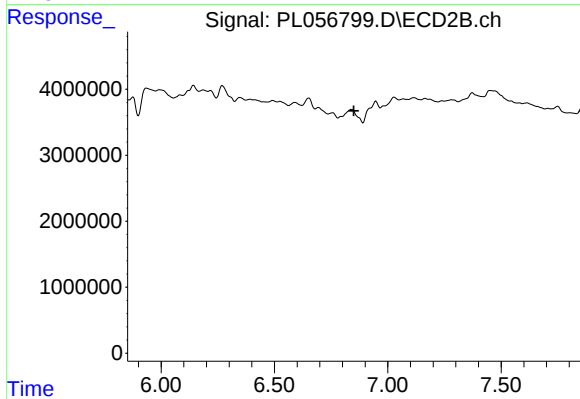

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.850 min
Response: 0
Conc: N.D.

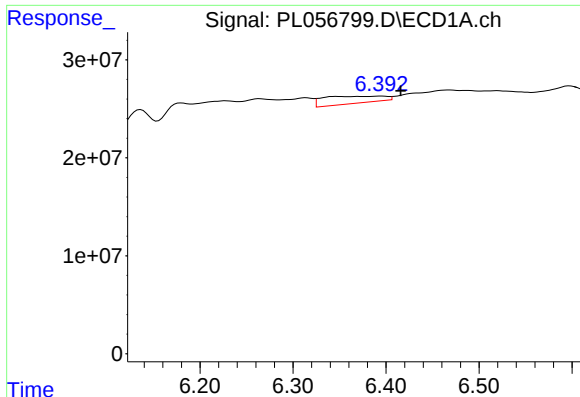

#17 4,4'-DDT


R.T.: 6.395 min
Delta R.T.: -0.021 min
Response: 33381676
Conc: 3.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
STOCKPILE

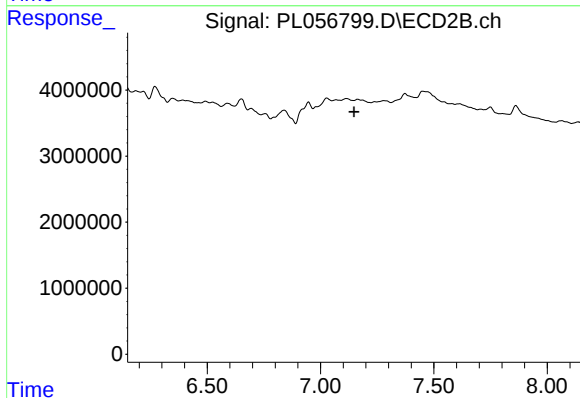


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.148 min
Response: 0
Conc: N.D.

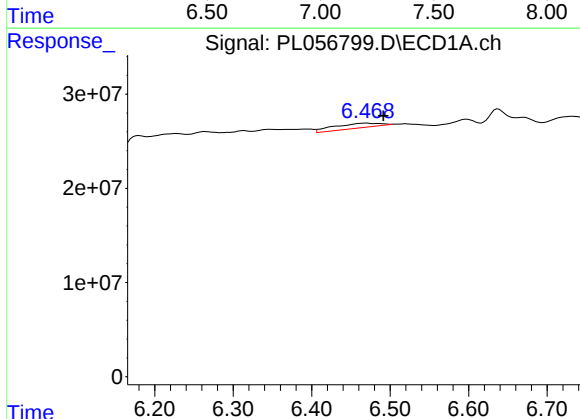


#18 Endrin aldehyde

R.T.: 6.469 min
Delta R.T.: -0.022 min
Response: 19948315
Conc: 1.84 ng/ml

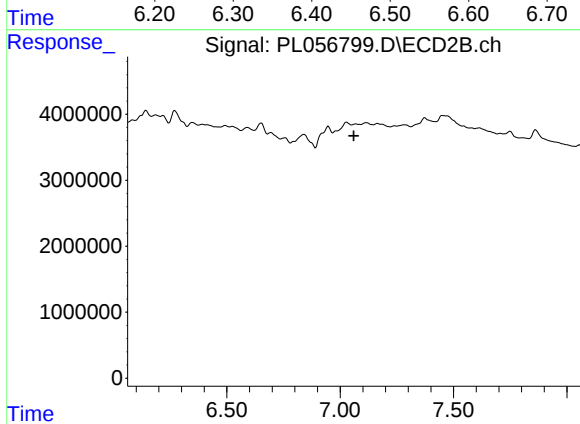

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 7.060 min
Response: 0
Conc: N.D.

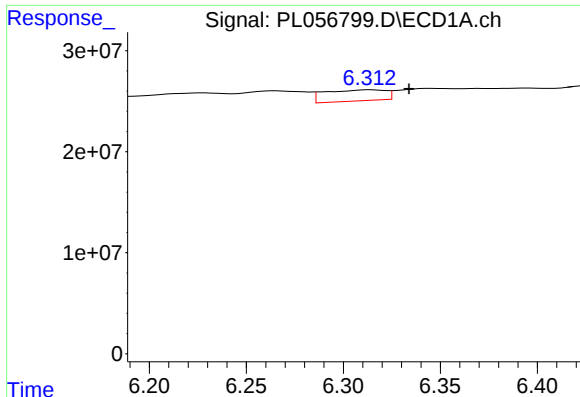

#27 Chlordane-5


R.T.: 6.314 min
Delta R.T.: -0.020 min
Response: 23852611
Conc: 72.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
STOCKPILE

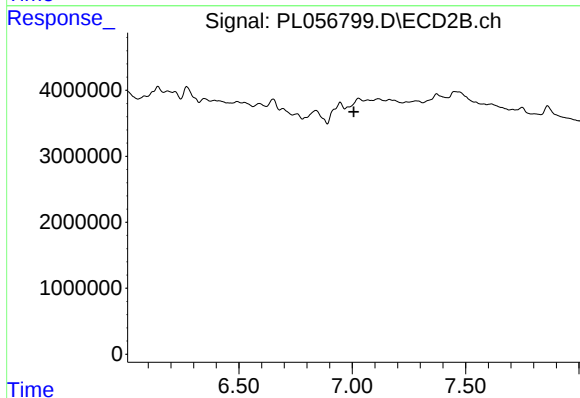


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 7.007 min
Response: 0
Conc: N.D.

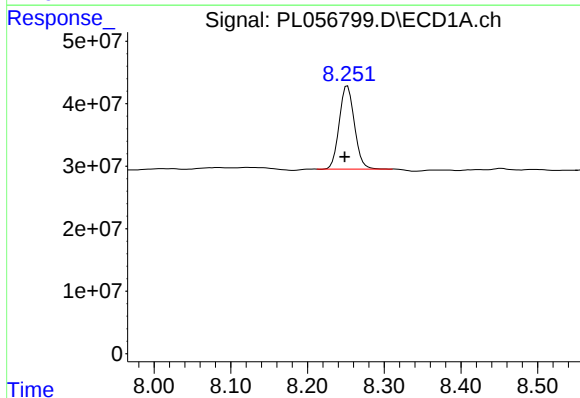

#28 Decachlorobiphenyl

R.T.: 8.252 min
Delta R.T.: 0.004 min
Response: 183041881
Conc: 15.39 ng/ml

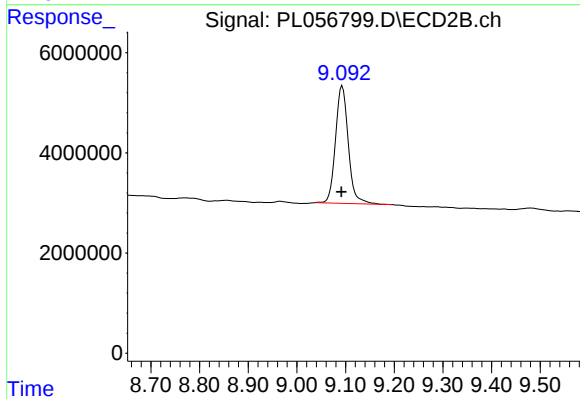

#28 Decachlorobiphenyl

R.T.: 9.093 min
Delta R.T.: 0.002 min
Response: 42704400
Conc: 20.32 ng/ml