

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022422\
 Data File : PL072959.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Feb 2022 00:16
 Operator : AR\AJ
 Sample : PIBLK203
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 06:24:38 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022422CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 01 06:18:13 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	4.650	5.516	6032073	32179816	19.301	19.530
27)	SA Decachlor...	10.434	11.386	8601254	26535624	20.444	20.435
Target Compounds							
6)	B beta-BHC	0.000	6.708	0	611672	N.D.	0.601
7)	B delta-BHC	0.000	6.988	0	2378721	N.D.	1.050
15)	B Endosulfa...	8.329f	0.000	3274446	0	7.643	N.D. #
16)	A 4,4'-DDD	0.000	8.977f	0	12443087	N.D.	9.718
20)	A Methoxychlor	0.000	9.782f	0	294986	N.D.	0.451


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022422\
Data File : PL072959.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Feb 2022 00:16
Operator : AR\AJ
Sample : PIBLK203
Misc :
ALS Vial : 19 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 06:24:38 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022422CLP.M
Quant Title : GC Extractables
QLast Update : Tue Mar 01 06:18:13 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

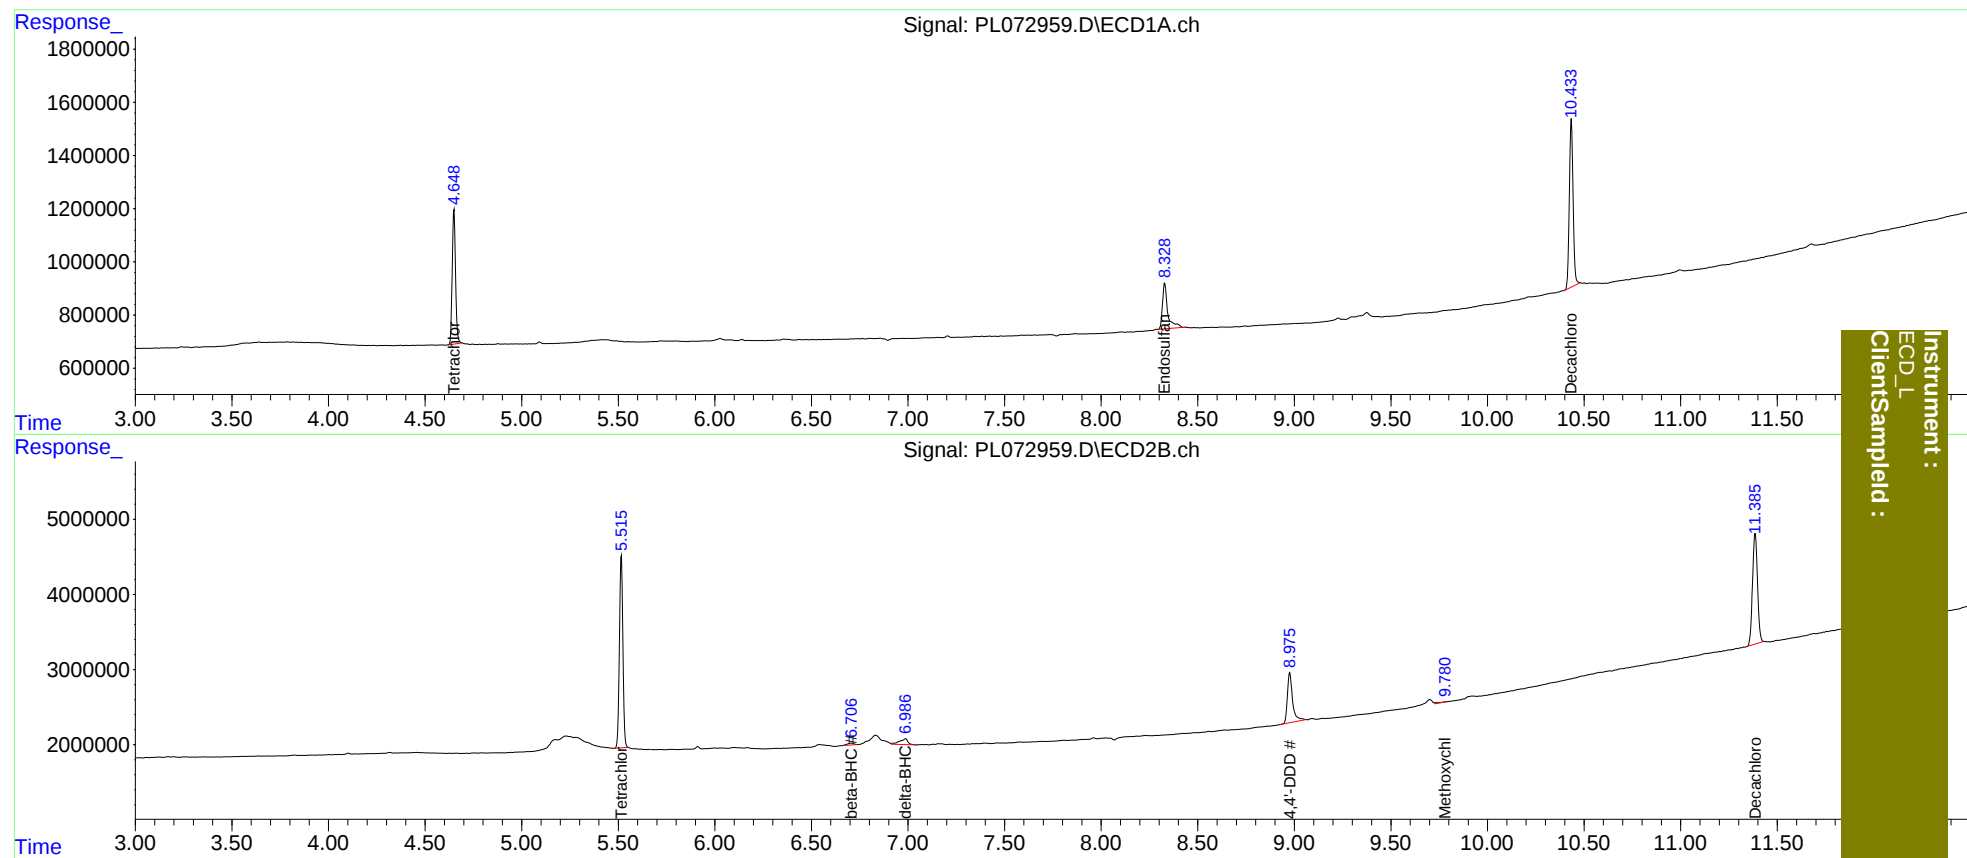


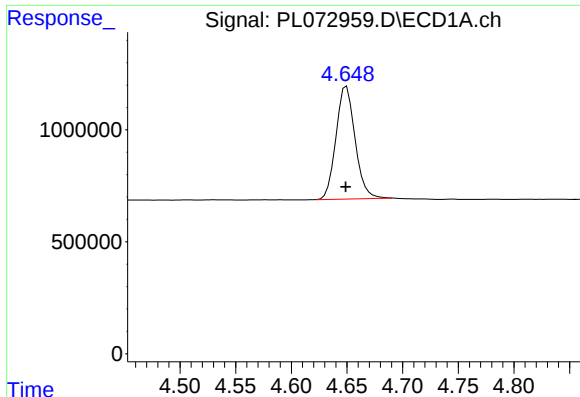

#1 Tetrachloro-m-xylene


R.T.: 4.650 min
Delta R.T.: 0.000 min
Response: 6032073
Conc: 19.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

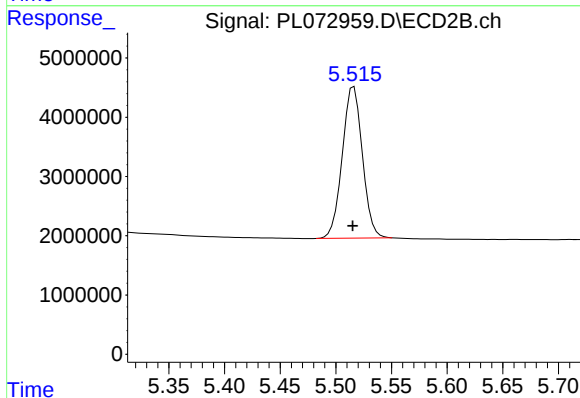


#1 Tetrachloro-m-xylene

R.T.: 5.516 min
Delta R.T.: 0.001 min
Response: 32179816
Conc: 19.53 ng/ml

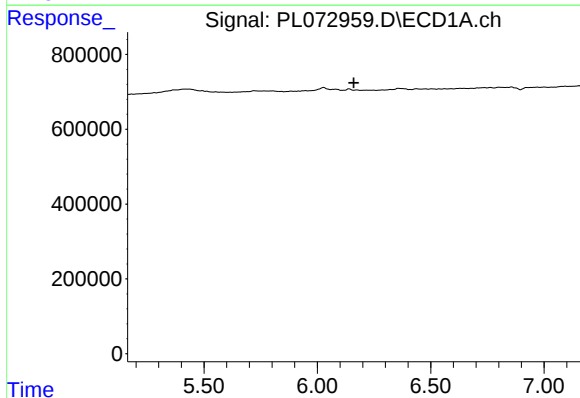


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.162 min
Response: 0
Conc: N.D.

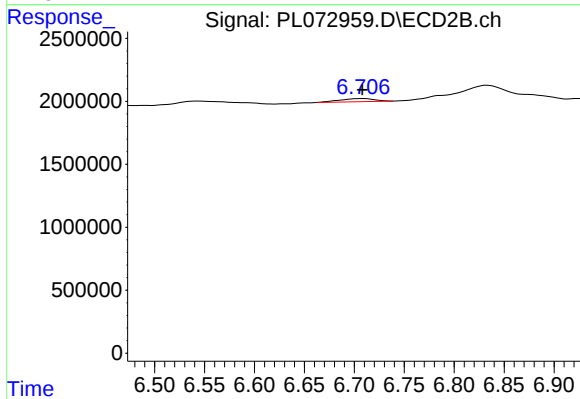

#6 beta-BHC


R.T.: 6.708 min
Delta R.T.: 0.000 min
Response: 611672
Conc: 0.60 ng/ml

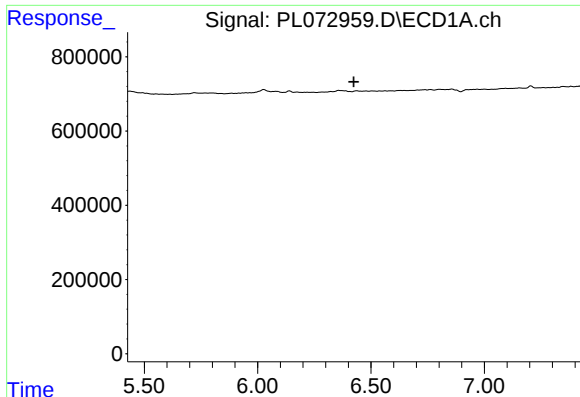

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.424 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

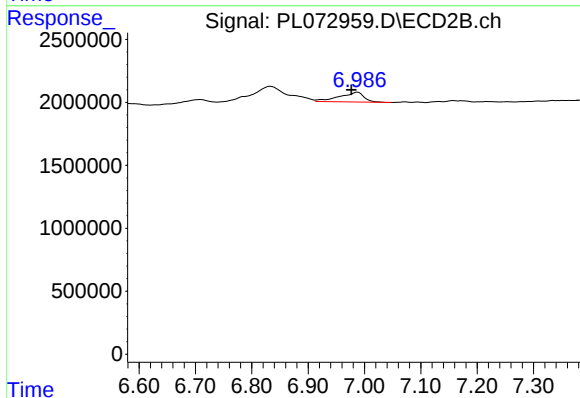


#7 delta-BHC

R.T.: 6.988 min
Delta R.T.: 0.011 min
Response: 2378721
Conc: 1.05 ng/ml

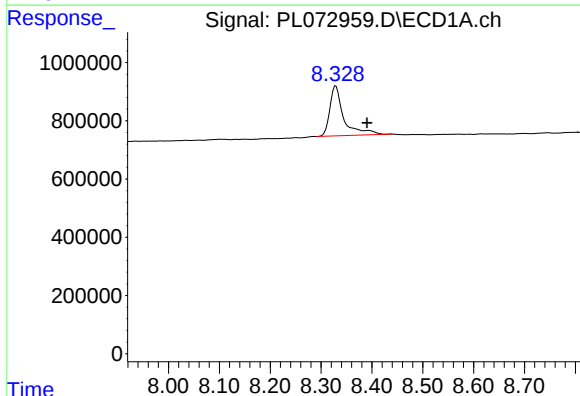


#15 Endosulfan II

R.T.: 8.329 min
Delta R.T.: -0.061 min
Response: 3274446
Conc: 7.64 ng/ml

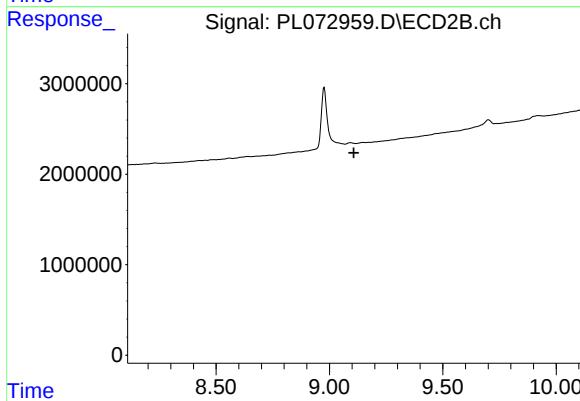

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 9.107 min
Response: 0
Conc: N.D.

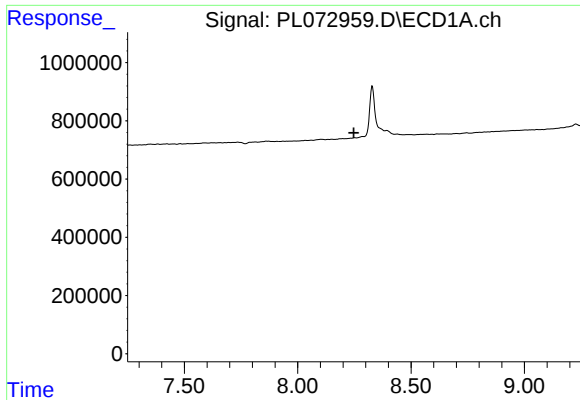

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 8.247 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

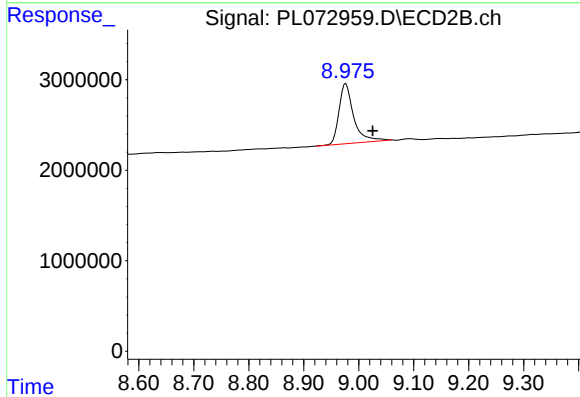


#16 4,4'-DDD

R.T.: 8.977 min
Delta R.T.: -0.049 min
Response: 12443087
Conc: 9.72 ng/ml

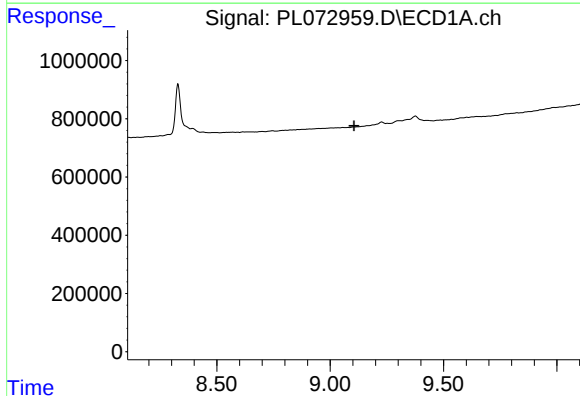


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 9.105 min
Response: 0
Conc: N.D.

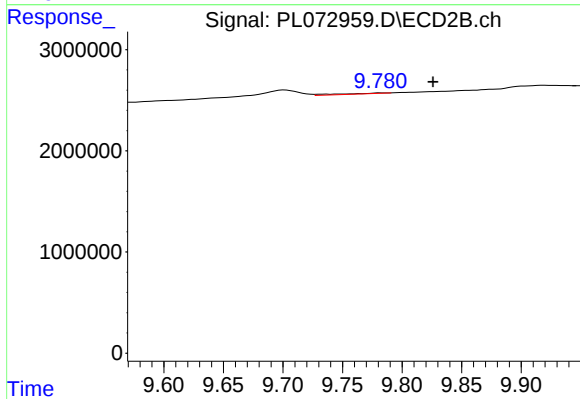

#20 Methoxychlor


R.T.: 9.782 min
Delta R.T.: -0.044 min
Response: 294986
Conc: 0.45 ng/ml

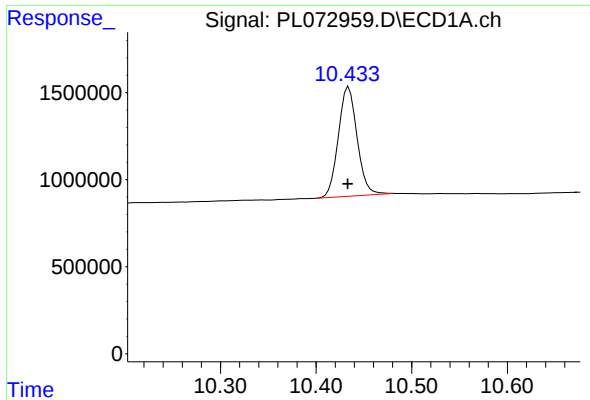

#27 Decachlorobiphenyl

R.T.: 10.434 min
Delta R.T.: 0.001 min
Response: 8601254
Conc: 20.44 ng/ml

Instrument :
ECD_L
ClientSampleId :

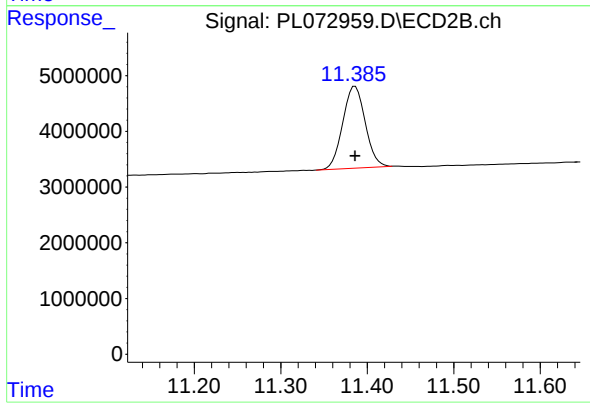

#27 Decachlorobiphenyl

R.T.: 11.386 min
Delta R.T.: 0.000 min
Response: 26535624
Conc: 20.43 ng/ml