

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022425\
 Data File : PL094379.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Feb 2025 16:11
 Operator : AR\AJ
 Sample : Q1411-03 10X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HR-03-02212025

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 02/25/2025
 Supervised By : Ankita Jodhani 02/25/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 25 02:31:10 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022125.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 21 14:52:19 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.536	2.772	6226648	7404027	2.452m	2.320
28) SA Decachlor...	9.050	7.906	4364540	5498236	2.052m	1.430 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022425\
Data File : PL094379.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Feb 2025 16:11
Operator : AR\AJ
Sample : Q1411-03 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
HR-03-02212025


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 02/25/2025
Supervised By : Ankita Jodhani 02/25/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 25 02:31:10 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022125.M
Quant Title : GC Extractables
QLast Update : Fri Feb 21 14:52:19 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

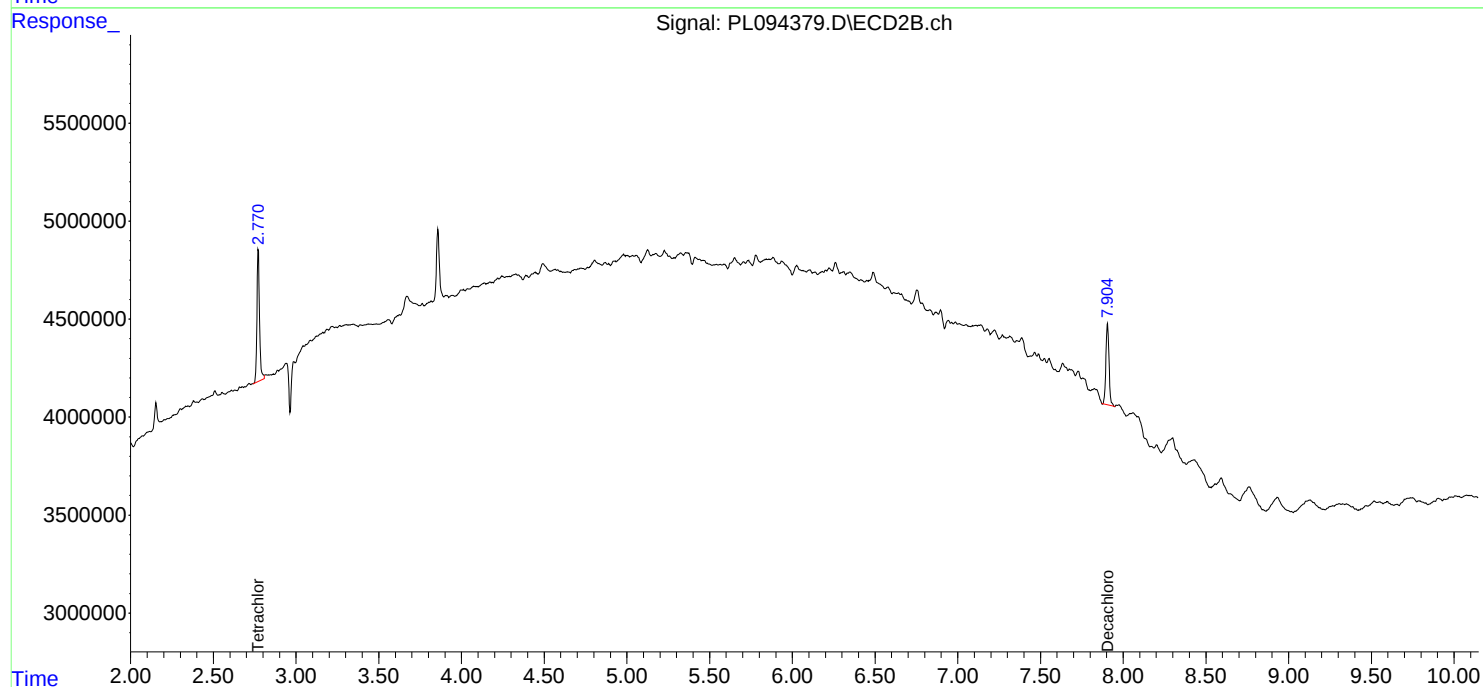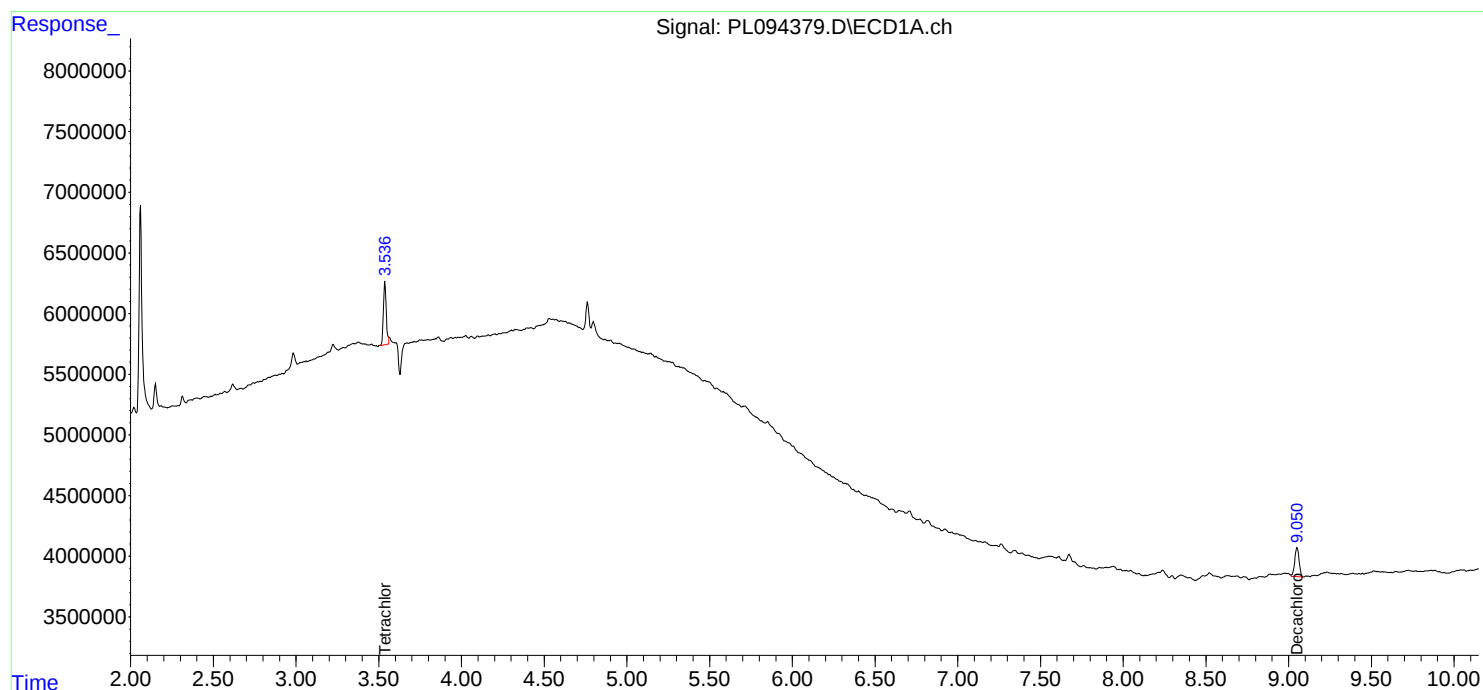

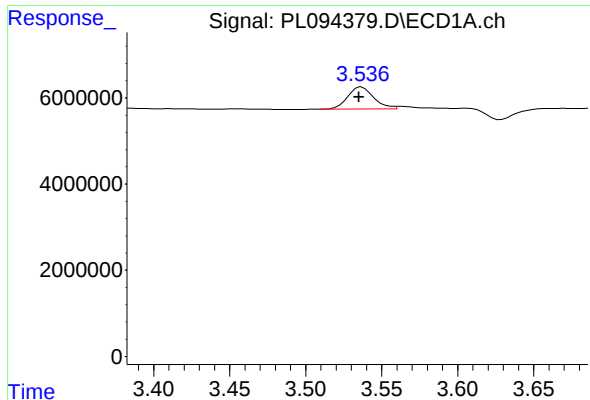


#1 Tetrachloro-m-xylene

R.T.: 3.536 min
Delta R.T.: 0.000 min
Response: 6226648
Conc: 2.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
HR-03-02212025


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/25/2025
Supervised By :Ankita Jodhani 02/25/2025

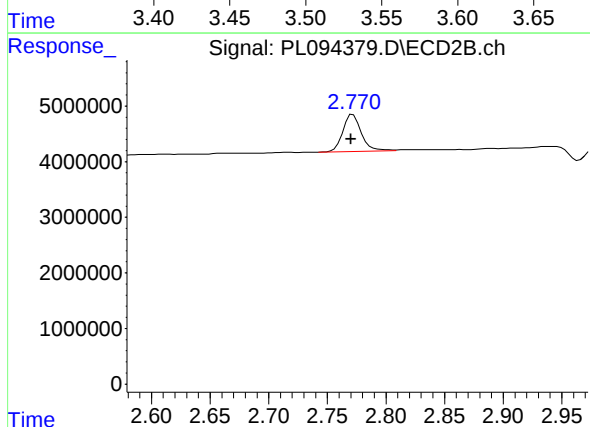


#1 Tetrachloro-m-xylene

R.T.: 2.772 min
Delta R.T.: 0.002 min
Response: 7404027
Conc: 2.32 ng/ml

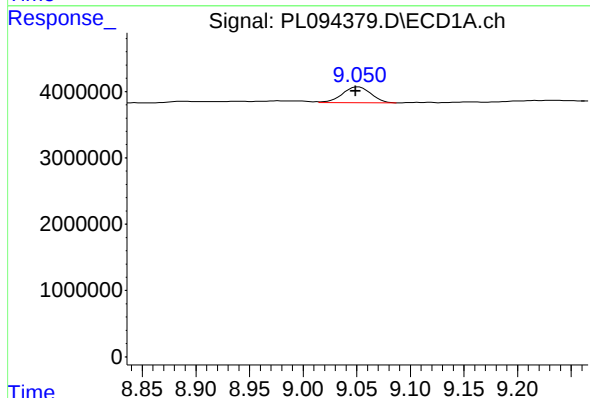

#28 Decachlorobiphenyl

R.T.: 9.050 min
Delta R.T.: 0.001 min
Response: 4364540
Conc: 2.05 ng/ml m

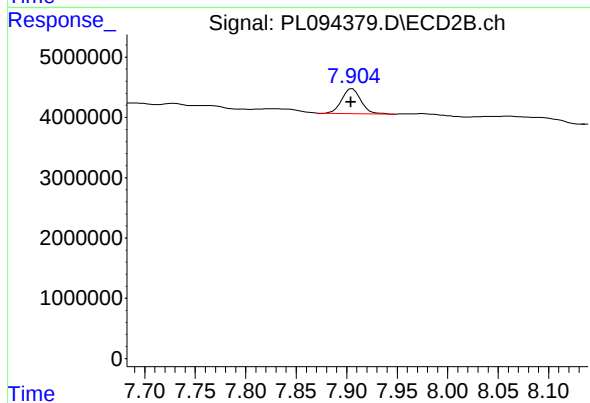

#28 Decachlorobiphenyl

R.T.: 7.906 min
Delta R.T.: 0.001 min
Response: 5498236
Conc: 1.43 ng/ml