

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022519\
 Data File : PL045057.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Feb 2019 15:00
 Operator : AJ\SJ
 Sample : K1348-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OK-03-022219-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 25 23:50:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 07 01:39:50 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.365	3.984	76400812	25372804	10.737	10.801
28)	SA Decachlor...	8.052	9.045	86873398	26437292	11.911	11.936
Target Compounds							
4)	MA Heptachlor	0.000	5.188f	0	5392435	N.D.	1.770 #
5)	MB Aldrin	0.000	5.442f	0	13732214	N.D.	4.956 #
8)	B Heptachlo...	0.000	5.876f	0	8545968	N.D.	3.418 #
10)	B gamma-Chl...	5.283f	6.092	215.3E6	34322269	22.310	12.364 #
11)	B alpha-Chl...	5.320	6.165	203.4E6	108.5E6	21.276	39.154 #
12)	B 4,4'-DDE	5.487	6.318	4288276	6423762	0.494	2.690 #
15)	B Endosulfa...	6.145	0.000	59592055	0	7.048	N.D. #
17)	MA 4,4'-DDT	6.233	7.110	7974080	2149490	1.112	1.096



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022519\
Data File : PL045057.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Feb 2019 15:00
Operator : AJ\SJ
Sample : K1348-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
OK-03-022219-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 25 23:50:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
Quant Title : GC Extractables
QLast Update : Thu Feb 07 01:39:50 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

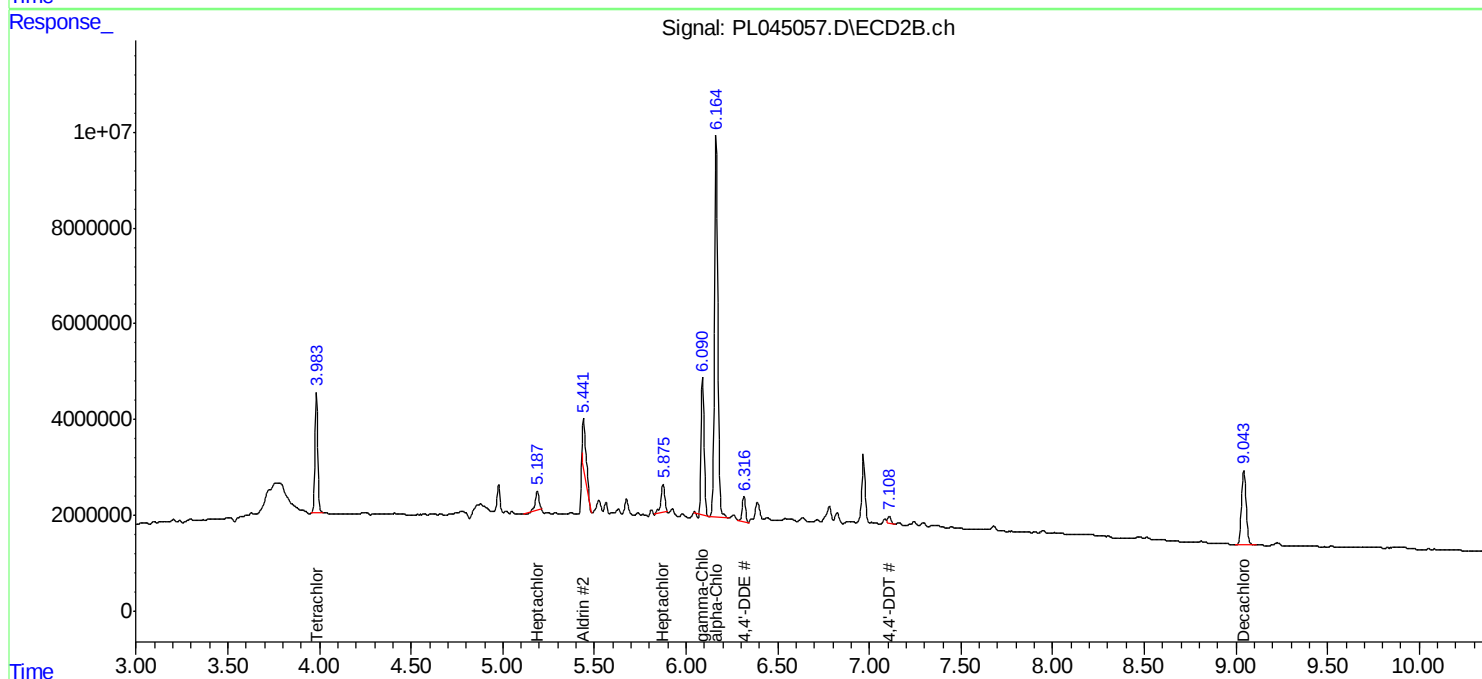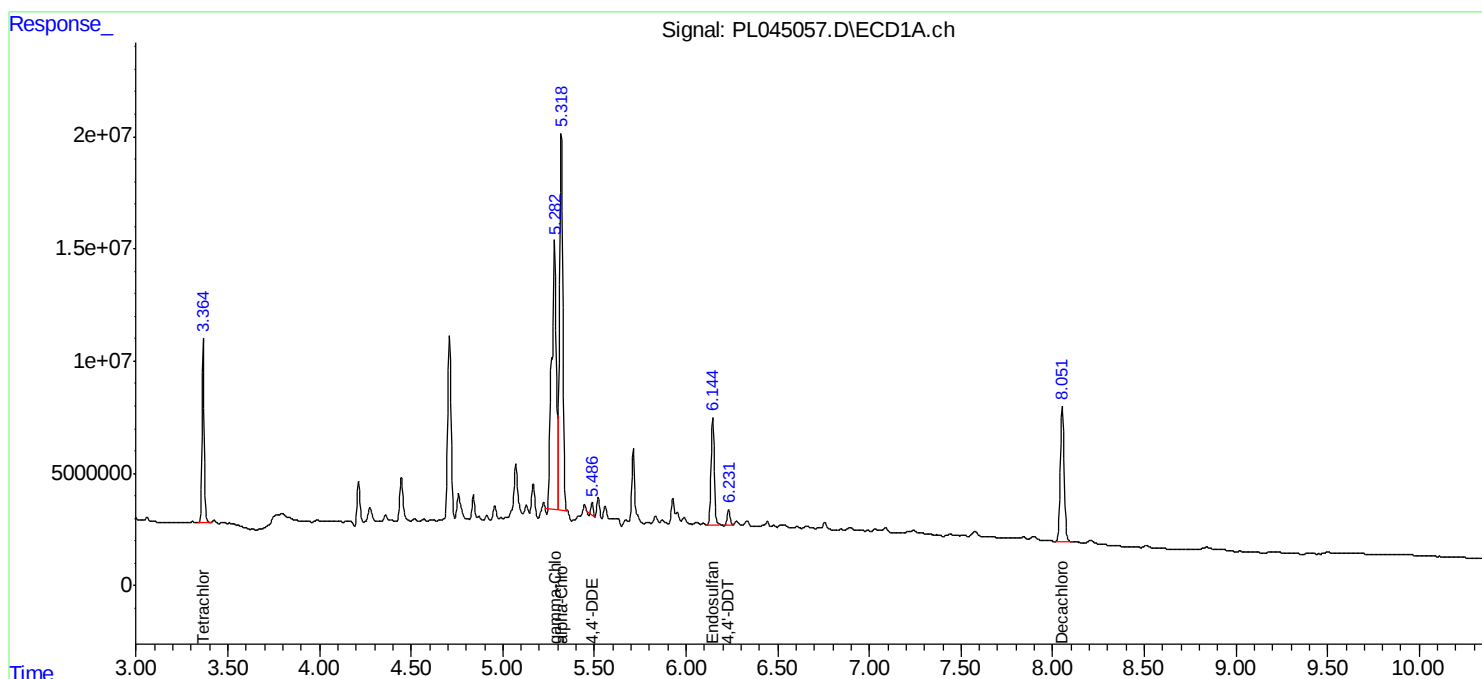


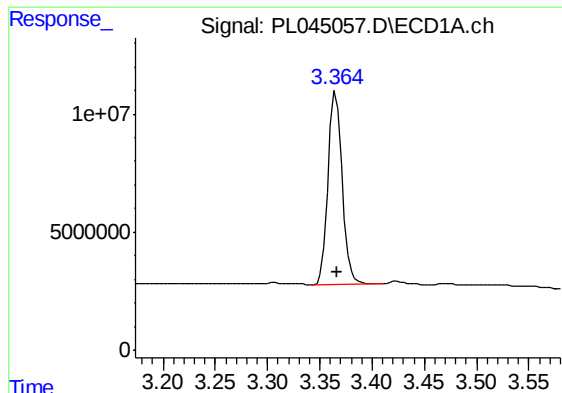

#1 Tetrachloro-m-xylene


R.T.: 3.365 min
Delta R.T.: 0.000 min
Response: 76400812
Conc: 10.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-03-022219-A

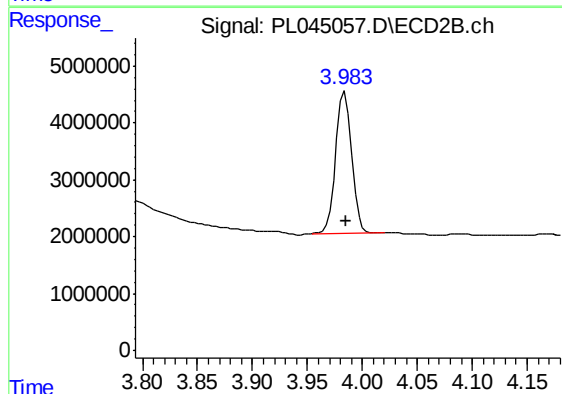


#1 Tetrachloro-m-xylene

R.T.: 3.984 min
Delta R.T.: 0.000 min
Response: 25372804
Conc: 10.80 ng/ml

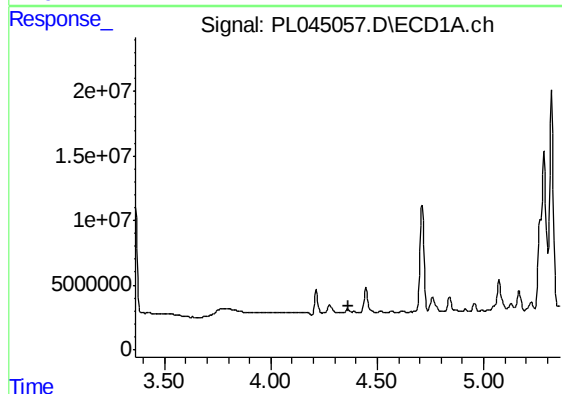


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.362 min
Response: 0
Conc: N.D.

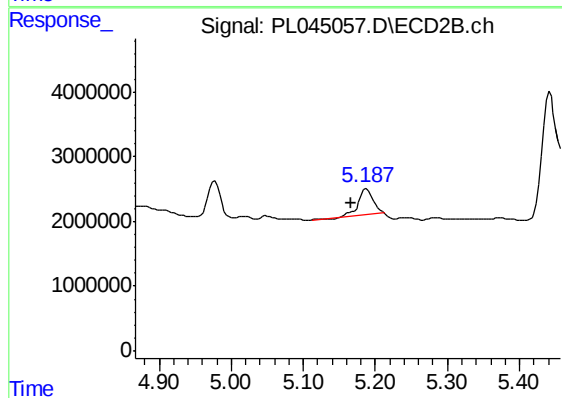

#4 Heptachlor


R.T.: 5.188 min
Delta R.T.: 0.022 min
Response: 5392435
Conc: 1.77 ng/ml

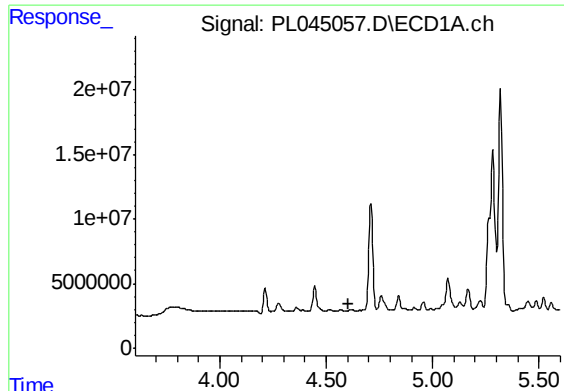

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 4.602 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
OK-03-022219-A

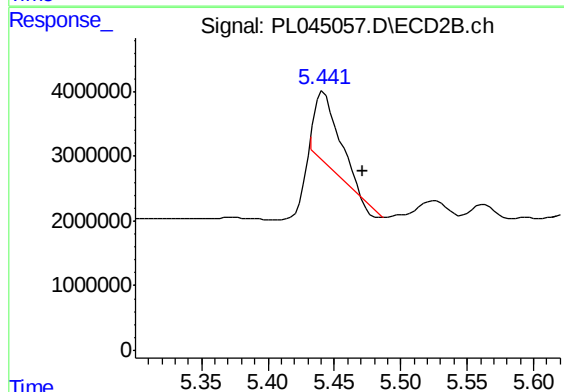


#5 Aldrin

R.T.: 5.442 min
Delta R.T.: -0.029 min
Response: 13732214
Conc: 4.96 ng/ml

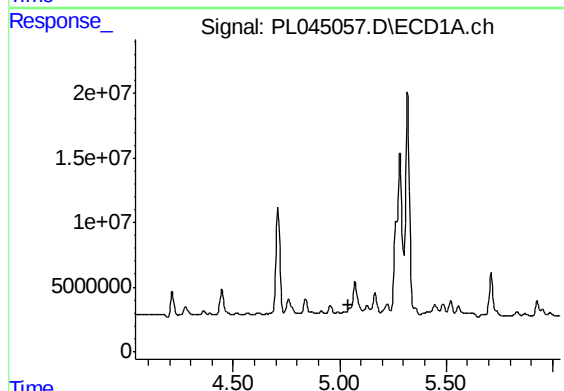


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.040 min
Response: 0
Conc: N.D.

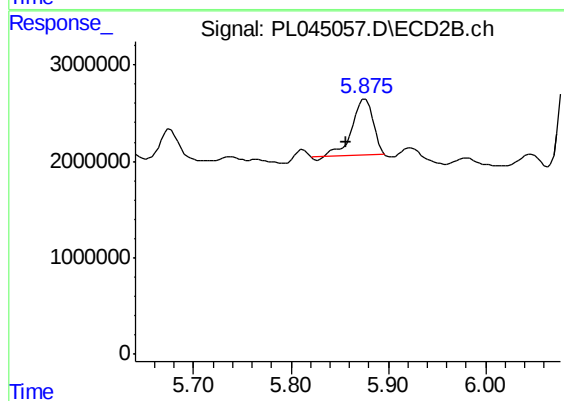

#8 Heptachlor epoxide


R.T.: 5.876 min
Delta R.T.: 0.019 min
Response: 8545968
Conc: 3.42 ng/ml

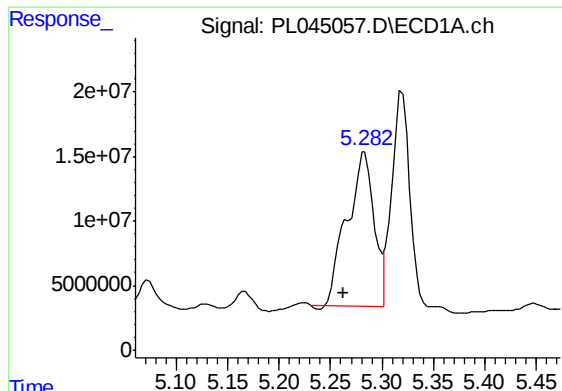

#10 gamma-Chlordane


R.T.: 5.283 min
Delta R.T.: 0.020 min
Response: 215315344
Conc: 22.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-03-022219-A

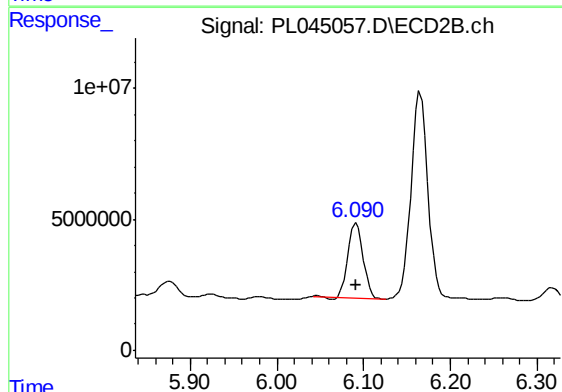


#10 gamma-Chlordane

R.T.: 6.092 min
Delta R.T.: 0.000 min
Response: 34322269
Conc: 12.36 ng/ml

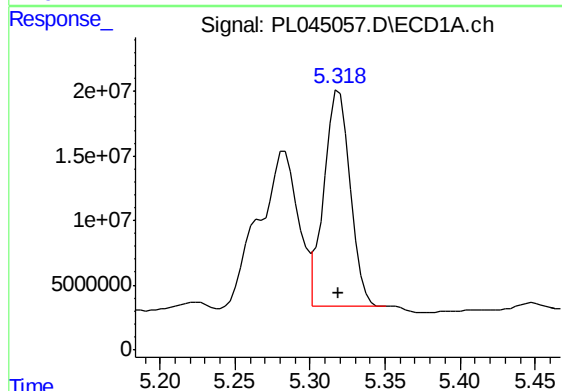


#11 alpha-Chlordane

R.T.: 5.320 min
Delta R.T.: 0.000 min
Response: 203430614
Conc: 21.28 ng/ml

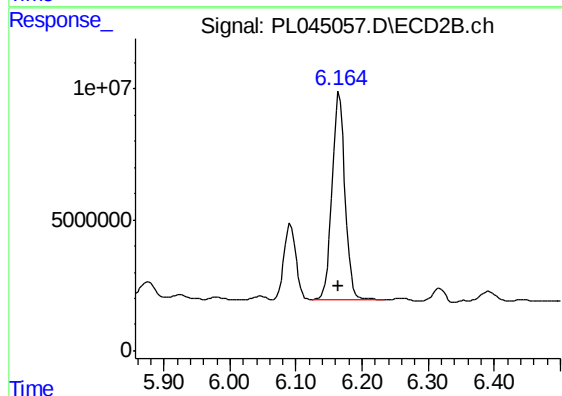

#11 alpha-Chlordane


R.T.: 6.165 min
Delta R.T.: 0.001 min
Response: 108488432
Conc: 39.15 ng/ml

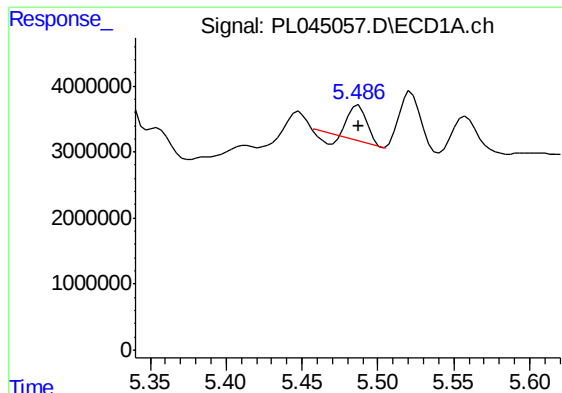

#12 4,4'-DDE


R.T.: 5.487 min
Delta R.T.: 0.000 min
Response: 4288276
Conc: 0.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-03-022219-A

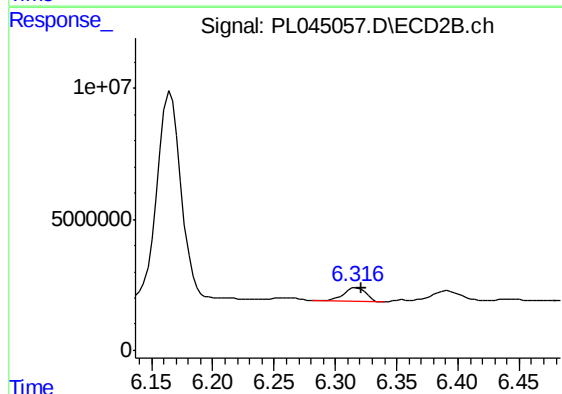


#12 4,4'-DDE

R.T.: 6.318 min
Delta R.T.: -0.003 min
Response: 6423762
Conc: 2.69 ng/ml

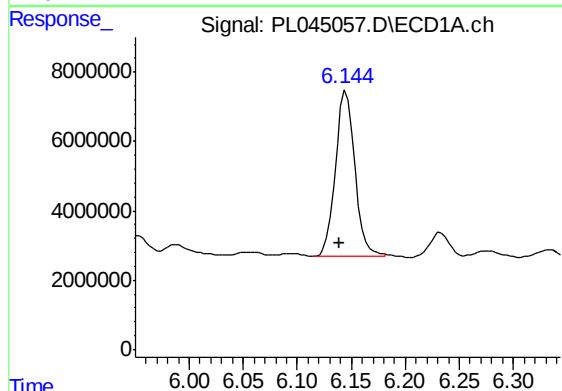


#15 Endosulfan II

R.T.: 6.145 min
Delta R.T.: 0.006 min
Response: 59592055
Conc: 7.05 ng/ml

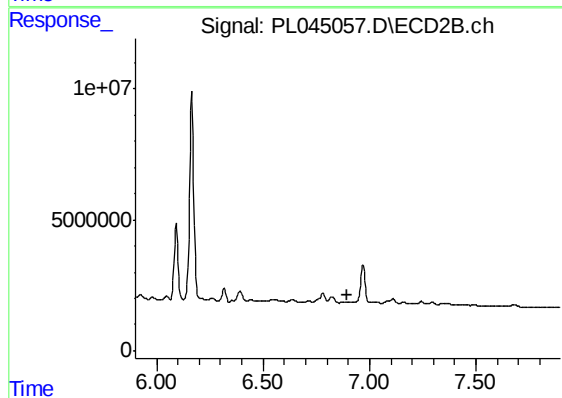

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.897 min
Response: 0
Conc: N.D.

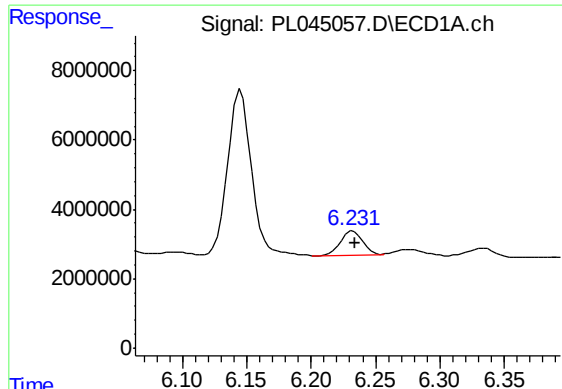

#17 4,4'-DDT


R.T.: 6.233 min
Delta R.T.: -0.001 min
Response: 7974080
Conc: 1.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-03-022219-A

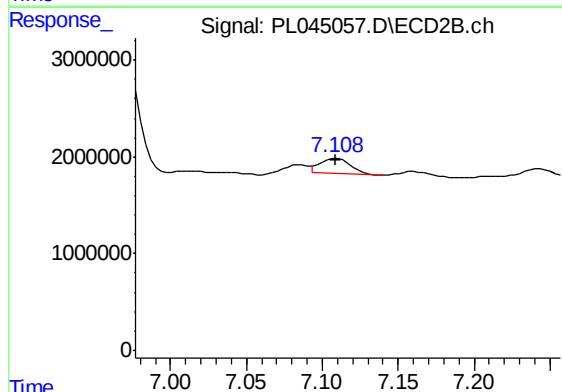


#17 4,4'-DDT

R.T.: 7.110 min
Delta R.T.: 0.000 min
Response: 2149490
Conc: 1.10 ng/ml

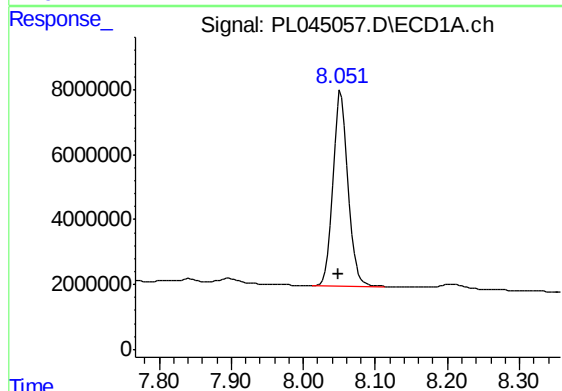

#28 Decachlorobiphenyl

R.T.: 8.052 min
Delta R.T.: 0.003 min
Response: 86873398
Conc: 11.91 ng/ml

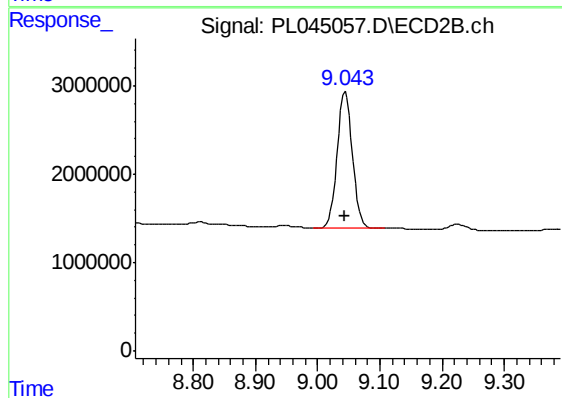

#28 Decachlorobiphenyl

R.T.: 9.045 min
Delta R.T.: 0.002 min
Response: 26437292
Conc: 11.94 ng/ml