

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022519\
 Data File : PL045071.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Feb 2019 18:18
 Operator : AJ\SJ
 Sample : K1596-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-13

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 25 23:54:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 07 01:39:50 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.365	3.983	69359959	23171431	9.747	9.864
28)	SA Decachlor...	8.051	9.042	73466963	25368007	10.073	11.454
Target Compounds							
8)	B Heptachlo...	0.000	5.846	0	1744269	N.D.	0.698 #
10)	B gamma-Chl...	5.282f	0.000	4792568	0	0.497	N.D. #
11)	B alpha-Chl...	0.000	6.164	0	4270615	N.D.	1.541 #
12)	B 4,4'-DDE	5.486	6.320	22627725	8541279	2.609	3.577 #
13)	MA Dieldrin	5.609	0.000	9630775	0	1.026	N.D. #
14)	MA Endrin	5.868	6.715f	4834997	1462749	0.552	0.651
16)	A 4,4'-DDD	0.000	6.815	0	3321124	N.D.	1.730 #
17)	MA 4,4'-DDT	6.232	7.108	36359173	5359359	5.070	2.732 #
19)	B Endosulfa...	6.512	0.000	3494346	0	0.481	N.D. #
20)	A Methoxychlor	6.758f	0.000	9770516	0	2.435	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022519\
Data File : PL045071.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Feb 2019 18:18
Operator : AJ\SJ
Sample : K1596-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
COMP-13

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 25 23:54:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
Quant Title : GC Extractables
QLast Update : Thu Feb 07 01:39:50 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

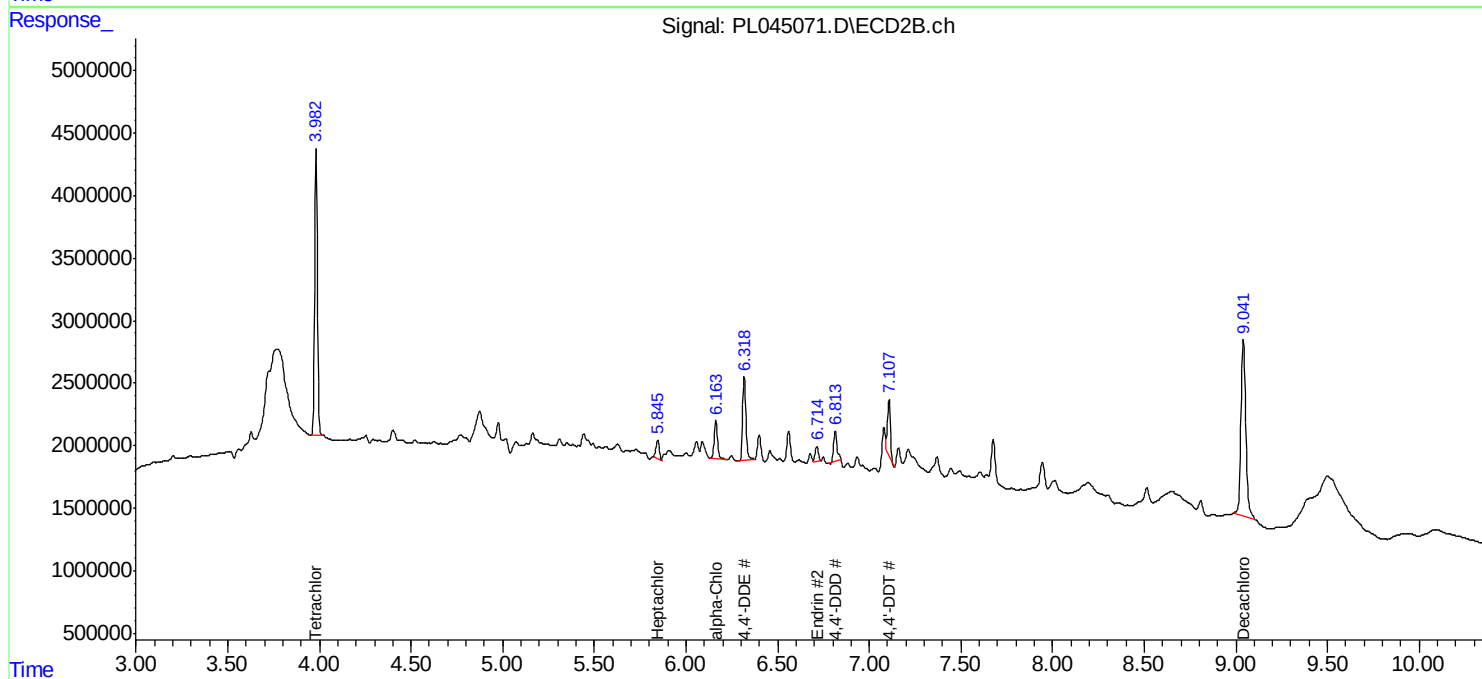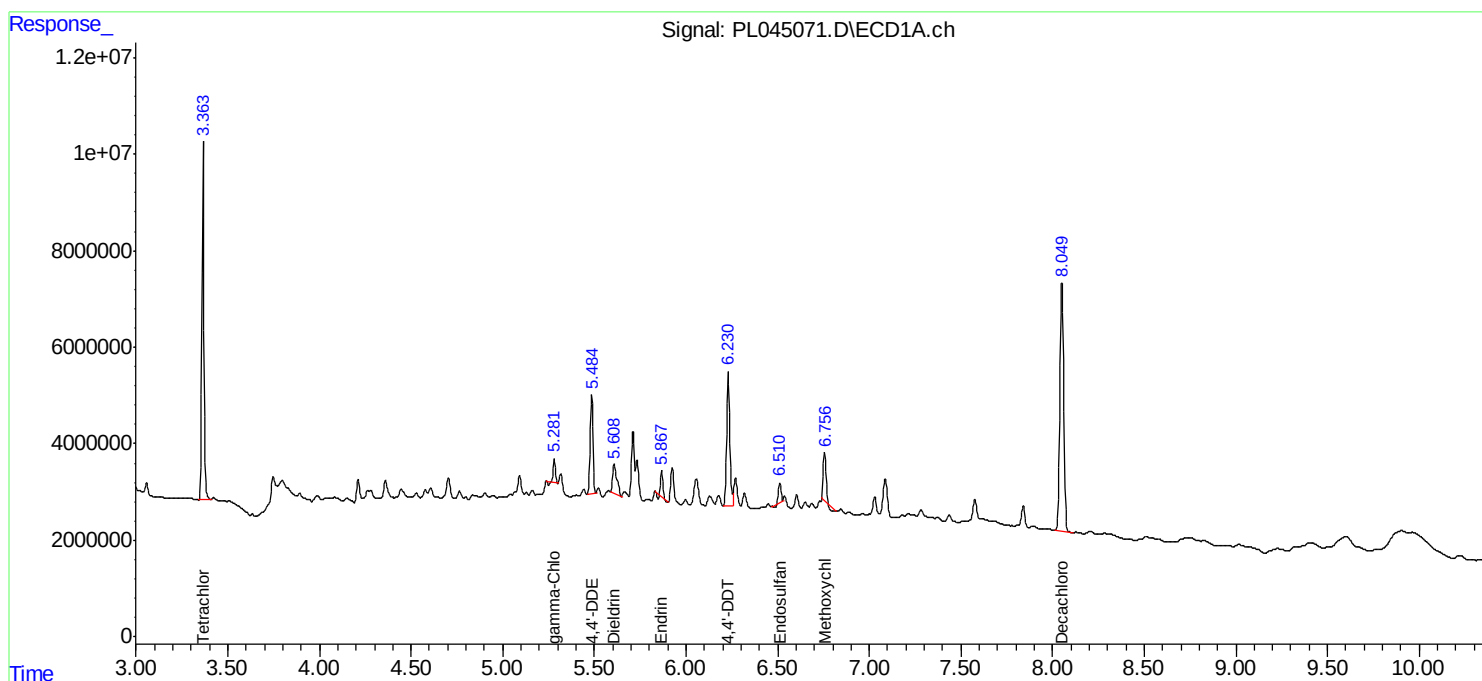


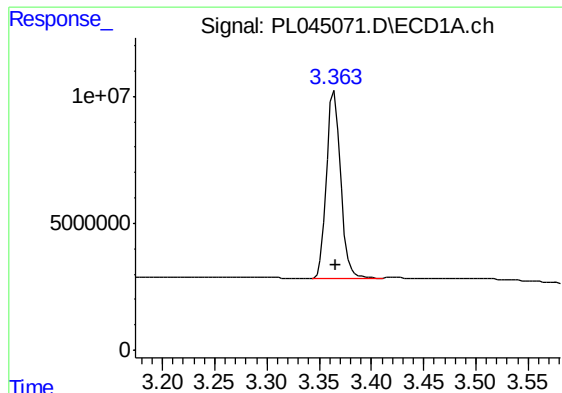

#1 Tetrachloro-m-xylene


R.T.: 3.365 min
Delta R.T.: -0.001 min
Response: 69359959
Conc: 9.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-13

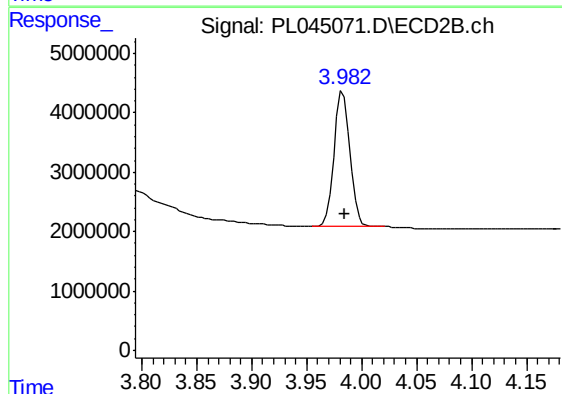


#1 Tetrachloro-m-xylene

R.T.: 3.983 min
Delta R.T.: -0.002 min
Response: 23171431
Conc: 9.86 ng/ml

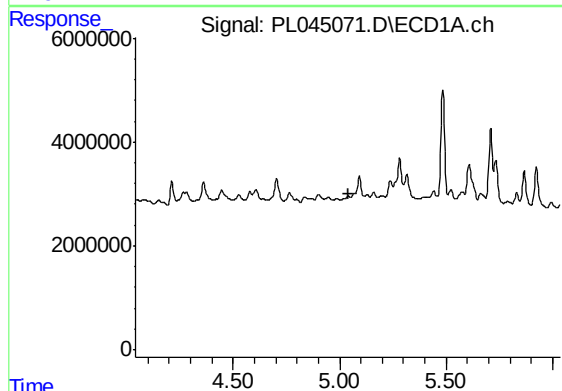


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.040 min
Response: 0
Conc: N.D.

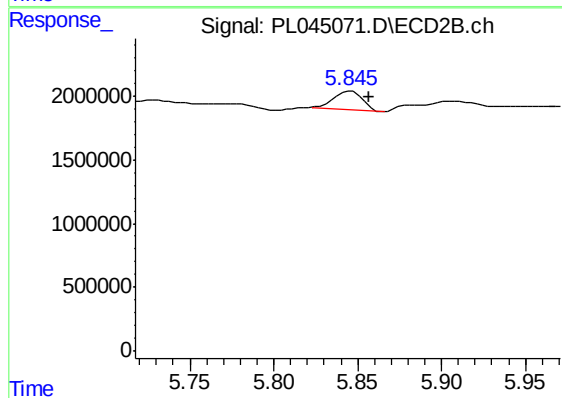

#8 Heptachlor epoxide


R.T.: 5.846 min
Delta R.T.: -0.011 min
Response: 1744269
Conc: 0.70 ng/ml

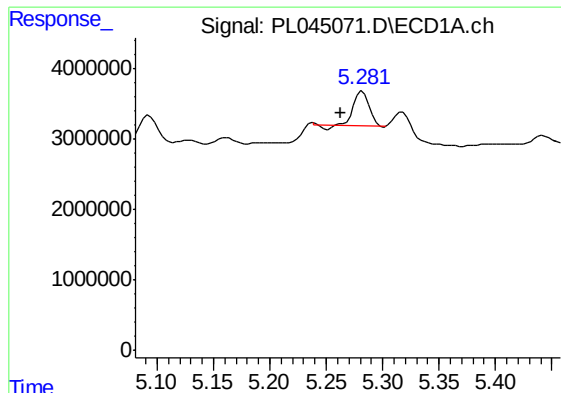

#10 gamma-Chlordane


R.T.: 5.282 min
Delta R.T.: 0.019 min
Response: 4792568
Conc: 0.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-13

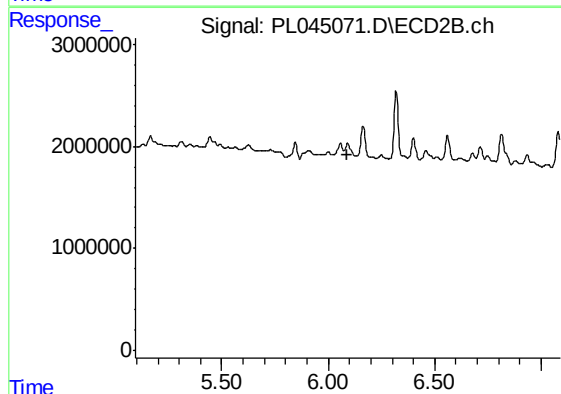


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.091 min
Response: 0
Conc: N.D.

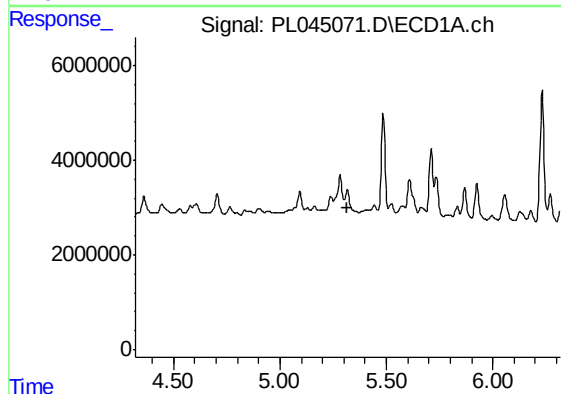


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.319 min
Response: 0
Conc: N.D.

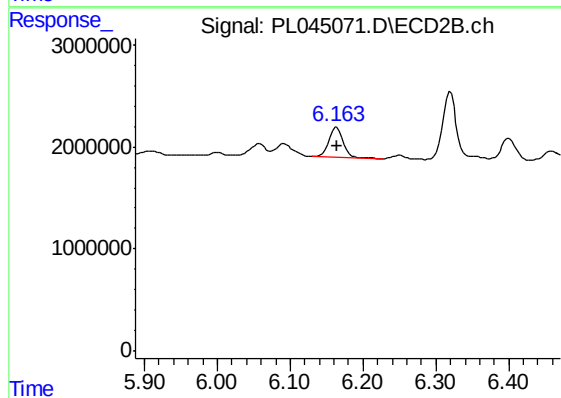

#11 alpha-Chlordane


R.T.: 6.164 min
Delta R.T.: 0.000 min
Response: 4270615
Conc: 1.54 ng/ml

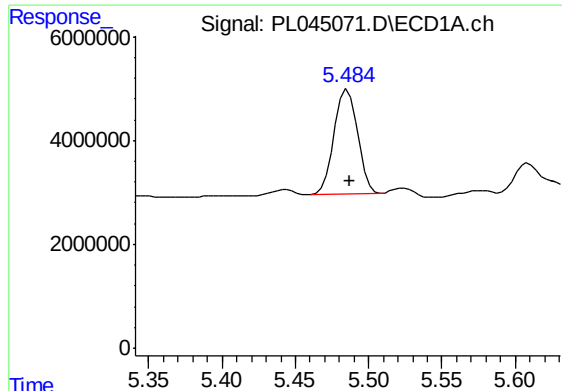

#12 4,4'-DDE


R.T.: 5.486 min
Delta R.T.: -0.001 min
Response: 22627725
Conc: 2.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-13

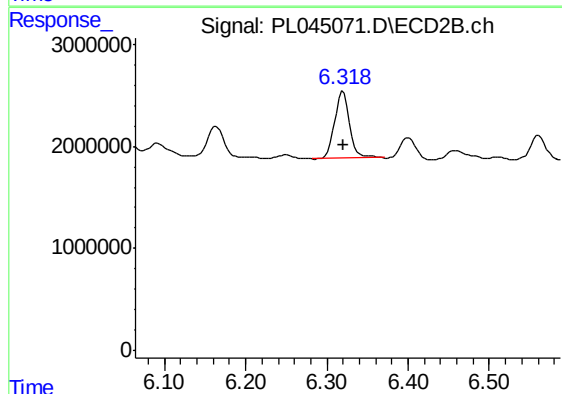


#12 4,4'-DDE

R.T.: 6.320 min
Delta R.T.: -0.001 min
Response: 8541279
Conc: 3.58 ng/ml

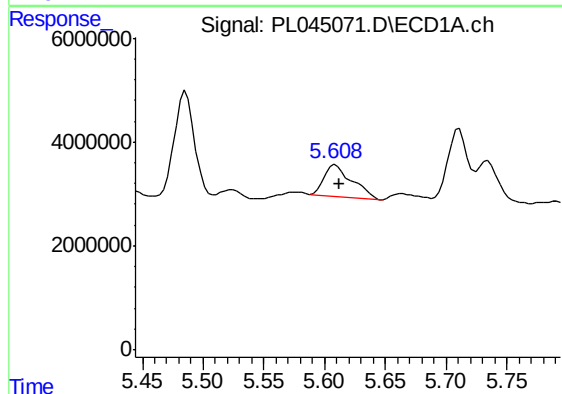


#13 Dieldrin

R.T.: 5.609 min
Delta R.T.: -0.003 min
Response: 9630775
Conc: 1.03 ng/ml

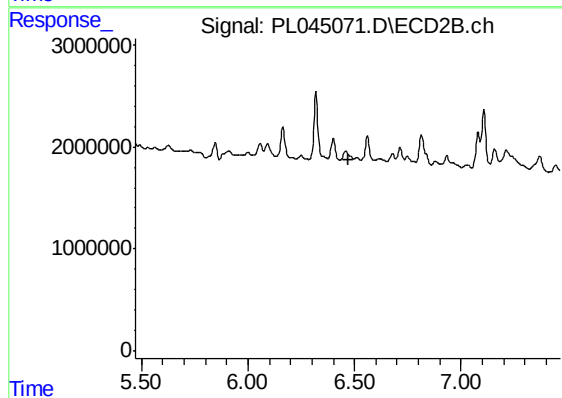

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.470 min
Response: 0
Conc: N.D.

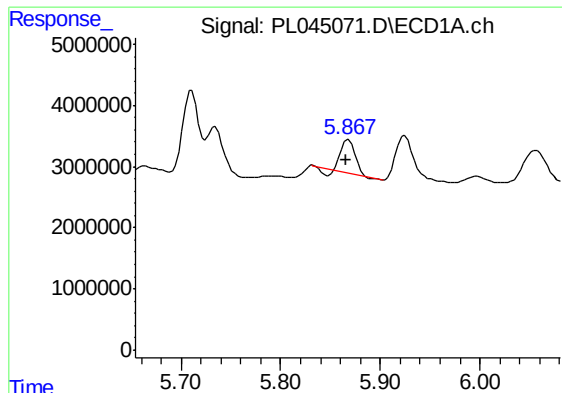

#14 Endrin


R.T.: 5.868 min
Delta R.T.: 0.003 min
Response: 4834997
Conc: 0.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-13

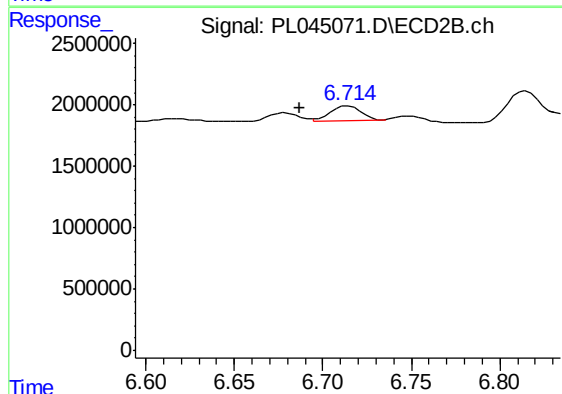


#14 Endrin

R.T.: 6.715 min
Delta R.T.: 0.028 min
Response: 1462749
Conc: 0.65 ng/ml

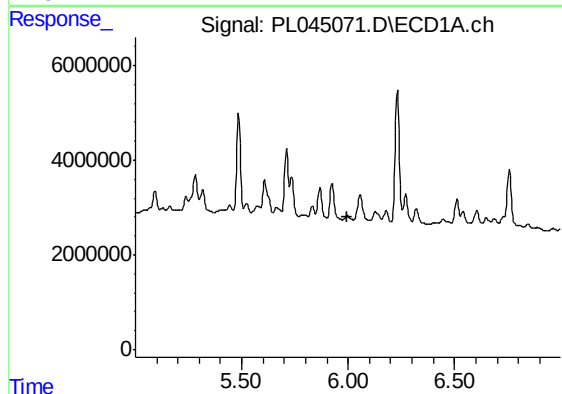


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.998 min
Response: 0
Conc: N.D.

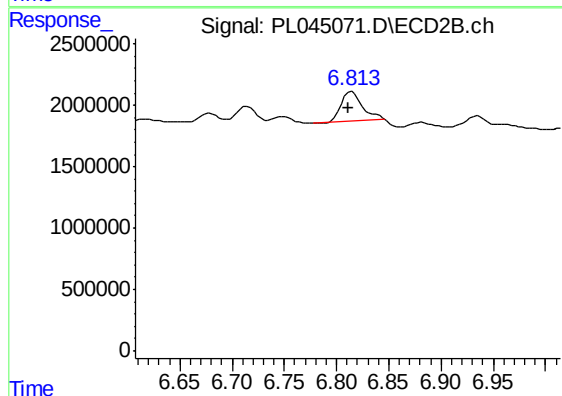

#16 4,4'-DDD


R.T.: 6.815 min
Delta R.T.: 0.004 min
Response: 3321124
Conc: 1.73 ng/ml

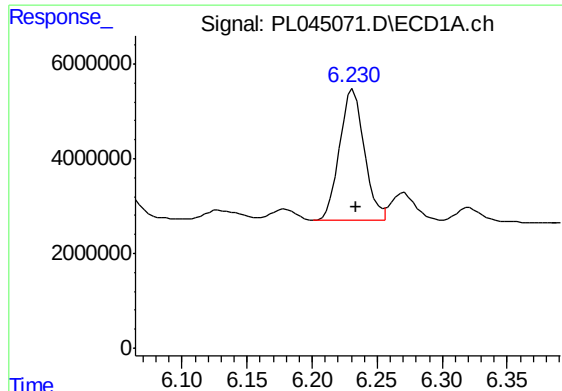

#17 4,4'-DDT


R.T.: 6.232 min
Delta R.T.: -0.002 min
Response: 36359173
Conc: 5.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-13

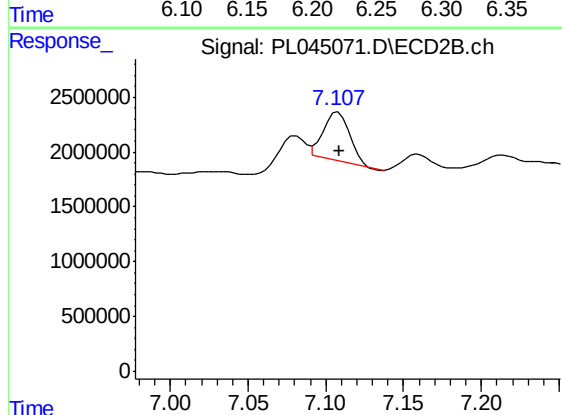


#17 4,4'-DDT

R.T.: 7.108 min
Delta R.T.: -0.001 min
Response: 5359359
Conc: 2.73 ng/ml

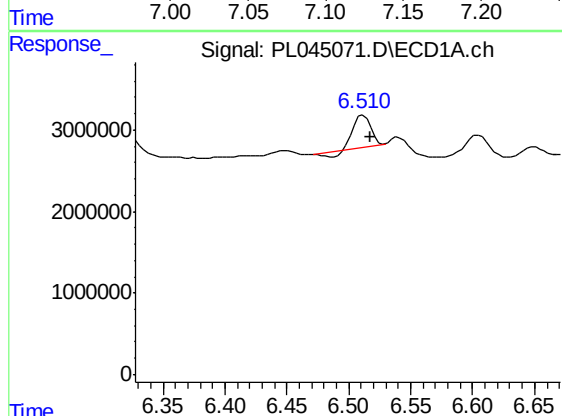


#19 Endosulfan Sulfate

R.T.: 6.512 min
Delta R.T.: -0.005 min
Response: 3494346
Conc: 0.48 ng/ml

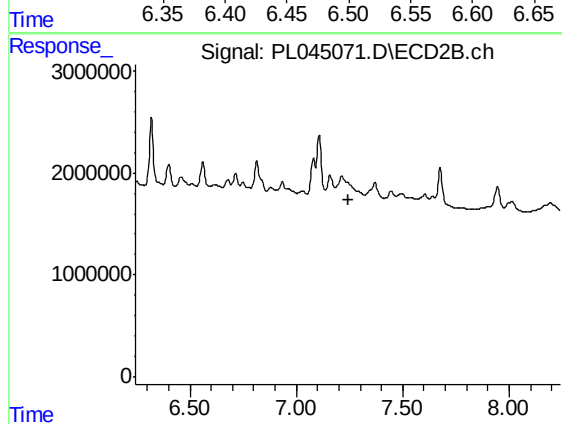

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.243 min
Response: 0
Conc: N.D.

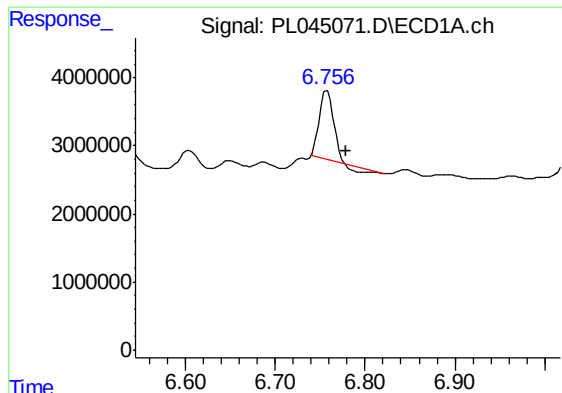

#20 Methoxychlor


R.T.: 6.758 min
Delta R.T.: -0.021 min
Response: 9770516
Conc: 2.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-13

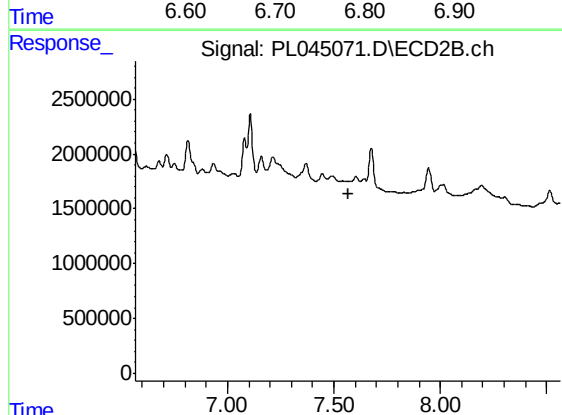


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.567 min
Response: 0
Conc: N.D.

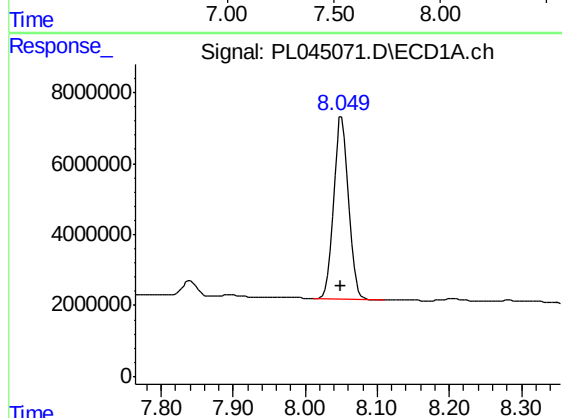

#28 Decachlorobiphenyl

R.T.: 8.051 min
Delta R.T.: 0.002 min
Response: 73466963
Conc: 10.07 ng/ml

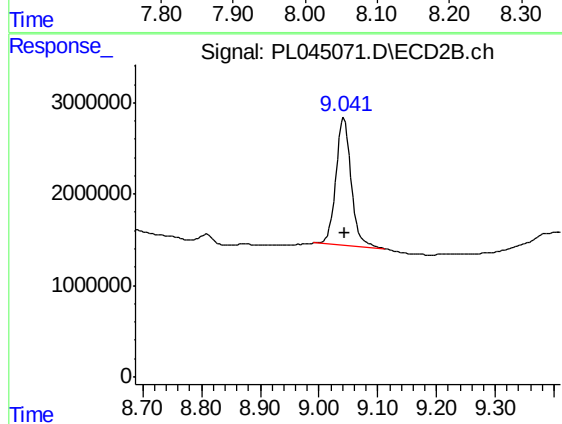

#28 Decachlorobiphenyl

R.T.: 9.042 min
Delta R.T.: 0.000 min
Response: 25368007
Conc: 11.45 ng/ml