

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022519\
 Data File : PL045072.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Feb 2019 18:32
 Operator : AJ\SJ
 Sample : K1596-02
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-14

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 25 23:54:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 07 01:39:50 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.365	3.984	60600606	20432811	8.516	8.698
28)	SA Decachlor...	8.050	9.042	72857765	23981715	9.989	10.828
Target Compounds							
4)	MA Heptachlor	4.360	5.165	5862110	1660135	0.569	0.545
8)	B Heptachlo...	0.000	5.847	0	2473038	N.D.	0.989 #
10)	B gamma-Chl...	5.283f	0.000	3231166	0	0.335	N.D. #
11)	B alpha-Chl...	0.000	6.164	0	4007873	N.D.	1.446 #
12)	B 4,4'-DDE	5.485	6.320	11736142	6151303	1.353	2.576 #
13)	MA Dieldrin	5.608	0.000	11530091	0	1.228	N.D. #
14)	MA Endrin	0.000	6.679	0	2557516	N.D.	1.138 #
16)	A 4,4'-DDD	0.000	6.816	0	3731794	N.D.	1.943 #
17)	MA 4,4'-DDT	6.229	7.081f	20045133	1602661	2.795	0.817 #
20)	A Methoxychlor	6.757f	0.000	9682302	0	2.413	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022519\
Data File : PL045072.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Feb 2019 18:32
Operator : AJ\SJ
Sample : K1596-02
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
COMP-14

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 25 23:54:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
Quant Title : GC Extractables
QLast Update : Thu Feb 07 01:39:50 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

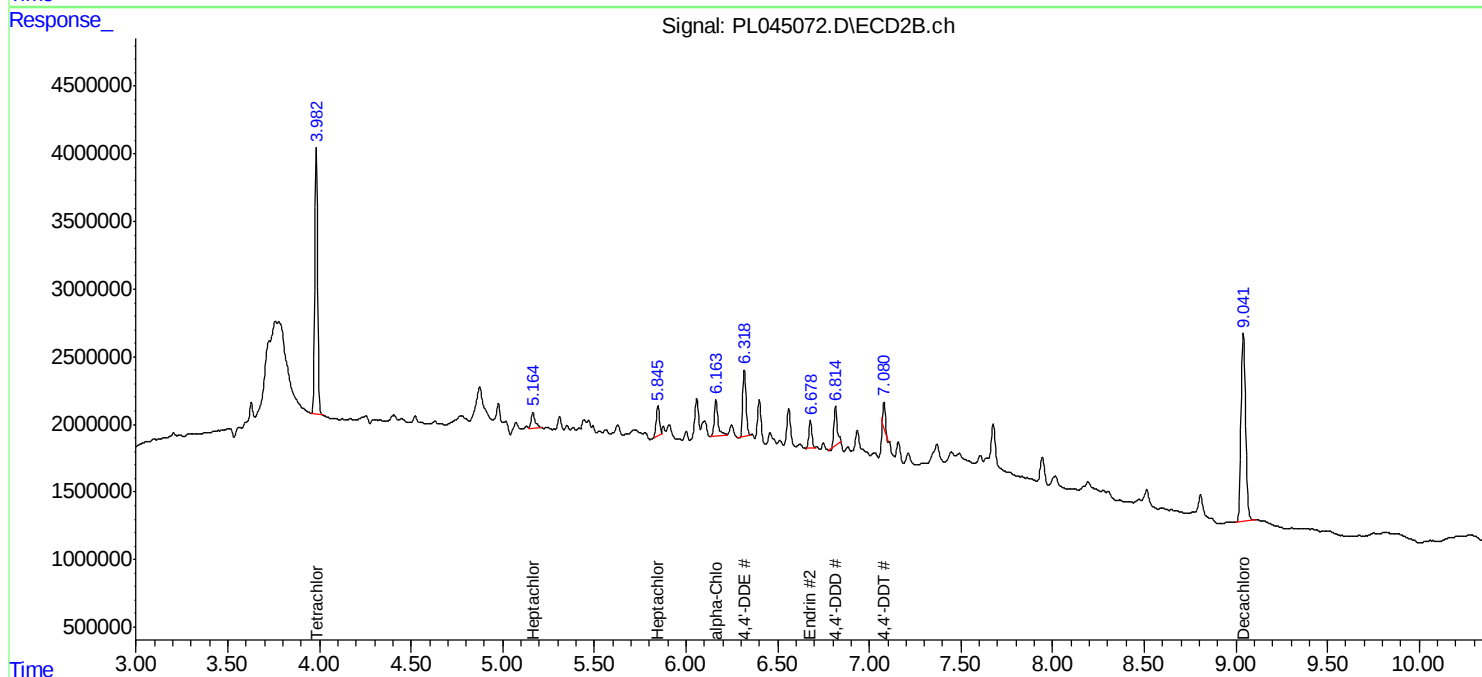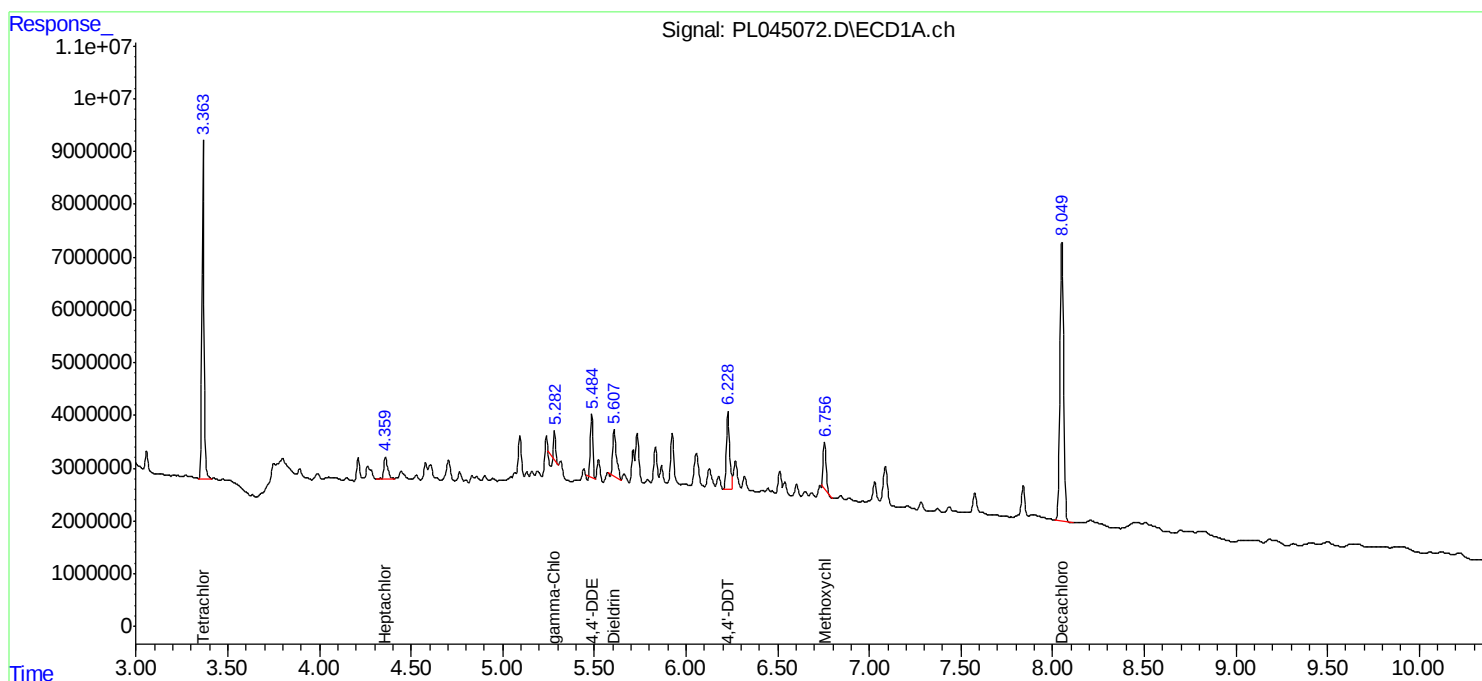


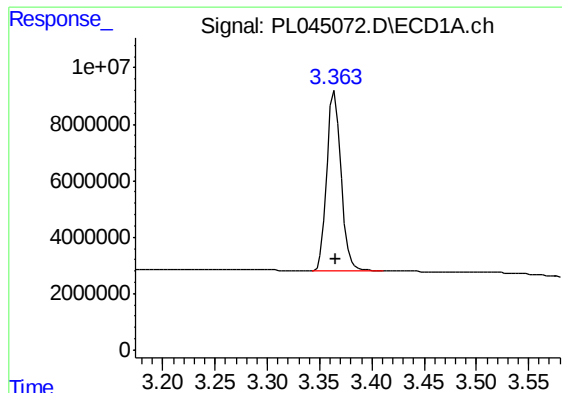

#1 Tetrachloro-m-xylene


R.T.: 3.365 min
Delta R.T.: -0.001 min
Response: 60600606
Conc: 8.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-14

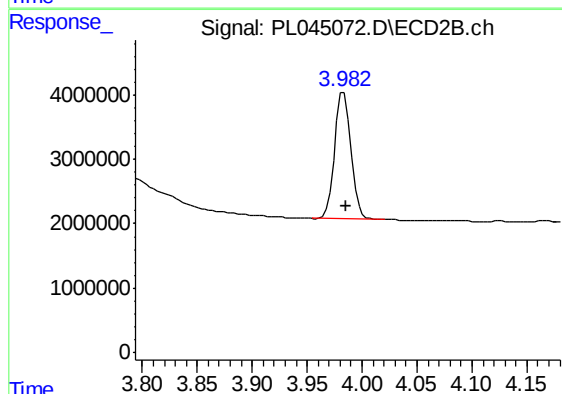


#1 Tetrachloro-m-xylene

R.T.: 3.984 min
Delta R.T.: -0.001 min
Response: 20432811
Conc: 8.70 ng/ml

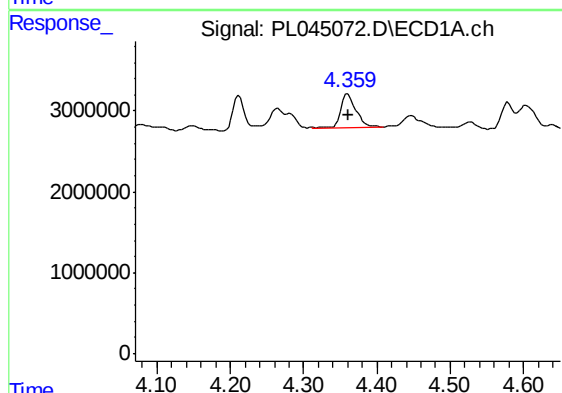


#4 Heptachlor

R.T.: 4.360 min
Delta R.T.: -0.002 min
Response: 5862110
Conc: 0.57 ng/ml

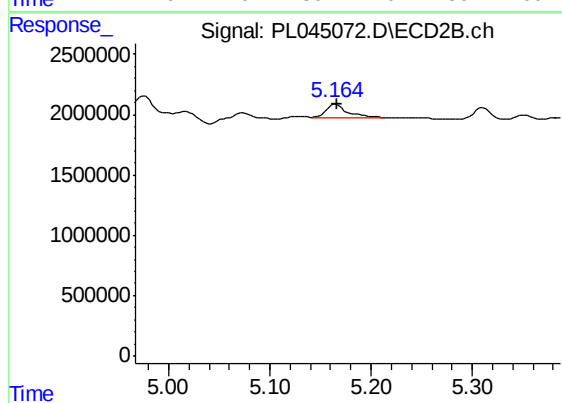

#4 Heptachlor


R.T.: 5.165 min
Delta R.T.: 0.000 min
Response: 1660135
Conc: 0.55 ng/ml

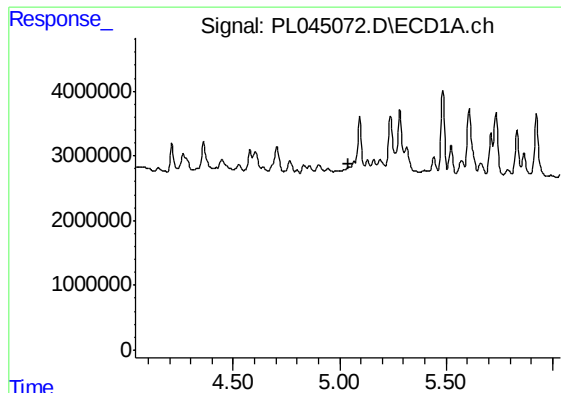

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.040 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
COMP-14

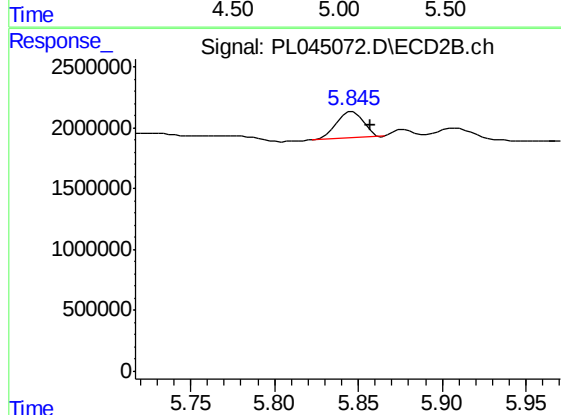


#8 Heptachlor epoxide

R.T.: 5.847 min
Delta R.T.: -0.010 min
Response: 2473038
Conc: 0.99 ng/ml

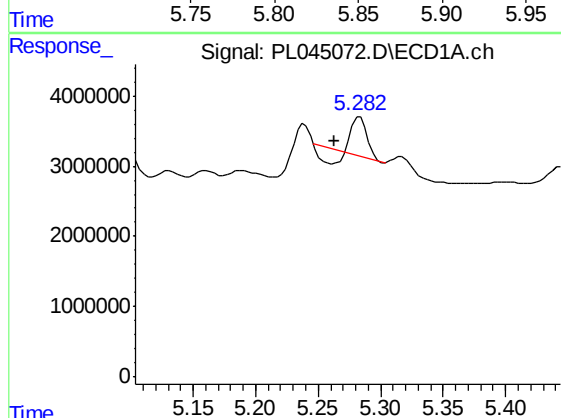


#10 gamma-Chlordane

R.T.: 5.283 min
Delta R.T.: 0.020 min
Response: 3231166
Conc: 0.33 ng/ml

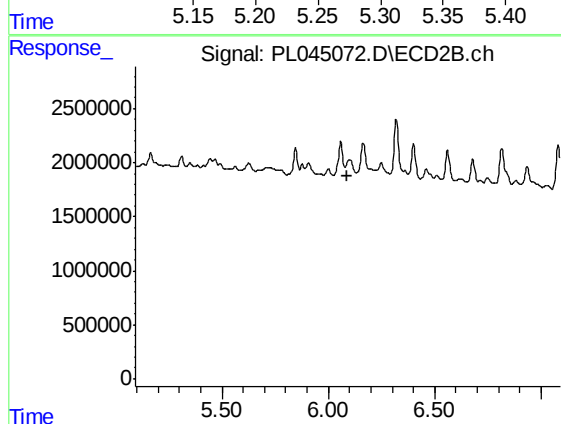

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.091 min
Response: 0
Conc: N.D.

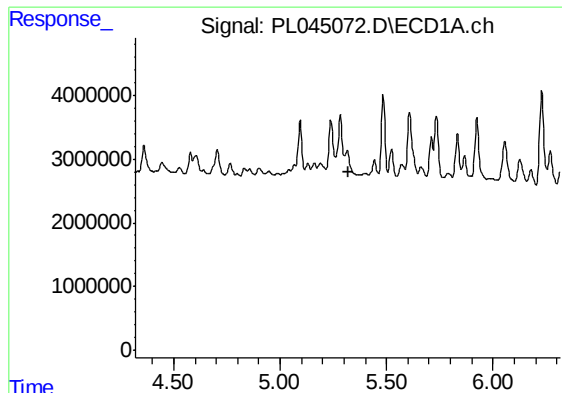

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.319 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
COMP-14

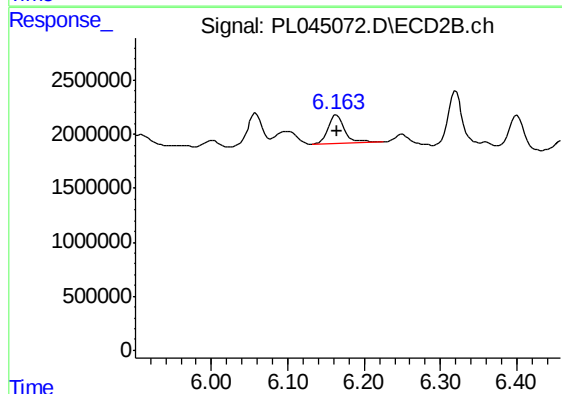


#11 alpha-Chlordane

R.T.: 6.164 min
Delta R.T.: 0.000 min
Response: 4007873
Conc: 1.45 ng/ml

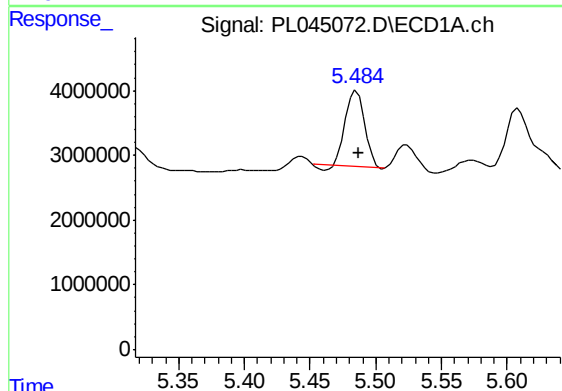


#12 4,4'-DDE

R.T.: 5.485 min
Delta R.T.: -0.002 min
Response: 11736142
Conc: 1.35 ng/ml

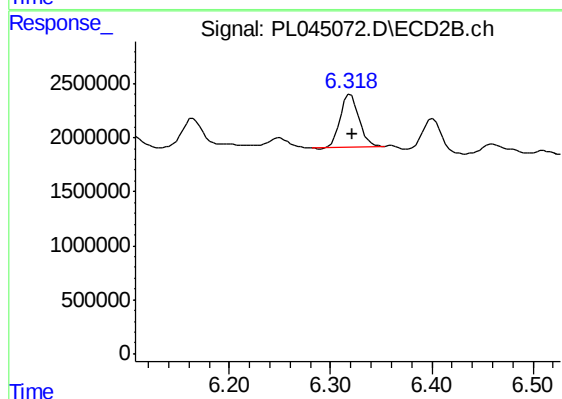

#12 4,4'-DDE


R.T.: 6.320 min
Delta R.T.: -0.001 min
Response: 6151303
Conc: 2.58 ng/ml

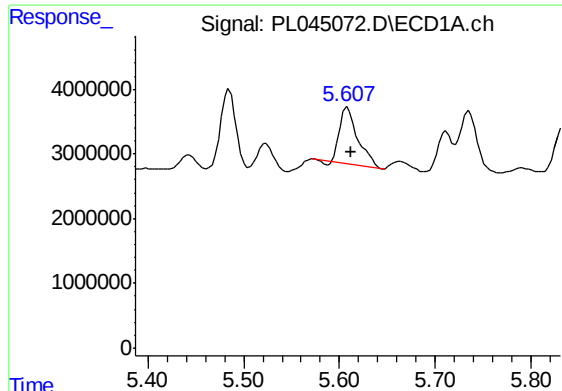

#13 Dieldrin


R.T.: 5.608 min
Delta R.T.: -0.004 min
Response: 11530091
Conc: 1.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-14

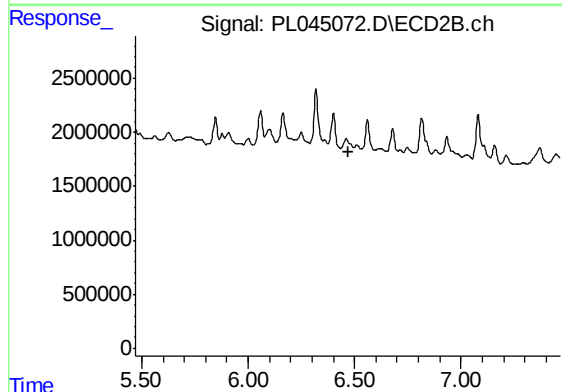


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.470 min
Response: 0
Conc: N.D.

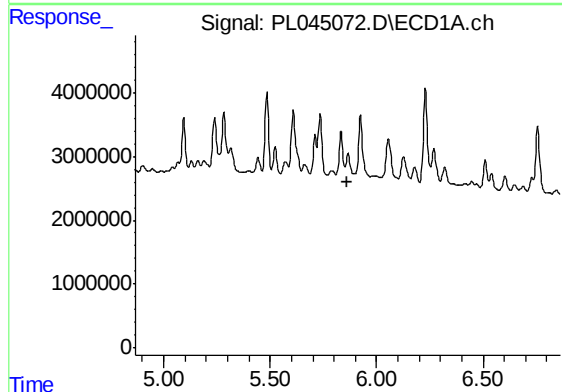


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 5.865 min
Response: 0
Conc: N.D.

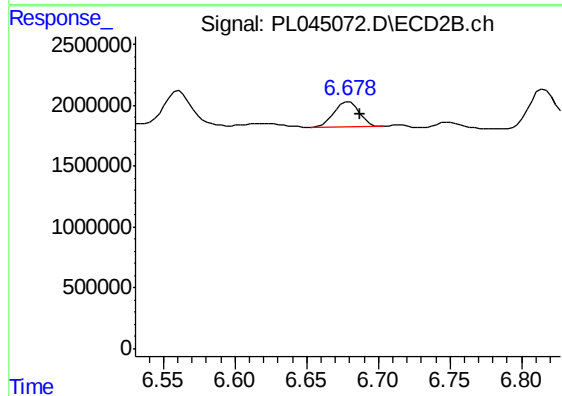

#14 Endrin


R.T.: 6.679 min
Delta R.T.: -0.008 min
Response: 2557516
Conc: 1.14 ng/ml

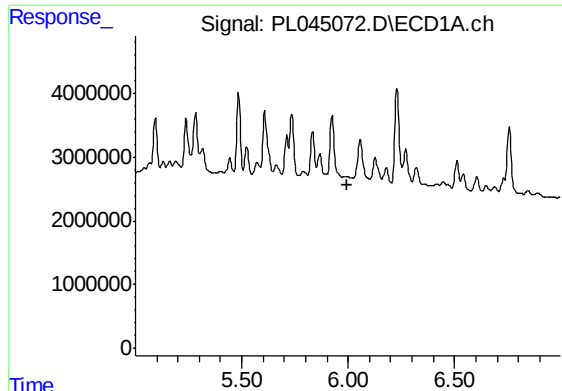

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.998 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
COMP-14

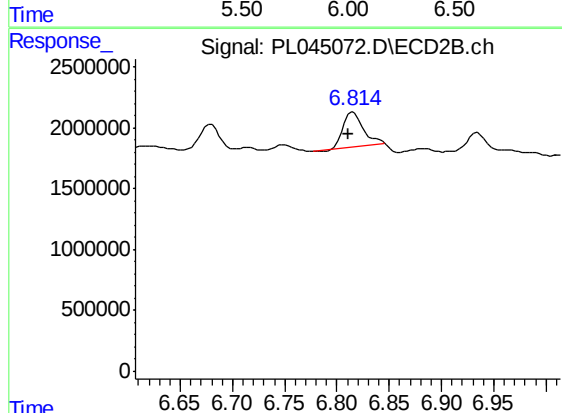


#16 4,4'-DDD

R.T.: 6.816 min
Delta R.T.: 0.005 min
Response: 3731794
Conc: 1.94 ng/ml

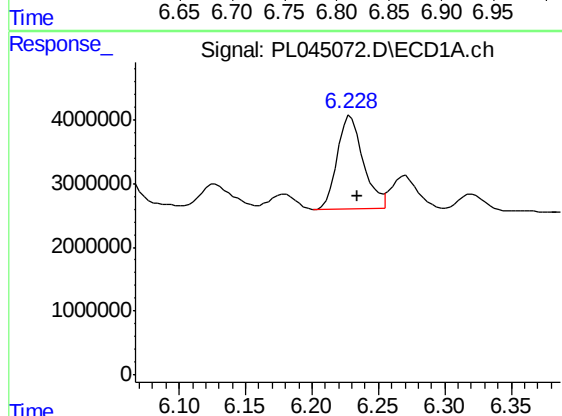


#17 4,4'-DDT

R.T.: 6.229 min
Delta R.T.: -0.005 min
Response: 20045133
Conc: 2.80 ng/ml

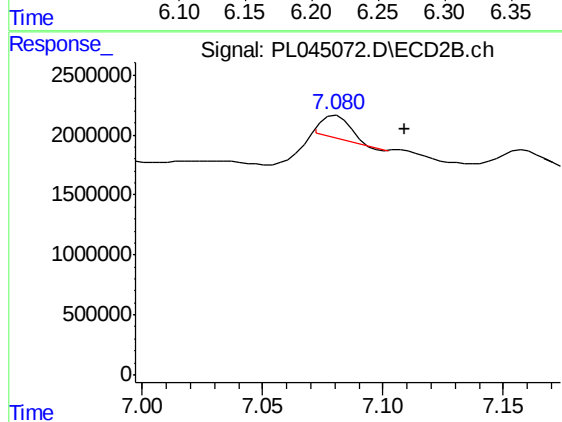

#17 4,4'-DDT


R.T.: 7.081 min
Delta R.T.: -0.028 min
Response: 1602661
Conc: 0.82 ng/ml

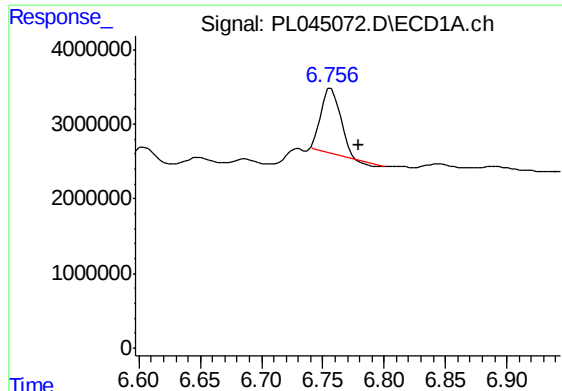

#20 Methoxychlor


R.T.: 6.757 min
Delta R.T.: -0.022 min
Response: 9682302
Conc: 2.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-14

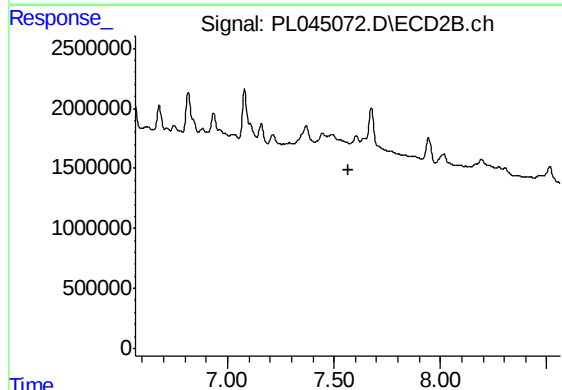


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.567 min
Response: 0
Conc: N.D.

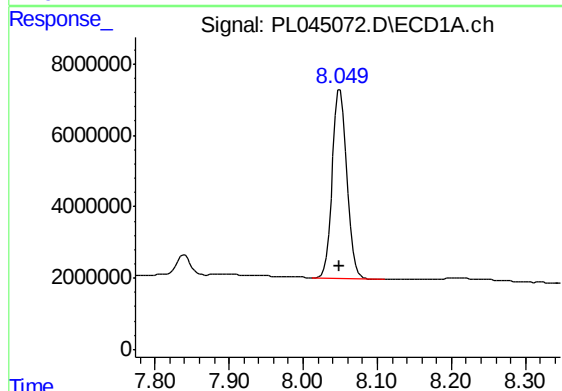

#28 Decachlorobiphenyl

R.T.: 8.050 min
Delta R.T.: 0.001 min
Response: 72857765
Conc: 9.99 ng/ml

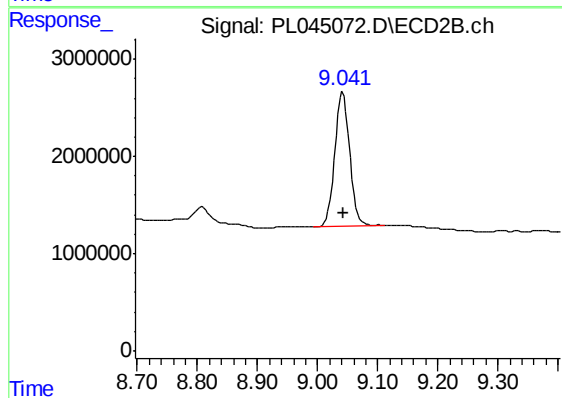

#28 Decachlorobiphenyl

R.T.: 9.042 min
Delta R.T.: 0.000 min
Response: 23981715
Conc: 10.83 ng/ml