

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022519\
 Data File : PL045074.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Feb 2019 19:00
 Operator : AJ\SJ
 Sample : K1597-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-25

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 25 23:55:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 07 01:39:50 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.365	3.984	41006283	13674934	5.763	5.821
28)	SA Decachlor...	8.051	9.043	69341780	21091809	9.507	9.523
Target Compounds							
16)	A 4,4'-DDD	0.000	6.817	0	1948615	N.D.	1.015 #
20)	A Methoxychlor	6.758f	0.000	6225261	0	1.551	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022519\
Data File : PL045074.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Feb 2019 19:00
Operator : AJ\SJ
Sample : K1597-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
TP-25

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 25 23:55:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
Quant Title : GC Extractables
QLast Update : Thu Feb 07 01:39:50 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

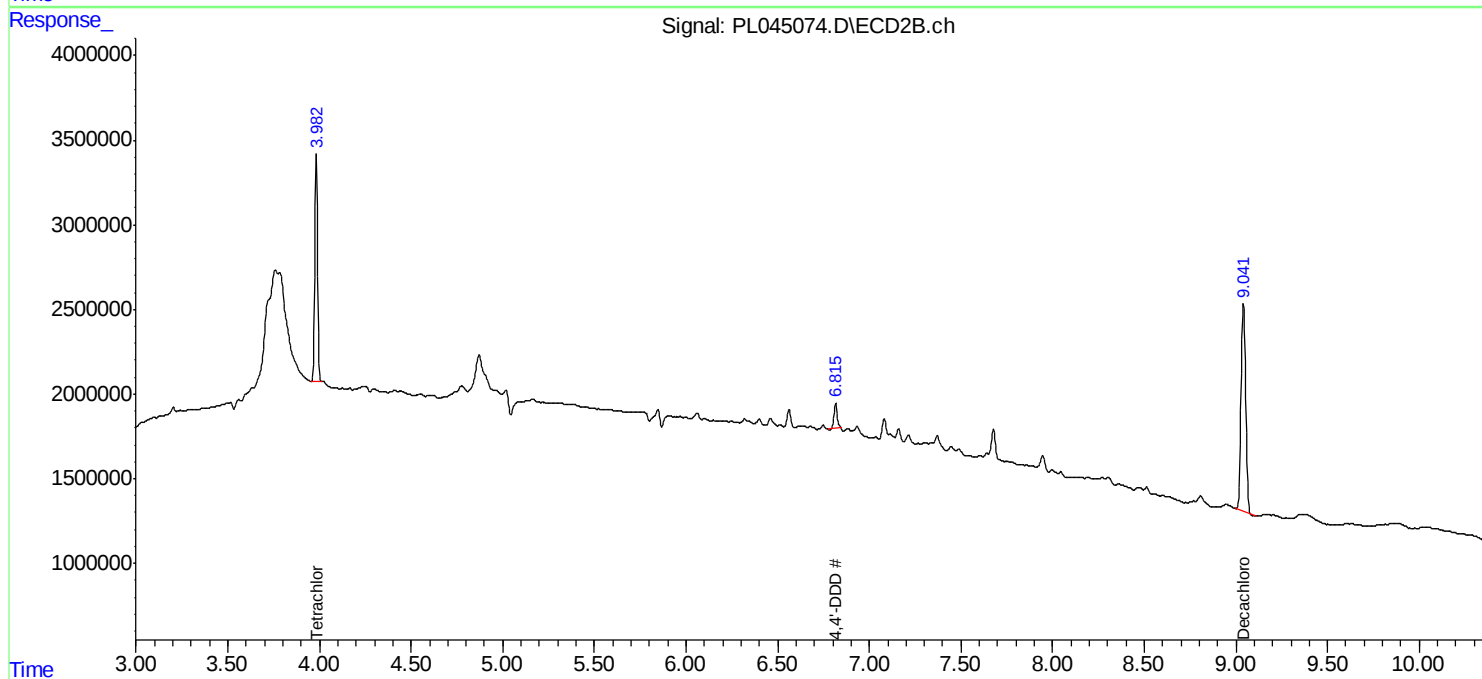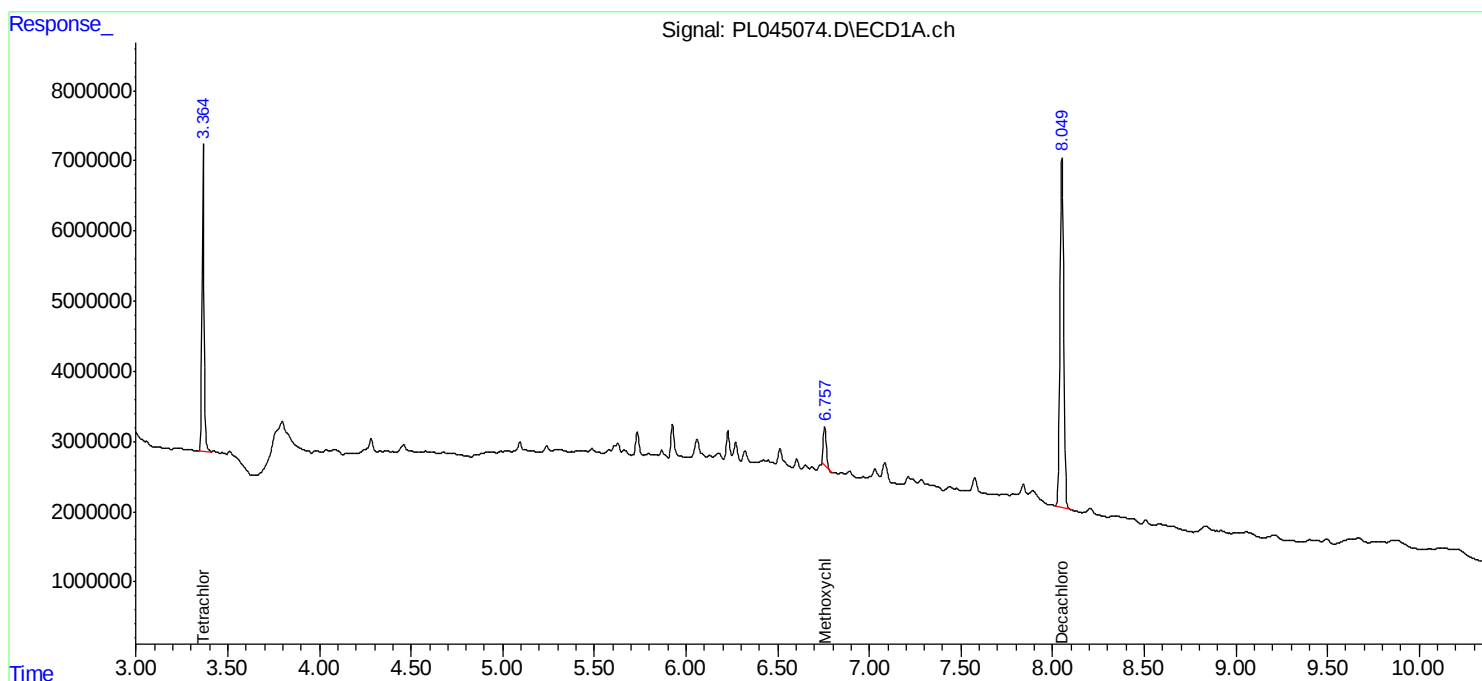


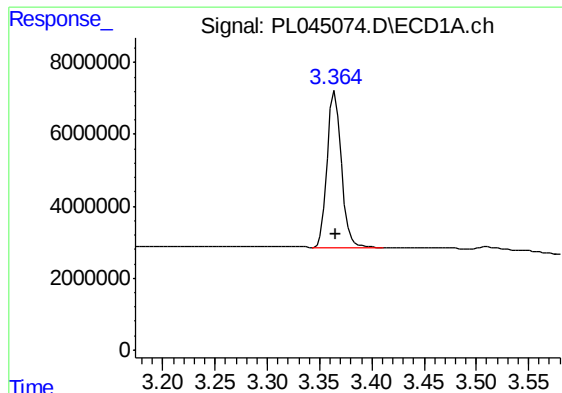

#1 Tetrachloro-m-xylene


R.T.: 3.365 min
Delta R.T.: -0.001 min
Response: 41006283
Conc: 5.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-25

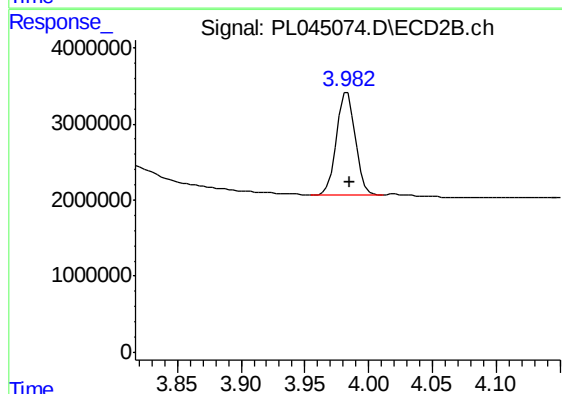


#1 Tetrachloro-m-xylene

R.T.: 3.984 min
Delta R.T.: -0.001 min
Response: 13674934
Conc: 5.82 ng/ml

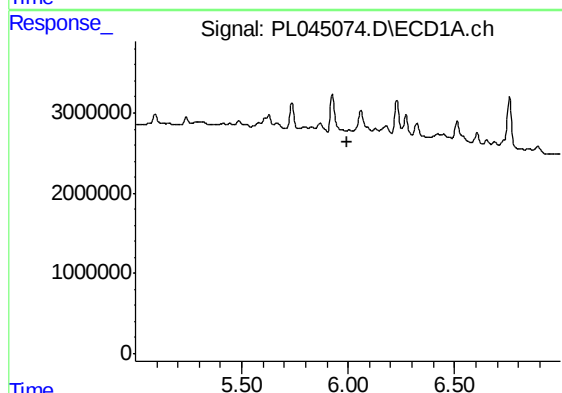


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.998 min
Response: 0
Conc: N.D.

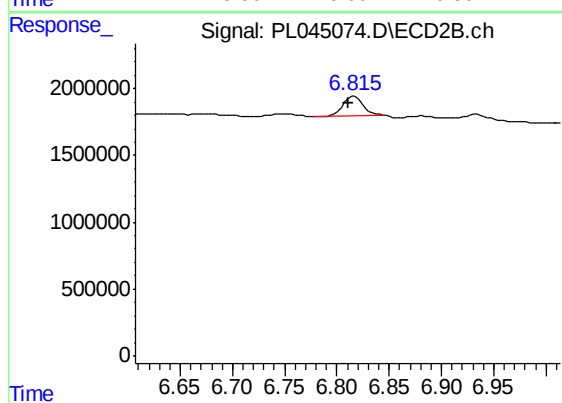

#16 4,4'-DDD


R.T.: 6.817 min
Delta R.T.: 0.006 min
Response: 1948615
Conc: 1.01 ng/ml

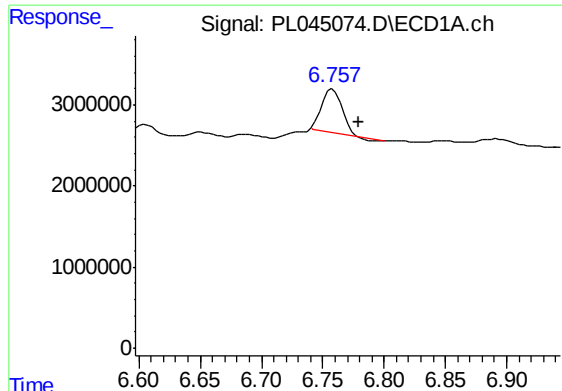

#20 Methoxychlor


R.T.: 6.758 min
Delta R.T.: -0.021 min
Response: 6225261
Conc: 1.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-25

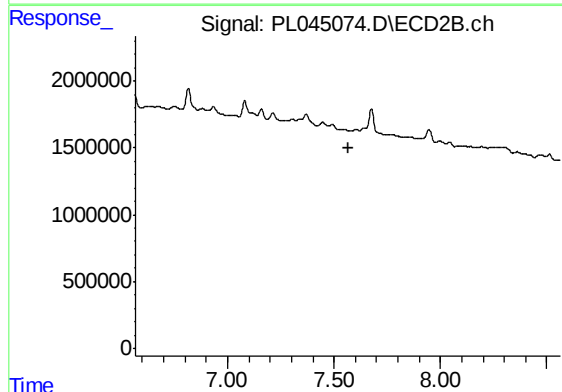


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.567 min
Response: 0
Conc: N.D.

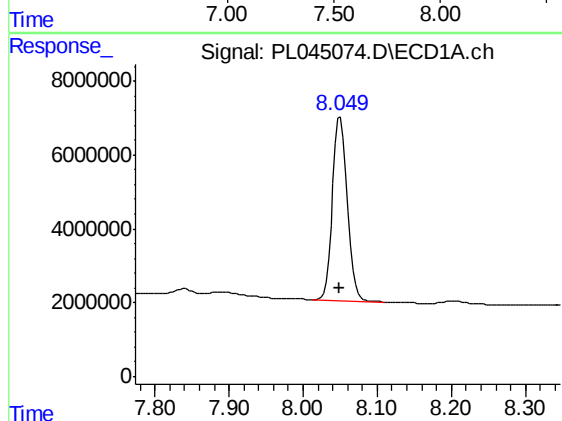

#28 Decachlorobiphenyl

R.T.: 8.051 min
Delta R.T.: 0.002 min
Response: 69341780
Conc: 9.51 ng/ml

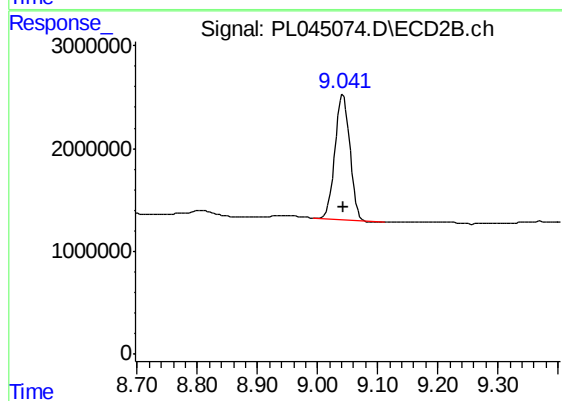

#28 Decachlorobiphenyl

R.T.: 9.043 min
Delta R.T.: 0.000 min
Response: 21091809
Conc: 9.52 ng/ml