

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022519\
 Data File : PL045078.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Feb 2019 19:56
 Operator : AJ\SJ
 Sample : K1597-15
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-23

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 25 23:55:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 07 01:39:50 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.365	3.984	111.1E6	35099119	15.616	14.941
28)	SA Decachlor...	8.050	9.042	59103047	16091663	8.103	7.265
Target Compounds							
7)	B delta-BHC	0.000	5.017f	0	4537014	N.D.	2.481 #
9)	A Endosulfan I	5.400f	0.000	7919760	0	0.908	N.D. #
10)	B gamma-Chl...	0.000	6.076	0	3516529	N.D.	1.267 #
13)	MA Dieldrin	5.599	6.466	14368696	1771813	1.531	0.687 #
15)	B Endosulfa...	0.000	6.913f	0	1890809	N.D.	0.821 #
19)	B Endosulfa...	6.500f	7.242	26240213	8675600	3.610	4.112



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022519\
Data File : PL045078.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Feb 2019 19:56
Operator : AJ\SJ
Sample : K1597-15
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-23

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 25 23:55:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
Quant Title : GC Extractables
QLast Update : Thu Feb 07 01:39:50 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

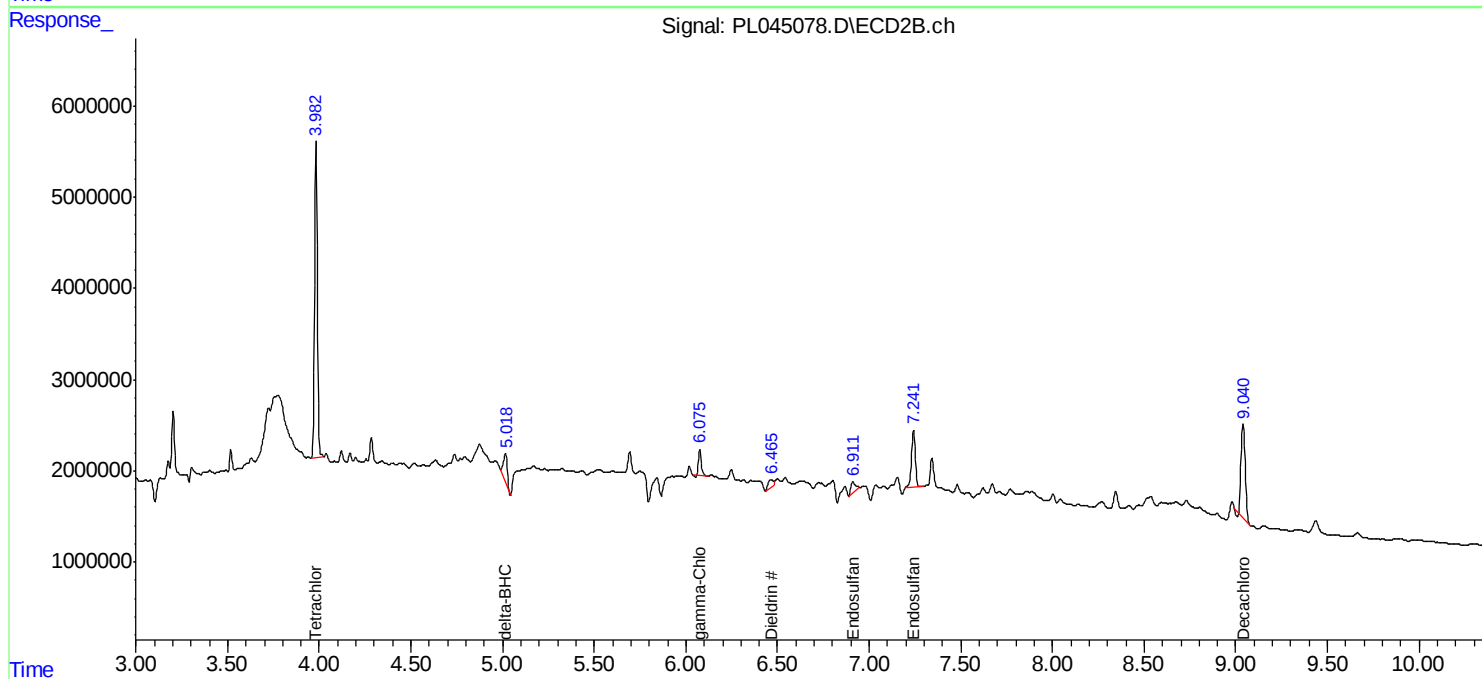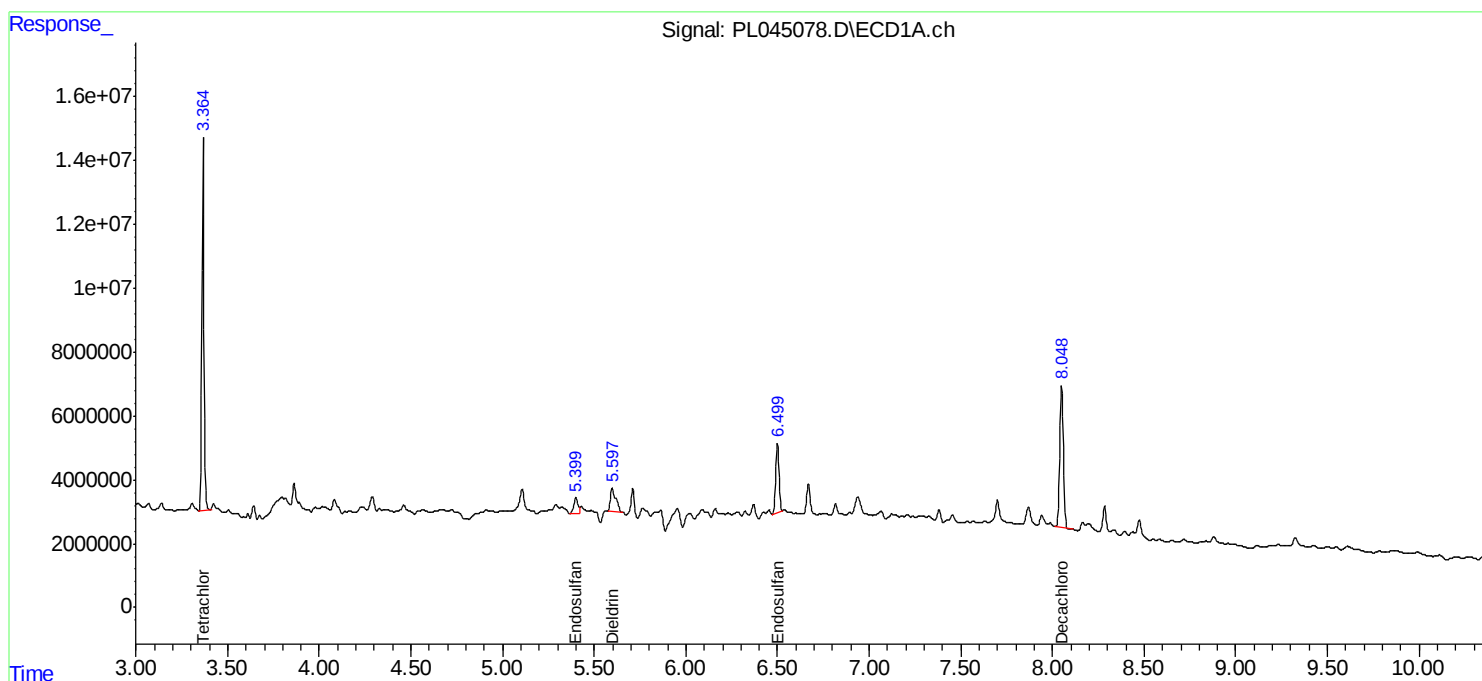


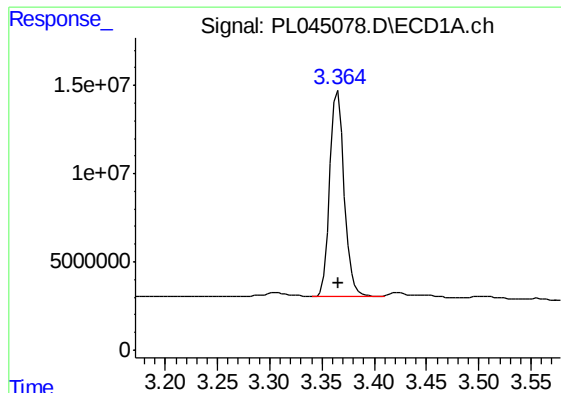

#1 Tetrachloro-m-xylene


R.T.: 3.365 min
Delta R.T.: 0.000 min
Response: 111119693
Conc: 15.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-23

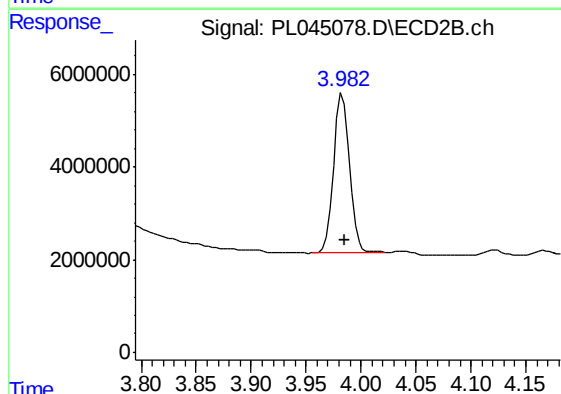


#1 Tetrachloro-m-xylene

R.T.: 3.984 min
Delta R.T.: -0.001 min
Response: 35099119
Conc: 14.94 ng/ml

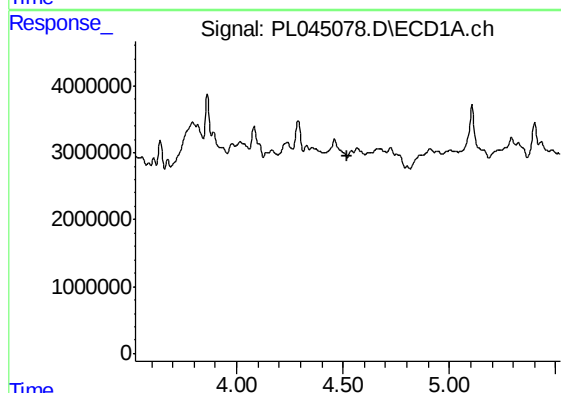


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.522 min
Response: 0
Conc: N.D.

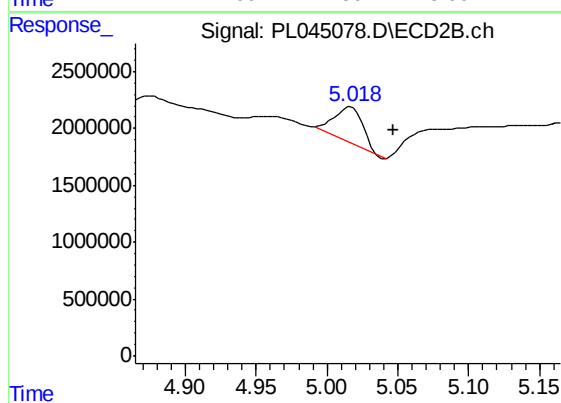

#7 delta-BHC


R.T.: 5.017 min
Delta R.T.: -0.030 min
Response: 4537014
Conc: 2.48 ng/ml

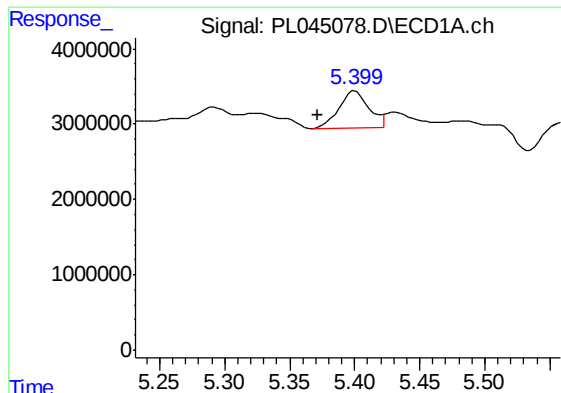

#9 Endosulfan I


R.T.: 5.400 min
Delta R.T.: 0.028 min
Response: 7919760
Conc: 0.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-23

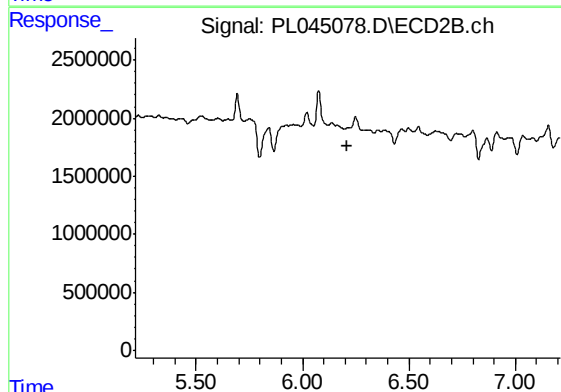


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.213 min
Response: 0
Conc: N.D.

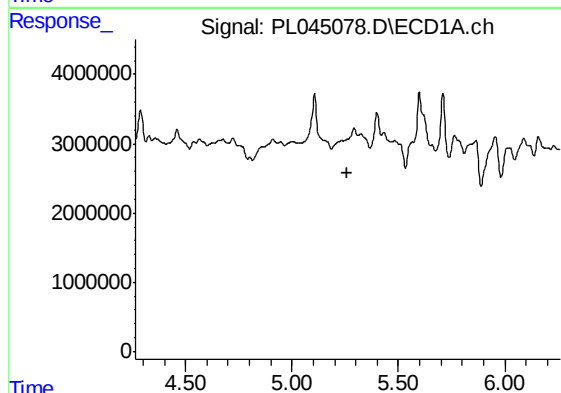


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.263 min
Response: 0
Conc: N.D.

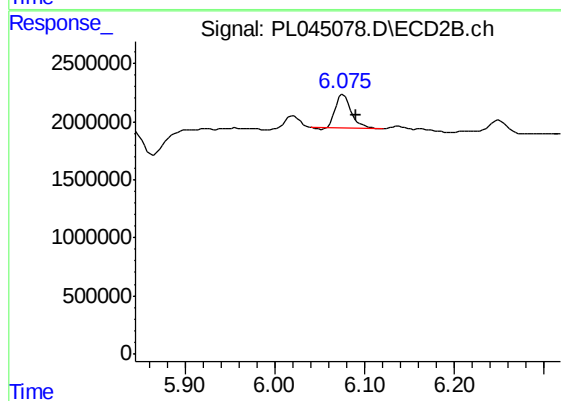

#10 gamma-Chlordane


R.T.: 6.076 min
Delta R.T.: -0.015 min
Response: 3516529
Conc: 1.27 ng/ml

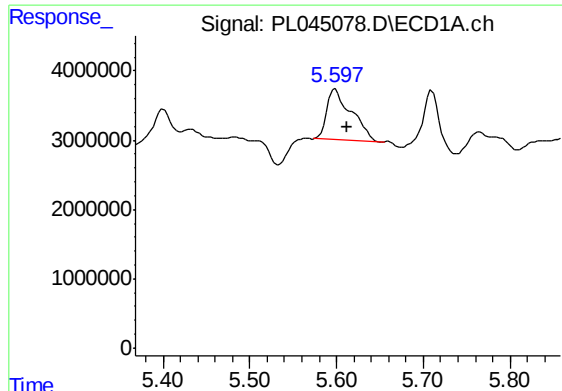

#13 Dieldrin


R.T.: 5.599 min
Delta R.T.: -0.013 min
Response: 14368696
Conc: 1.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-23

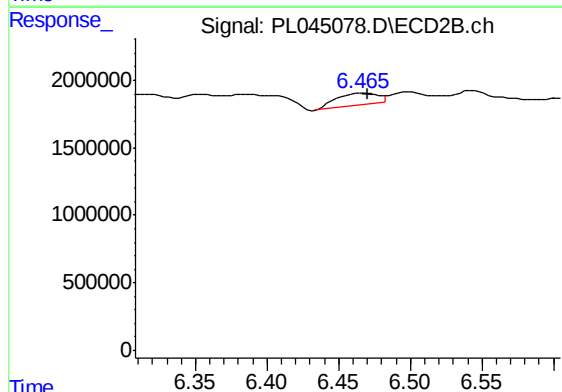


#13 Dieldrin

R.T.: 6.466 min
Delta R.T.: -0.004 min
Response: 1771813
Conc: 0.69 ng/ml

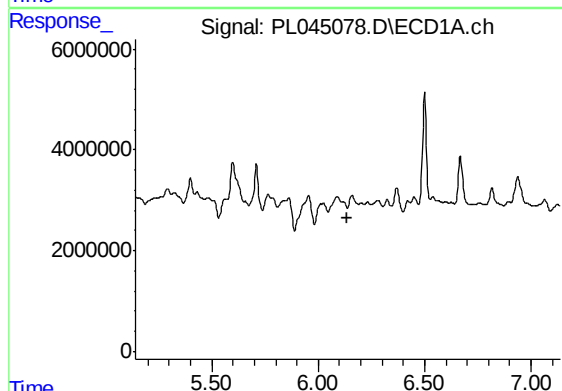


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.139 min
Response: 0
Conc: N.D.

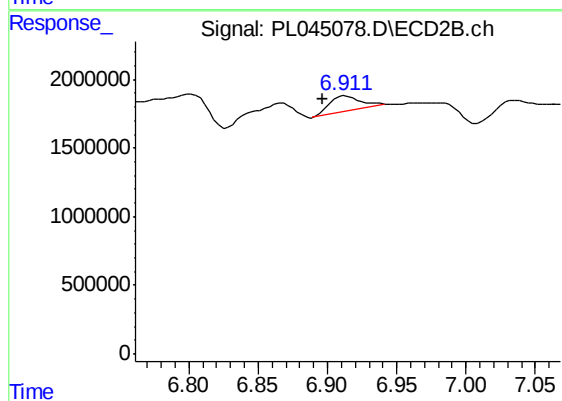

#15 Endosulfan II


R.T.: 6.913 min
Delta R.T.: 0.016 min
Response: 1890809
Conc: 0.82 ng/ml

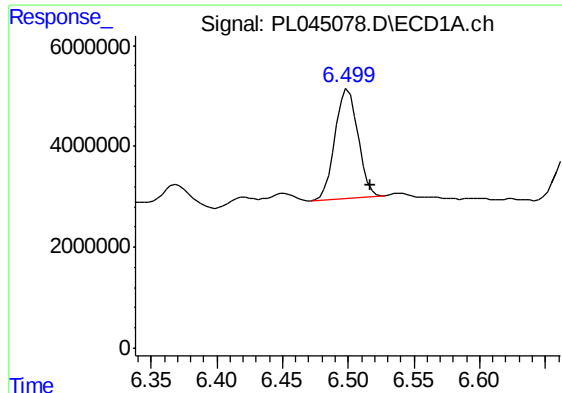

#19 Endosulfan Sulfate


R.T.: 6.500 min
Delta R.T.: -0.017 min
Response: 26240213
Conc: 3.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-23

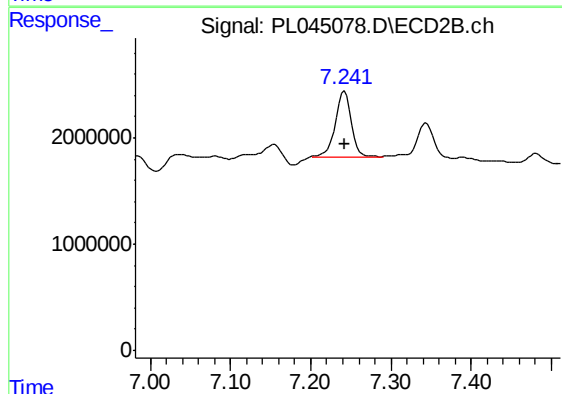


#19 Endosulfan Sulfate

R.T.: 7.242 min
Delta R.T.: 0.000 min
Response: 8675600
Conc: 4.11 ng/ml

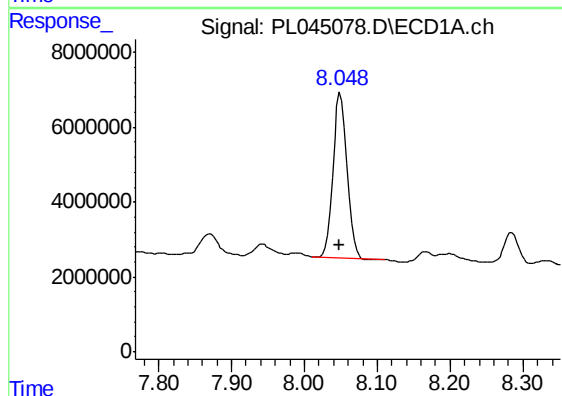

#28 Decachlorobiphenyl

R.T.: 8.050 min
Delta R.T.: 0.000 min
Response: 59103047
Conc: 8.10 ng/ml

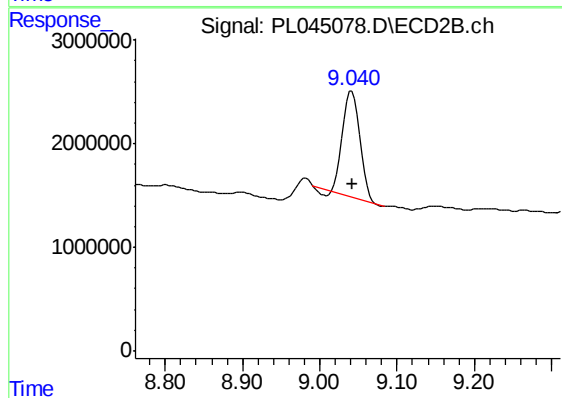

#28 Decachlorobiphenyl

R.T.: 9.042 min
Delta R.T.: -0.001 min
Response: 16091663
Conc: 7.27 ng/ml