

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022519\
 Data File : PL045095.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Feb 2019 23:56
 Operator : AJ\SJ
 Sample : K1595-06
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-E-WALL-GRADE-BEAM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 26 03:29:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 07 01:39:50 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.366	3.984	131.0E6	41391583	18.409	17.620
28)	SA Decachlor...	8.050	9.042	148.1E6	44580787	20.300	20.128

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022519\
Data File : PL045095.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Feb 2019 23:56
Operator : AJ\SJ
Sample : K1595-06
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-E-WALL-GRADE-BEAM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 26 03:29:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
Quant Title : GC Extractables
QLast Update : Thu Feb 07 01:39:50 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

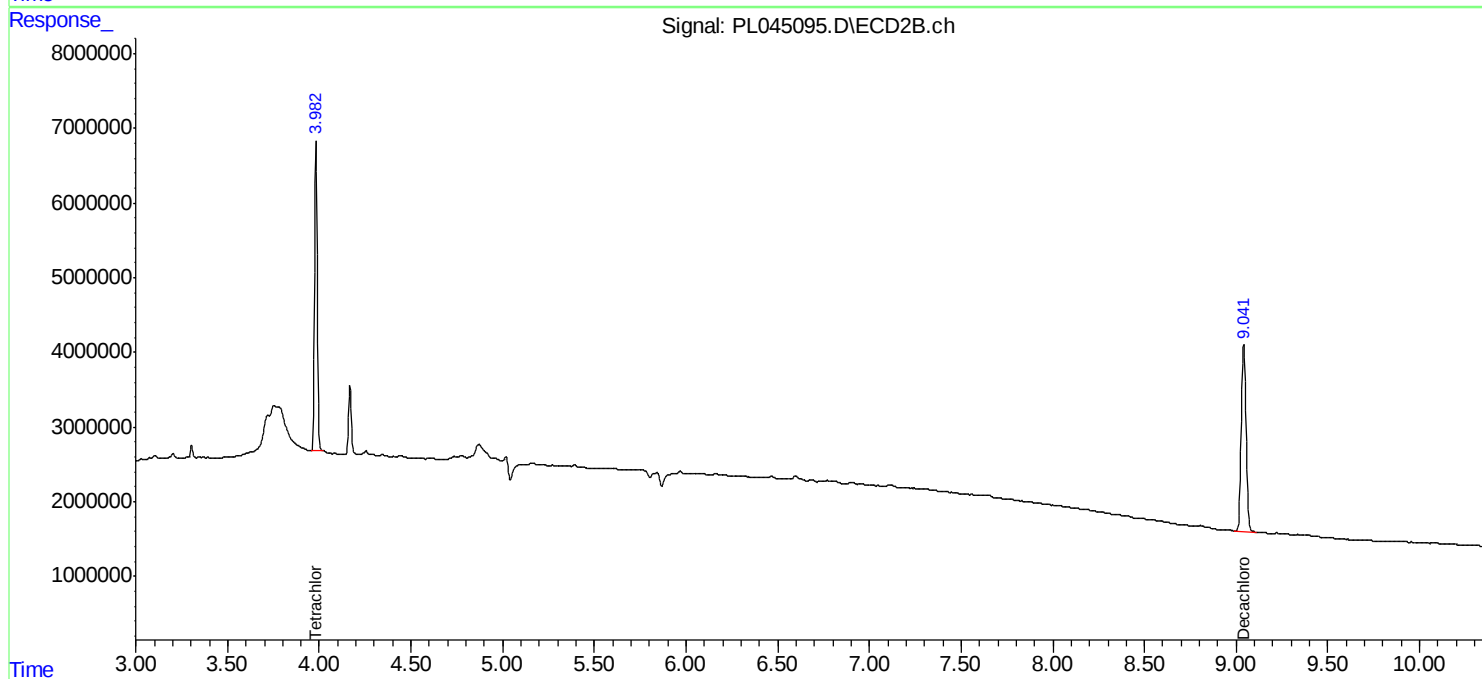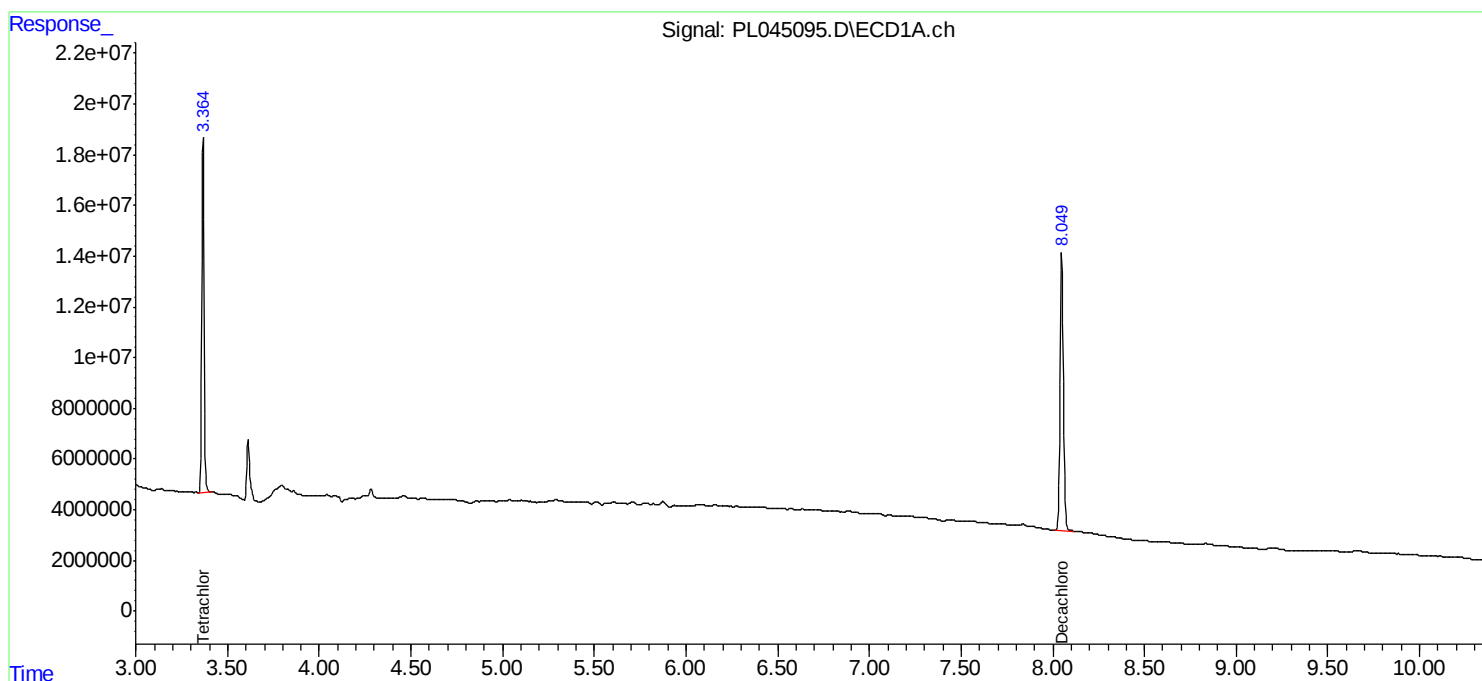


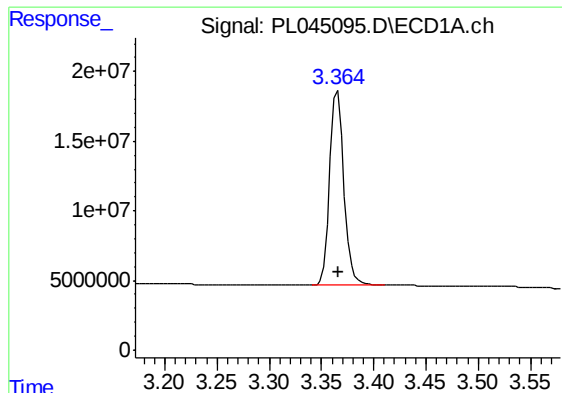

#1 Tetrachloro-m-xylene


R.T.: 3.366 min
Delta R.T.: 0.000 min
Response: 130994586
Conc: 18.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-E-WALL-GRADE-BEAM

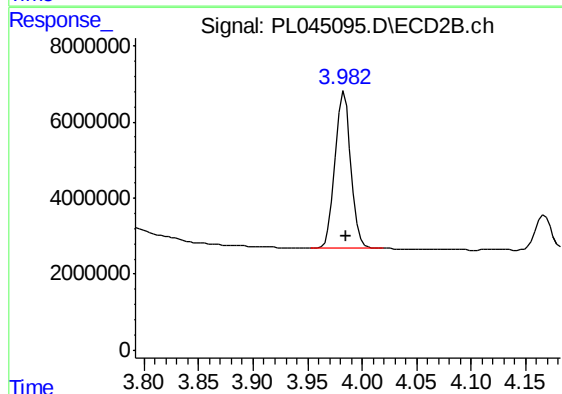


#1 Tetrachloro-m-xylene

R.T.: 3.984 min
Delta R.T.: -0.001 min
Response: 41391583
Conc: 17.62 ng/ml

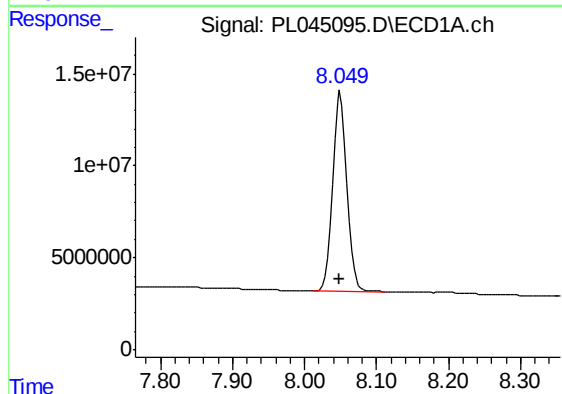

#28 Decachlorobiphenyl

R.T.: 8.050 min
Delta R.T.: 0.000 min
Response: 148060601
Conc: 20.30 ng/ml

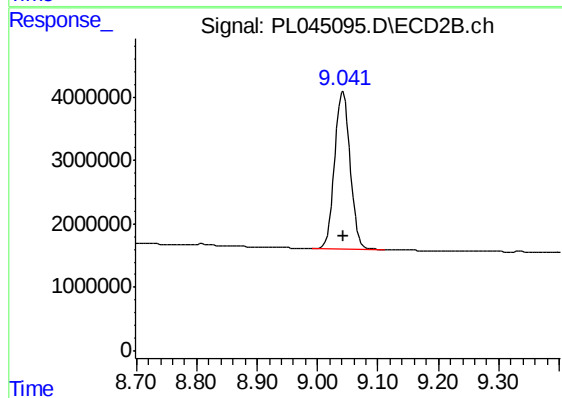

#28 Decachlorobiphenyl

R.T.: 9.042 min
Delta R.T.: 0.000 min
Response: 44580787
Conc: 20.13 ng/ml