

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022520\
 Data File : PL056807.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Feb 2020 10:41
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 26 04:32:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021920.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 20 02:32:45 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

8) B	Heptachlo...	0.000	5.899	0	21320634	N.D.	7.292 #
9) A	Endosulfan I	5.555	0.000	77837793	0	5.823	N.D. #
12) B	4,4'-DDE	5.685f	0.000	85664998	0	6.090	N.D. #
13) MA	Dieldrin	5.782	0.000	91869464	0	6.164	N.D. #
14) MA	Endrin	6.063	6.720	15622886	11304156	1.157	4.589 #
15) B	Endosulfa...	6.306f	0.000	69771291	0	5.618	N.D. #
17) MA	4,4'-DDT	6.425	0.000	105.7E6	0	9.708	N.D. #
27)	Chlordane-5	6.306f	0.000	69771291	0	213.083	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022520\
Data File : PL056807.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Feb 2020 10:41
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 26 04:32:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021920.M
Quant Title : GC Extractables
QLast Update : Thu Feb 20 02:32:45 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

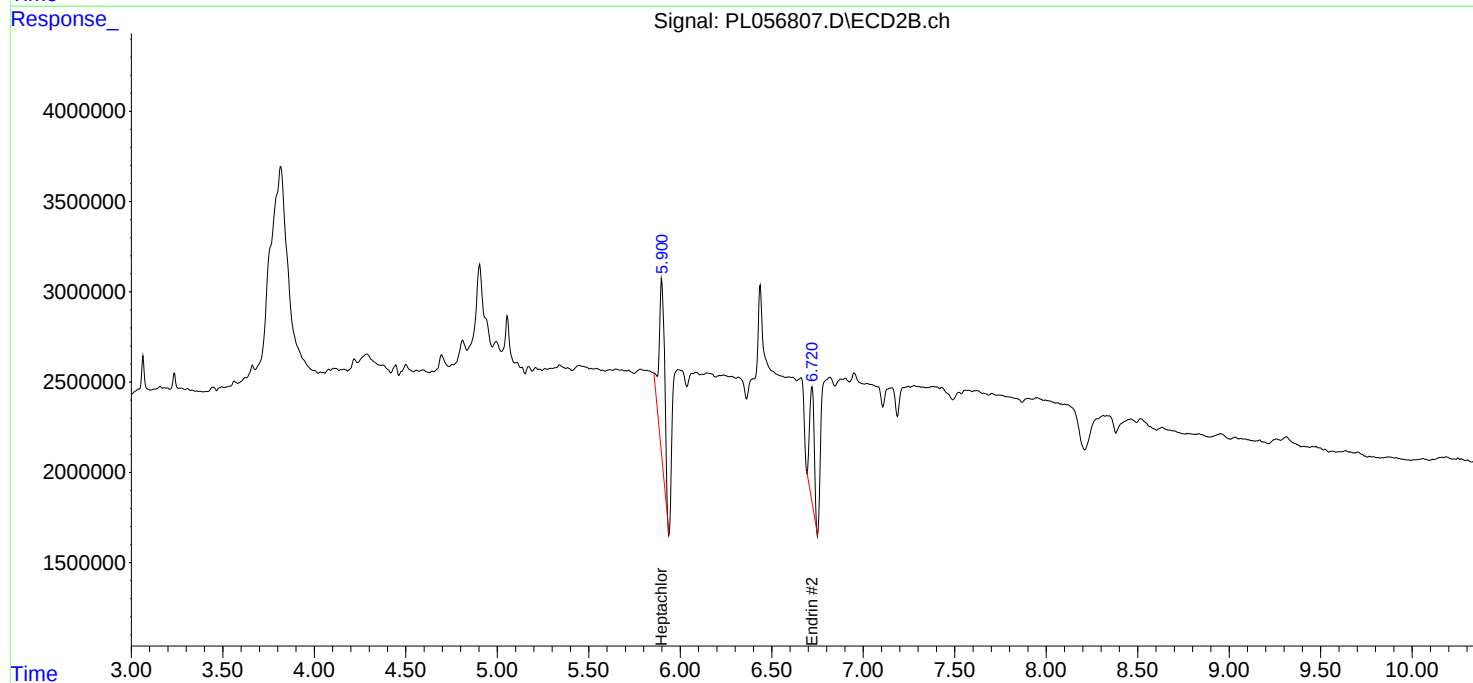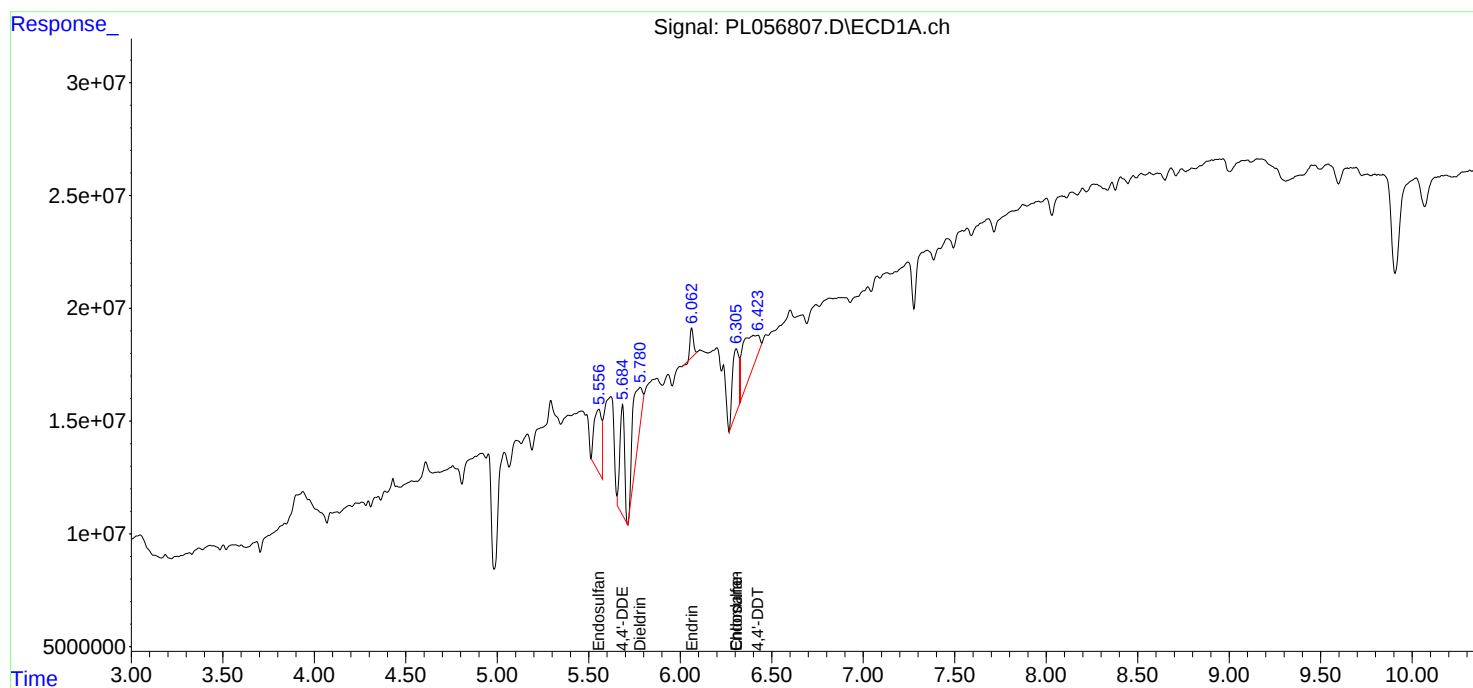


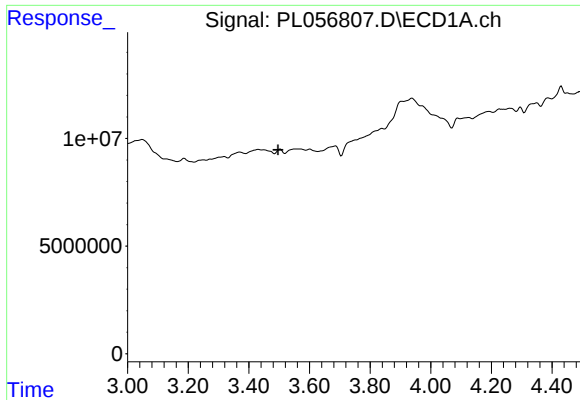

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.496 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

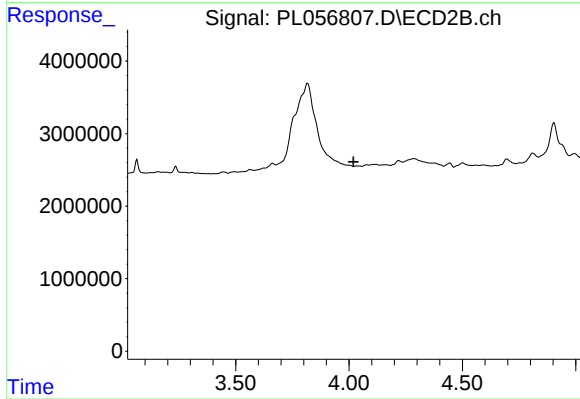


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.020 min
Response: 0
Conc: N.D.

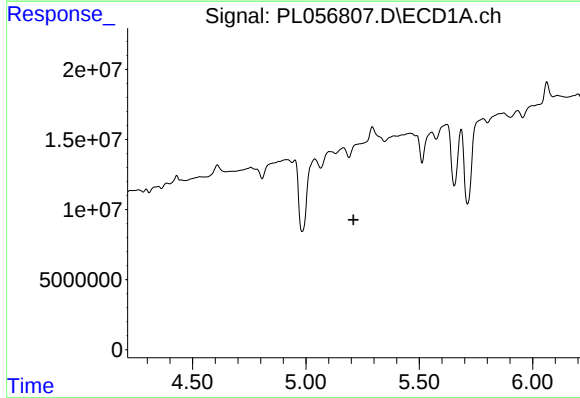


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.210 min
Response: 0
Conc: N.D.

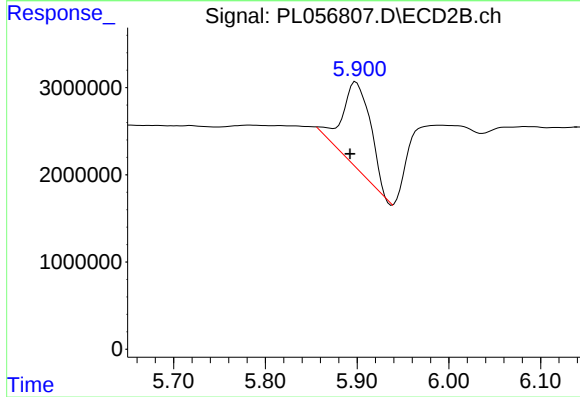

#8 Heptachlor epoxide


R.T.: 5.899 min
Delta R.T.: 0.006 min
Response: 21320634
Conc: 7.29 ng/ml

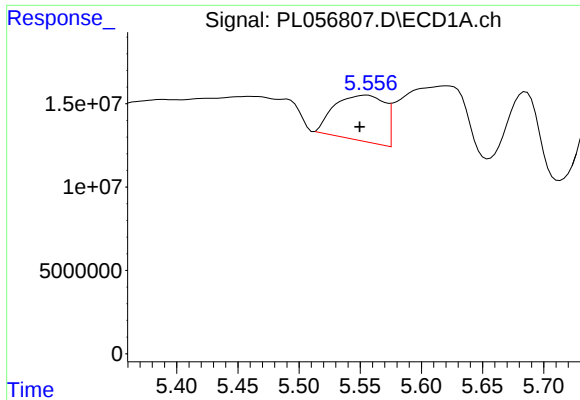

#9 Endosulfan I


R.T.: 5.555 min
Delta R.T.: 0.006 min
Response: 77837793
Conc: 5.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

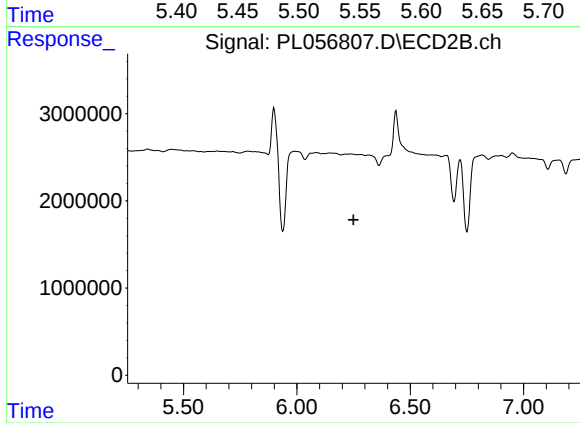


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.250 min
Response: 0
Conc: N.D.

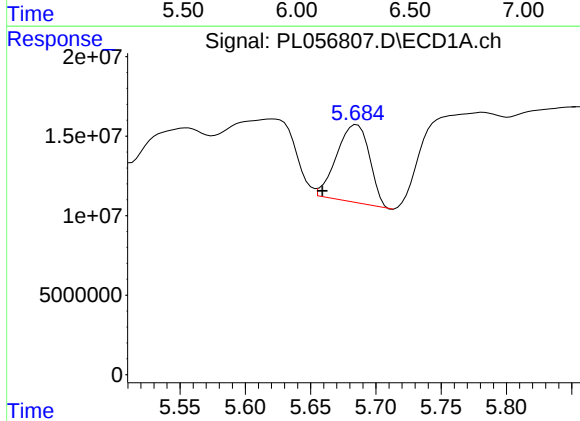


#12 4,4'-DDE

R.T.: 5.685 min
Delta R.T.: 0.026 min
Response: 85664998
Conc: 6.09 ng/ml

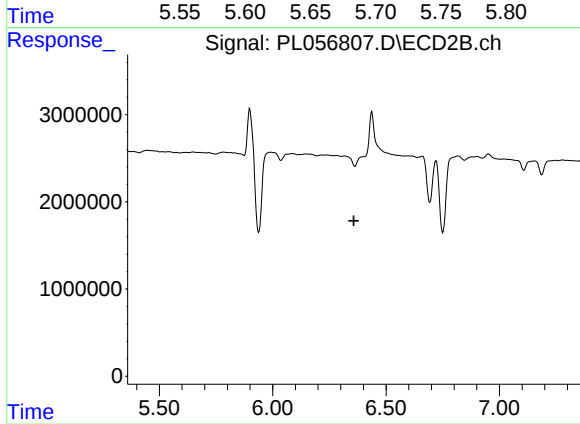

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T. : 6.358 min
Response: 0
Conc: N.D.

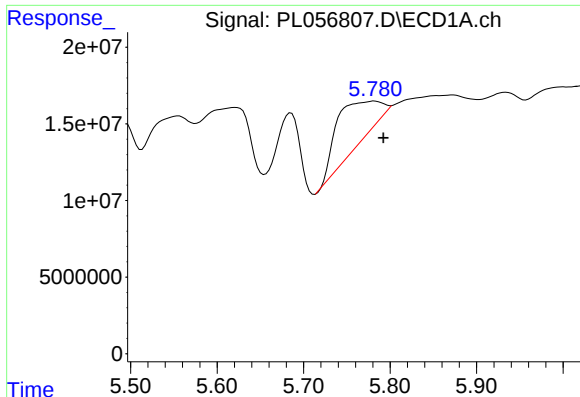

#13 Dieldrin


R.T.: 5.782 min
Delta R.T.: -0.010 min
Response: 91869464
Conc: 6.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

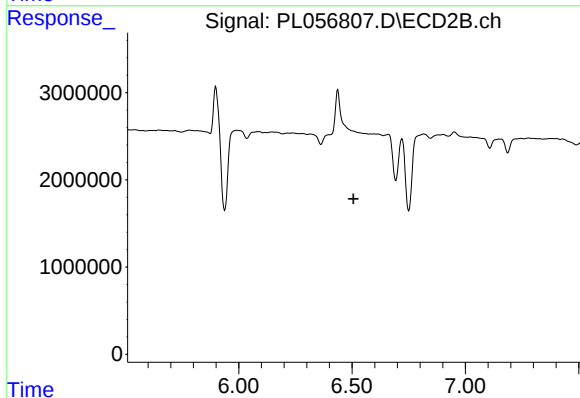


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.506 min
Response: 0
Conc: N.D.

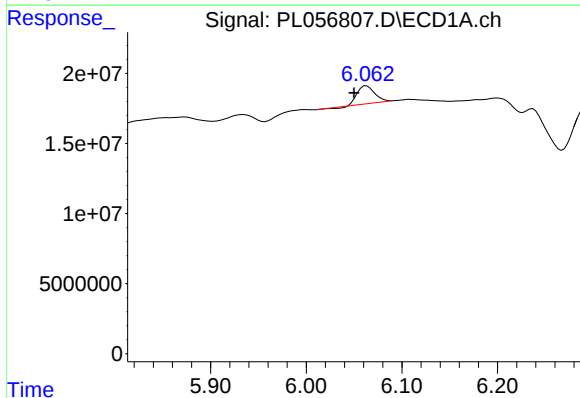


#14 Endrin

R.T.: 6.063 min
Delta R.T.: 0.013 min
Response: 15622886
Conc: 1.16 ng/ml

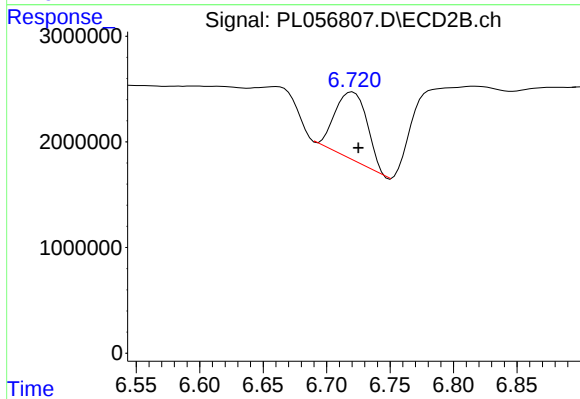

#14 Endrin


R.T.: 6.720 min
Delta R.T.: -0.005 min
Response: 11304156
Conc: 4.59 ng/ml

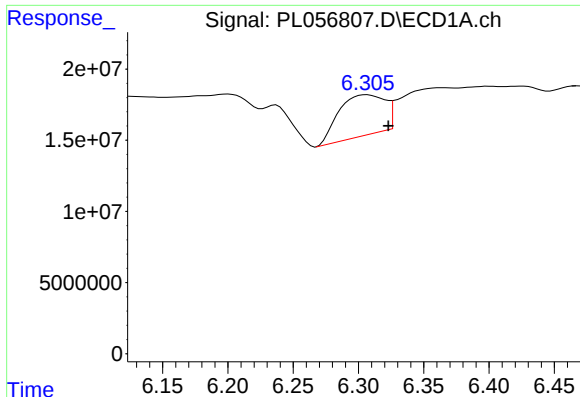

#15 Endosulfan II


R.T.: 6.306 min
Delta R.T.: -0.017 min
Response: 69771291
Conc: 5.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

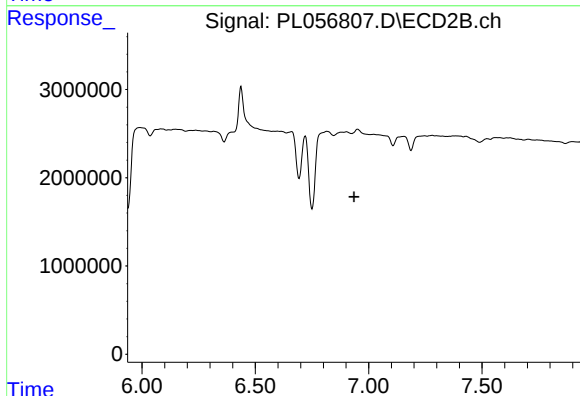


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.936 min
Response: 0
Conc: N.D.

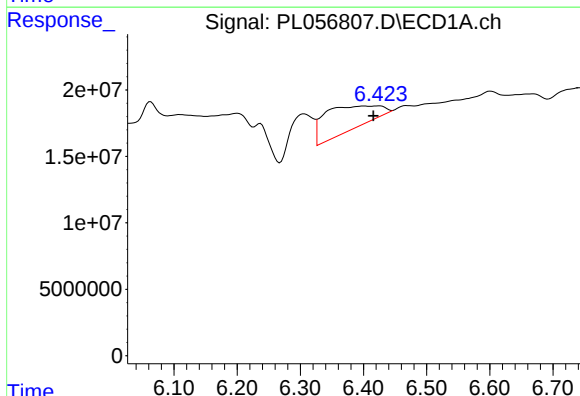


#17 4,4'-DDT

R.T.: 6.425 min
Delta R.T.: 0.009 min
Response: 105726256
Conc: 9.71 ng/ml

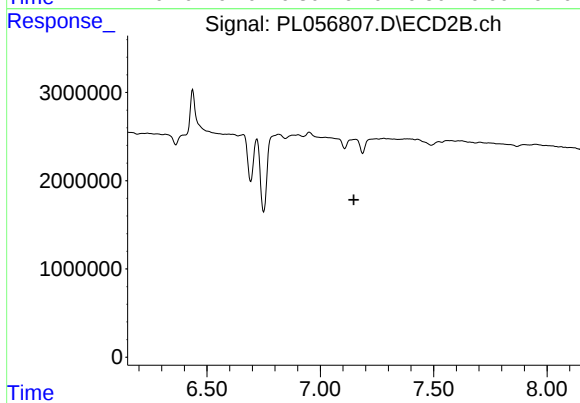

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 7.148 min
Response: 0
Conc: N.D.

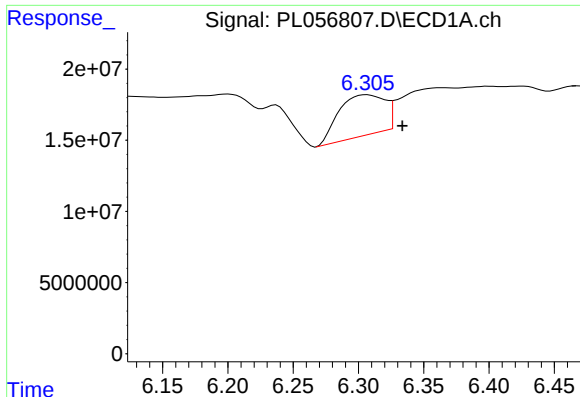

#27 Chlordane-5


R.T.: 6.306 min
Delta R.T.: -0.027 min
Response: 69771291
Conc: 213.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

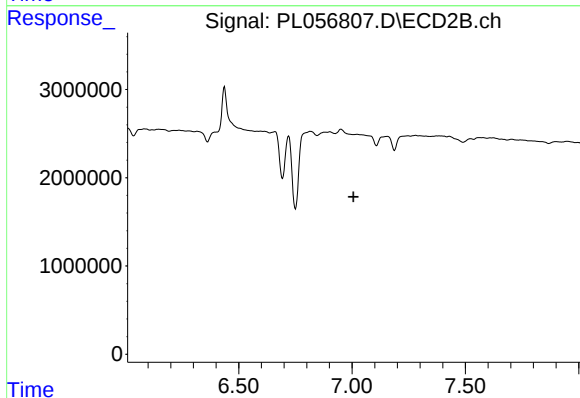


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.007 min
Response: 0
Conc: N.D.

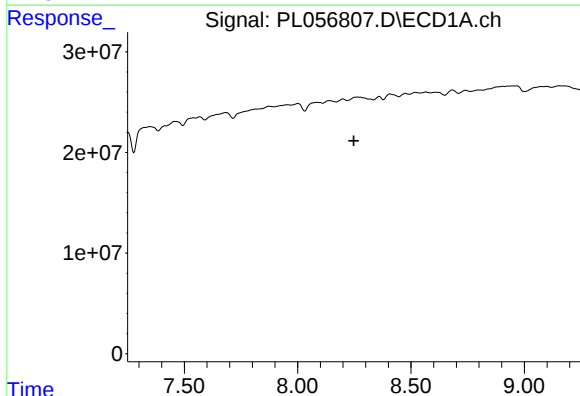

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.248 min
Response: 0
Conc: N.D.

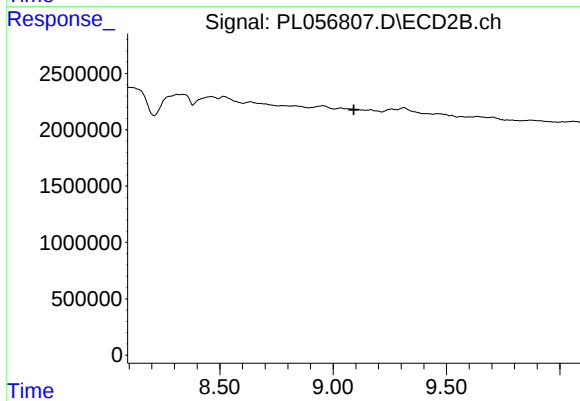

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.091 min
Response: 0
Conc: N.D.