

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022521\
 Data File : PL064942.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Feb 2021 11:03
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 24 15:45:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 09 04:41:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

6) B	beta-BHC	4.400	0.000	2900996	0	1.697	N.D.	#
8) B	Heptachlo...	0.000	6.001	0	15507227	N.D.	7.029	#
9) A	Endosulfan I	5.484f	0.000	1971044	0	0.615	N.D.	#
14) MA	Endrin	5.959	0.000	22535167	0	7.503	N.D.	#
15) B	Endosulfa...	6.210f	0.000	3387624	0	1.176	N.D.	#
23)	Chlordane-1	4.306f	0.000	5152942	0	45.330	N.D.	#
24)	Chlordane-2	4.798f	0.000	18336369	0	148.196	N.D.	#
27)	Chlordane-5	6.246	0.000	1640630	0	16.215	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022521\
Data File : PL064942.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Feb 2021 11:03
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 24 15:45:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
Quant Title : GC Extractables
QLast Update : Tue Feb 09 04:41:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

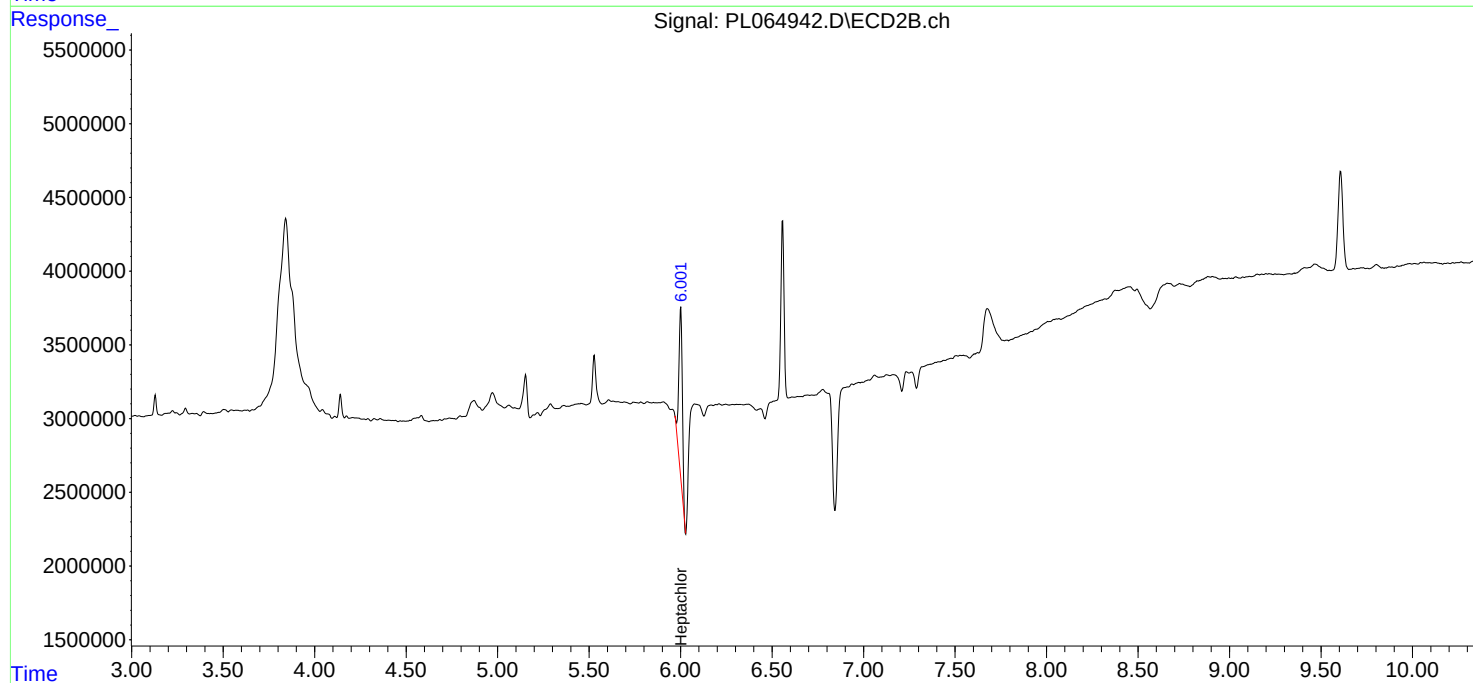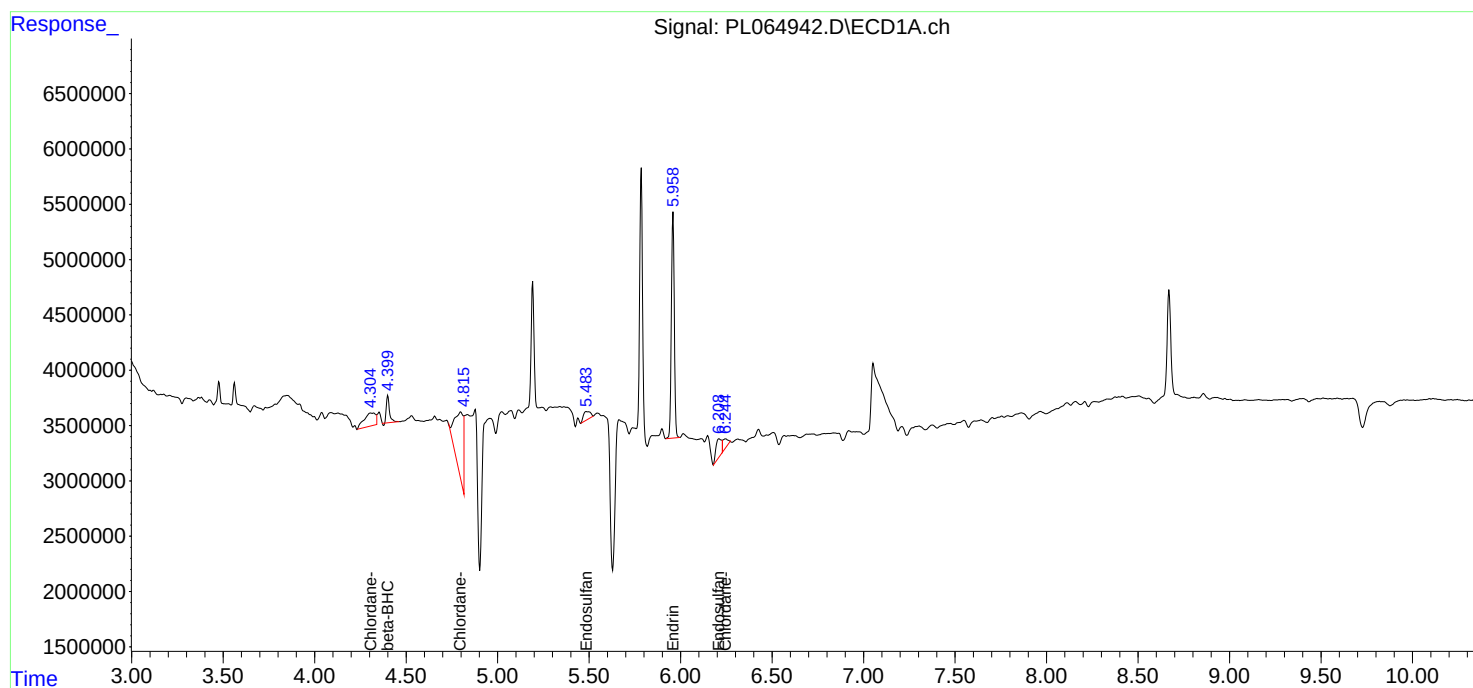


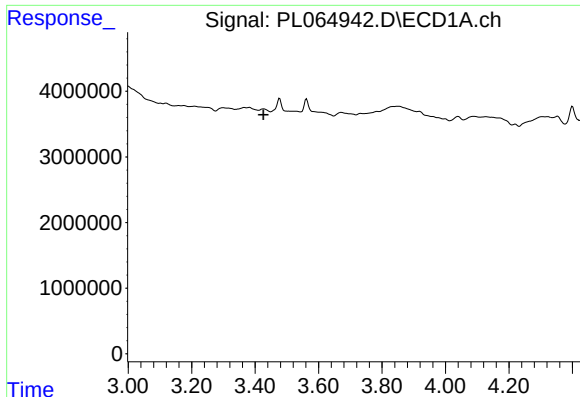

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.426 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

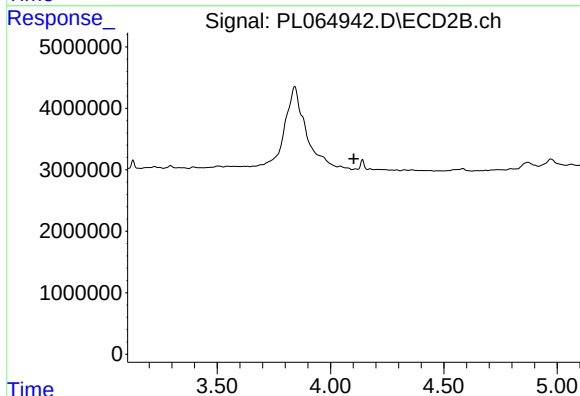


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 4.102 min
Response: 0
Conc: N.D.

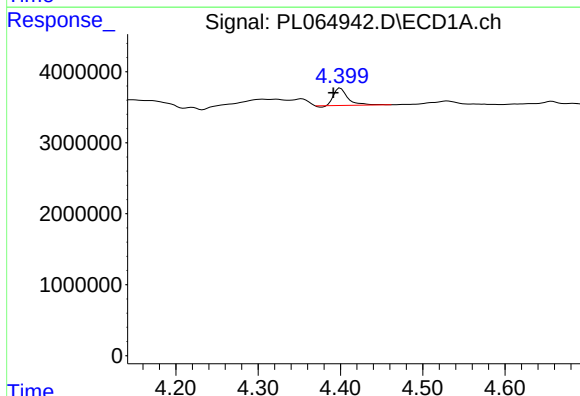


#6 beta-BHC

R.T.: 4.400 min
Delta R.T.: 0.009 min
Response: 2900996
Conc: 1.70 ng/ml

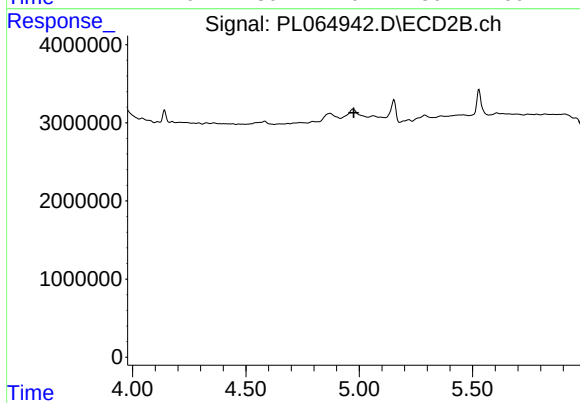

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.976 min
Response: 0
Conc: N.D.

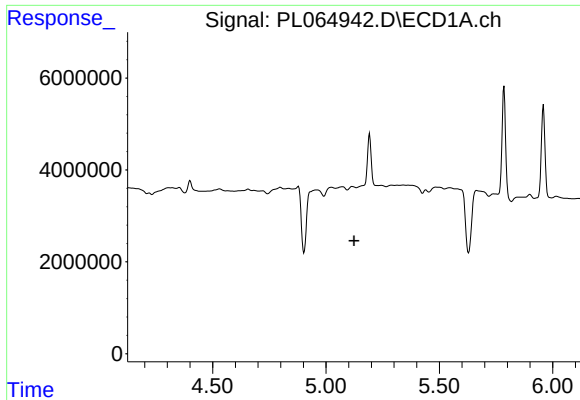

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.123 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

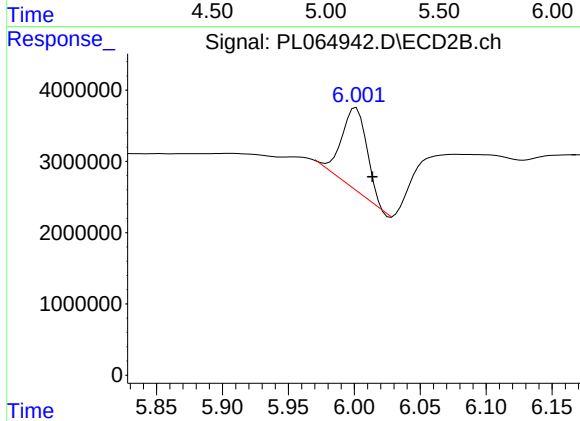


#8 Heptachlor epoxide

R.T.: 6.001 min
Delta R.T.: -0.012 min
Response: 15507227
Conc: 7.03 ng/ml

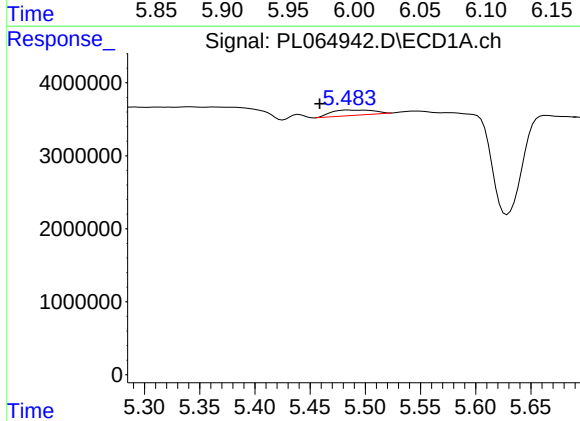


#9 Endosulfan I

R.T.: 5.484 min
Delta R.T.: 0.026 min
Response: 1971044
Conc: 0.61 ng/ml

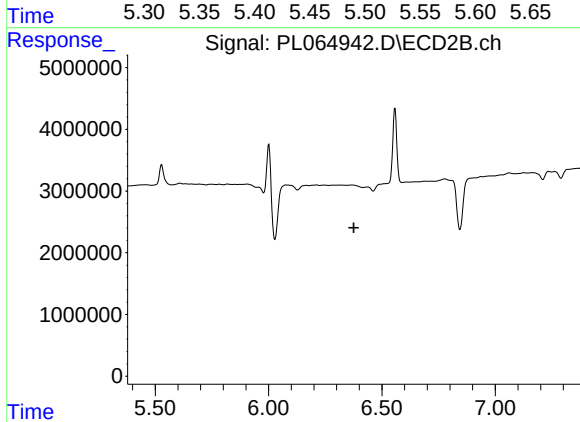

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.376 min
Response: 0
Conc: N.D.

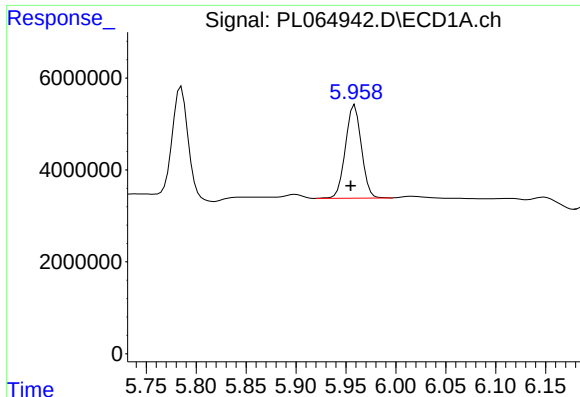

#14 Endrin


R.T.: 5.959 min
Delta R.T.: 0.004 min
Response: 22535167
Conc: 7.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

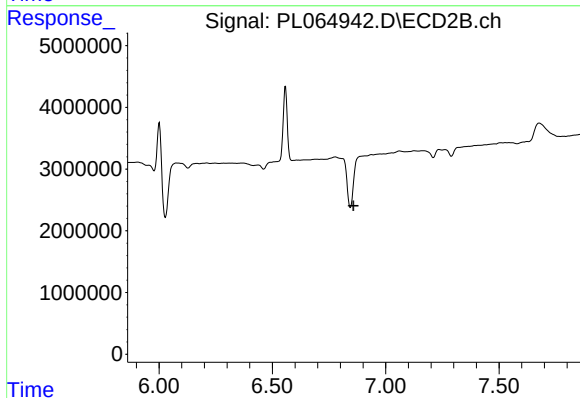


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.858 min
Response: 0
Conc: N.D.

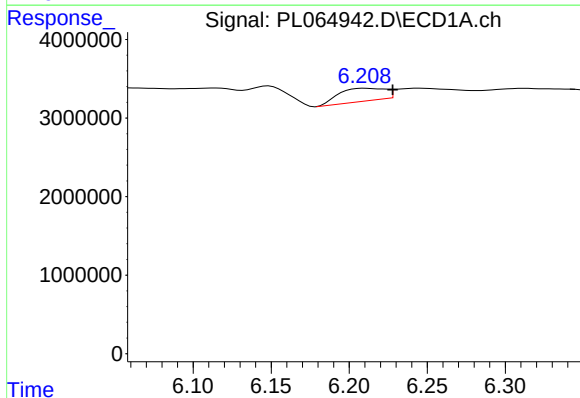


#15 Endosulfan II

R.T.: 6.210 min
Delta R.T.: -0.018 min
Response: 3387624
Conc: 1.18 ng/ml

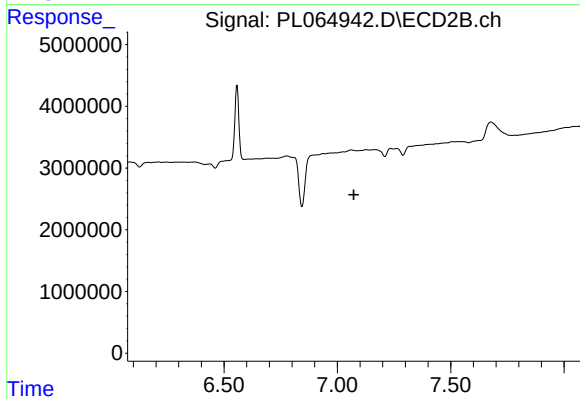

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 7.073 min
Response: 0
Conc: N.D.

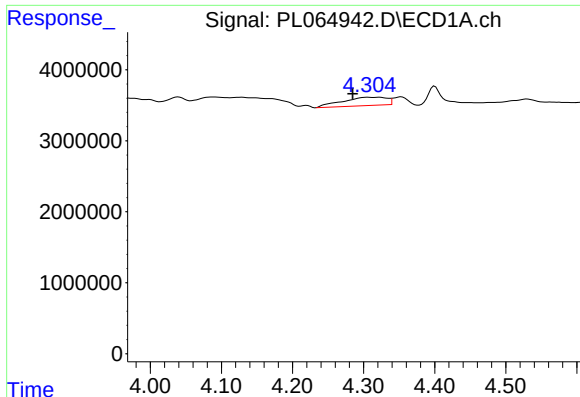

#23 Chlordane-1


R.T.: 4.306 min
Delta R.T.: 0.021 min
Response: 5152942
Conc: 45.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

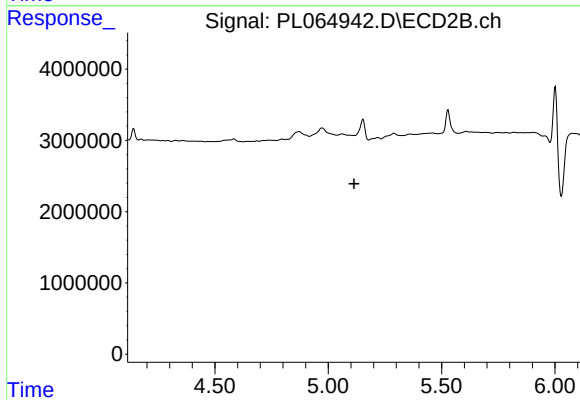


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.114 min
Response: 0
Conc: N.D.

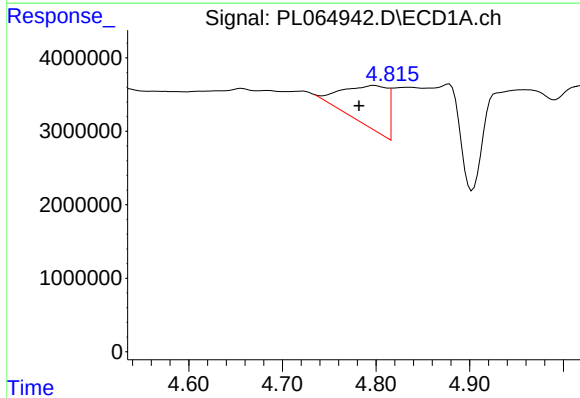


#24 Chlordane-2

R.T.: 4.798 min
Delta R.T.: 0.016 min
Response: 18336369
Conc: 148.20 ng/ml

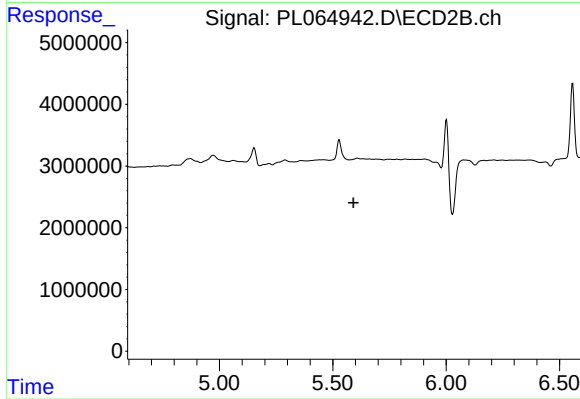

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.592 min
Response: 0
Conc: N.D.

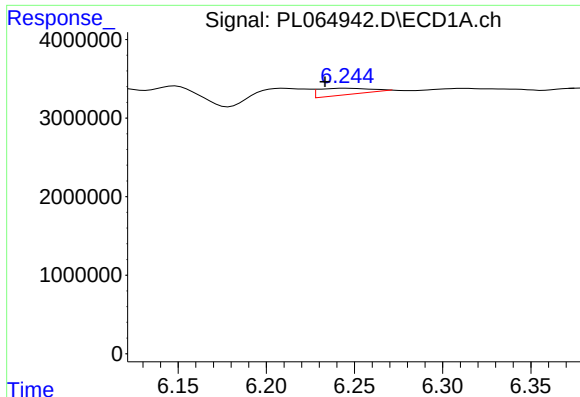

#27 Chlordane-5


R.T.: 6.246 min
Delta R.T.: 0.013 min
Response: 1640630
Conc: 16.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

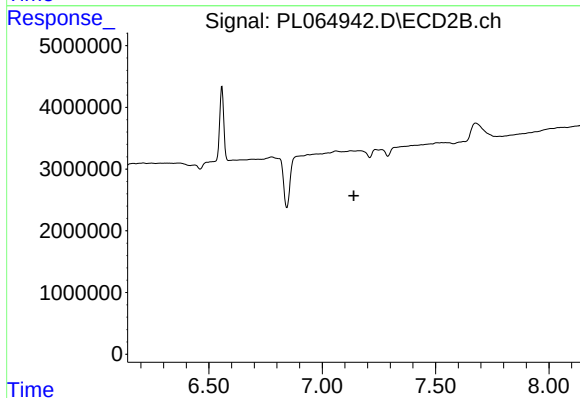


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.139 min
Response: 0
Conc: N.D.

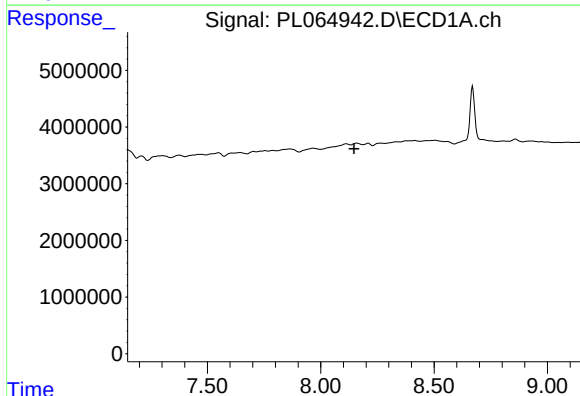

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.148 min
Response: 0
Conc: N.D.

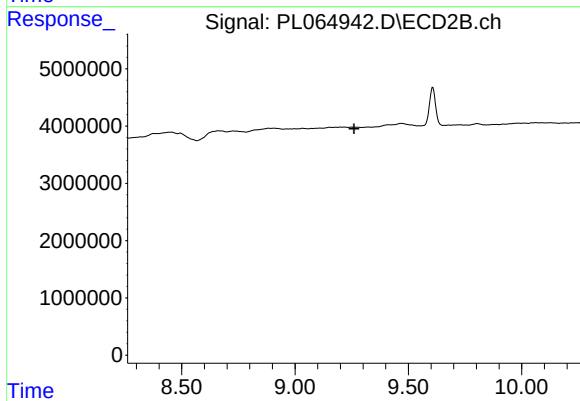

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.261 min
Response: 0
Conc: N.D.