

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022521\
 Data File : PL064943.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Feb 2021 11:17
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 24 15:45:55 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 09 04:41:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.423	4.098	65159231	54149536	23.159	25.067
28)	SA Decachlor...	8.142	9.254	59407186	46012067	26.417	24.225
Target Compounds							
6)	B beta-BHC	0.000	4.974	0	5086949	N.D.	0.157 #
23)	Chlordane-1	4.309f	0.000	1473856	0	12.965	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022521\
Data File : PL064943.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Feb 2021 11:17
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 24 15:45:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
Quant Title : GC Extractables
QLast Update : Tue Feb 09 04:41:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

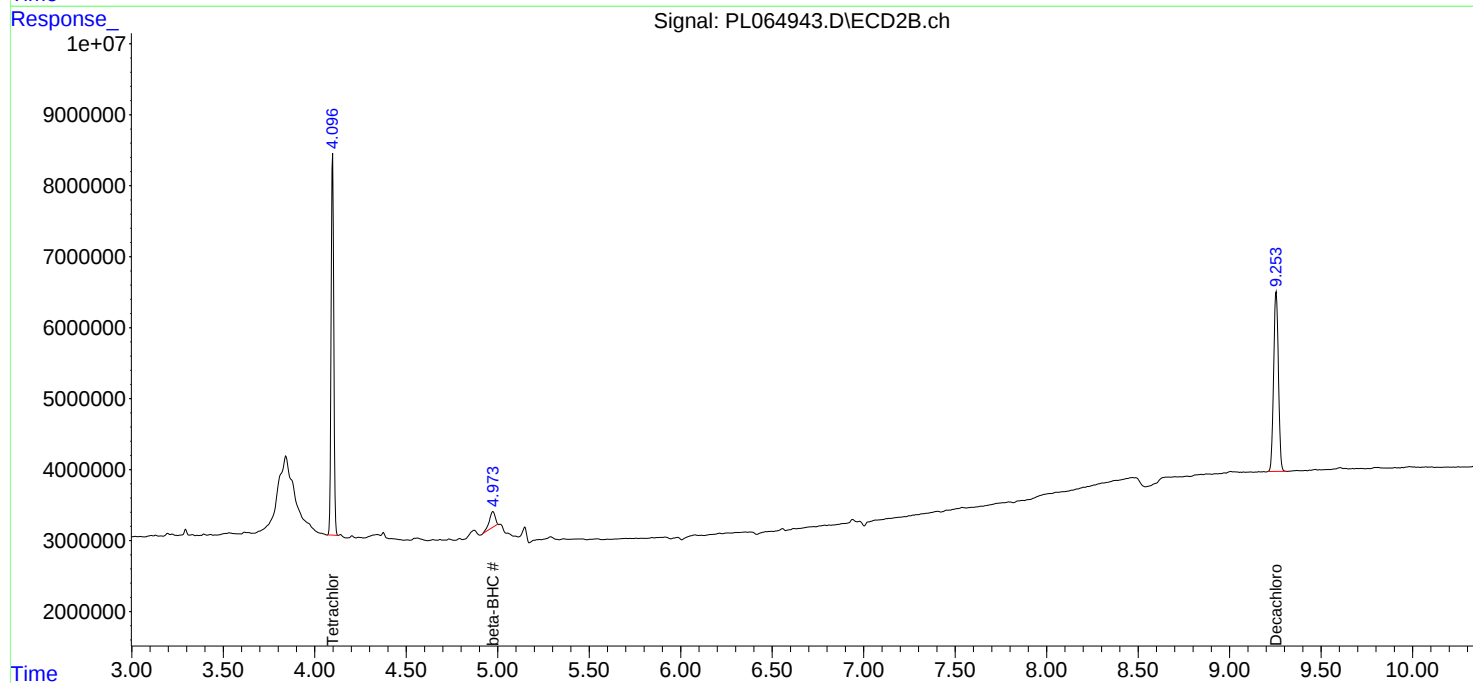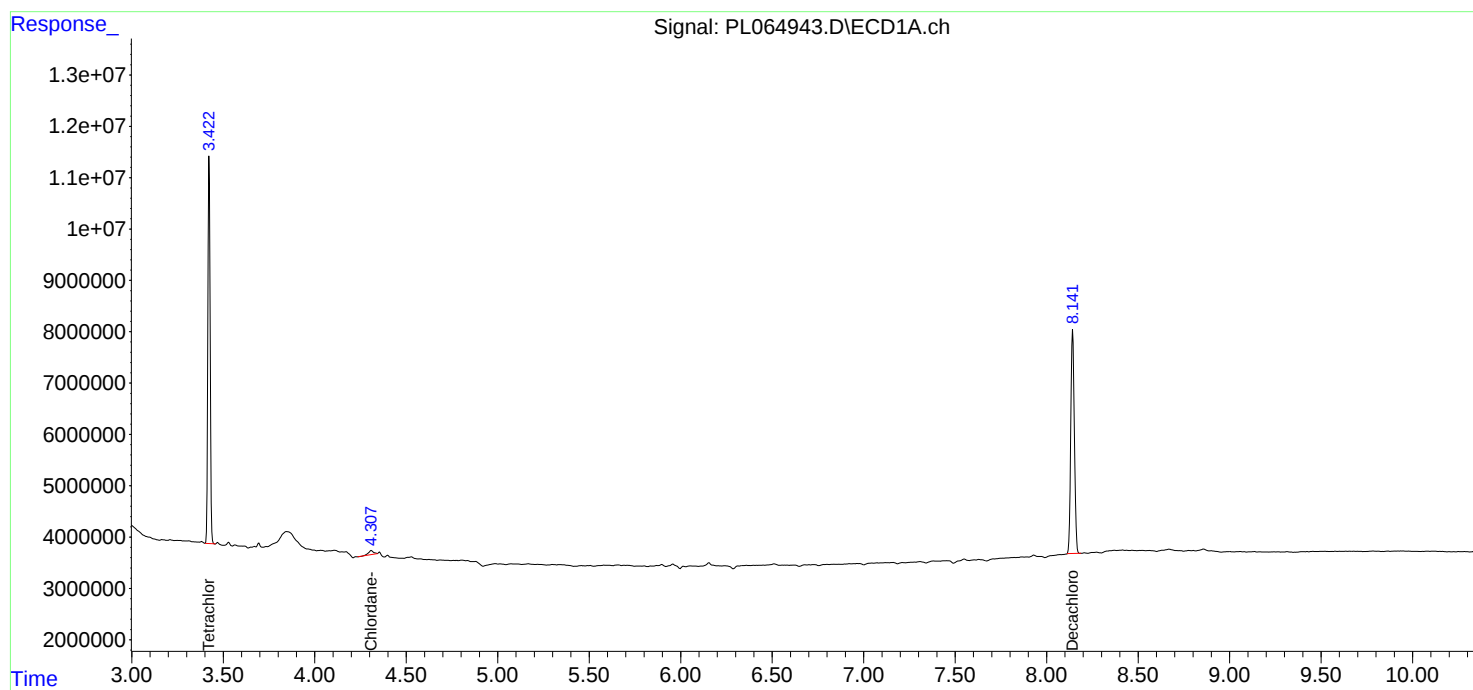


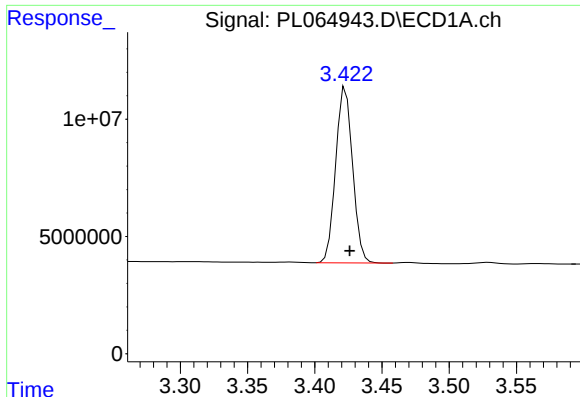

#1 Tetrachloro-m-xylene


R.T.: 3.423 min
Delta R.T.: -0.003 min
Response: 65159231
Conc: 23.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

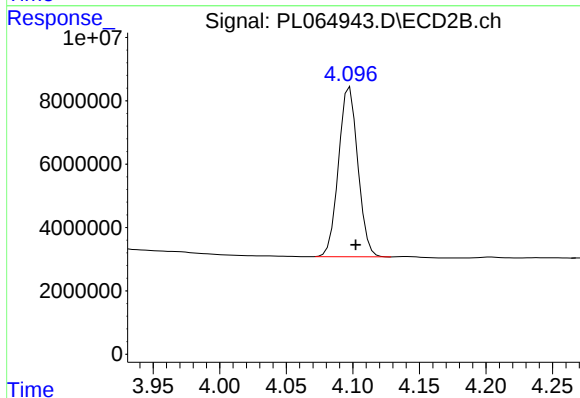


#1 Tetrachloro-m-xylene

R.T.: 4.098 min
Delta R.T.: -0.004 min
Response: 54149536
Conc: 25.07 ng/ml

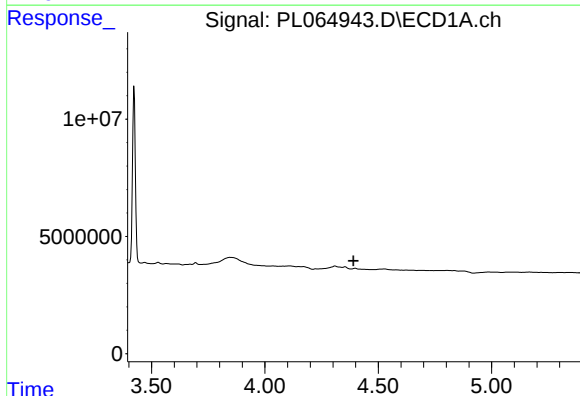


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.391 min
Response: 0
Conc: N.D.

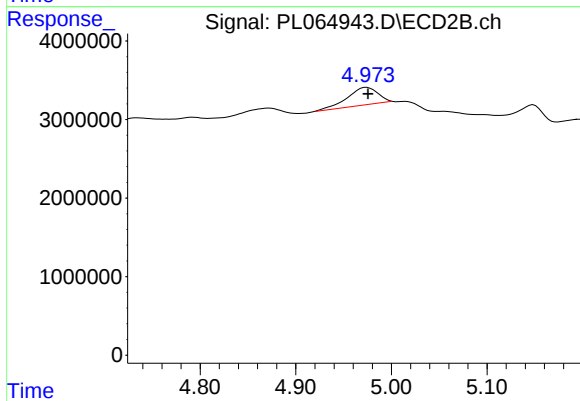

#6 beta-BHC


R.T.: 4.974 min
Delta R.T.: -0.001 min
Response: 5086949
Conc: 0.16 ng/ml

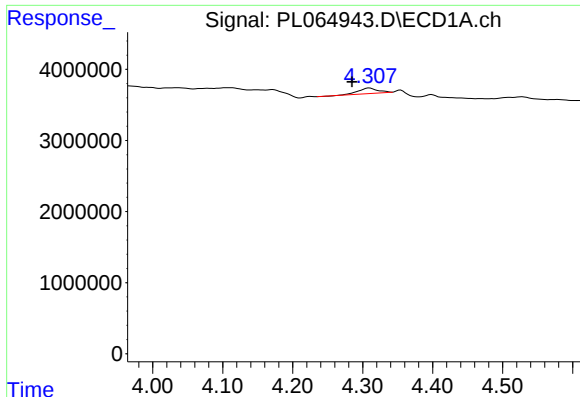

#23 Chlordane-1


R.T.: 4.309 min
Delta R.T.: 0.025 min
Response: 1473856
Conc: 12.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

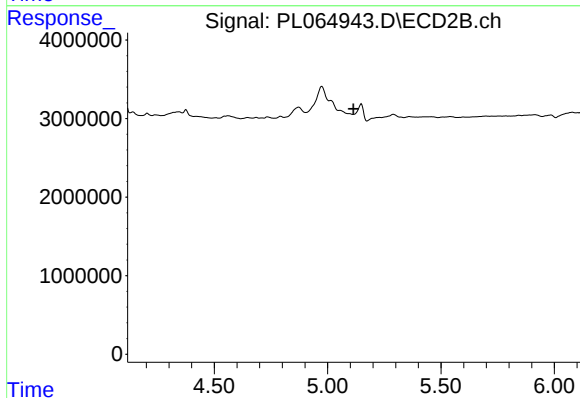


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.114 min
Response: 0
Conc: N.D.

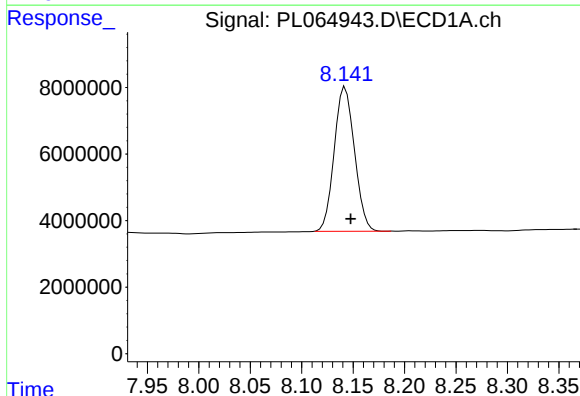

#28 Decachlorobiphenyl

R.T.: 8.142 min
Delta R.T.: -0.006 min
Response: 59407186
Conc: 26.42 ng/ml

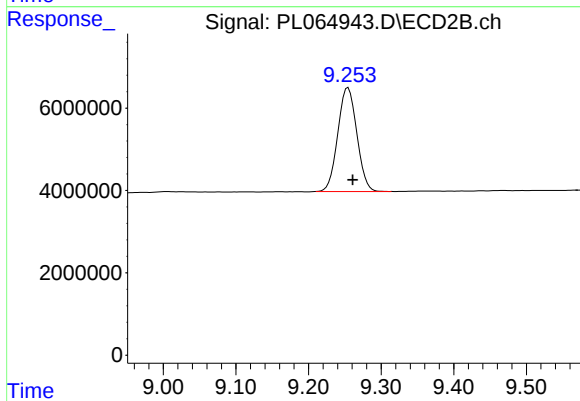

#28 Decachlorobiphenyl

R.T.: 9.254 min
Delta R.T.: -0.006 min
Response: 46012067
Conc: 24.22 ng/ml