

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022521\
 Data File : PL064951.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Feb 2021 13:37
 Operator : AR\AJ
 Sample : M1469-0110X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TR-08-022321

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 24 15:47:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 09 04:41:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.423	4.098	7964807	5630031	2.831	2.606
28)	SA Decachlor...	8.142	9.257	5384258	3673160	2.394	1.934
Target Compounds							
9)	A Endosulfan I	5.475f	0.000	2847571	0	0.888	N.D. #
13)	MA Dieldrin	5.694	0.000	2252882	0	0.687	N.D. #
20)	A Methoxychlor	6.897f	0.000	1403406	0	1.084	N.D. #
23)	Chlordane-1	4.296	0.000	2158637	0	18.989	N.D. #
24)	Chlordane-2	4.785	0.000	2291623	0	18.521	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022521\
Data File : PL064951.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Feb 2021 13:37
Operator : AR\AJ
Sample : M1469-0110X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TR-08-022321

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 24 15:47:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
Quant Title : GC Extractables
QLast Update : Tue Feb 09 04:41:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

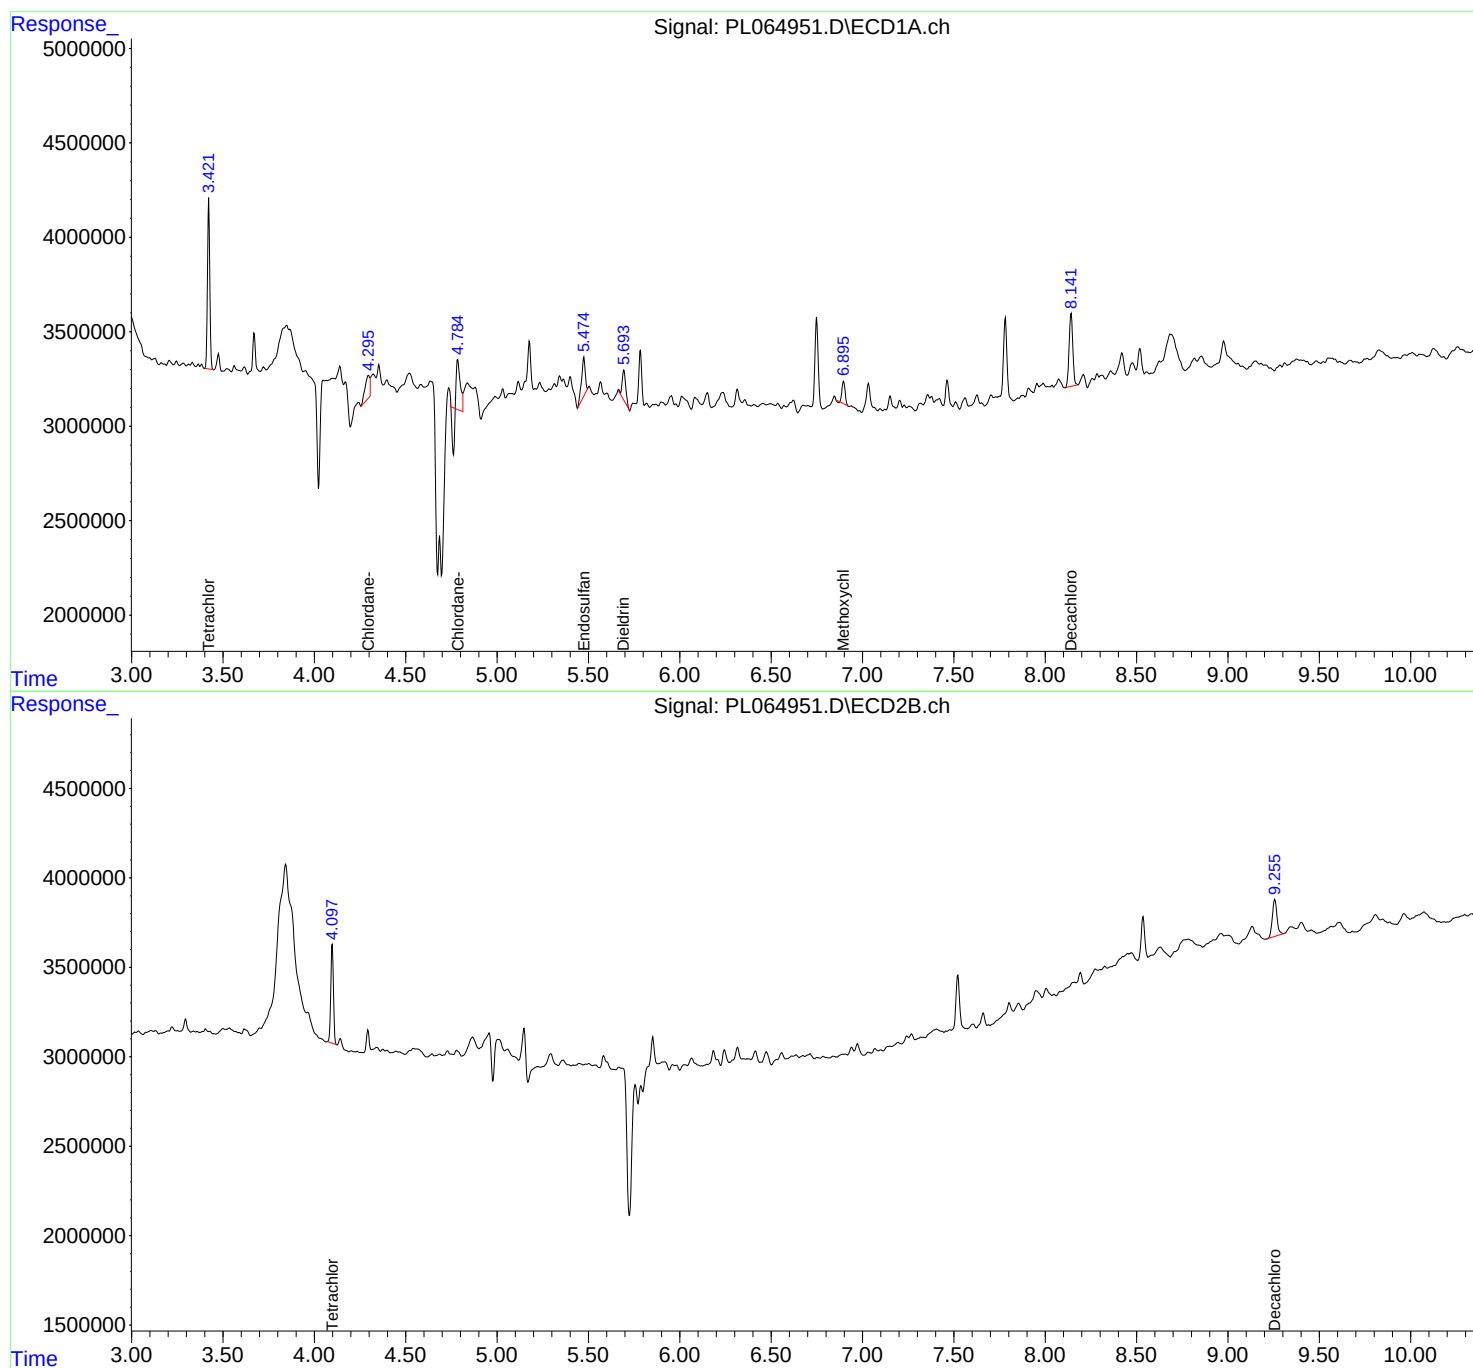


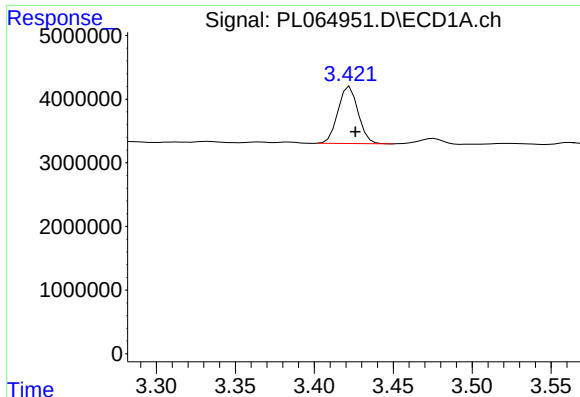

#1 Tetrachloro-m-xylene


R.T.: 3.423 min
Delta R.T.: -0.003 min
Response: 7964807
Conc: 2.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-08-022321

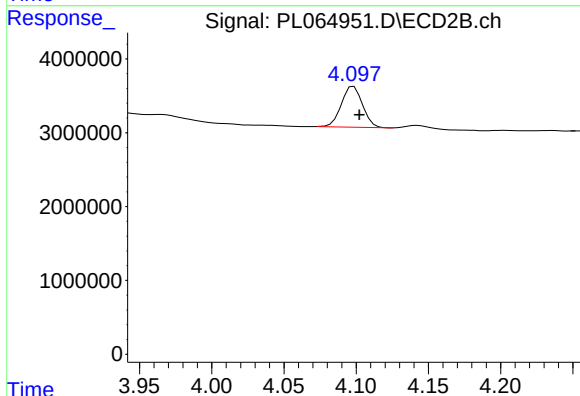


#1 Tetrachloro-m-xylene

R.T.: 4.098 min
Delta R.T.: -0.004 min
Response: 5630031
Conc: 2.61 ng/ml

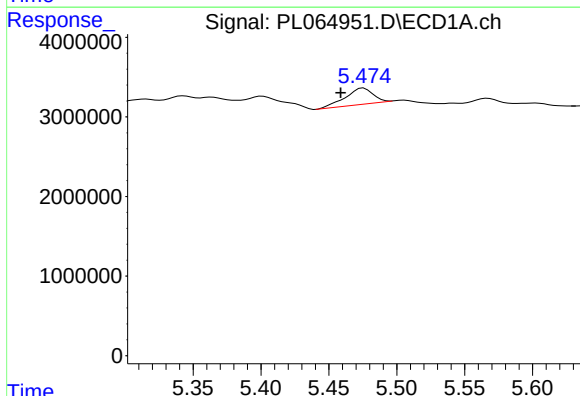


#9 Endosulfan I

R.T.: 5.475 min
Delta R.T.: 0.017 min
Response: 2847571
Conc: 0.89 ng/ml

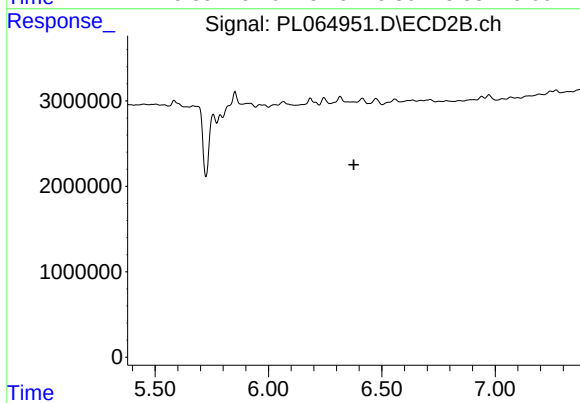

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.376 min
Response: 0
Conc: N.D.

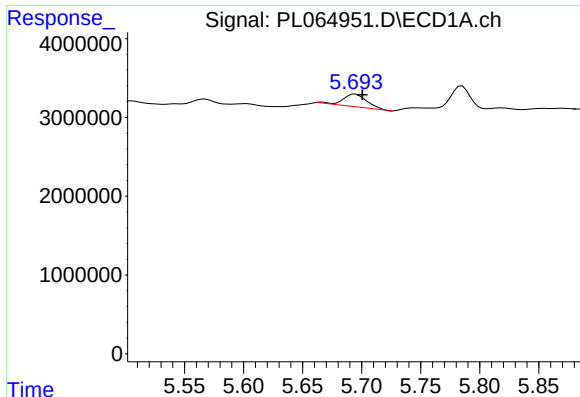

#13 Dieldrin


R.T.: 5.694 min
Delta R.T.: -0.006 min
Response: 2252882
Conc: 0.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-08-022321

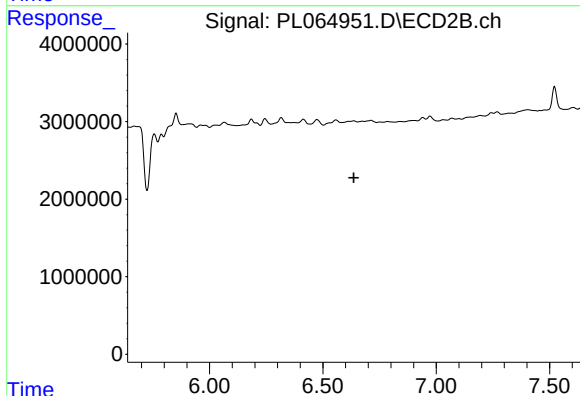


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.637 min
Response: 0
Conc: N.D.

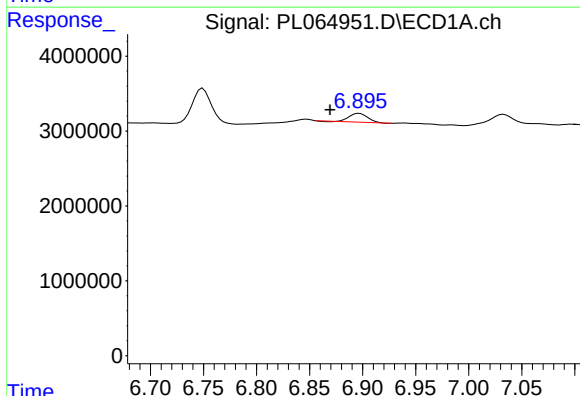


#20 Methoxychlor

R.T.: 6.897 min
Delta R.T.: 0.027 min
Response: 1403406
Conc: 1.08 ng/ml

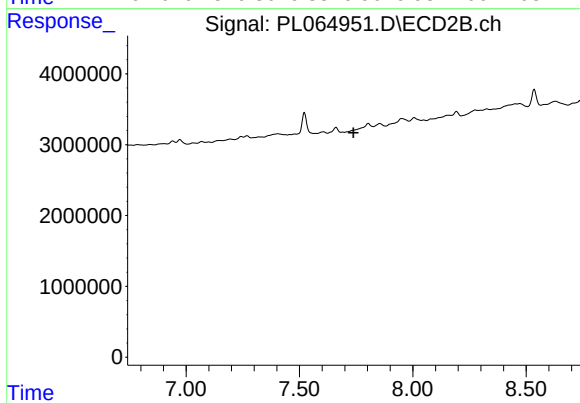

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.739 min
Response: 0
Conc: N.D.

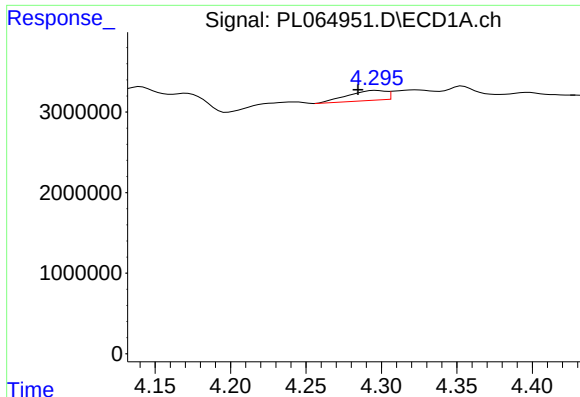

#23 Chlordane-1


R.T.: 4.296 min
Delta R.T.: 0.012 min
Response: 2158637
Conc: 18.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-08-022321

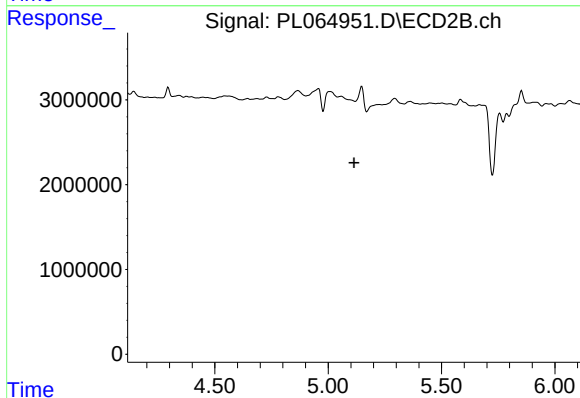


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.114 min
Response: 0
Conc: N.D.

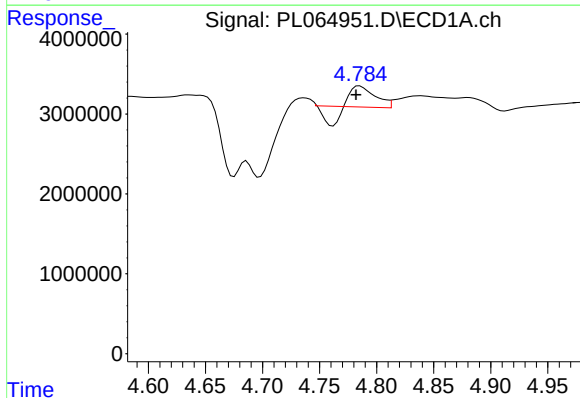


#24 Chlordane-2

R.T.: 4.785 min
Delta R.T.: 0.003 min
Response: 2291623
Conc: 18.52 ng/ml

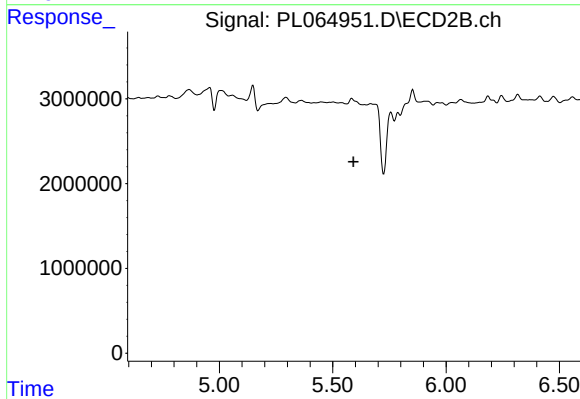

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.592 min
Response: 0
Conc: N.D.

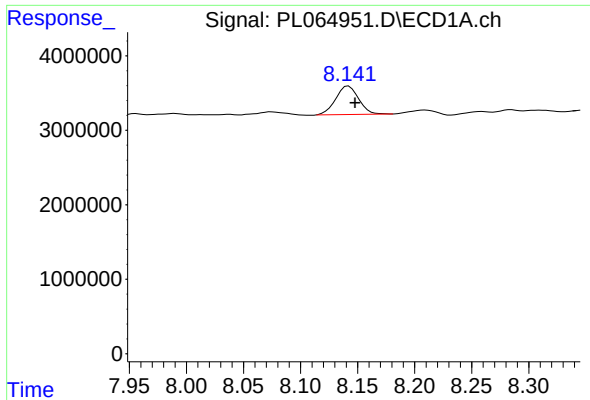

#28 Decachlorobiphenyl

R.T.: 8.142 min
Delta R.T.: -0.006 min
Response: 5384258
Conc: 2.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-08-022321

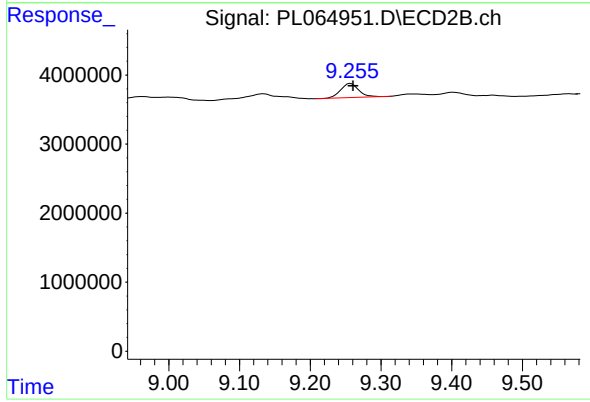

#28 Decachlorobiphenyl

R.T.: 9.257 min
Delta R.T.: -0.004 min
Response: 3673160
Conc: 1.93 ng/ml