

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022521\
 Data File : PL064954.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Feb 2021 14:20
 Operator : AR\AJ
 Sample : M1472-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMPOSITE-01(TP2-TP1)

Manual Integrations
 APPROVED

Ankita
 2/25/2021 9:07:19 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 24 15:48:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 09 04:41:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.423	4.098	36587092	23244098	13.004m	10.760m
28)	SA Decachlor...	8.143	9.256	33698667	28897522	14.985	15.214
Target Compounds							
10)	B gamma-Chl...	5.345	6.244	2315430	2475685	0.660m	1.071m#
11)	B alpha-Chl...	5.402	6.317	1964481	6617750	0.567m	2.875 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022521\
Data File : PL064954.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Feb 2021 14:20
Operator : AR\AJ
Sample : M1472-03
Misc :
ALS Vial : 13 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampleId :
COMPOSITE-01(TP2-TP1)


Manual Integrations
APPROVED

Ankita
2/25/2021 9:07:19 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 24 15:48:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
Quant Title : GC Extractables
QLast Update : Tue Feb 09 04:41:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

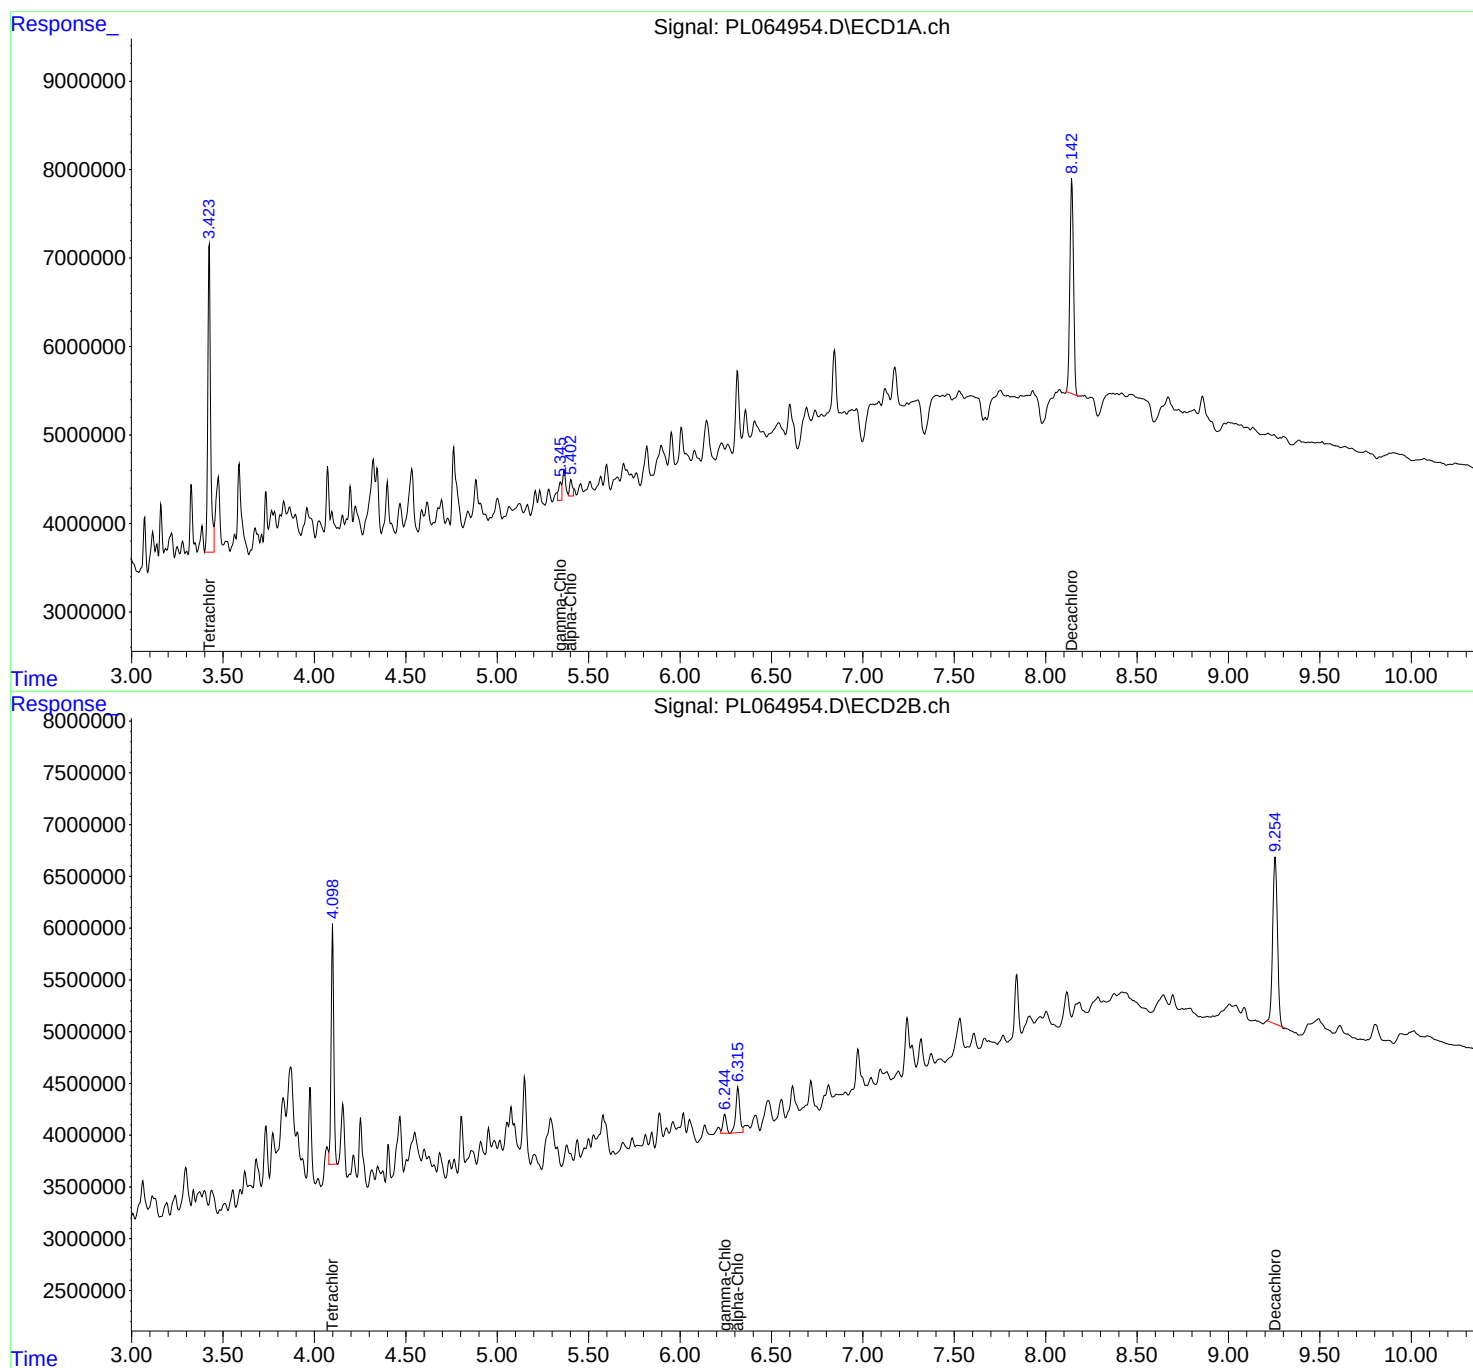

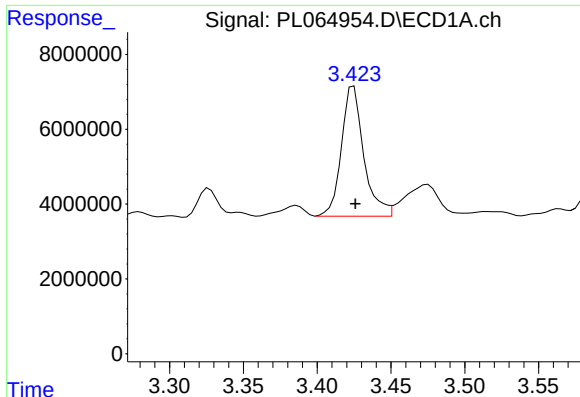


#1 Tetrachloro-m-xylene

R.T.: 3.423 min
Delta R.T.: -0.003 min
Response: 36587092
Conc: 13.00 ng/ml m

Instrument :
ECD_L
ClientSampleId :
COMPOSITE-01(TP2-TP1)


Manual Integrations
APPROVED

Ankita
2/25/2021 9:07:19 AM

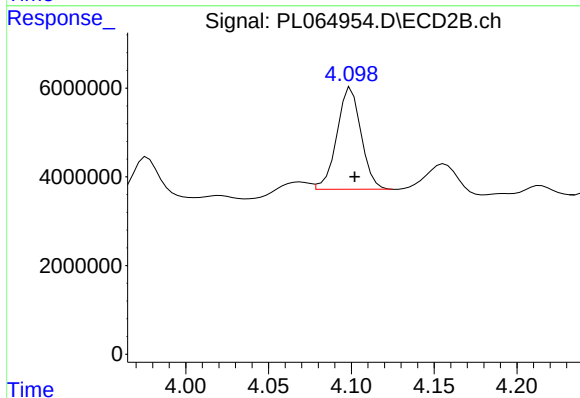


#1 Tetrachloro-m-xylene

R.T.: 4.098 min
Delta R.T.: -0.004 min
Response: 23244098
Conc: 10.76 ng/ml m

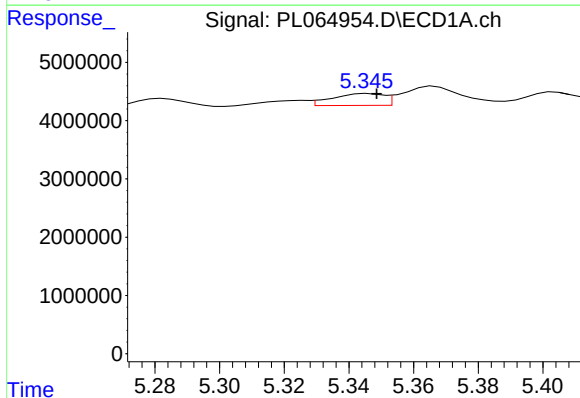


#10 gamma-Chlordane

R.T.: 5.345 min
Delta R.T.: -0.004 min
Response: 2315430
Conc: 0.66 ng/ml m

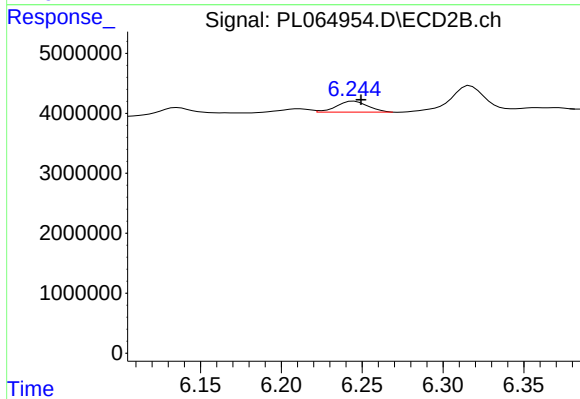

#10 gamma-Chlordane

R.T.: 6.244 min
Delta R.T.: -0.006 min
Response: 2475685
Conc: 1.07 ng/ml m

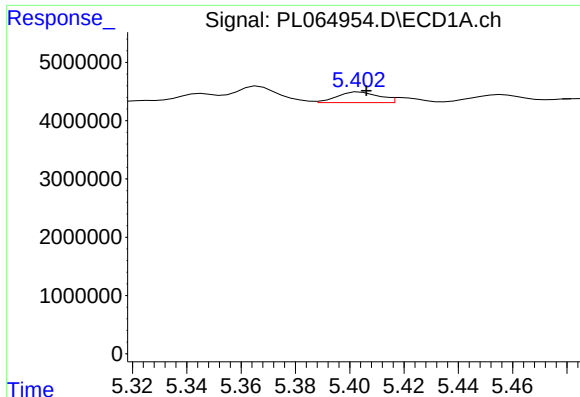


#11 alpha-Chlordane

R.T.: 5.402 min
Delta R.T.: -0.004 min
Response: 1964481
Conc: 0.57 ng/ml m

Instrument :
ECD_L
ClientSampleId :
COMPOSITE-01(TP2-TP1)


Manual Integrations
APPROVED

Ankita
2/25/2021 9:07:19 AM

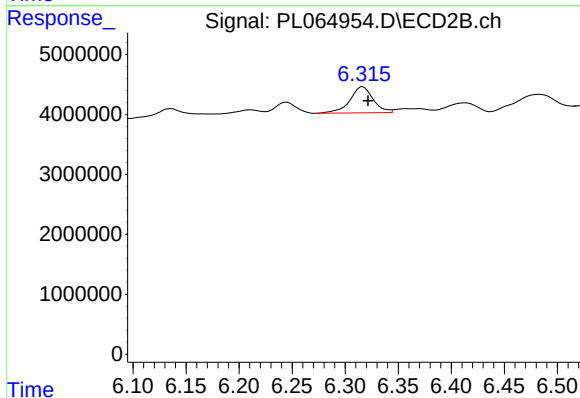


#11 alpha-Chlordane

R.T.: 6.317 min
Delta R.T.: -0.005 min
Response: 6617750
Conc: 2.87 ng/ml

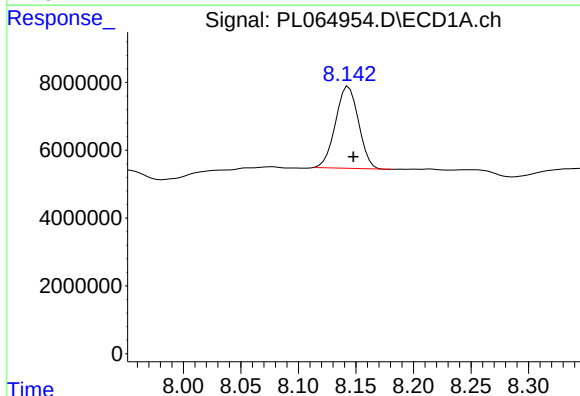

#28 Decachlorobiphenyl

R.T.: 8.143 min
Delta R.T.: -0.004 min
Response: 33698667
Conc: 14.99 ng/ml

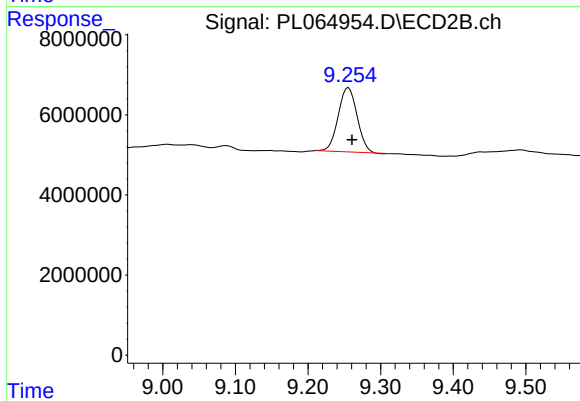

#28 Decachlorobiphenyl

R.T.: 9.256 min
Delta R.T.: -0.005 min
Response: 28897522
Conc: 15.21 ng/ml