

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022522\
 Data File : PL072986.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Feb 2022 23:47
 Operator : AR\AJ
 Sample : N1331-02
 Misc : TOX MDL
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MDL-WATER-QT1-2022-02

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 03/01/2022
 Supervised By : Ankita Jodhani 03/02/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 02:05:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022522CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 01 01:47:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	4.648	5.489	6254732	28389116	18.188	18.185
27)	SA Decachlor...	10.428	11.326	18534874	62828753	38.549	38.872
Target Compounds							
22)	Toxaphene-1	7.749	8.504	229990	1018311	97.969m	105.846m
23)	Toxaphene-2	7.925	9.023	278116	2264596	94.386m	108.201m
24)	Toxaphene-3	8.423	9.251	655960	1264289	81.067m	92.337m
25)	Toxaphene-4	8.691	9.424	809992	2232570	92.372m	98.060m
26)	Toxaphene-5	9.211	9.854	1098417	1825099	109.747m	107.527

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022522\
Data File : PL072986.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Feb 2022 23:47
Operator : AR\AJ
Sample : N1331-02
Misc : TOX MDL
ALS Vial : 23 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 02:05:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022522CLP.M
Quant Title : GC Extractables
QLast Update : Tue Mar 01 01:47:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

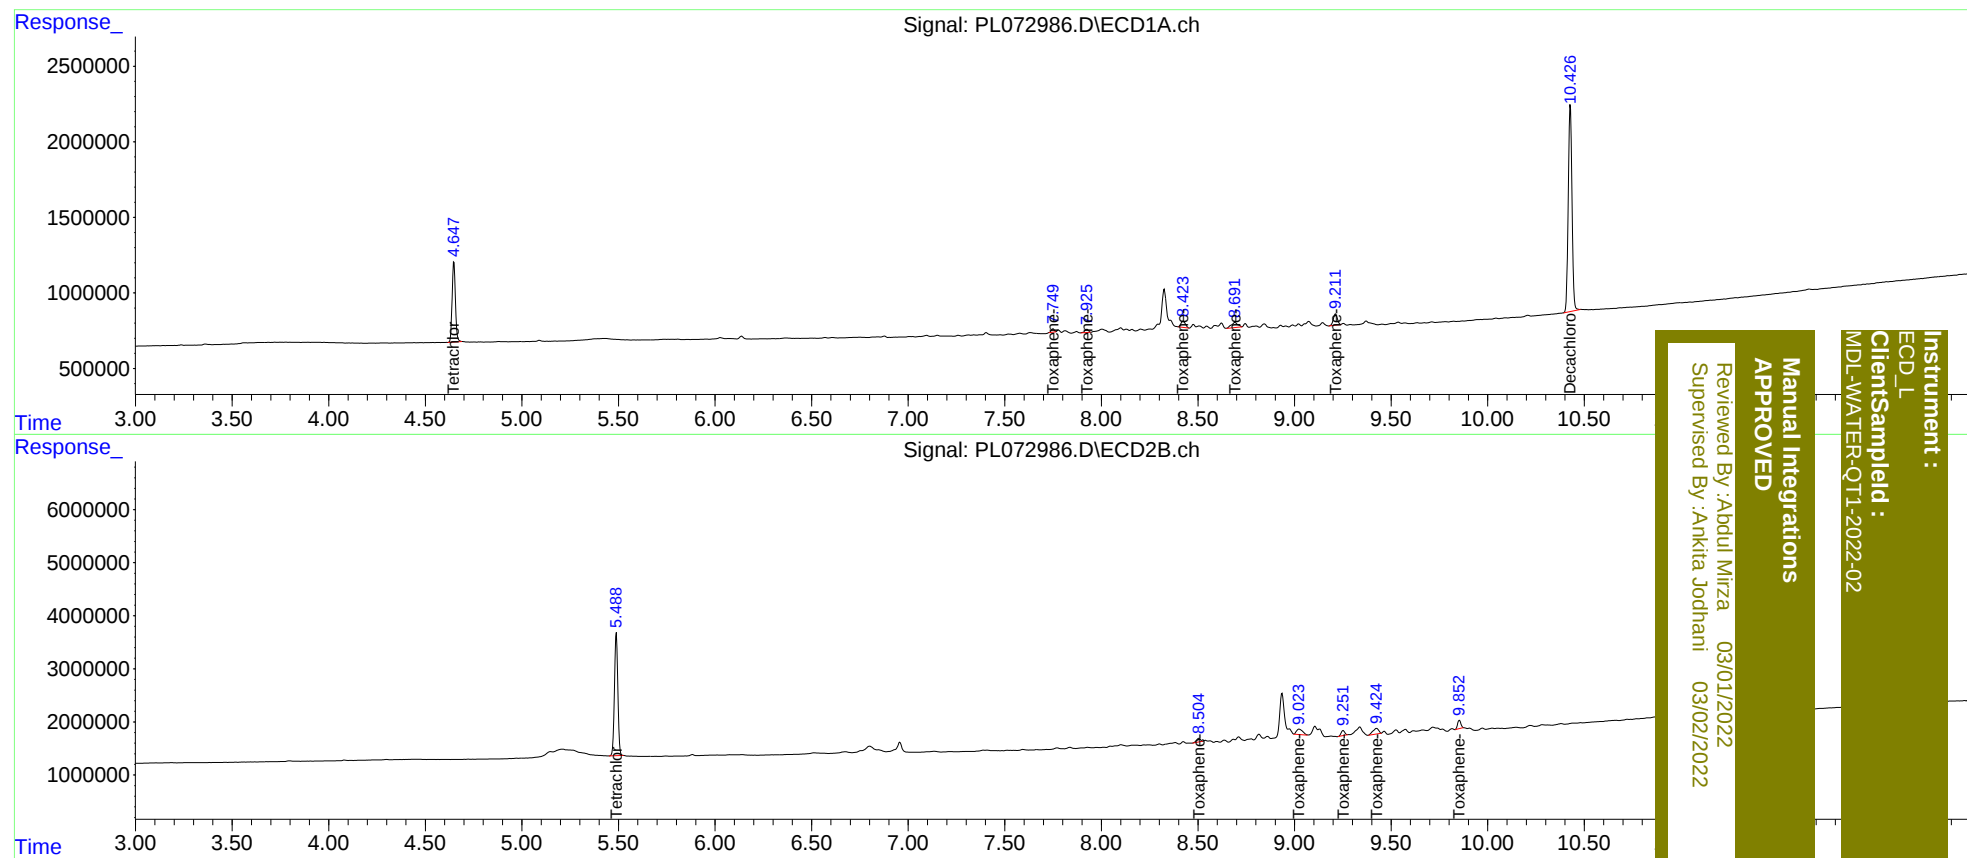

Reviewed By: Abdul Mirza 03/01/2022
Supervised By: Ankita Jodhani 03/02/2022

Manual Integrations
APPROVED

Instrument :
ECD_L
Client Sample :
MDL-WATER-QT1-2022-02