

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022522\
 Data File : PL072985.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Feb 2022 23:30
 Operator : AR\AJ
 Sample : N1331-02
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MDL-WATER-QT1-2022-02

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 03/01/2022
 Supervised By : Ankita Jodhani 03/02/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 02:15:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022522CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 01 01:47:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	4.647	5.490	6348913	28764428	18.462	18.425
27)	SA Decachlor...	10.427	11.325	18693641	63315243	38.879	39.173
Target Compounds							
2)	A alpha-BHC	5.355	6.052	449557	1858176	1.080	0.961
3)	MA gamma-BHC...	5.779	6.441	536129	1932493	1.220	1.020
4)	MA Heptachlor	6.192	7.099	627844	2423317	1.328	1.195
5)	MB Aldrin	6.517	7.467	613543	2279423	1.356	1.261
6)	B beta-BHC	6.157	6.677	342813	1574190	1.397m	1.609
7)	B delta-BHC	6.420	6.947	479895	4652704	1.114	2.406 #
8)	B Heptachlo...	7.094	7.923	670108	2336813	1.429	1.373
9)	A Endosulfan I	7.498	8.322	600492	2054902	1.329	1.289
10)	B trans-Chl...	7.372	8.190	636126	2443104	1.334	1.400
11)	B cis-Chlor...	7.442	8.273	661375	2261034	1.386	1.324
12)	B 4,4'-DDE	7.656	8.457	487942	1825917	1.263	1.206
13)	MA Dieldrin	7.784	8.608	577742	2102790	1.233	1.267
14)	MA Endrin	8.075	8.842	548440	1702391	1.349	1.274
15)	B Endosulfa...	8.385	9.064	962301	2098417	2.054	1.448 #
16)	A 4,4'-DDD	8.242	8.982	428752	2202691	1.214	1.677m#
17)	MA 4,4'-DDT	8.504	9.302	434871	1690190	1.121	1.282
18)	B Endrin al...	8.574	9.198	473879	1590804	1.425	1.487
19)	B Endosulfa...	8.805	9.435	633146	2030450	1.447	1.476
20)	A Methoxychlor	9.099	9.782	322942	1080892	1.318	1.411
21)	B Endrin ke...	9.324	9.923	593881	1795214	1.245	1.267

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022522\
Data File : PL072985.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Feb 2022 23:30
Operator : AR\AJ
Sample : N1331-02
Misc :
ALS Vial : 22 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 02:15:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022522CLP.M
Quant Title : GC Extractables
QLast Update : Tue Mar 01 01:47:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

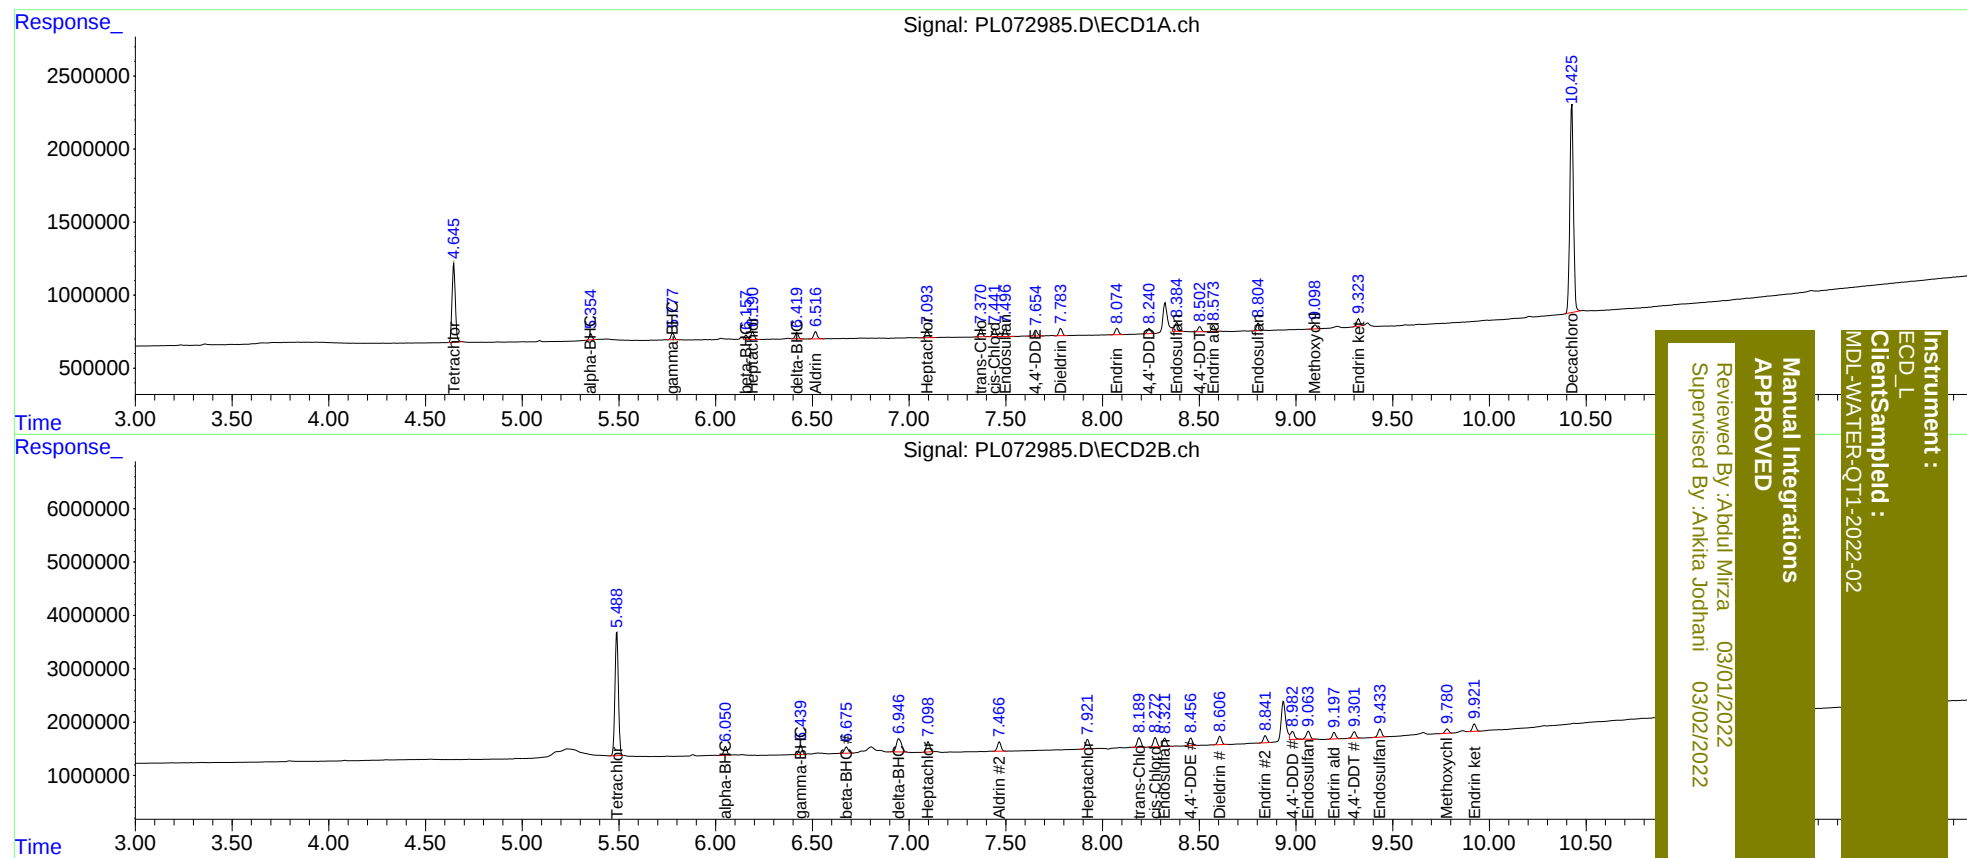

Reviewed By: Abdul Mirza 03/01/2022
Supervised By: Ankita Jodhani 03/02/2022

Manual Integrations
APPROVED

Instrument :
ECD_L
Client Sample :
MDL-WATER-QT1-2022-02