

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022525\
 Data File : PL094390.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Feb 2025 14:04
 Operator : AR\AJ
 Sample : Q1416-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OK-01-022425

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 02/26/2025
 Supervised By : Ankita Jodhani 02/26/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 26 00:09:38 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022125.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 21 14:52:19 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.541	2.772	35565084	48356598	14.007m	15.153
28) SA Decachlor...	9.061	7.909	31605282	41023841	14.857	10.668 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022525\
Data File : PL094390.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Feb 2025 14:04
Operator : AR\AJ
Sample : Q1416-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
OK-01-022425


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 02/26/2025
Supervised By : Ankita Jodhani 02/26/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 26 00:09:38 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022125.M
Quant Title : GC Extractables
QLast Update : Fri Feb 21 14:52:19 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

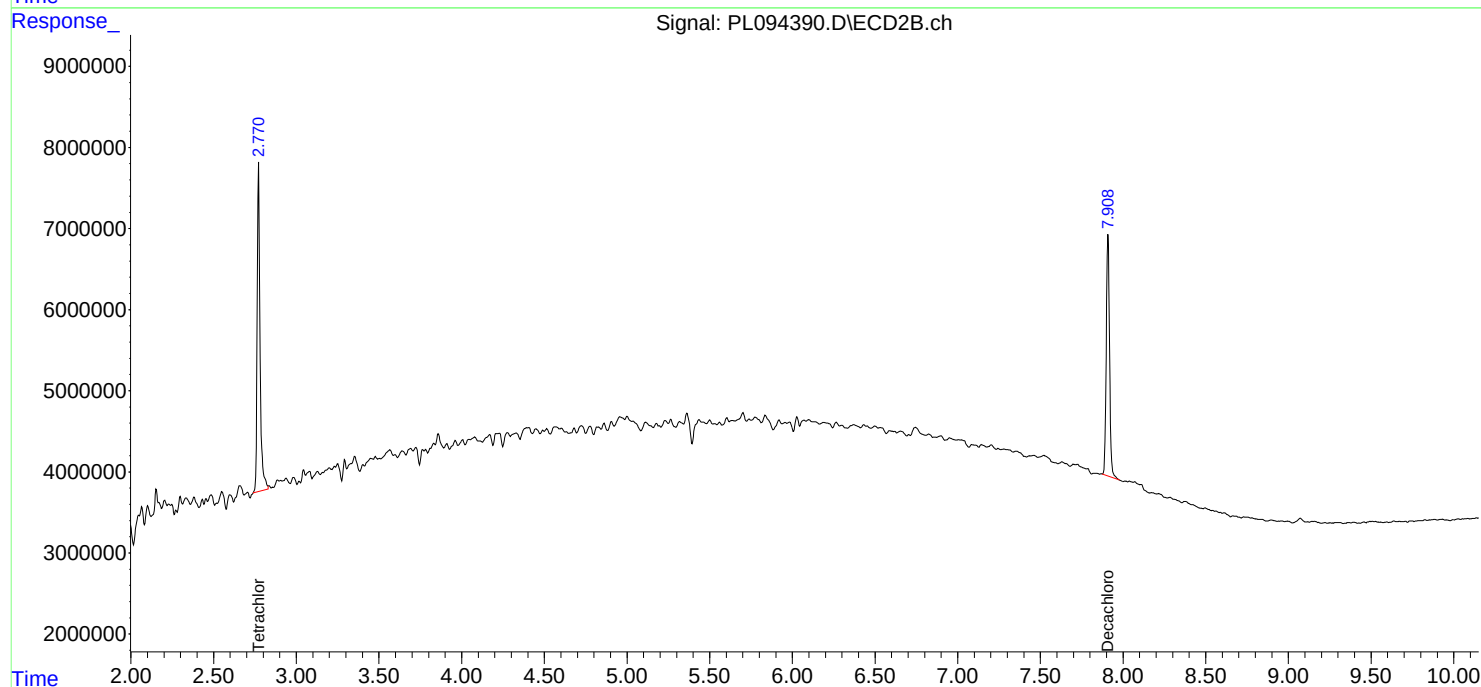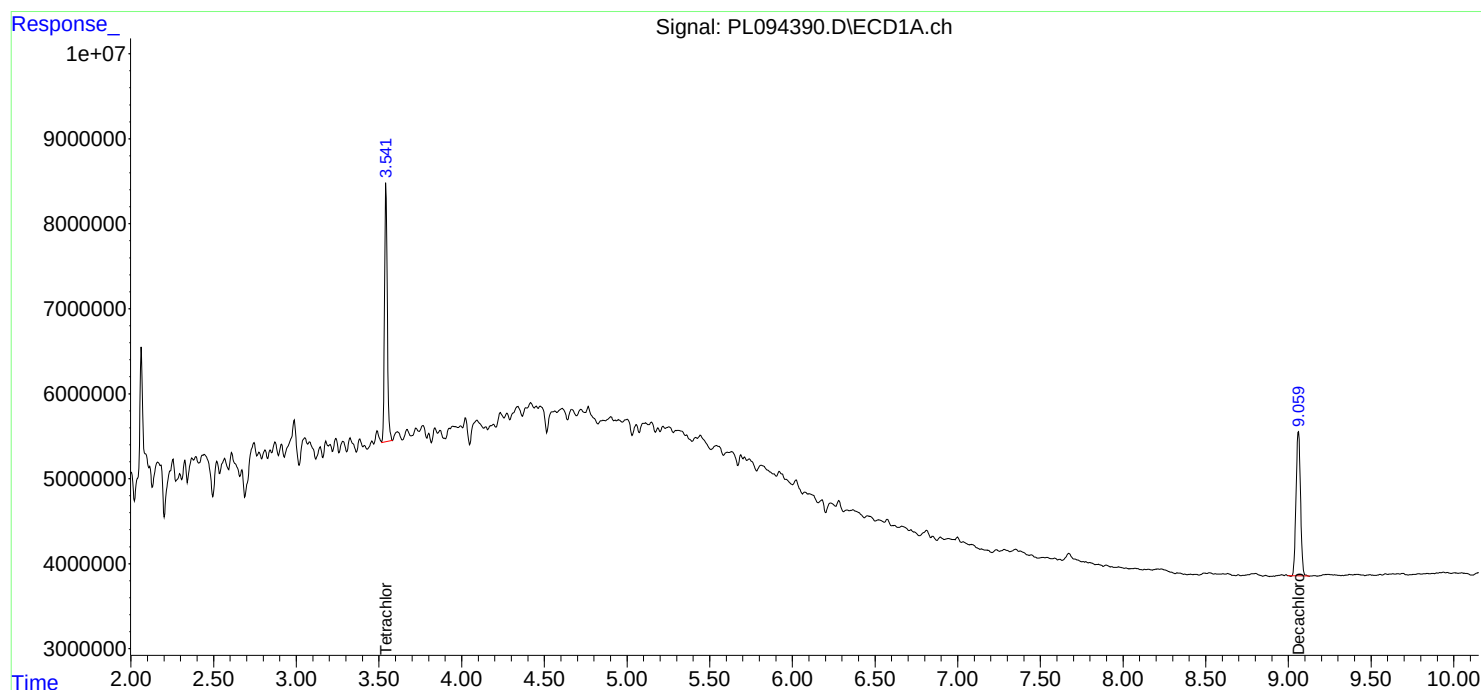

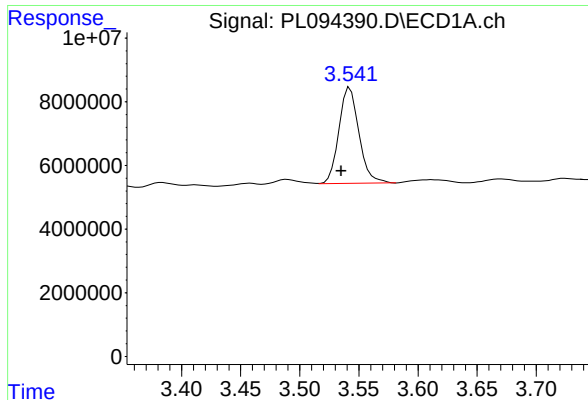


#1 Tetrachloro-m-xylene

R.T.: 3.541 min
Delta R.T.: 0.006 min
Response: 35565084
Conc: 14.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-01-022425


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/26/2025
Supervised By :Ankita Jodhani 02/26/2025

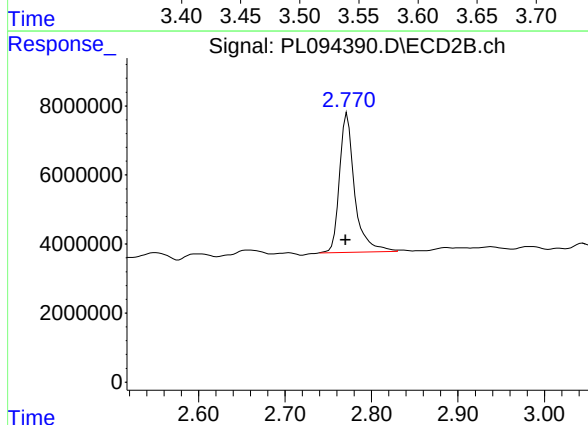


#1 Tetrachloro-m-xylene

R.T.: 2.772 min
Delta R.T.: 0.002 min
Response: 48356598
Conc: 15.15 ng/ml

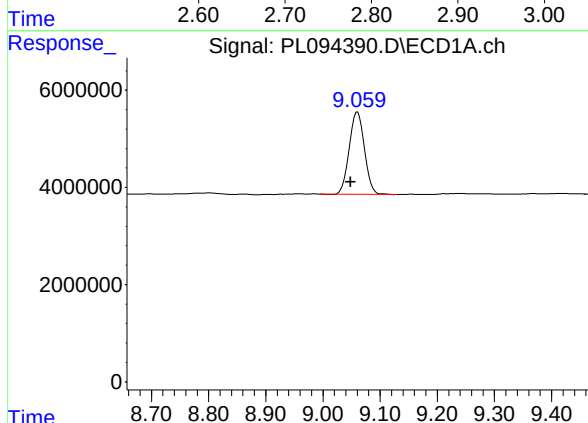

#28 Decachlorobiphenyl

R.T.: 9.061 min
Delta R.T.: 0.012 min
Response: 31605282
Conc: 14.86 ng/ml

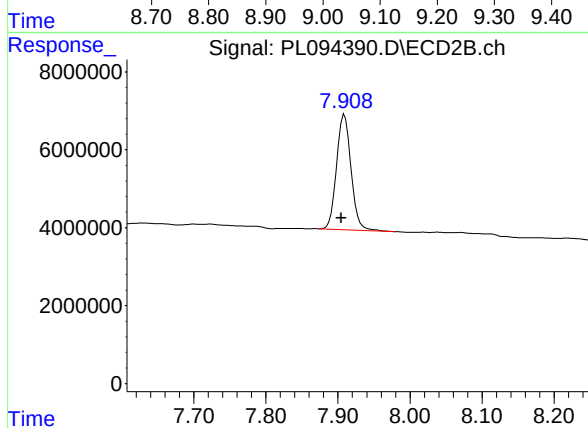

#28 Decachlorobiphenyl

R.T.: 7.909 min
Delta R.T.: 0.005 min
Response: 41023841
Conc: 10.67 ng/ml