

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022525\
 Data File : PL094391.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Feb 2025 14:17
 Operator : AR\AJ
 Sample : Q1418-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TR-06-02242025

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 02/26/2025
 Supervised By : Ankita Jodhani 02/26/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 26 00:10:02 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022125.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 21 14:52:19 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.536	2.772	32980273	45832485	12.989m	14.362
28) SA Decachlor...	9.056	7.907	26517380	36665592	12.465	9.534

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022525\
Data File : PL094391.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Feb 2025 14:17
Operator : AR\AJ
Sample : Q1418-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TR-06-02242025


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 02/26/2025
Supervised By : Ankita Jodhani 02/26/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 26 00:10:02 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022125.M
Quant Title : GC Extractables
QLast Update : Fri Feb 21 14:52:19 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

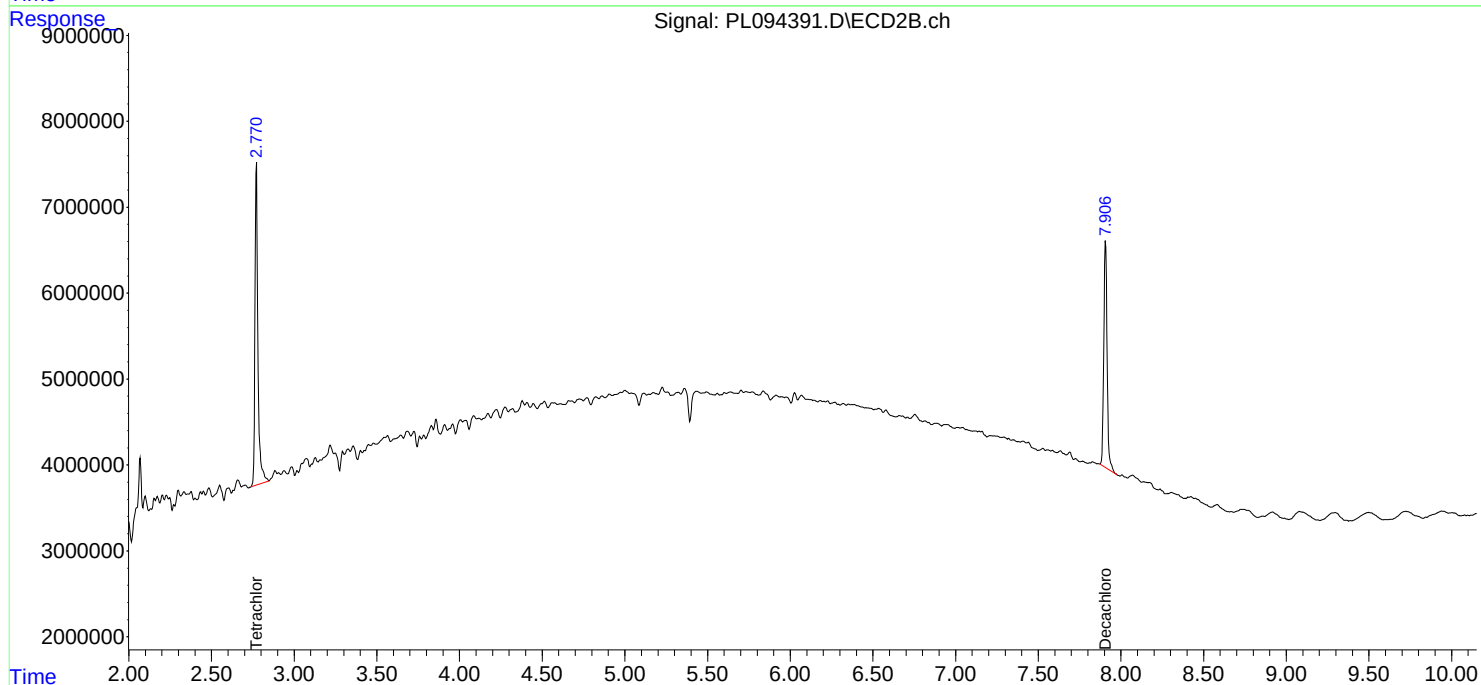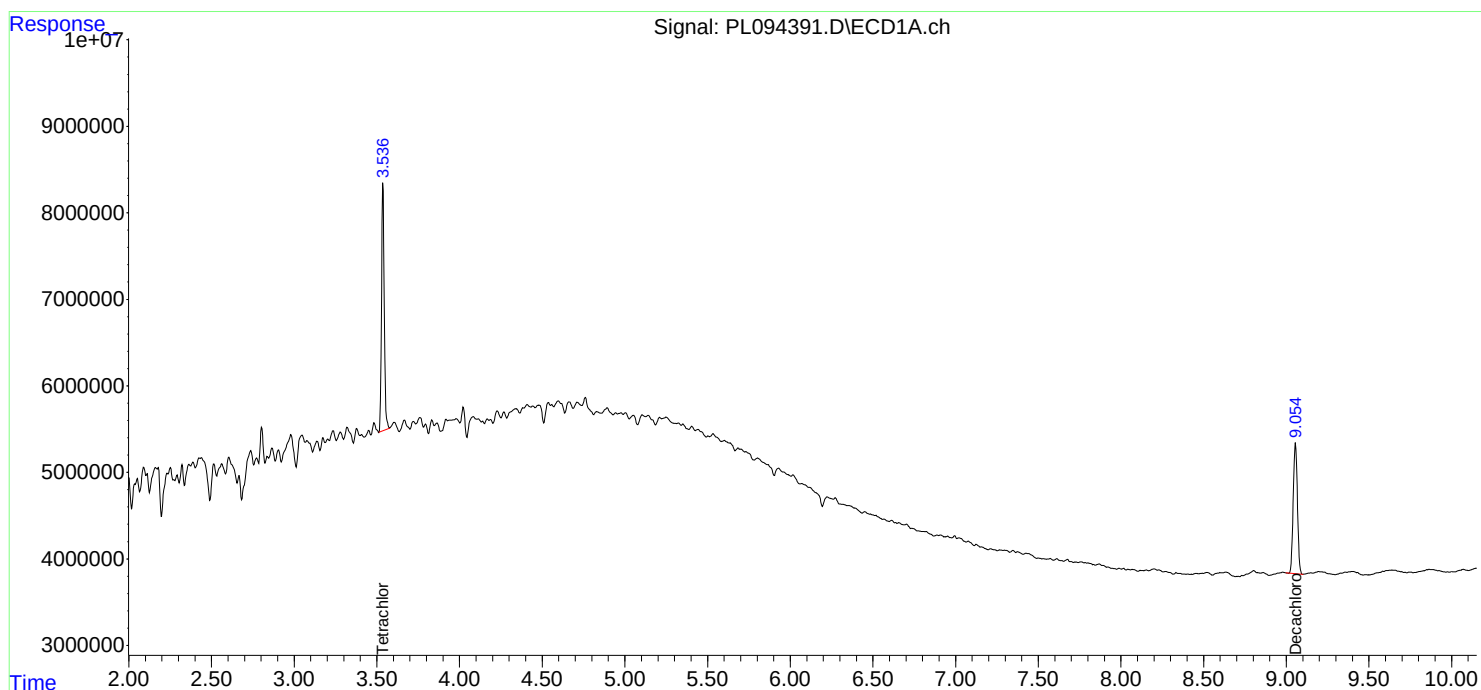

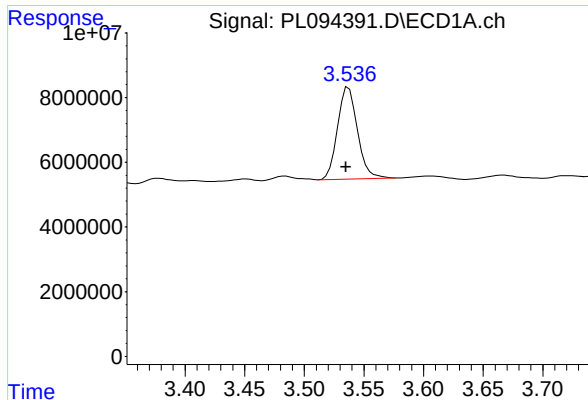


#1 Tetrachloro-m-xylene

R.T.: 3.536 min
Delta R.T.: 0.000 min
Response: 32980273
Conc: 12.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-06-02242025


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/26/2025
Supervised By :Ankita Jodhani 02/26/2025

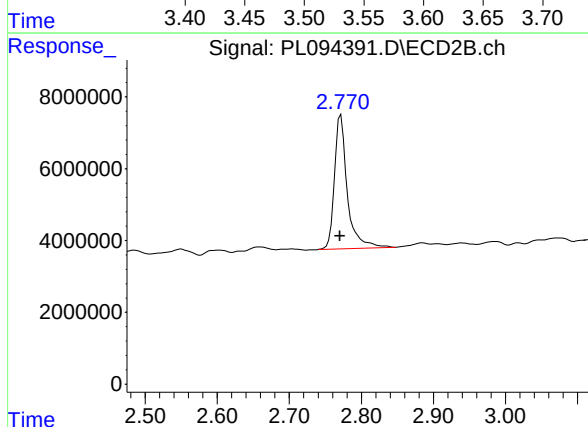


#1 Tetrachloro-m-xylene

R.T.: 2.772 min
Delta R.T.: 0.001 min
Response: 45832485
Conc: 14.36 ng/ml

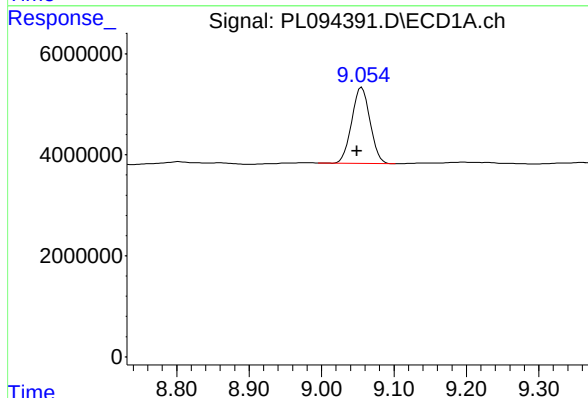

#28 Decachlorobiphenyl

R.T.: 9.056 min
Delta R.T.: 0.007 min
Response: 26517380
Conc: 12.47 ng/ml

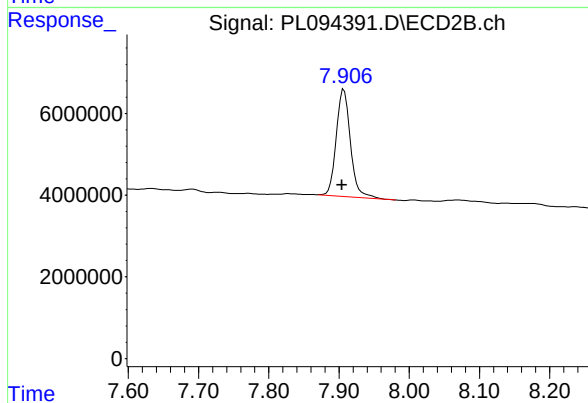

#28 Decachlorobiphenyl

R.T.: 7.907 min
Delta R.T.: 0.003 min
Response: 36665592
Conc: 9.53 ng/ml