

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022620\
 Data File : PL056826.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Feb 2020 11:02
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 27 00:31:15 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021920.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 20 02:32:45 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
12) B	4,4'-DDE	5.686f	0.000	65627728	0	4.666	N.D. #
15) B	Endosulfa...	6.305f	0.000	3474974	0	0.280	N.D. #
27)	Chlordane-5	6.305f	0.000	3474974	0	10.613	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022620\
Data File : PL056826.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Feb 2020 11:02
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 27 00:31:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021920.M
Quant Title : GC Extractables
QLast Update : Thu Feb 20 02:32:45 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

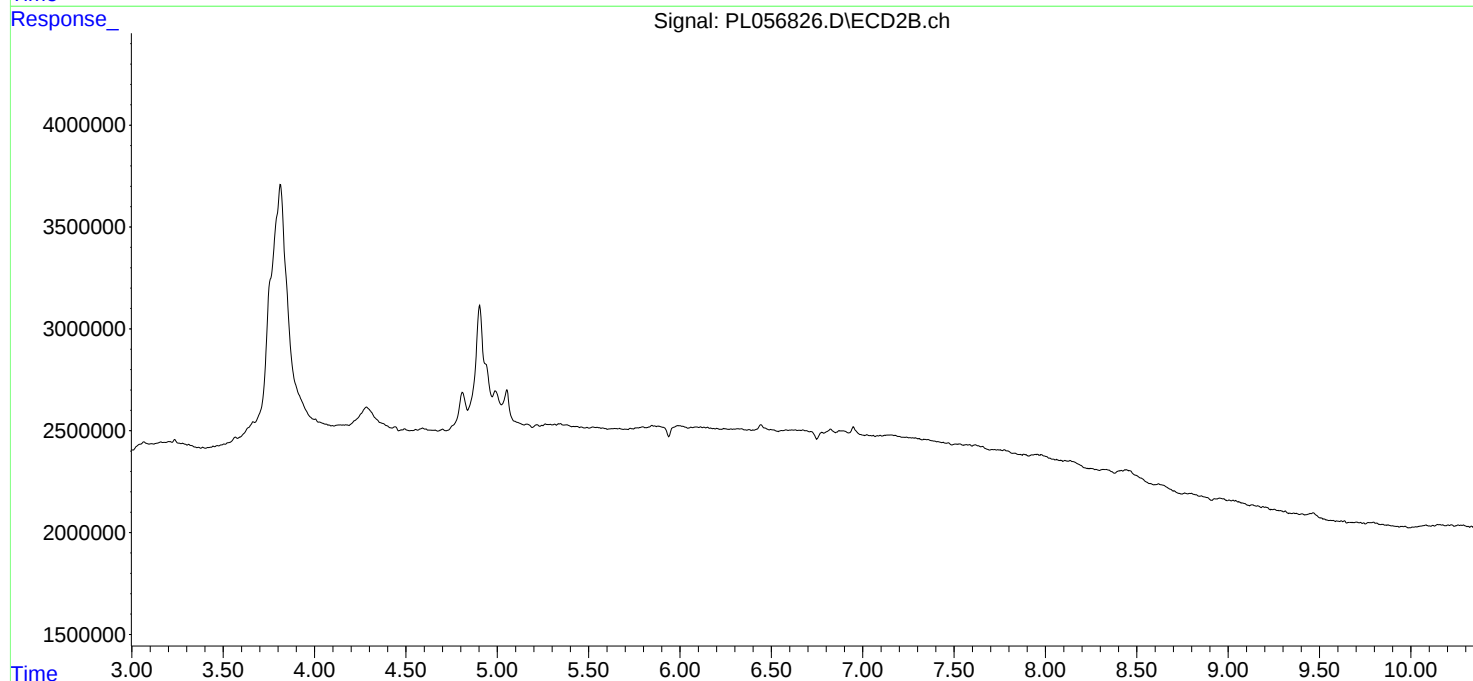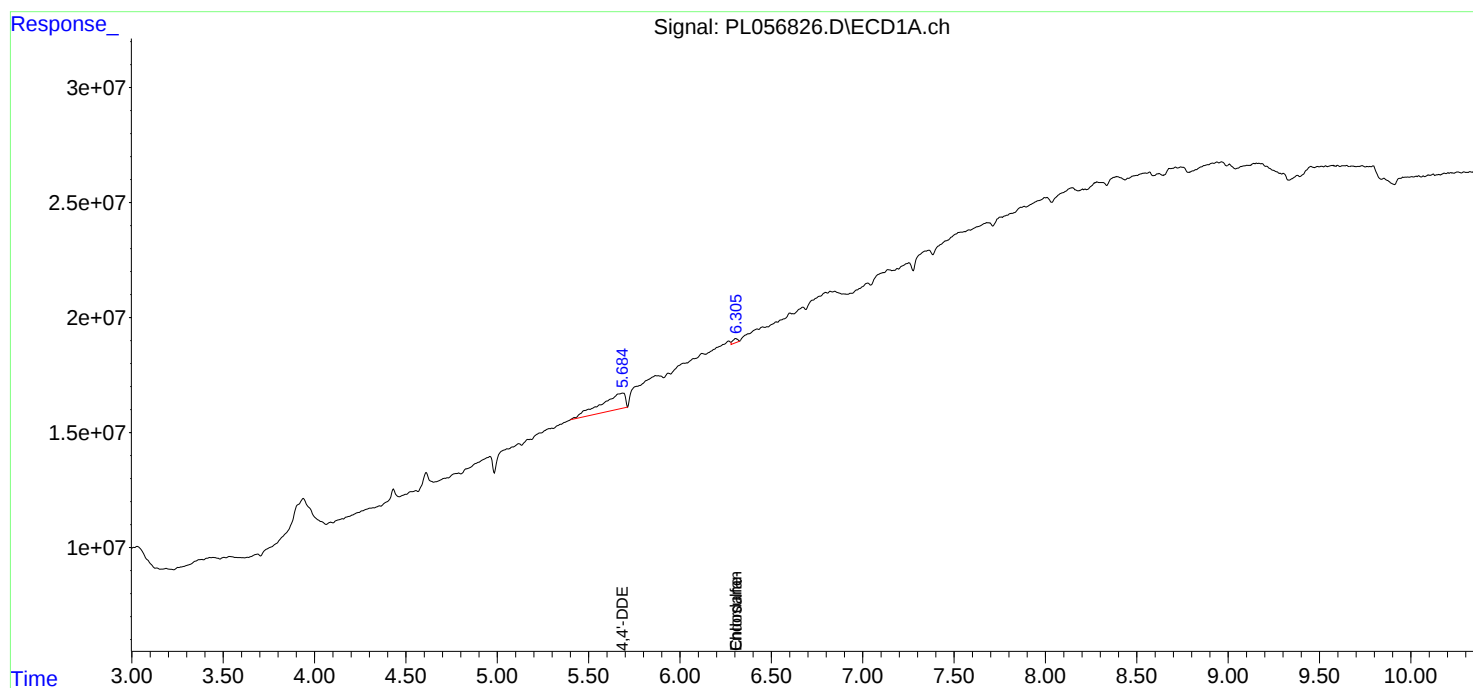


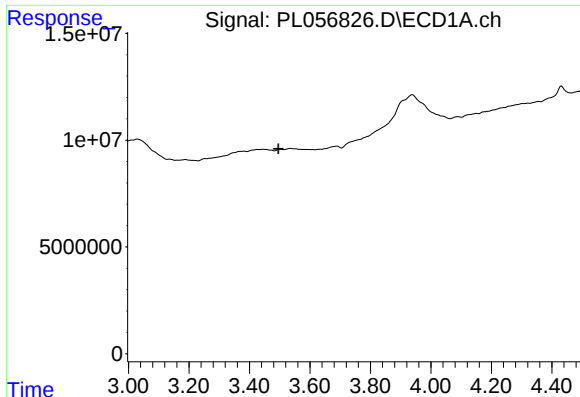

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.496 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

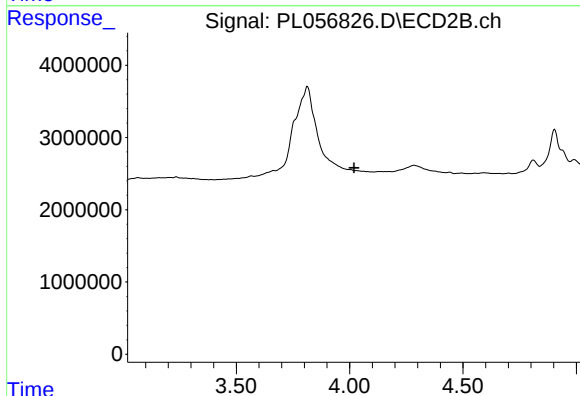


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 4.020 min
Response: 0
Conc: N.D.

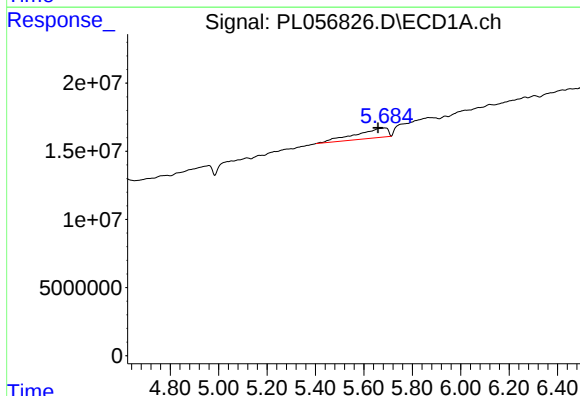


#12 4,4'-DDE

R.T.: 5.686 min
Delta R.T.: 0.027 min
Response: 65627728
Conc: 4.67 ng/ml

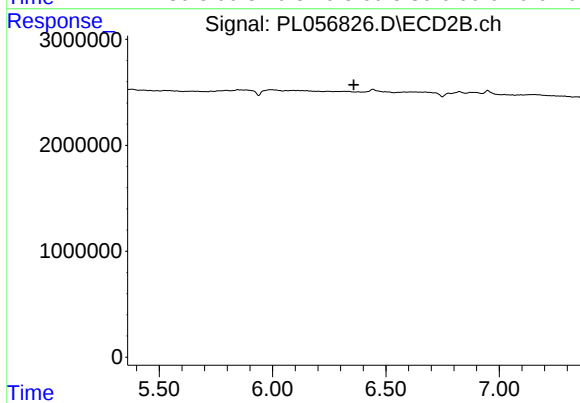

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 6.358 min
Response: 0
Conc: N.D.

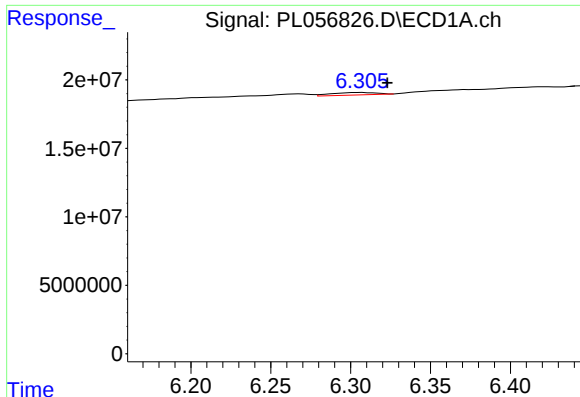

#15 Endosulfan II


R.T.: 6.305 min
Delta R.T.: -0.018 min
Response: 3474974
Conc: 0.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

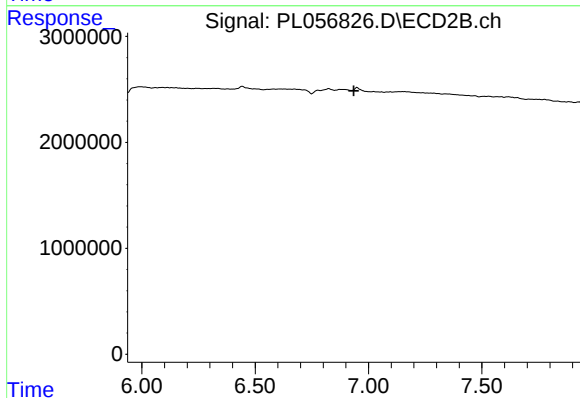


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.936 min
Response: 0
Conc: N.D.

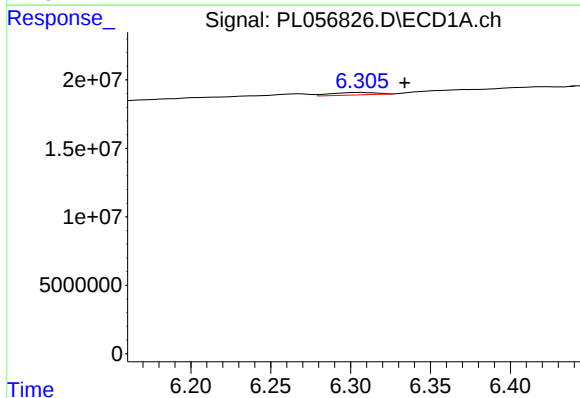


#27 Chlordane-5

R.T.: 6.305 min
Delta R.T.: -0.029 min
Response: 3474974
Conc: 10.61 ng/ml

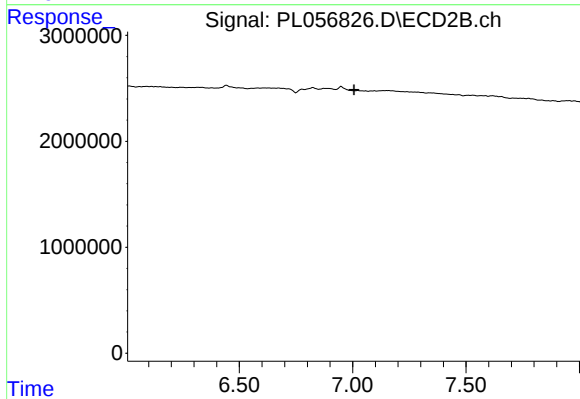

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 7.007 min
Response: 0
Conc: N.D.

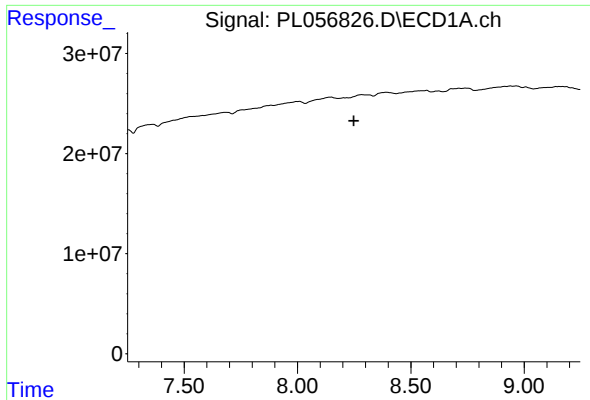

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.248 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

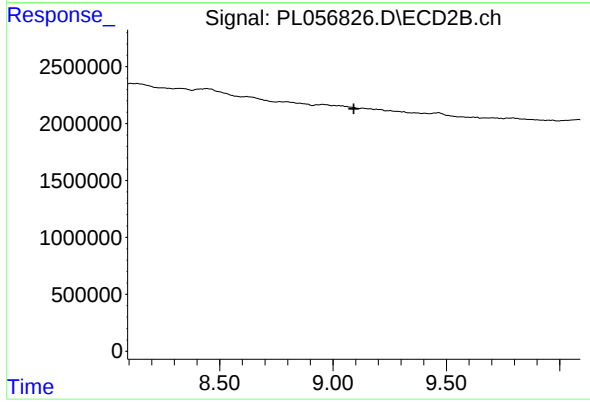

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.091 min
Response: 0
Conc: N.D.