

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022620\
 Data File : PL056834.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Feb 2020 13:48
 Operator : AJ\MA
 Sample : L1681-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SH-BORING-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 27 00:33:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021920.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 20 02:32:45 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.498	4.020	184.1E6	62281019	21.290	25.002
28)	SA Decachlor...	8.251	9.093	154.3E6	34972165	12.971	16.643 #
Target Compounds							
13)	MA Dieldrin	5.801	0.000	10178893	0	0.683	N.D. #
15)	B Endosulfa...	6.338	0.000	8940994	0	0.720	N.D. #
17)	MA 4,4'-DDT	6.414	0.000	9608411	0	0.882	N.D. #
18)	B Endrin al...	6.510f	0.000	1982179	0	0.183	N.D. #
19)	B Endosulfa...	6.725f	0.000	997.7E6	0	84.143	N.D. #
27)	Chlordane-5	6.338	0.000	8940994	0	27.306	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022620\
Data File : PL056834.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Feb 2020 13:48
Operator : AJ\MA
Sample : L1681-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SH-BORING-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 27 00:33:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021920.M
Quant Title : GC Extractables
QLast Update : Thu Feb 20 02:32:45 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

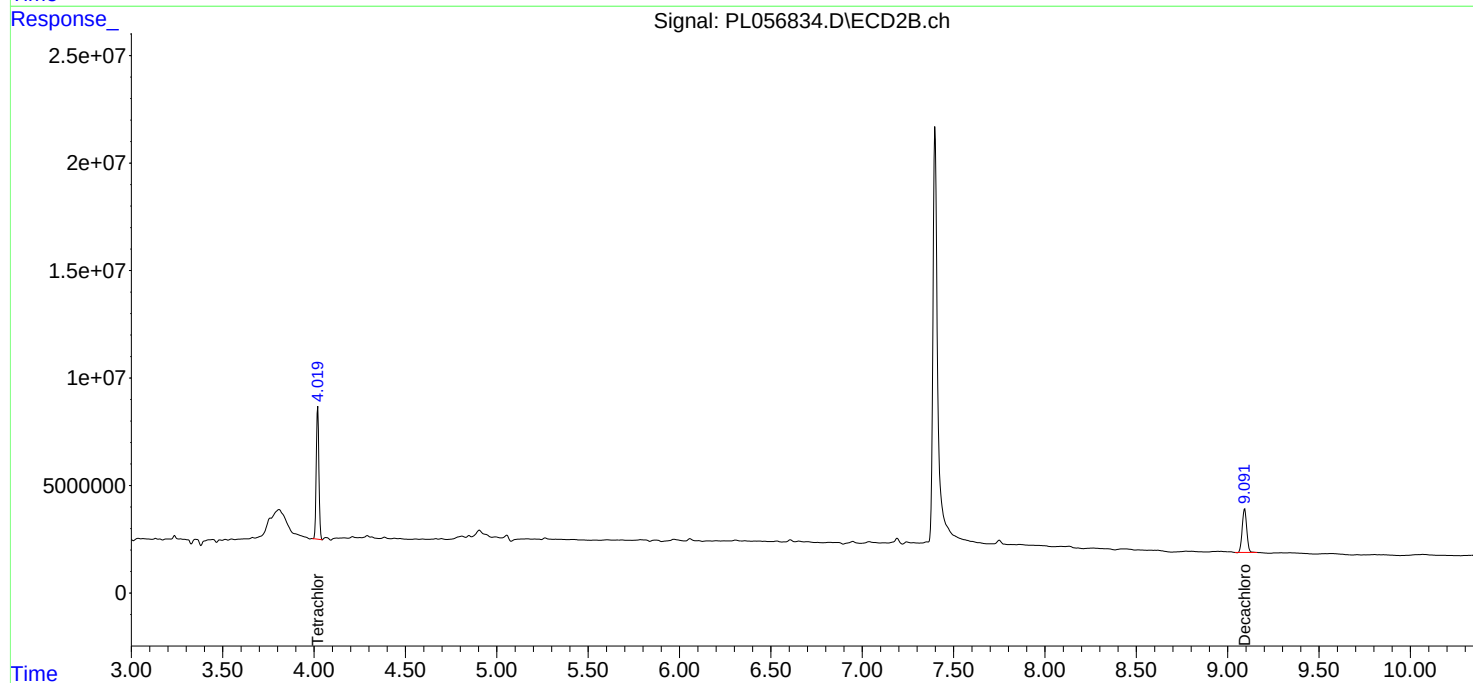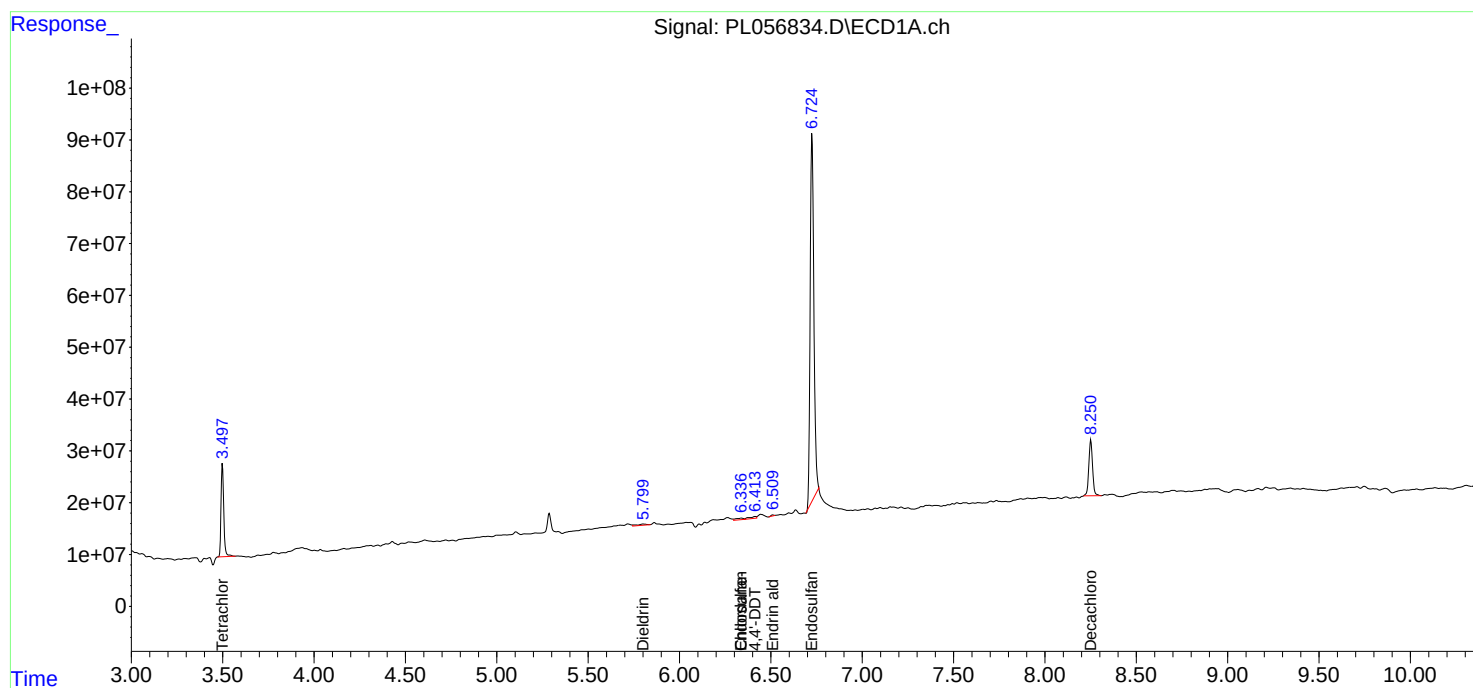


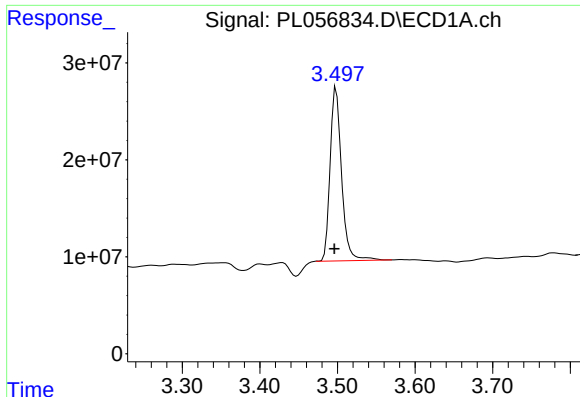

#1 Tetrachloro-m-xylene


R.T.: 3.498 min
Delta R.T.: 0.002 min
Response: 184110861
Conc: 21.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
SH-BORING-2

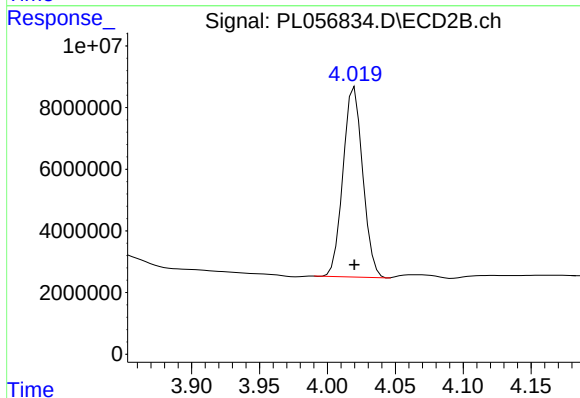


#1 Tetrachloro-m-xylene

R.T.: 4.020 min
Delta R.T.: 0.000 min
Response: 62281019
Conc: 25.00 ng/ml

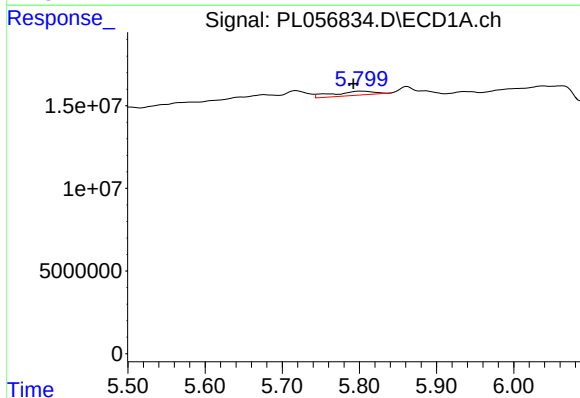


#13 Dieldrin

R.T.: 5.801 min
Delta R.T.: 0.008 min
Response: 10178893
Conc: 0.68 ng/ml

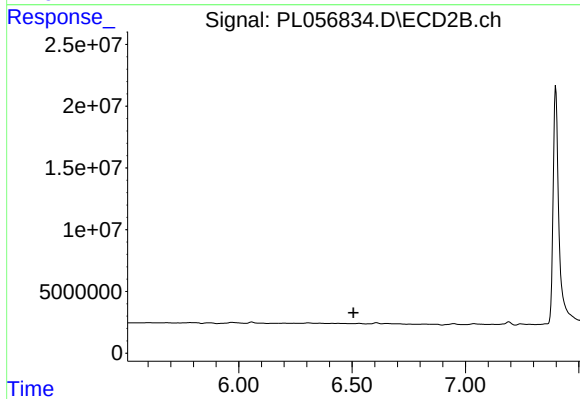

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.506 min
Response: 0
Conc: N.D.

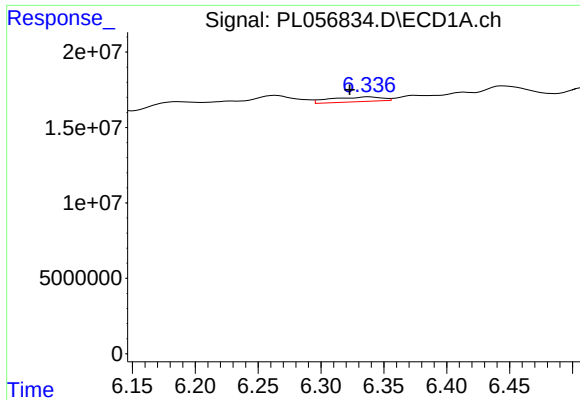

#15 Endosulfan II


R.T.: 6.338 min
Delta R.T.: 0.015 min
Response: 8940994
Conc: 0.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
SH-BORING-2

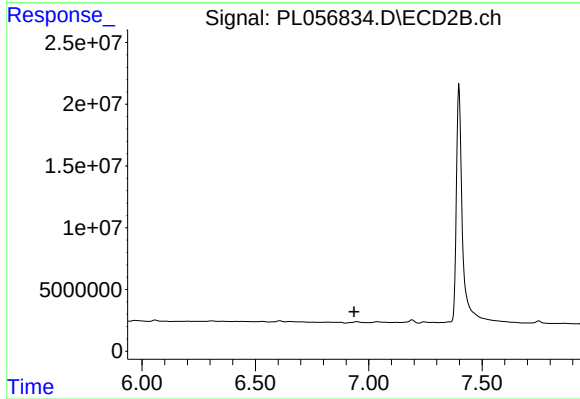


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.936 min
Response: 0
Conc: N.D.

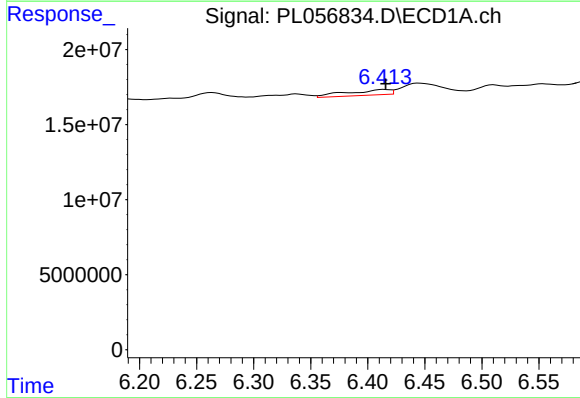


#17 4,4'-DDT

R.T.: 6.414 min
Delta R.T.: -0.001 min
Response: 9608411
Conc: 0.88 ng/ml

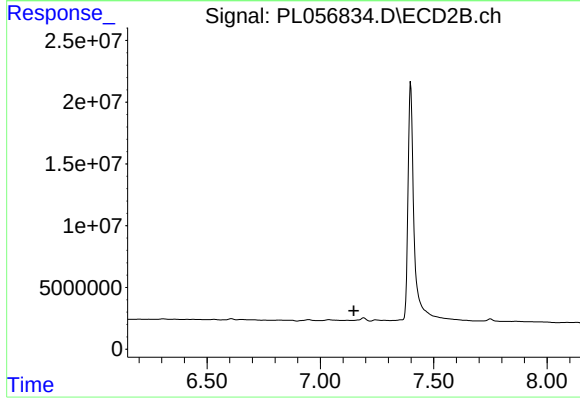

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 7.148 min
Response: 0
Conc: N.D.

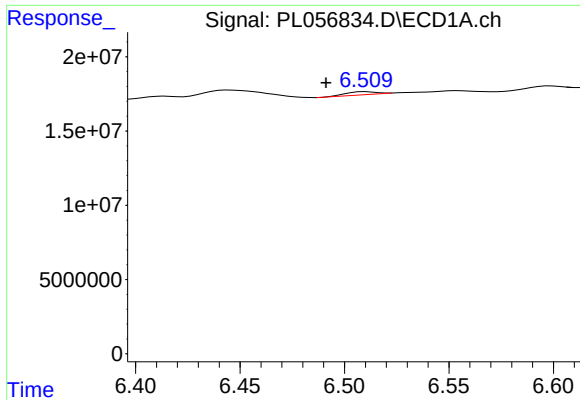

#18 Endrin aldehyde


R.T.: 6.510 min
Delta R.T.: 0.019 min
Response: 1982179
Conc: 0.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
SH-BORING-2

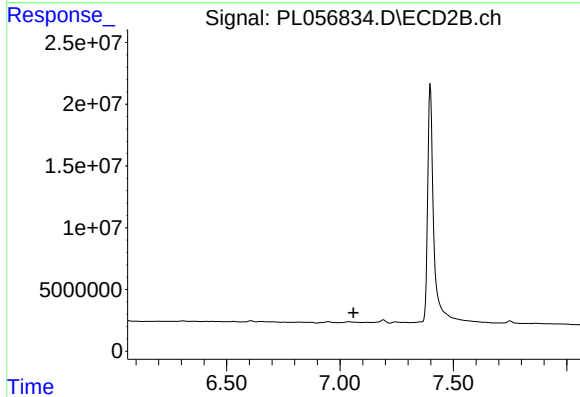


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 7.060 min
Response: 0
Conc: N.D.

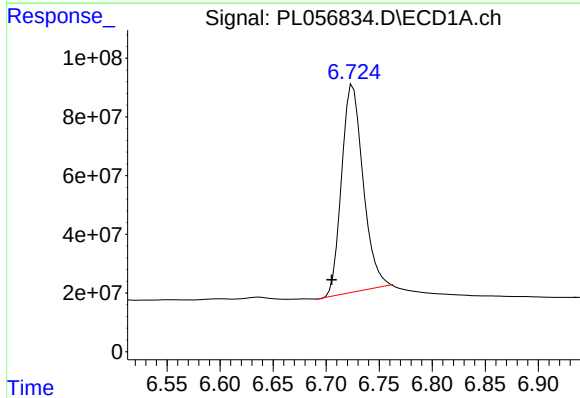


#19 Endosulfan Sulfate

R.T.: 6.725 min
Delta R.T.: 0.020 min
Response: 997669103
Conc: 84.14 ng/ml

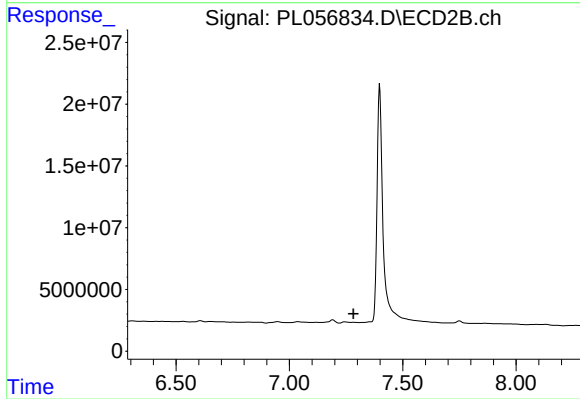

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.283 min
Response: 0
Conc: N.D.

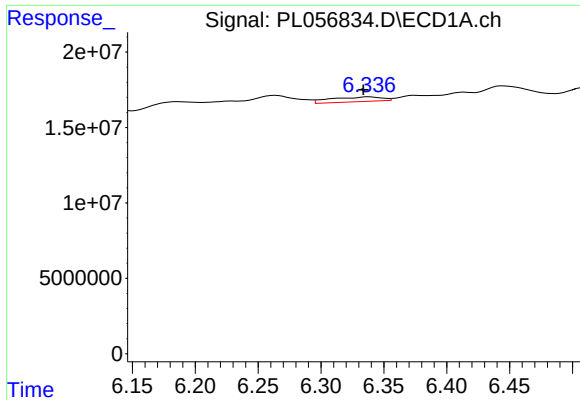

#27 Chlordane-5


R.T.: 6.338 min
Delta R.T.: 0.004 min
Response: 8940994
Conc: 27.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
SH-BORING-2

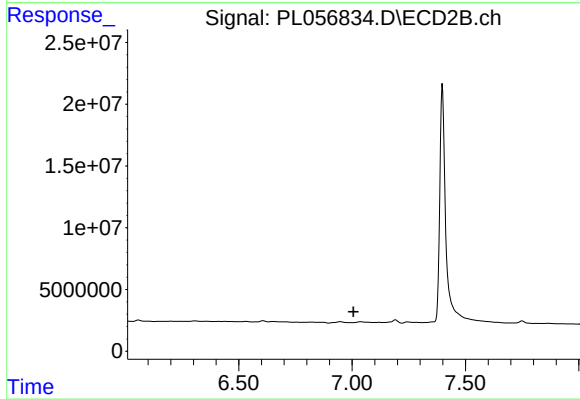


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 7.007 min
Response: 0
Conc: N.D.

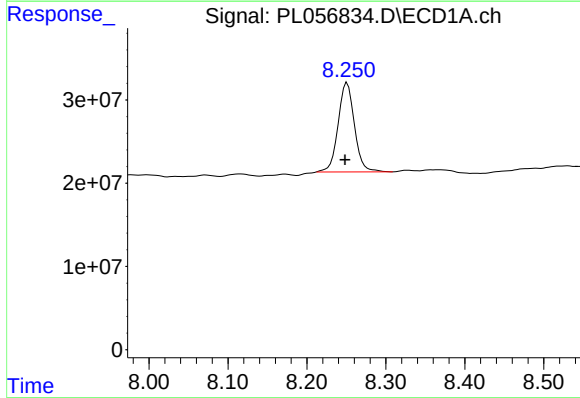

#28 Decachlorobiphenyl

R.T.: 8.251 min
Delta R.T.: 0.003 min
Response: 154293824
Conc: 12.97 ng/ml

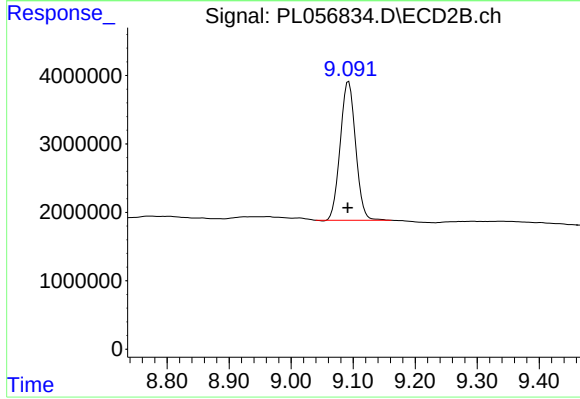

#28 Decachlorobiphenyl

R.T.: 9.093 min
Delta R.T.: 0.002 min
Response: 34972165
Conc: 16.64 ng/ml