

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022620\
 Data File : PL056847.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Feb 2020 18:31
 Operator : AJ\MA
 Sample : L1367-08
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OK-02-022420

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 27 00:36:03 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021920.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 20 02:32:45 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.498	4.020	198.8E6	60838394	22.983	24.423
28)	SA Decachlor...	8.252	9.093	214.4E6	47748975	18.025	22.723 #
Target Compounds							
15)	B Endosulfa...	6.335	0.000	39842003	0	3.208	N.D. #
27)	Chlordane-5	6.335	0.000	39842003	0	121.678	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022620\
Data File : PL056847.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Feb 2020 18:31
Operator : AJ\MA
Sample : L1367-08
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
OK-02-022420

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 27 00:36:03 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021920.M
Quant Title : GC Extractables
QLast Update : Thu Feb 20 02:32:45 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

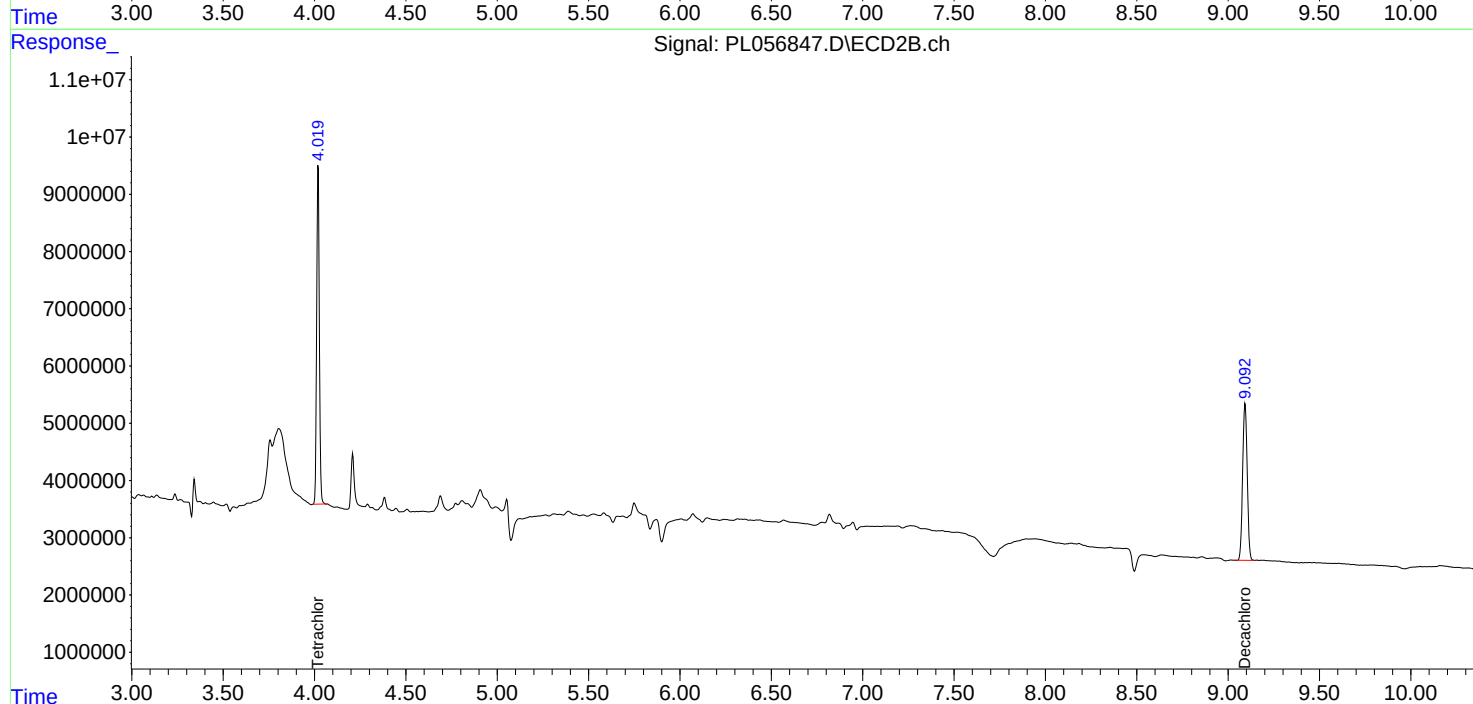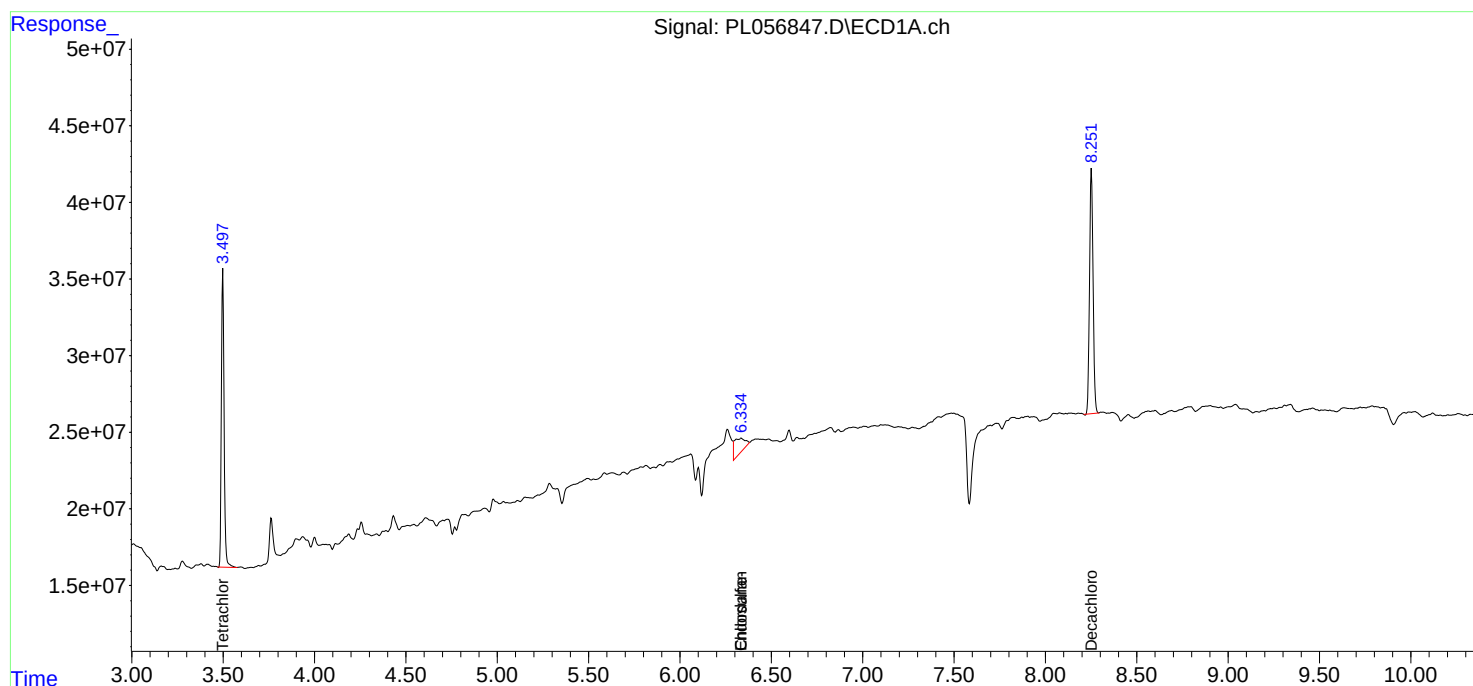


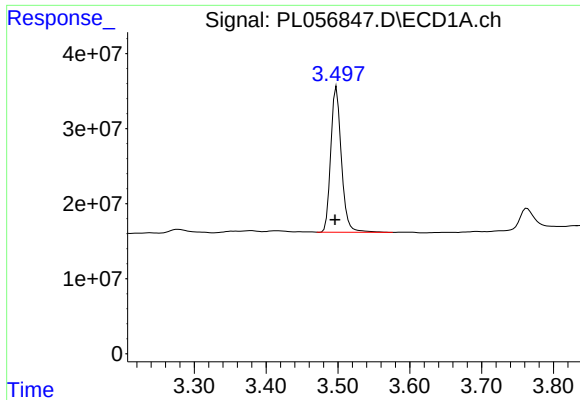

#1 Tetrachloro-m-xylene


R.T.: 3.498 min
Delta R.T.: 0.002 min
Response: 198751622
Conc: 22.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-02-022420

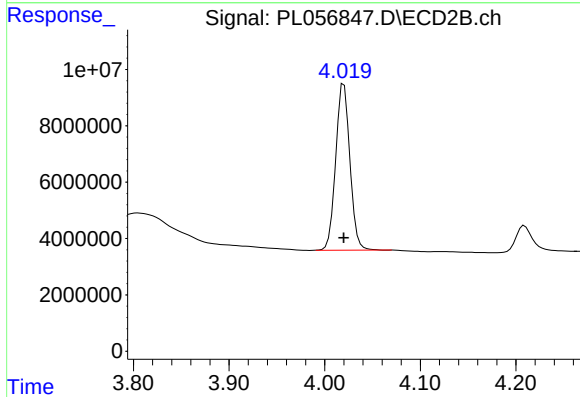


#1 Tetrachloro-m-xylene

R.T.: 4.020 min
Delta R.T.: 0.000 min
Response: 60838394
Conc: 24.42 ng/ml

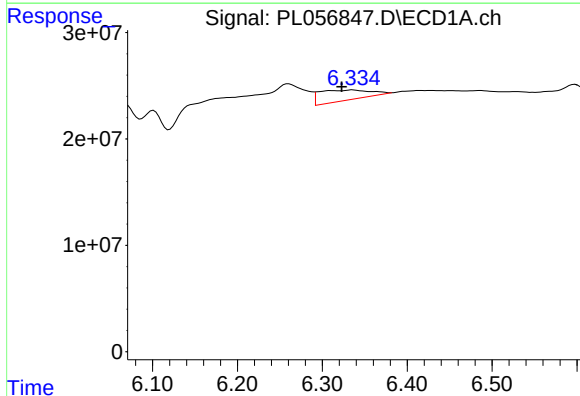


#15 Endosulfan II

R.T.: 6.335 min
Delta R.T.: 0.013 min
Response: 39842003
Conc: 3.21 ng/ml

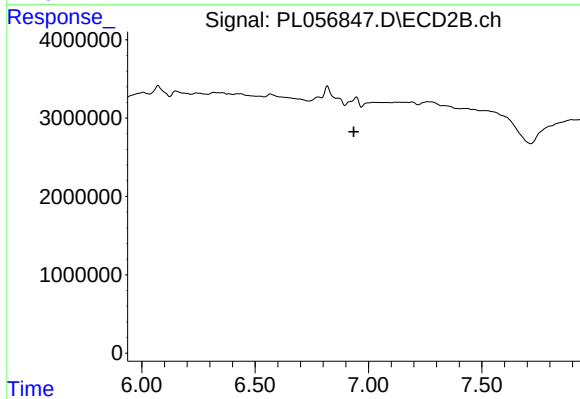

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.936 min
Response: 0
Conc: N.D.

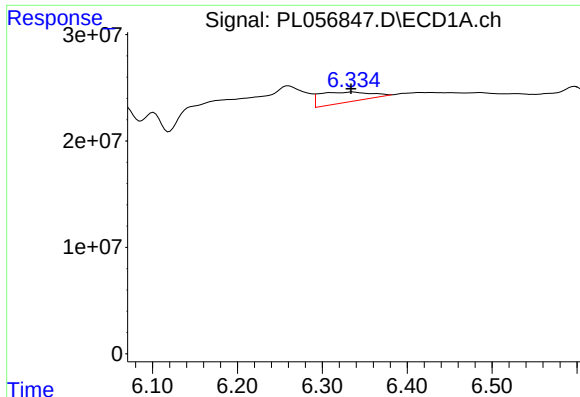

#27 Chlordane-5


R.T.: 6.335 min
Delta R.T.: 0.002 min
Response: 39842003
Conc: 121.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-02-022420

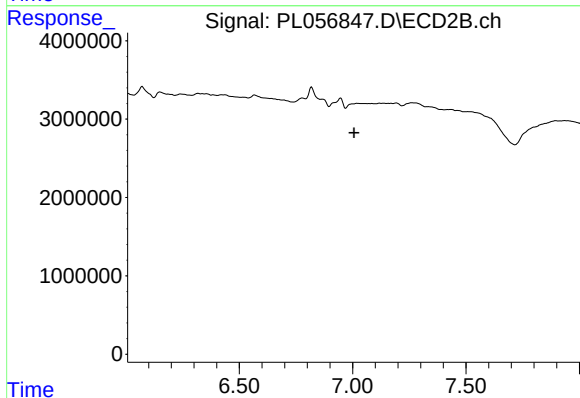


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 7.007 min
Response: 0
Conc: N.D.

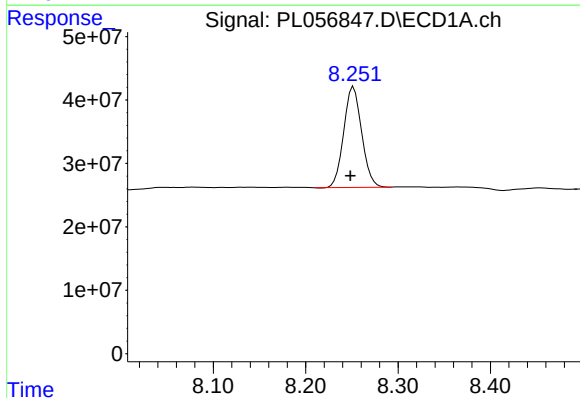

#28 Decachlorobiphenyl

R.T.: 8.252 min
Delta R.T.: 0.004 min
Response: 214411761
Conc: 18.03 ng/ml

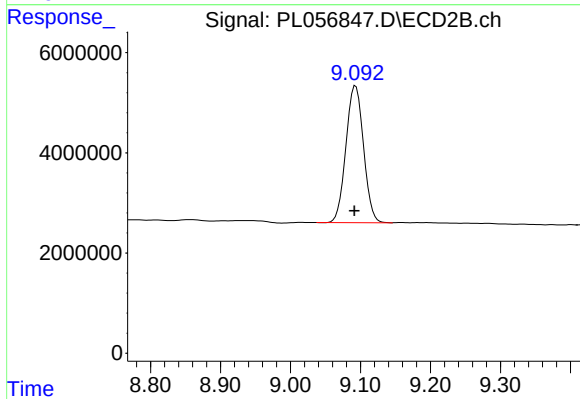

#28 Decachlorobiphenyl

R.T.: 9.093 min
Delta R.T.: 0.002 min
Response: 47748975
Conc: 22.72 ng/ml