

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022622\
 Data File : PL073003.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Feb 2022 04:30
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 27 10:54:57 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022622.M
 Quant Title : GC Extractables
 QLast Update : Sun Feb 27 10:54:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.649	5.490	40460364	158.4E6	100.860	101.250
28)	SA Decachlor...	10.428	11.326	48356669	163.1E6	98.709	99.135
Target Compounds							
23)	Chlordane-1	5.982	6.862	14207598	65790988	998.388	1004.387
24)	Chlordane-2	6.671	7.444	18758755	71385215	982.942	986.136
25)	Chlordane-3	7.373	8.193	51141456	281.7E6	1019.801	1023.605
26)	Chlordane-4	7.442	8.279	54319250	337.1E6	1017.831	1014.927
27)	Chlordane-5	8.392	9.147	19544620	55073822	1002.837	1012.761



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022622\
Data File : PL073003.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Feb 2022 04:30
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 27 10:54:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022622.M
Quant Title : GC Extractables
QLast Update : Sun Feb 27 10:54:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

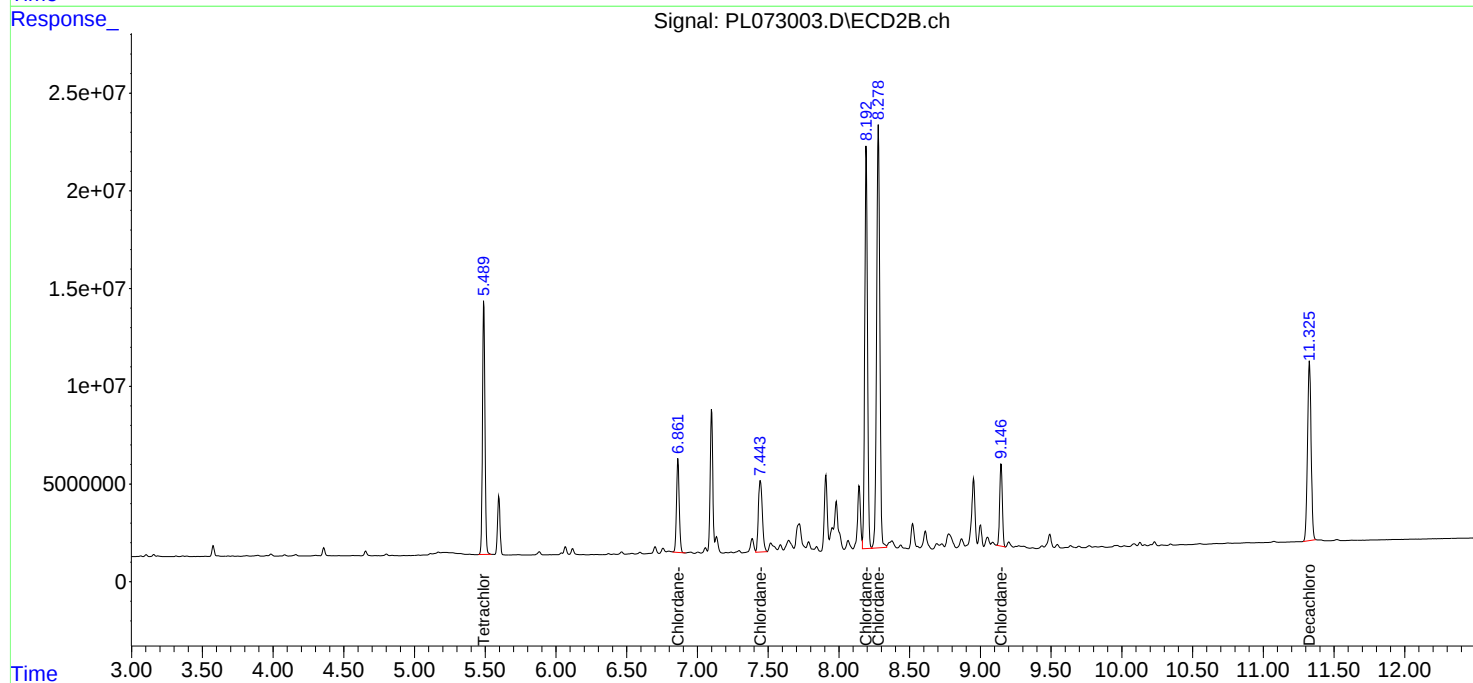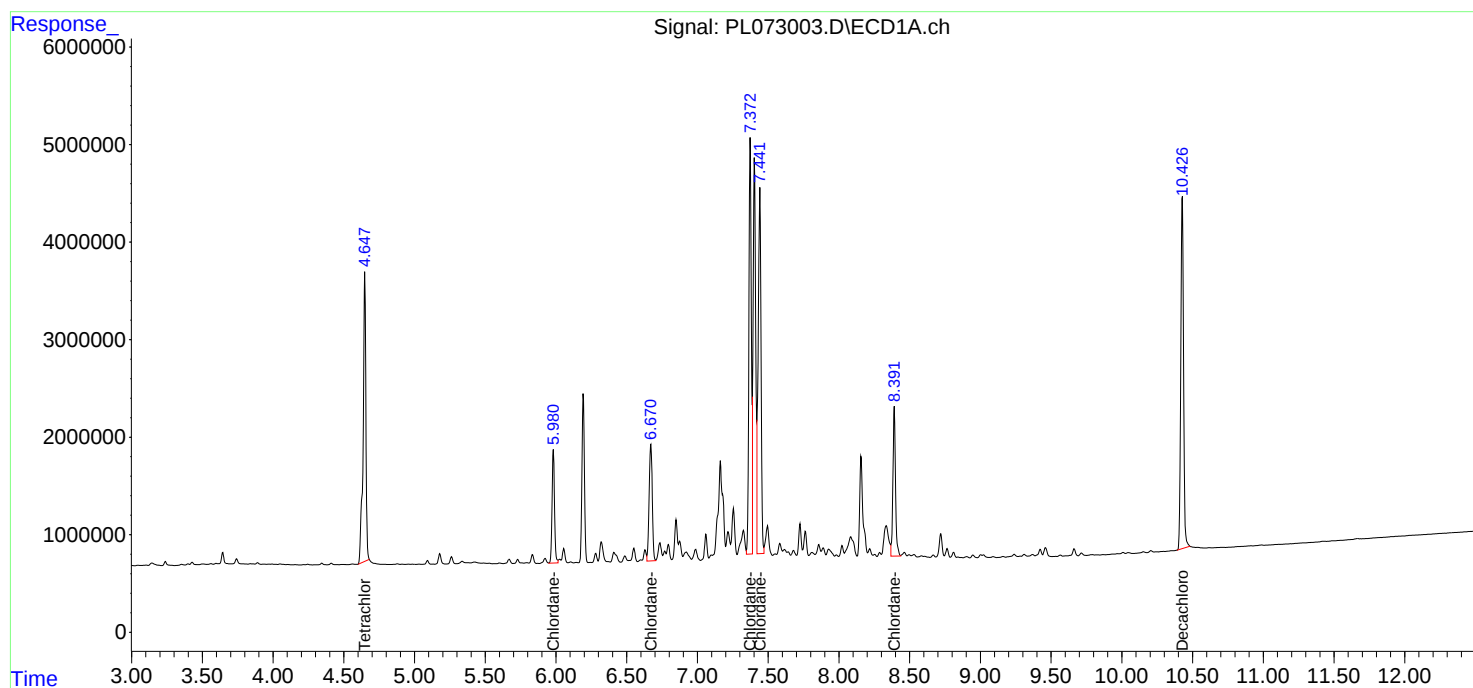


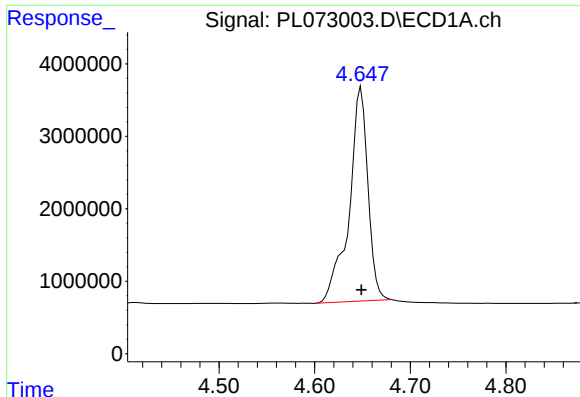

#1 Tetrachloro-m-xylene


R.T.: 4.649 min
Delta R.T.: 0.000 min
Response: 40460364
Conc: 100.86 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

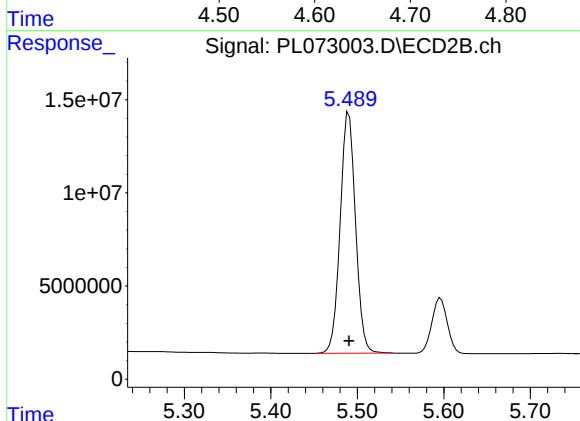


#1 Tetrachloro-m-xylene

R.T.: 5.490 min
Delta R.T.: 0.000 min
Response: 158413035
Conc: 101.25 ng/ml

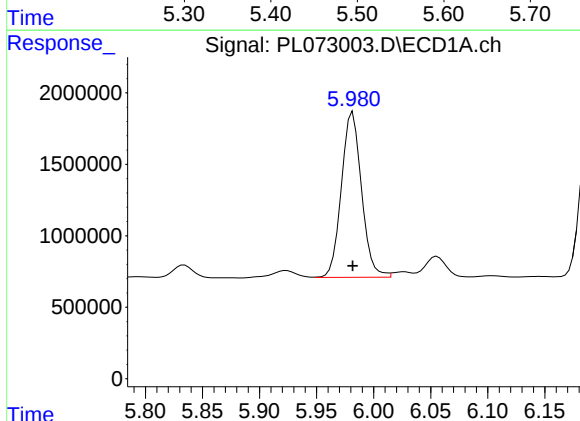


#23 Chlordane-1

R.T.: 5.982 min
Delta R.T.: 0.000 min
Response: 14207598
Conc: 998.39 ng/ml

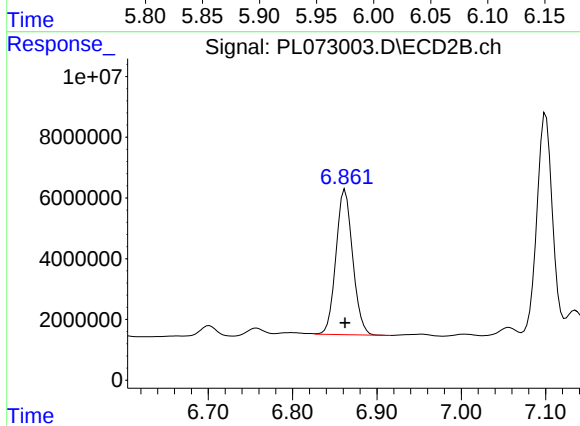

#23 Chlordane-1


R.T.: 6.862 min
Delta R.T.: 0.000 min
Response: 65790988
Conc: 1004.39 ng/ml

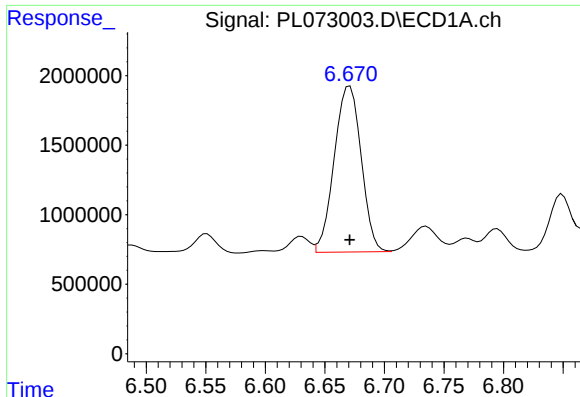

#24 Chlordane-2


R.T.: 6.671 min
Delta R.T.: 0.000 min
Response: 18758755
Conc: 982.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

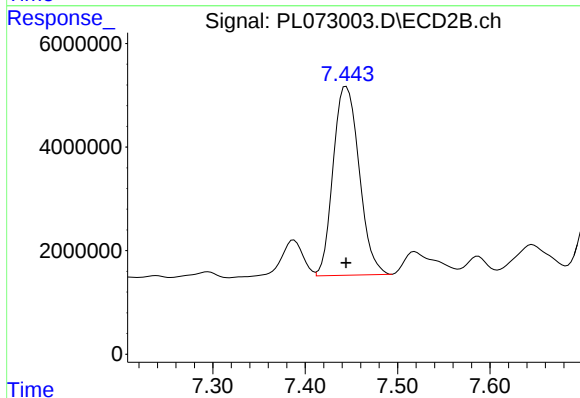


#24 Chlordane-2

R.T.: 7.444 min
Delta R.T.: 0.000 min
Response: 71385215
Conc: 986.14 ng/ml

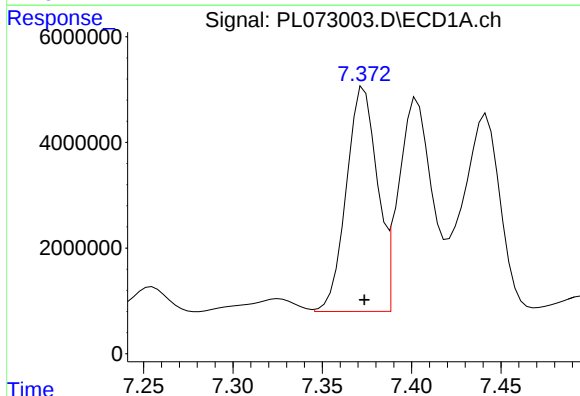


#25 Chlordane-3

R.T.: 7.373 min
Delta R.T.: 0.000 min
Response: 51141456
Conc: 1019.80 ng/ml

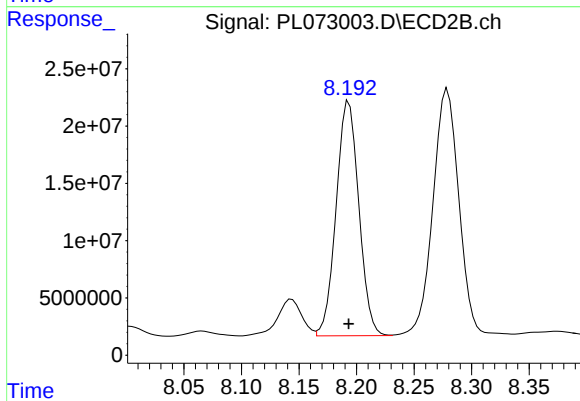

#25 Chlordane-3


R.T.: 8.193 min
Delta R.T.: 0.000 min
Response: 281679689
Conc: 1023.60 ng/ml

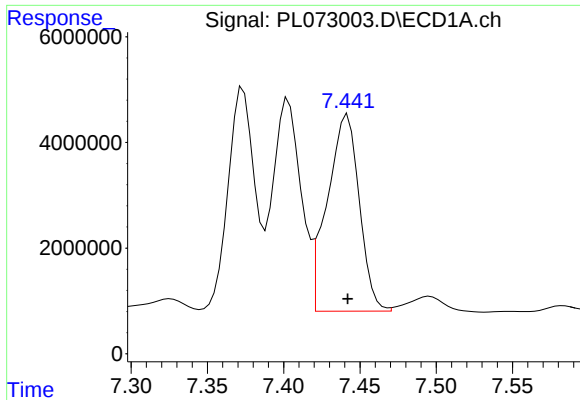

#26 Chlordane-4


R.T.: 7.442 min
Delta R.T.: 0.000 min
Response: 54319250
Conc: 1017.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

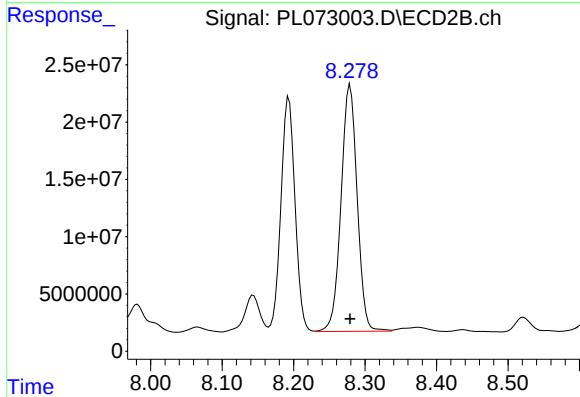


#26 Chlordane-4

R.T.: 8.279 min
Delta R.T.: 0.000 min
Response: 337119416
Conc: 1014.93 ng/ml

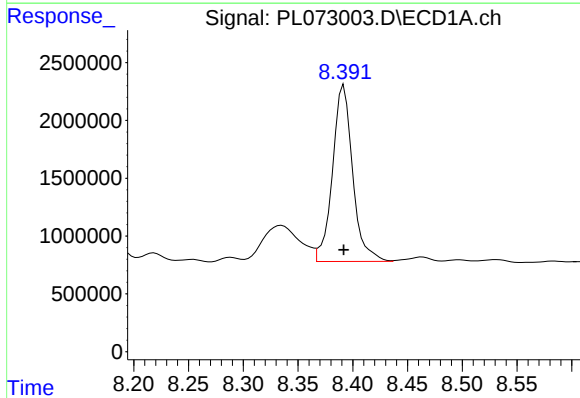


#27 Chlordane-5

R.T.: 8.392 min
Delta R.T.: 0.000 min
Response: 19544620
Conc: 1002.84 ng/ml

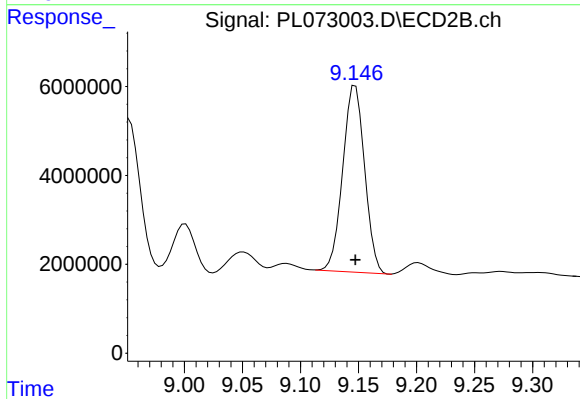

#27 Chlordane-5


R.T.: 9.147 min
Delta R.T.: 0.000 min
Response: 55073822
Conc: 1012.76 ng/ml

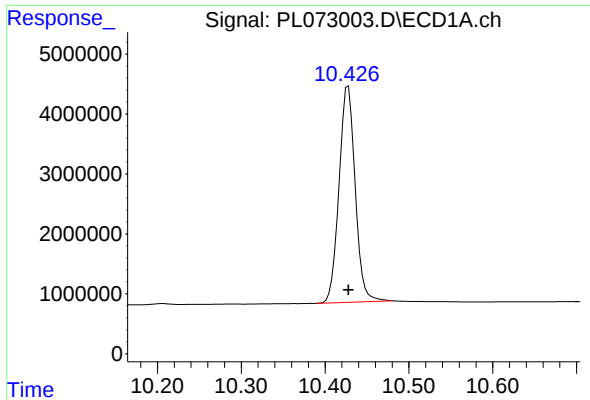

#28 Decachlorobiphenyl

R.T.: 10.428 min
Delta R.T.: 0.000 min
Response: 48356669
Conc: 98.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

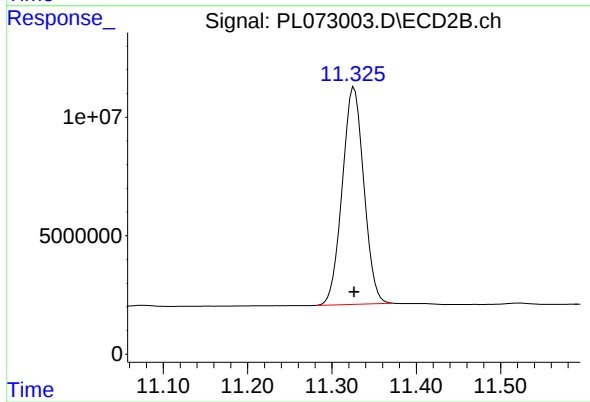

#28 Decachlorobiphenyl

R.T.: 11.326 min
Delta R.T.: 0.000 min
Response: 163062001
Conc: 99.13 ng/ml