

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022622\
 Data File : PL073004.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Feb 2022 04:47
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 27 10:57:29 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022622.M
 Quant Title : GC Extractables
 QLast Update : Sun Feb 27 10:57:20 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.648	5.490	29308450	114.6E6	73.696	73.823
28)	SA Decachlor...	10.427	11.327	35823046	120.2E6	73.739	73.720
Target Compounds							
23)	Chlordane-1	5.981	6.862	10382008	47558568	736.247	733.858
24)	Chlordane-2	6.671	7.445	13927761	52986422	736.413	737.883
25)	Chlordane-3	7.373	8.193	36968777	202.0E6	741.409	739.188
26)	Chlordane-4	7.442	8.279	39164460	243.9E6	739.163	739.470
27)	Chlordane-5	8.391	9.147	14306557	39740118	739.305	737.081



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022622\
Data File : PL073004.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Feb 2022 04:47
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 27 10:57:29 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022622.M
Quant Title : GC Extractables
QLast Update : Sun Feb 27 10:57:20 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

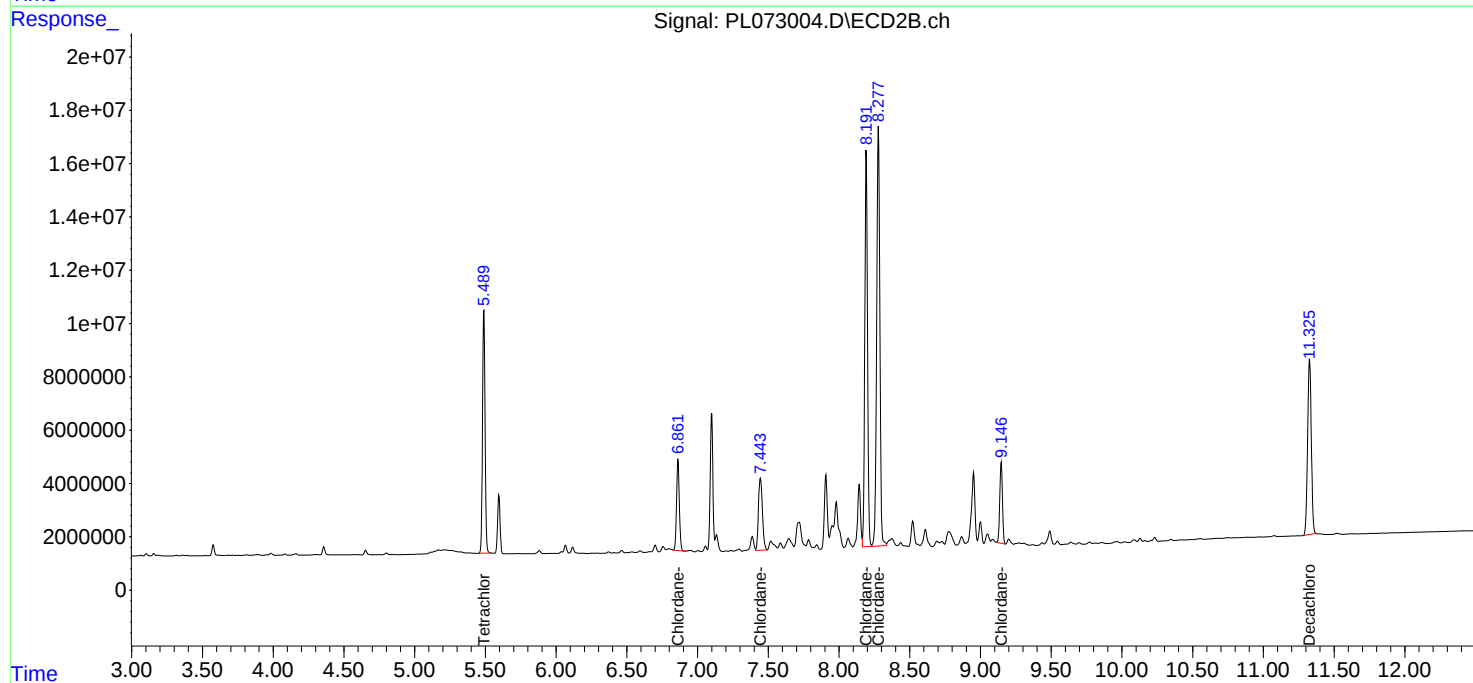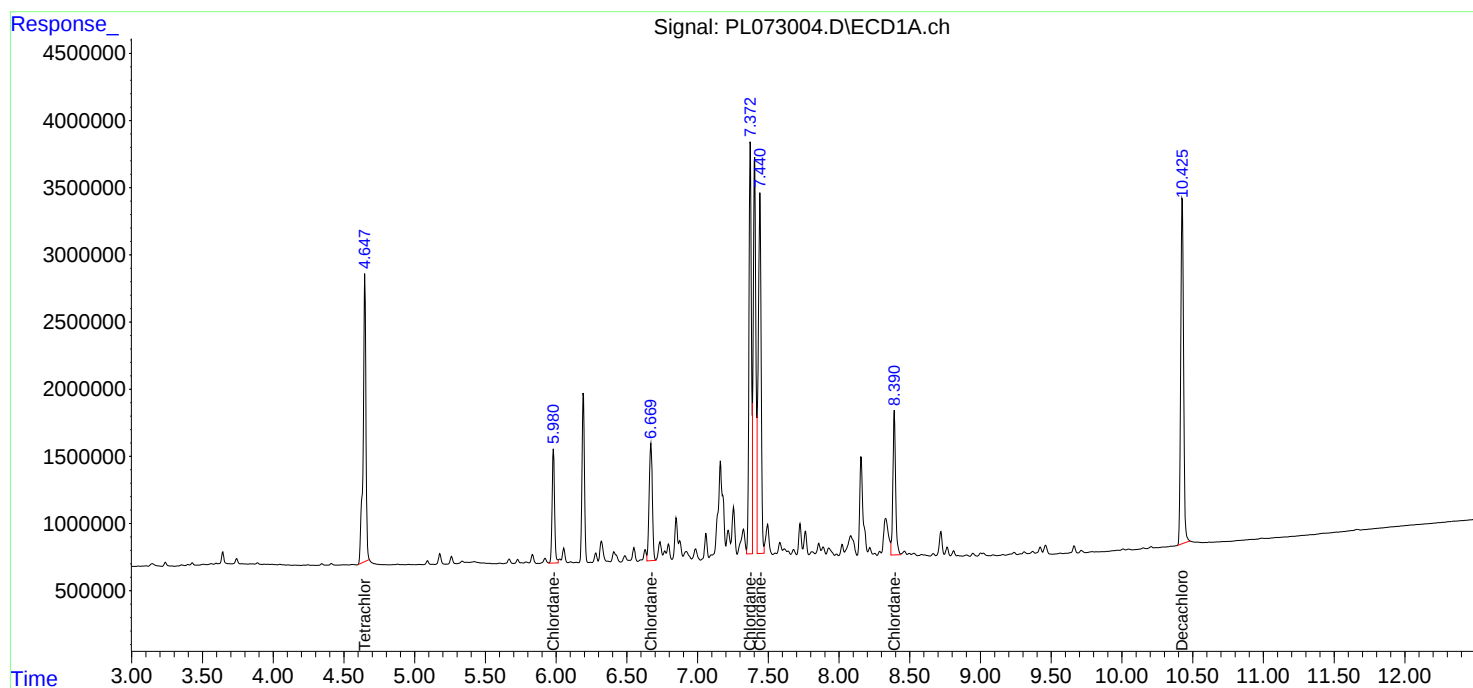


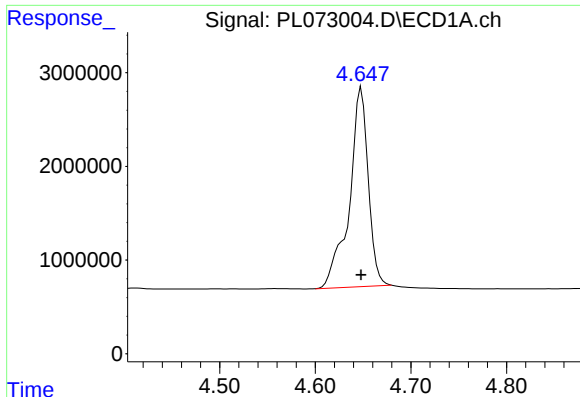

#1 Tetrachloro-m-xylene


R.T.: 4.648 min
Delta R.T.: 0.000 min
Response: 29308450
Conc: 73.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

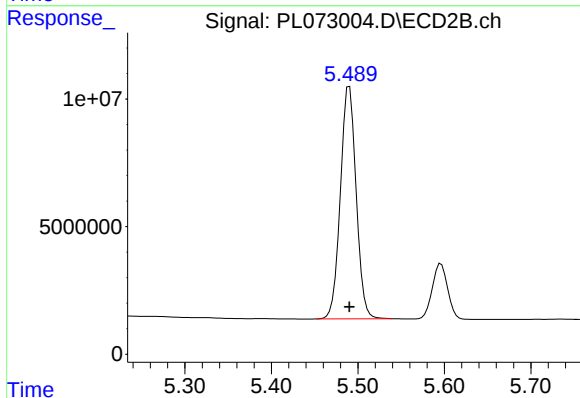


#1 Tetrachloro-m-xylene

R.T.: 5.490 min
Delta R.T.: 0.000 min
Response: 114601665
Conc: 73.82 ng/ml

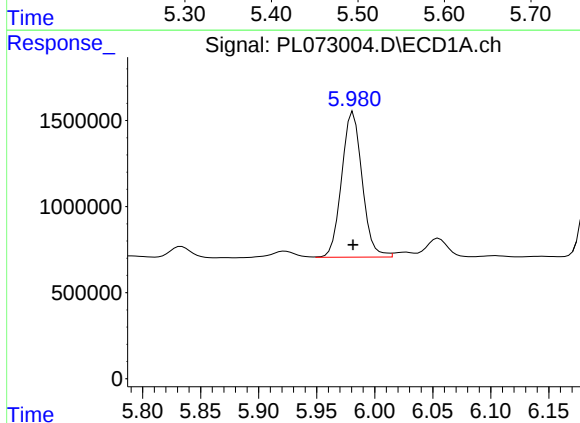


#23 Chlordane-1

R.T.: 5.981 min
Delta R.T.: 0.000 min
Response: 10382008
Conc: 736.25 ng/ml

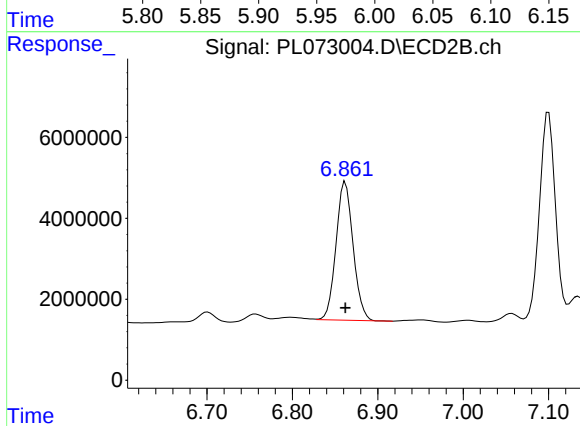

#23 Chlordane-1


R.T.: 6.862 min
Delta R.T.: 0.000 min
Response: 47558568
Conc: 733.86 ng/ml

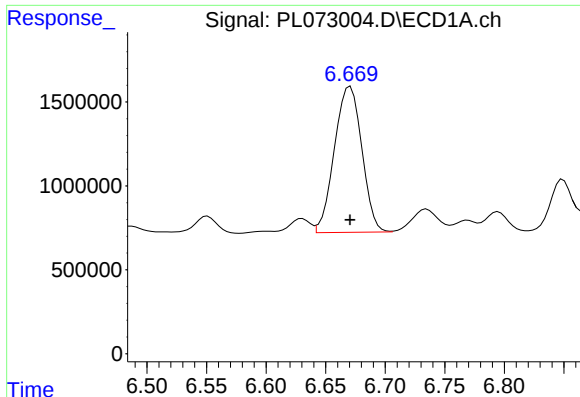

#24 Chlordane-2


R.T.: 6.671 min
Delta R.T.: 0.000 min
Response: 13927761
Conc: 736.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

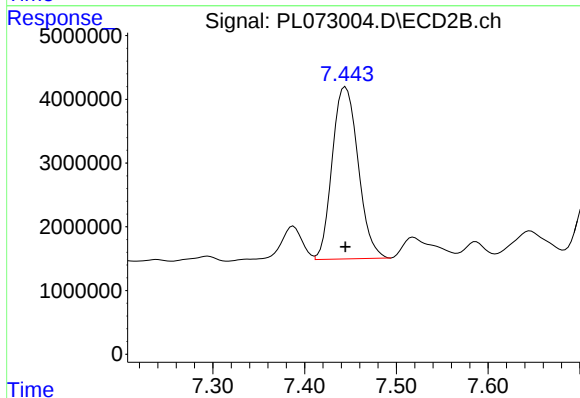


#24 Chlordane-2

R.T.: 7.445 min
Delta R.T.: 0.000 min
Response: 52986422
Conc: 737.88 ng/ml

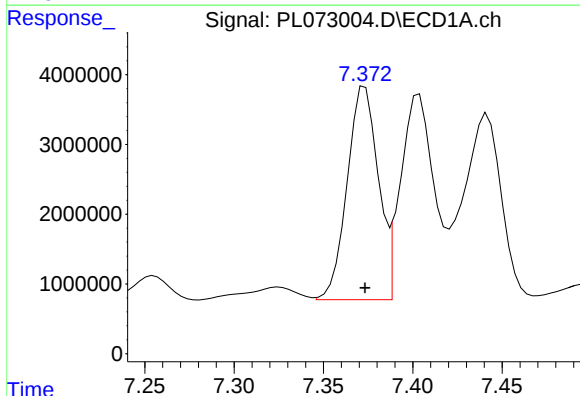


#25 Chlordane-3

R.T.: 7.373 min
Delta R.T.: 0.000 min
Response: 36968777
Conc: 741.41 ng/ml

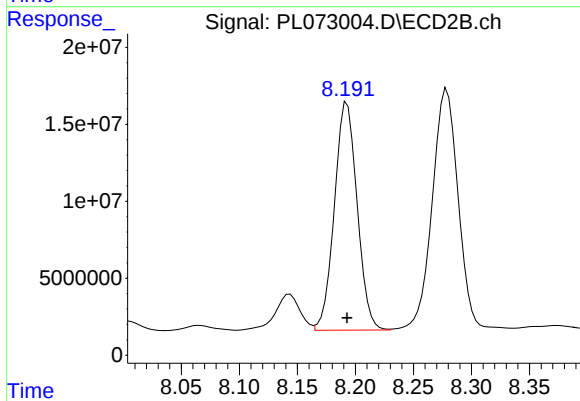

#25 Chlordane-3


R.T.: 8.193 min
Delta R.T.: 0.000 min
Response: 201956919
Conc: 739.19 ng/ml

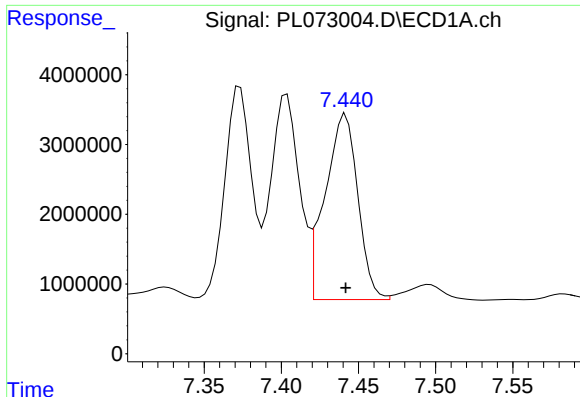

#26 Chlordane-4


R.T.: 7.442 min
Delta R.T.: 0.000 min
Response: 39164460
Conc: 739.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

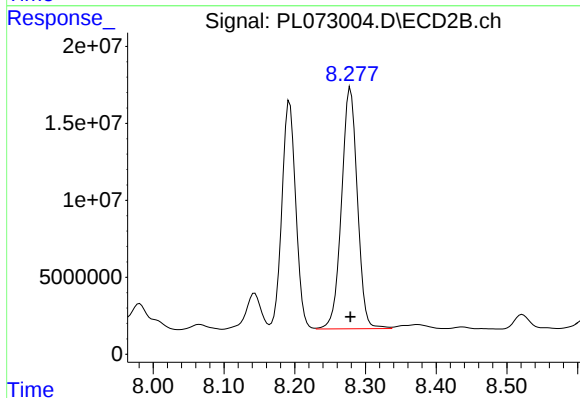


#26 Chlordane-4

R.T.: 8.279 min
Delta R.T.: 0.000 min
Response: 243911247
Conc: 739.47 ng/ml

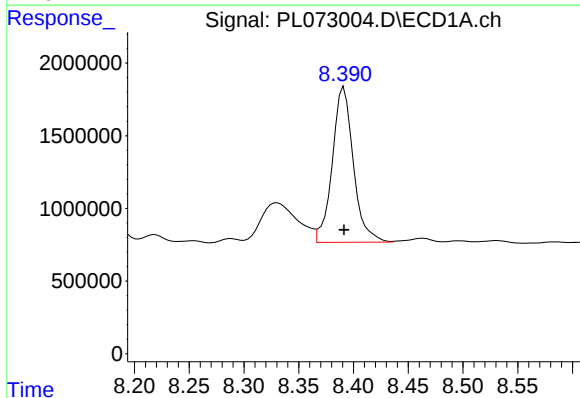


#27 Chlordane-5

R.T.: 8.391 min
Delta R.T.: 0.000 min
Response: 14306557
Conc: 739.31 ng/ml

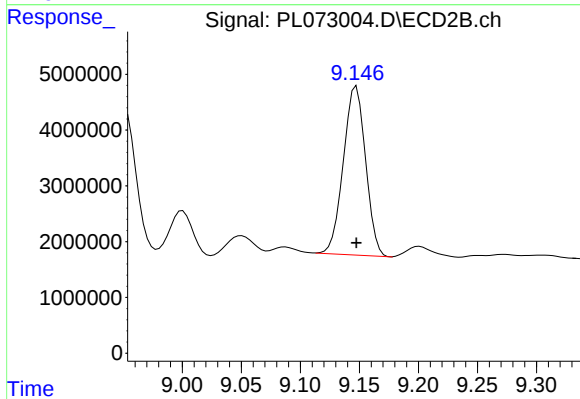

#27 Chlordane-5


R.T.: 9.147 min
Delta R.T.: 0.000 min
Response: 39740118
Conc: 737.08 ng/ml

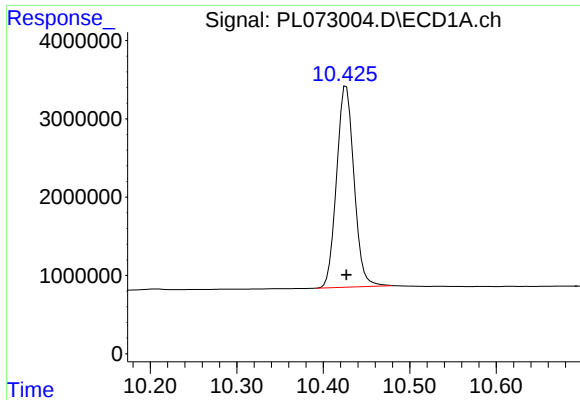

#28 Decachlorobiphenyl

R.T.: 10.427 min
Delta R.T.: 0.000 min
Response: 35823046
Conc: 73.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

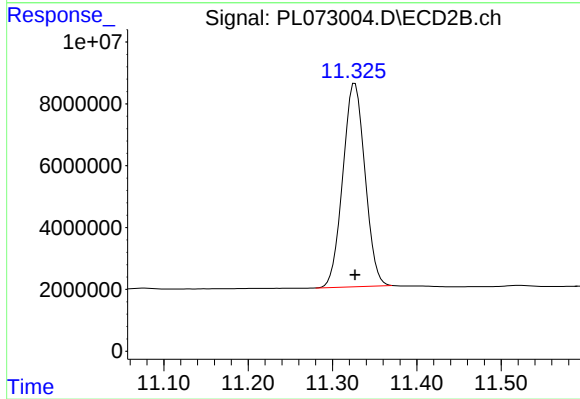

#28 Decachlorobiphenyl

R.T.: 11.327 min
Delta R.T.: 0.000 min
Response: 120232752
Conc: 73.72 ng/ml