

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022622\
 Data File : PL073005.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Feb 2022 05:03
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 26 14:31:04 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022622.M
 Quant Title : GC Extractables
 QLast Update : Sat Feb 26 14:29:27 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.647	5.491	19885280	77250554	50.000	50.000
28)	SA Decachlor...	10.426	11.326	24810992	82954557	50.000	50.000
Target Compounds							
23)	Chlordane-1	5.980	6.862	7126739	32608110	500.000	500.000
24)	Chlordane-2	6.669	7.444	9704923	36696233	500.000	500.000
25)	Chlordane-3	7.372	8.193	24577716	134.3E6	500.000	500.000
26)	Chlordane-4	7.441	8.279	26208020	163.6E6	500.000	500.000
27)	Chlordane-5	8.391	9.147	9717024	26842963	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022622\
Data File : PL073005.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Feb 2022 05:03
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 26 14:31:04 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022622.M
Quant Title : GC Extractables
QLast Update : Sat Feb 26 14:29:27 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

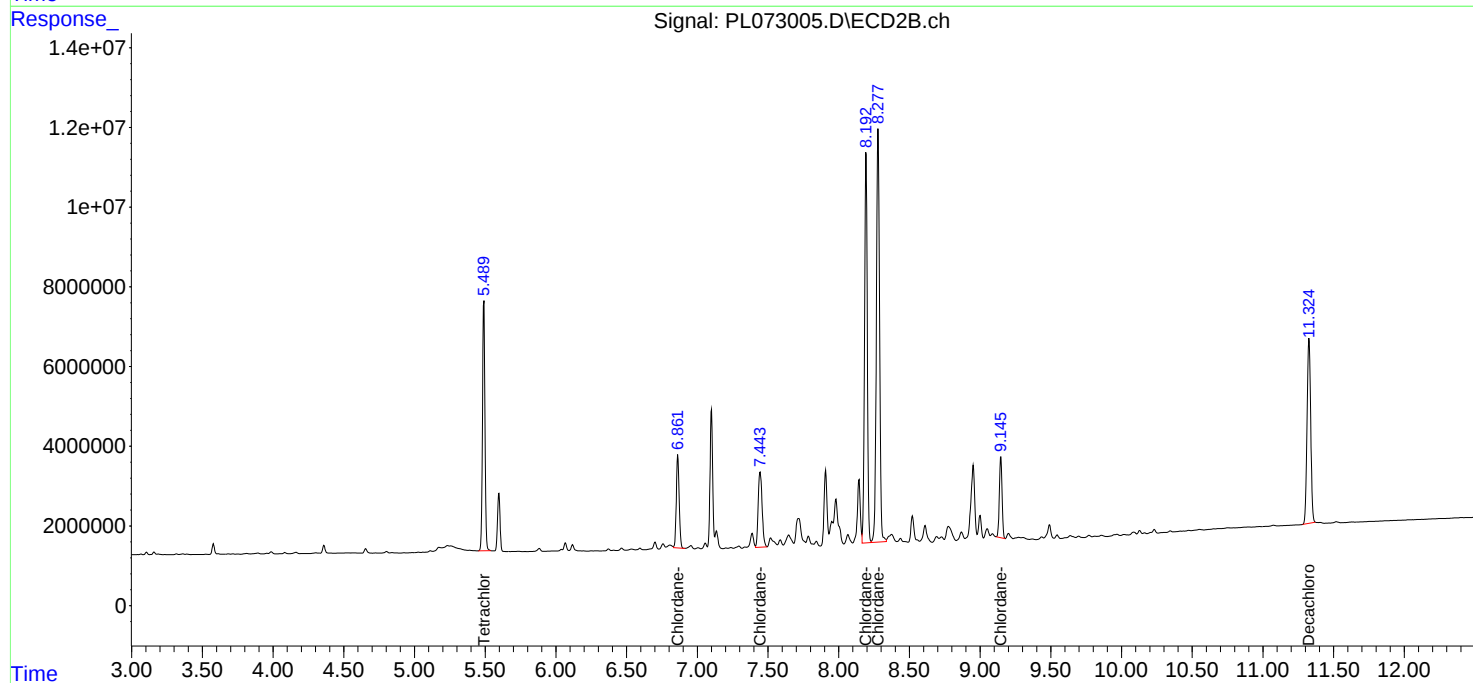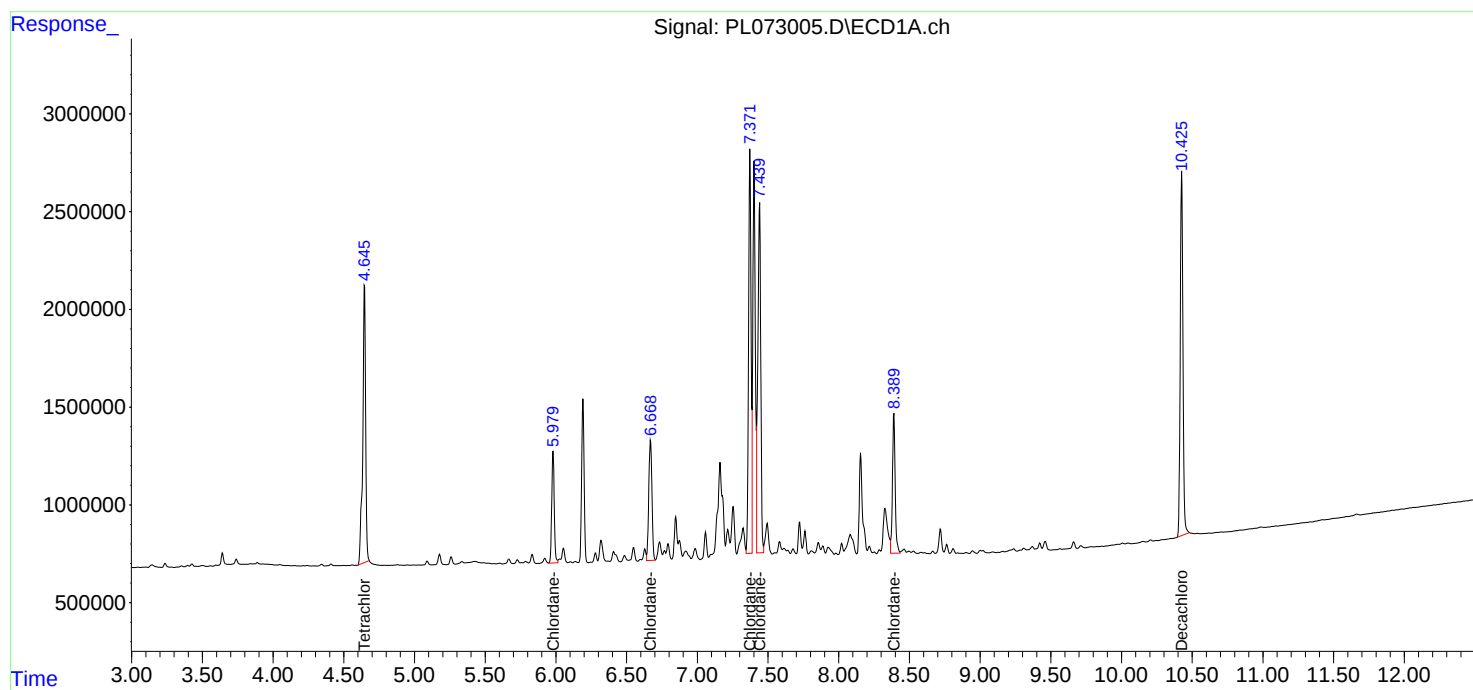


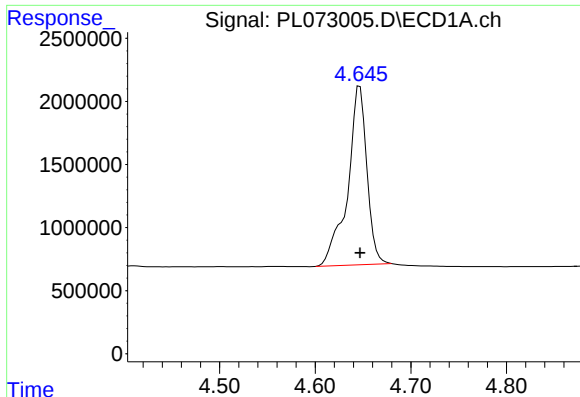

#1 Tetrachloro-m-xylene


R.T.: 4.647 min
Delta R.T.: 0.000 min
Response: 19885280
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

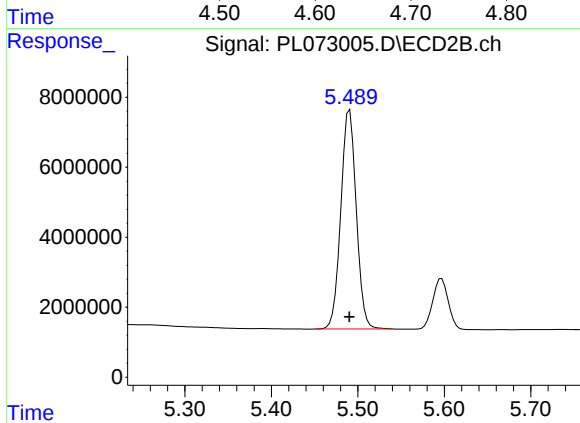


#1 Tetrachloro-m-xylene

R.T.: 5.491 min
Delta R.T.: 0.000 min
Response: 77250554
Conc: 50.00 ng/ml

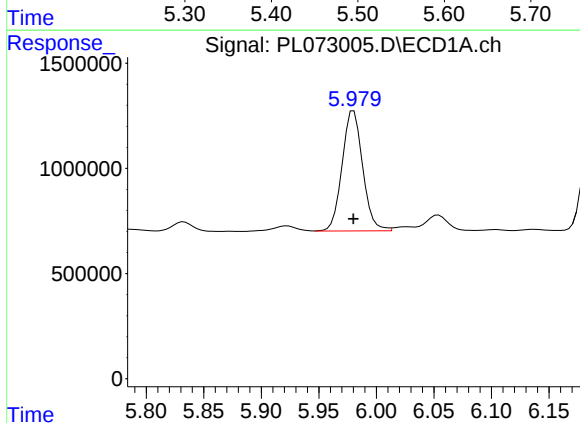


#23 Chlordane-1

R.T.: 5.980 min
Delta R.T.: 0.000 min
Response: 7126739
Conc: 500.00 ng/ml

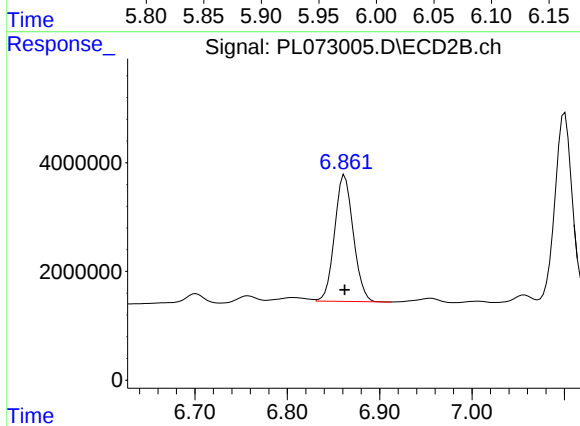

#23 Chlordane-1


R.T.: 6.862 min
Delta R.T.: 0.000 min
Response: 32608110
Conc: 500.00 ng/ml

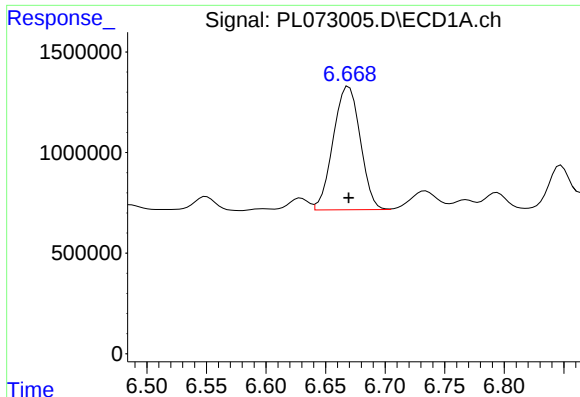

#24 Chlordane-2


R.T.: 6.669 min
Delta R.T.: 0.000 min
Response: 9704923
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

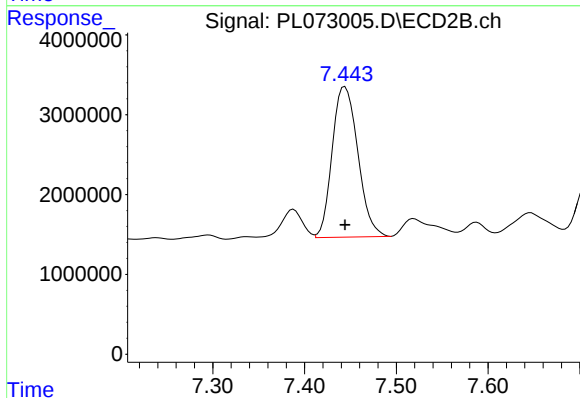


#24 Chlordane-2

R.T.: 7.444 min
Delta R.T.: 0.000 min
Response: 36696233
Conc: 500.00 ng/ml

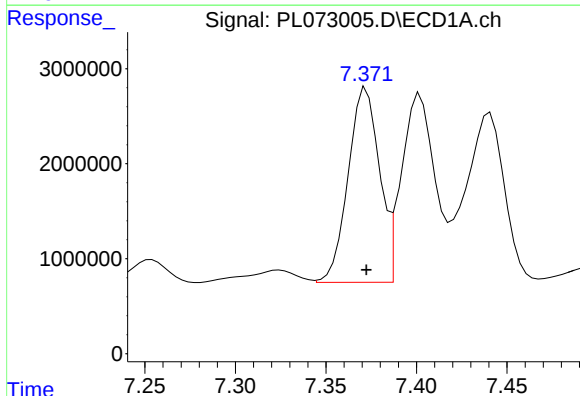


#25 Chlordane-3

R.T.: 7.372 min
Delta R.T.: 0.000 min
Response: 24577716
Conc: 500.00 ng/ml

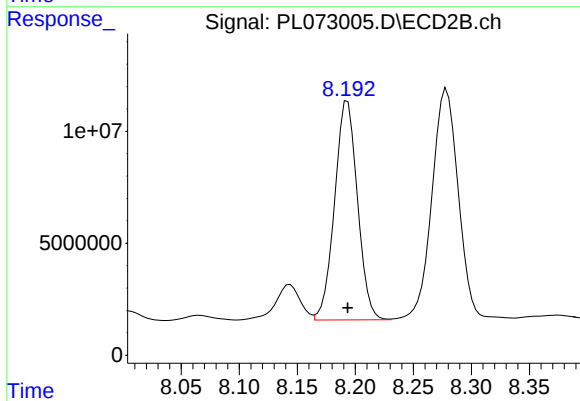

#25 Chlordane-3


R.T.: 8.193 min
Delta R.T.: 0.000 min
Response: 134344184
Conc: 500.00 ng/ml

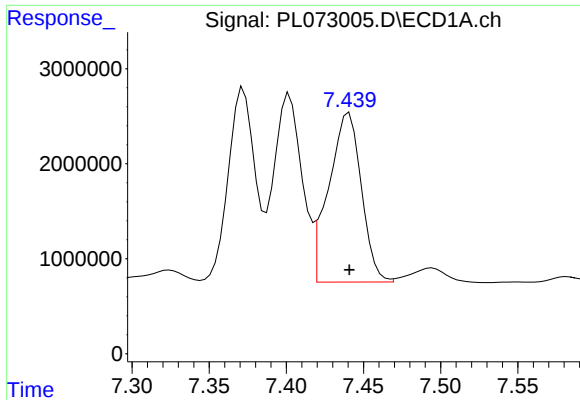

#26 Chlordane-4


R.T.: 7.441 min
Delta R.T.: 0.000 min
Response: 26208020
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

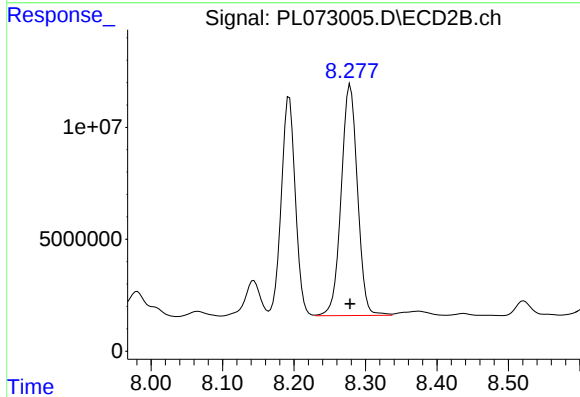


#26 Chlordane-4

R.T.: 8.279 min
Delta R.T.: 0.000 min
Response: 163601687
Conc: 500.00 ng/ml

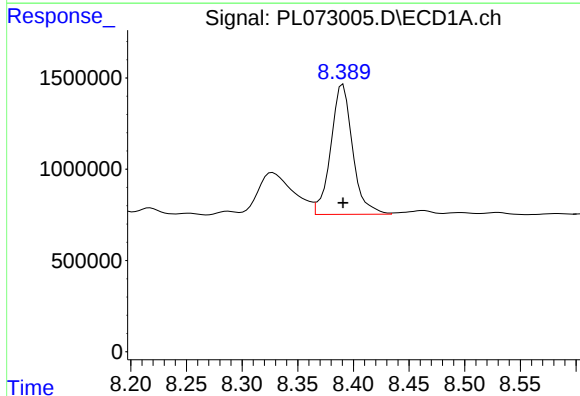


#27 Chlordane-5

R.T.: 8.391 min
Delta R.T.: 0.000 min
Response: 9717024
Conc: 500.00 ng/ml

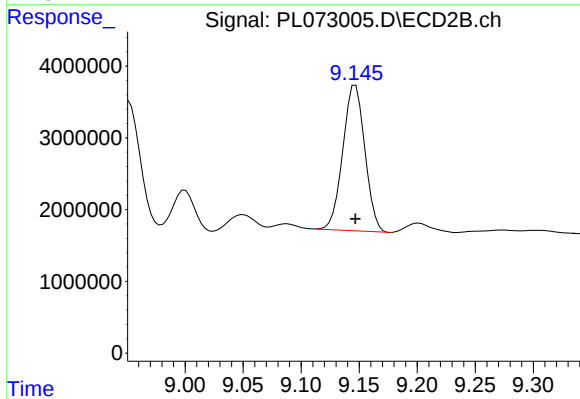

#27 Chlordane-5


R.T.: 9.147 min
Delta R.T.: 0.000 min
Response: 26842963
Conc: 500.00 ng/ml

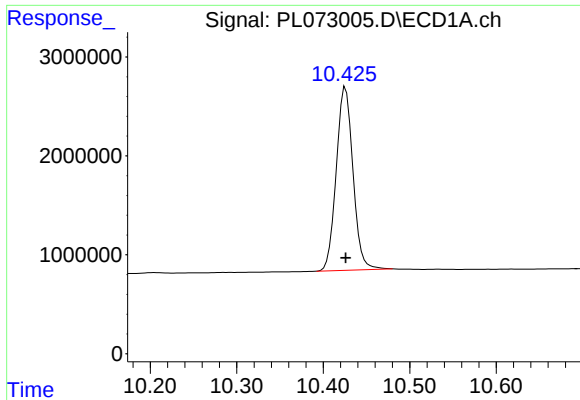

#28 Decachlorobiphenyl

R.T.: 10.426 min
Delta R.T.: 0.000 min
Response: 24810992
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

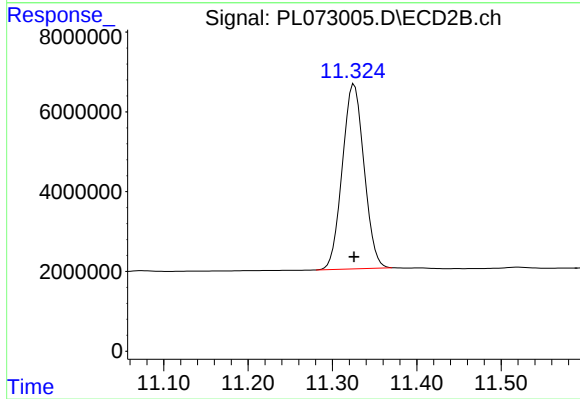

#28 Decachlorobiphenyl

R.T.: 11.326 min
Delta R.T.: 0.000 min
Response: 82954557
Conc: 50.00 ng/ml