

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022622\
 Data File : PL073006.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Feb 2022 05:20
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 27 10:59:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022622.M
 Quant Title : GC Extractables
 QLast Update : Sun Feb 27 10:59:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.648	5.490	9698916	37883179	24.538	24.550
28)	SA Decachlor...	10.426	11.325	12806468	43070030	26.007	26.041
Target Compounds							
23)	Chlordane-1	5.981	6.862	3657241	16482989	256.952	253.243
24)	Chlordane-2	6.671	7.444	5107936	19107701	264.760	261.878
25)	Chlordane-3	7.373	8.193	11919781	65151498	241.698	241.246
26)	Chlordane-4	7.442	8.279	12852071	80829874	244.379	246.272
27)	Chlordane-5	8.391	9.146	5139393	13403315	261.508	248.947


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022622\
Data File : PL073006.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Feb 2022 05:20
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 27 10:59:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022622.M
Quant Title : GC Extractables
QLast Update : Sun Feb 27 10:59:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

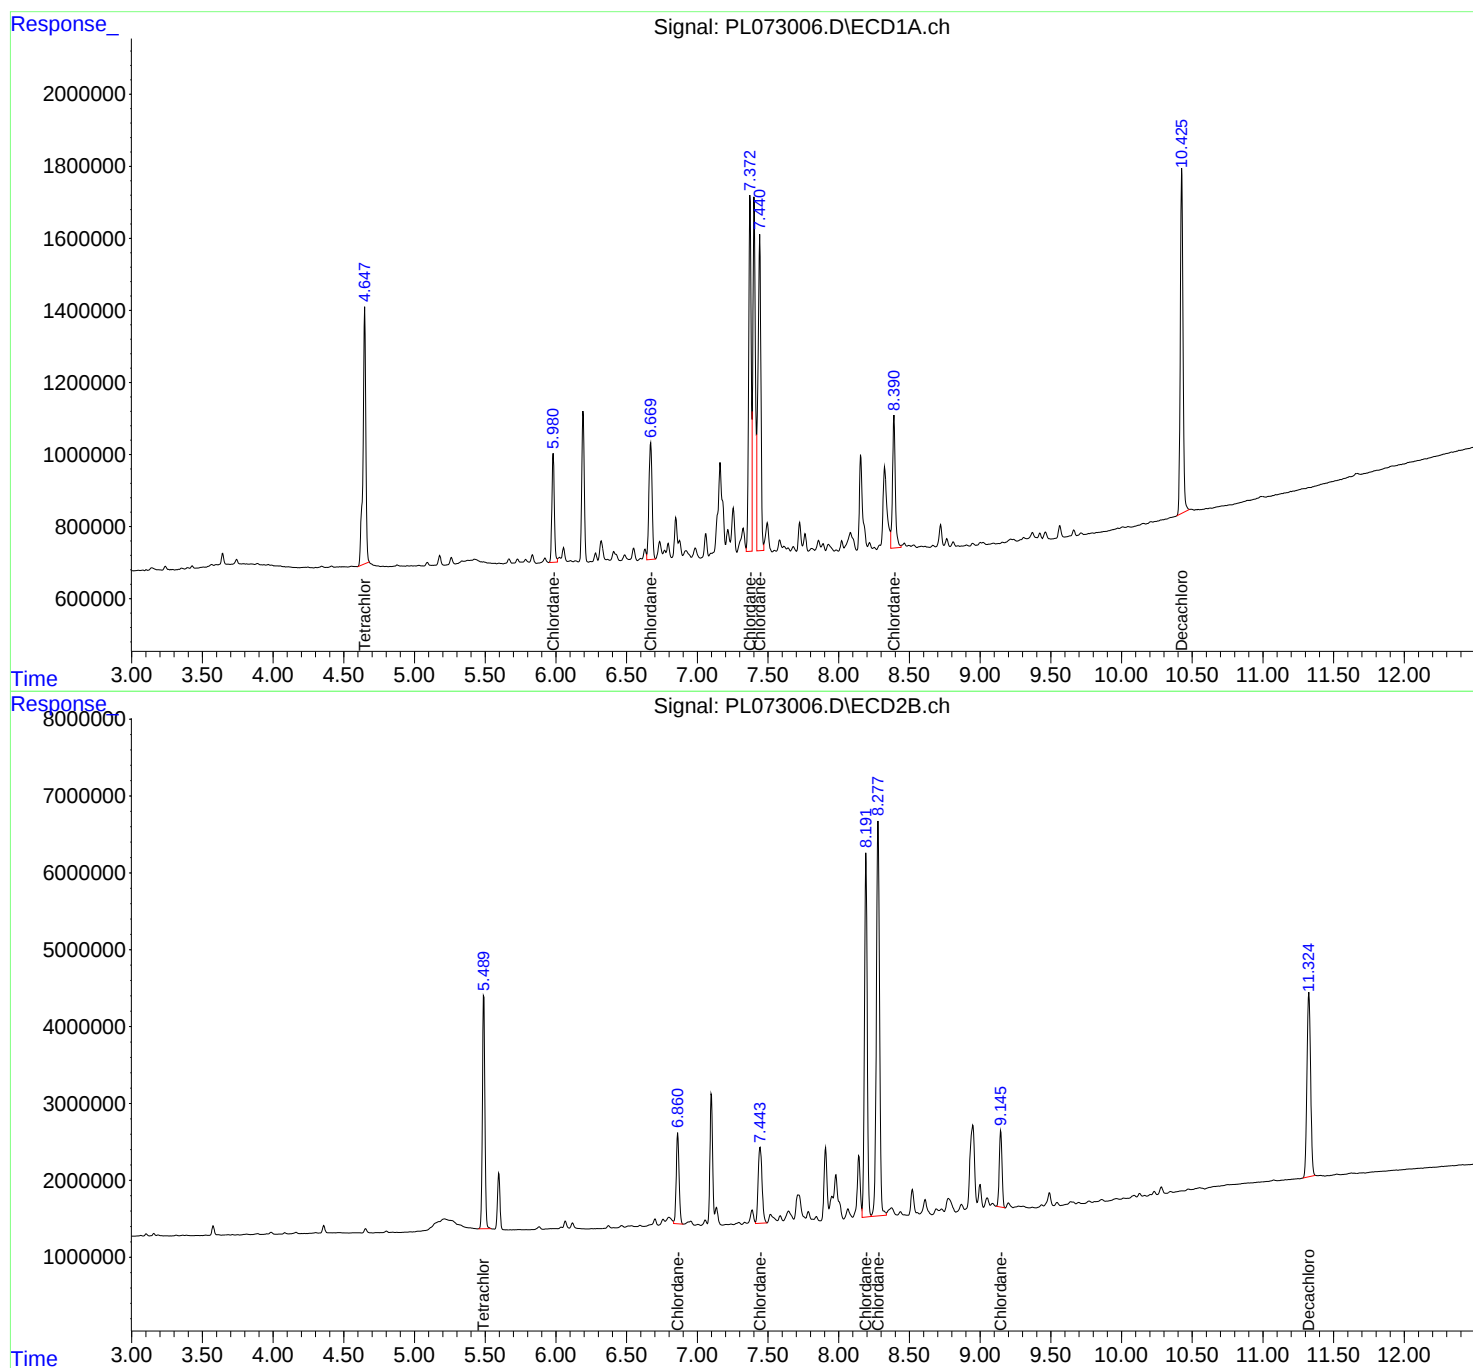


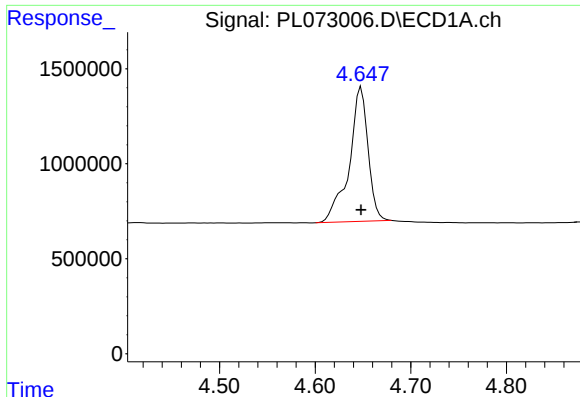

#1 Tetrachloro-m-xylene


R.T.: 4.648 min
Delta R.T.: 0.000 min
Response: 9698916
Conc: 24.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

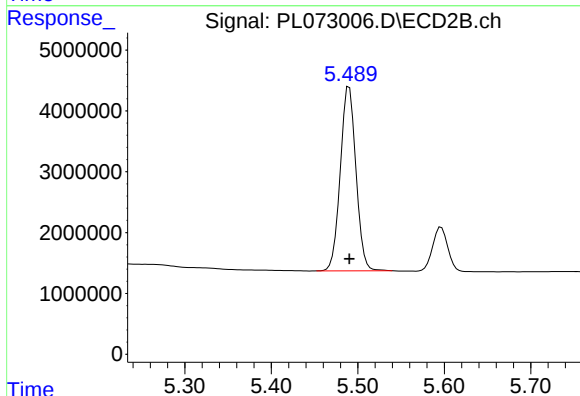


#1 Tetrachloro-m-xylene

R.T.: 5.490 min
Delta R.T.: 0.000 min
Response: 37883179
Conc: 24.55 ng/ml

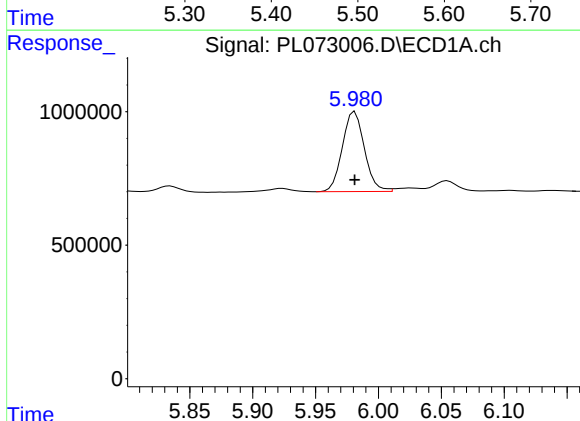


#23 Chlordane-1

R.T.: 5.981 min
Delta R.T.: 0.000 min
Response: 3657241
Conc: 256.95 ng/ml

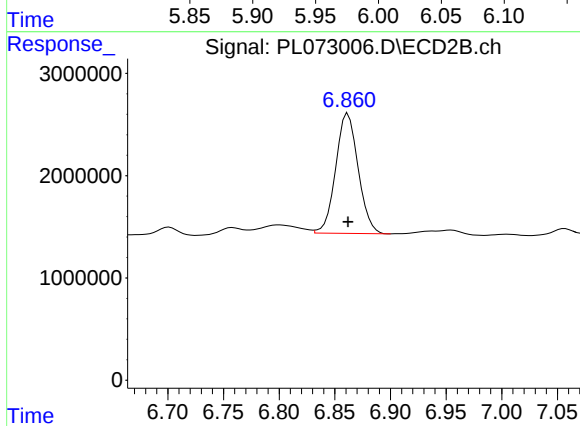

#23 Chlordane-1


R.T.: 6.862 min
Delta R.T.: 0.000 min
Response: 16482989
Conc: 253.24 ng/ml

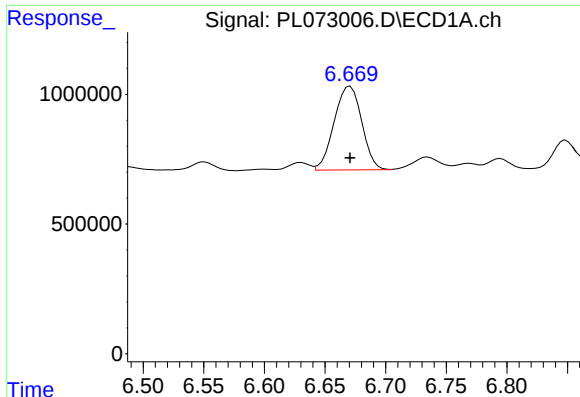

#24 Chlordane-2


R.T.: 6.671 min
Delta R.T.: 0.000 min
Response: 5107936
Conc: 264.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

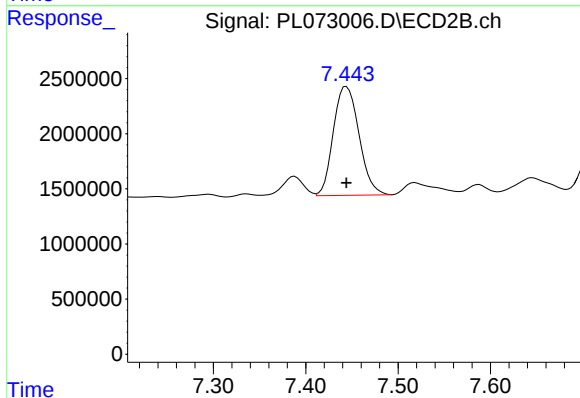


#24 Chlordane-2

R.T.: 7.444 min
Delta R.T.: 0.000 min
Response: 19107701
Conc: 261.88 ng/ml

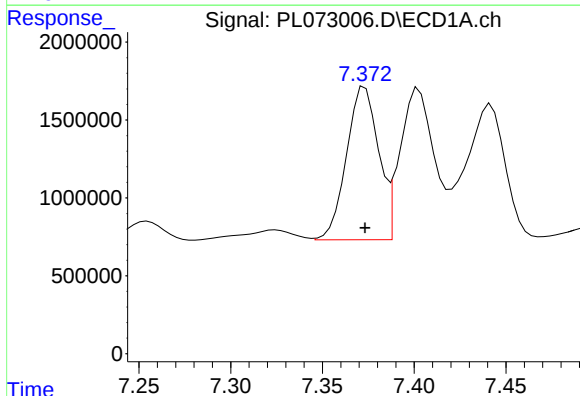


#25 Chlordane-3

R.T.: 7.373 min
Delta R.T.: 0.000 min
Response: 11919781
Conc: 241.70 ng/ml

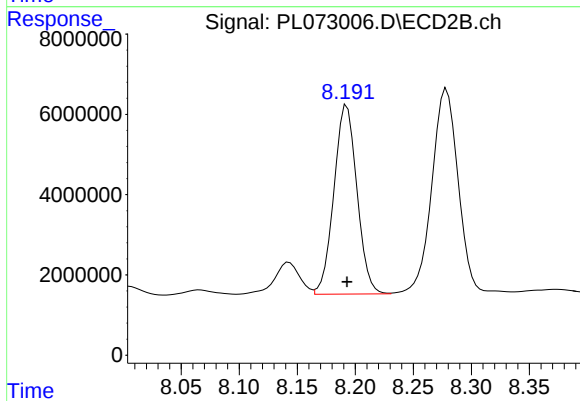

#25 Chlordane-3


R.T.: 8.193 min
Delta R.T.: 0.000 min
Response: 65151498
Conc: 241.25 ng/ml

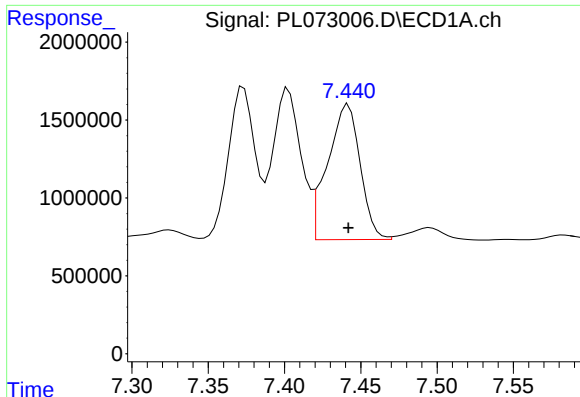

#26 Chlordane-4


R.T.: 7.442 min
Delta R.T.: 0.000 min
Response: 12852071
Conc: 244.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

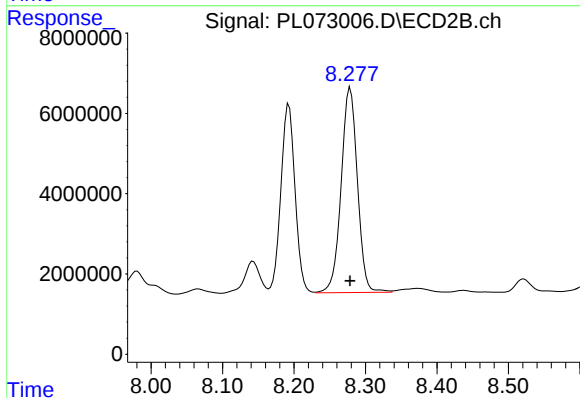


#26 Chlordane-4

R.T.: 8.279 min
Delta R.T.: 0.000 min
Response: 80829874
Conc: 246.27 ng/ml

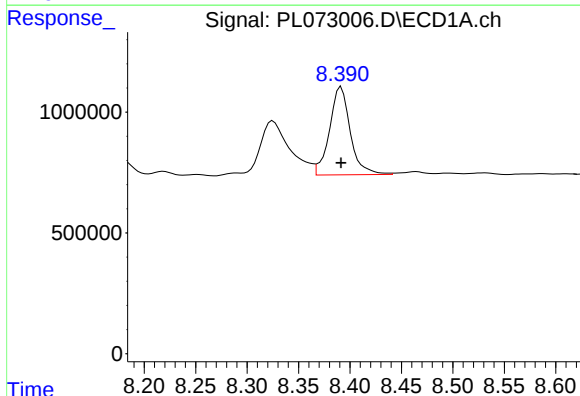


#27 Chlordane-5

R.T.: 8.391 min
Delta R.T.: 0.000 min
Response: 5139393
Conc: 261.51 ng/ml

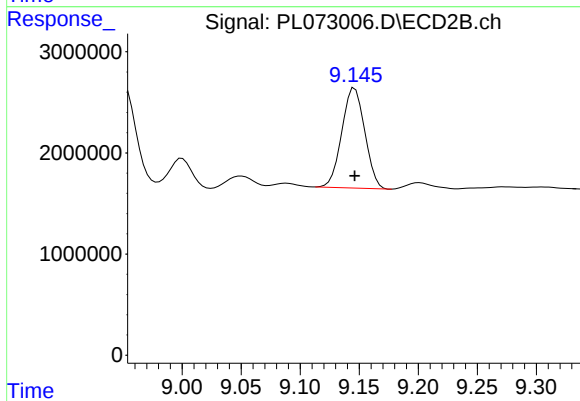

#27 Chlordane-5


R.T.: 9.146 min
Delta R.T.: 0.000 min
Response: 13403315
Conc: 248.95 ng/ml

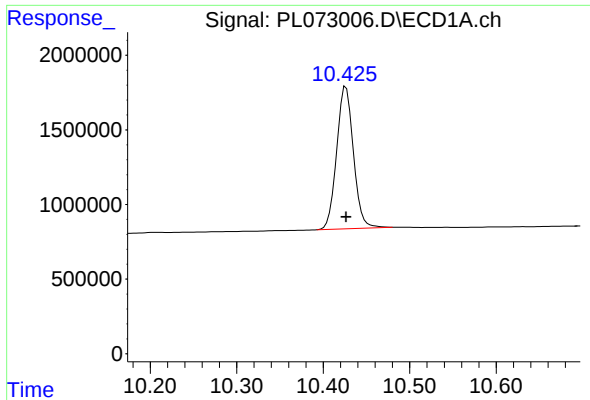

#28 Decachlorobiphenyl

R.T.: 10.426 min
Delta R.T.: 0.000 min
Response: 12806468
Conc: 26.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

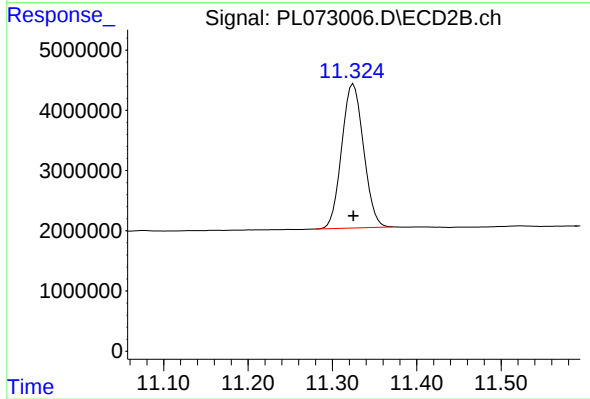

#28 Decachlorobiphenyl

R.T.: 11.325 min
Delta R.T.: 0.000 min
Response: 43070030
Conc: 26.04 ng/ml