

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022624\
Data File : PL088291.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Feb 2024 16:19
Operator : AR\AJ
Sample : P1524-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
20240768-AMENDED-COMP-39N-N-3-03

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 26 23:56:35 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021524.M
Quant Title : GC Extractables
QLast Update : Fri Feb 16 21:46:54 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.634	2.853	53557262	28306443	19.499	20.183
28)	SA Decachlor...	9.300	8.083	41730177	24122953	21.668	18.945

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022624\
Data File : PL088291.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Feb 2024 16:19
Operator : AR\AJ
Sample : P1524-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
20240768-AMENDED-COMP-39N-N-3-03

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 26 23:56:35 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021524.M
Quant Title : GC Extractables
QLast Update : Fri Feb 16 21:46:54 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

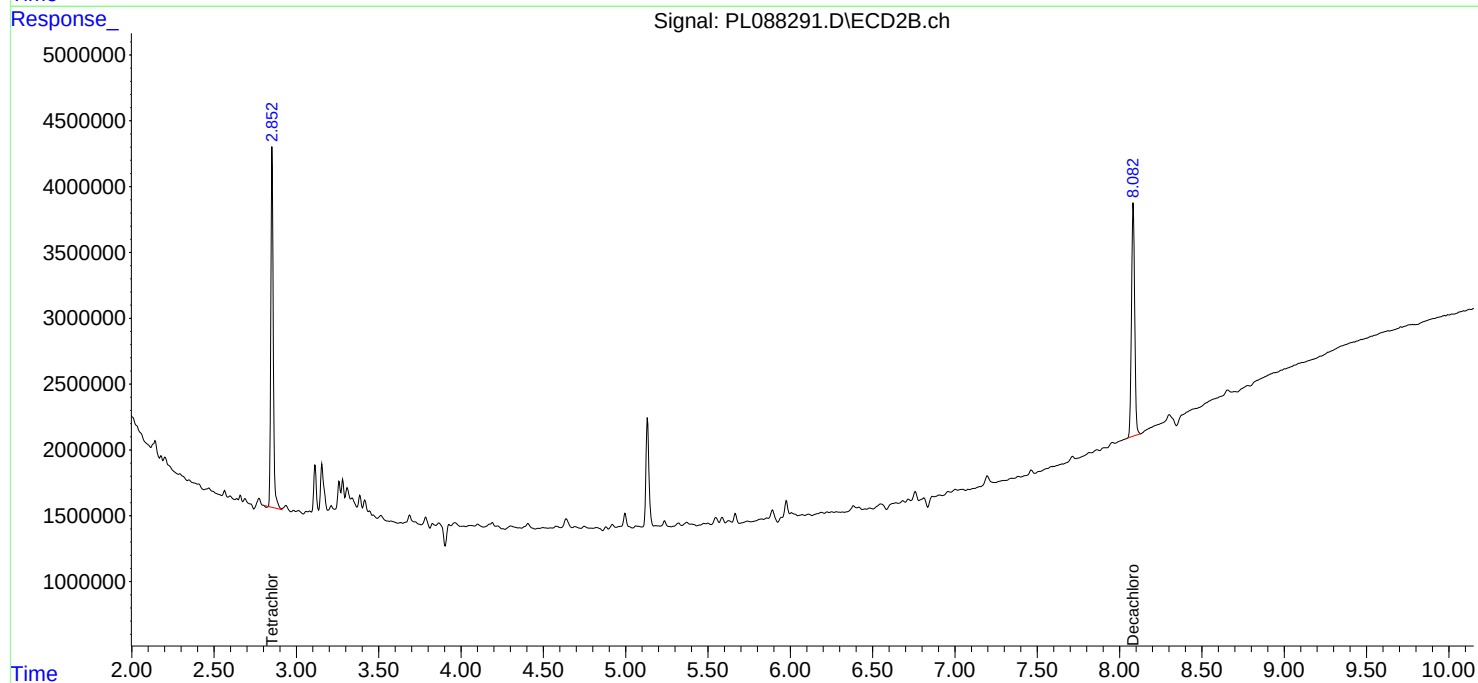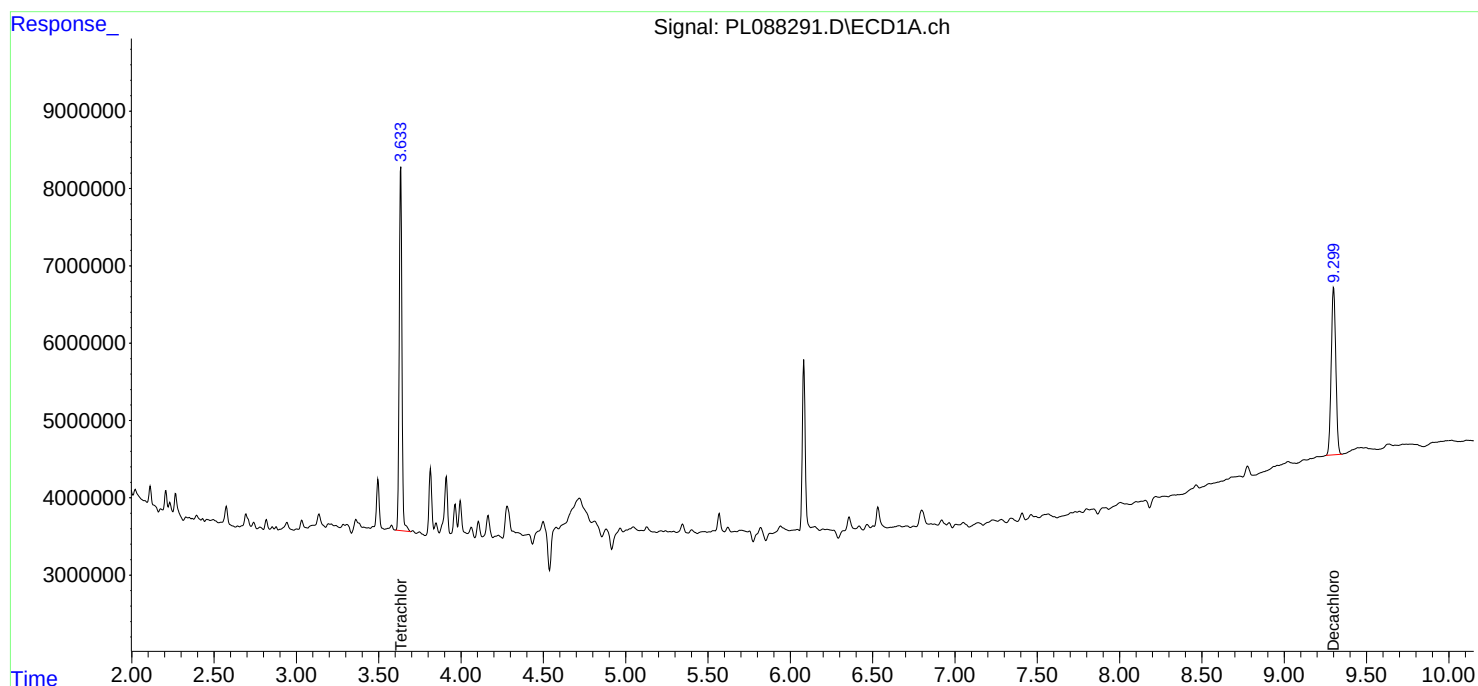


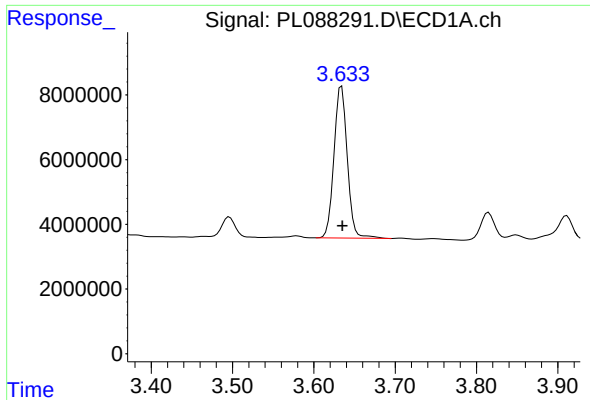

#1 Tetrachloro-m-xylene


R.T.: 3.634 min
Delta R.T.: 0.000 min
Response: 53557262
Conc: 19.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
20240768-AMENDED-COMP-39N-N-3-03

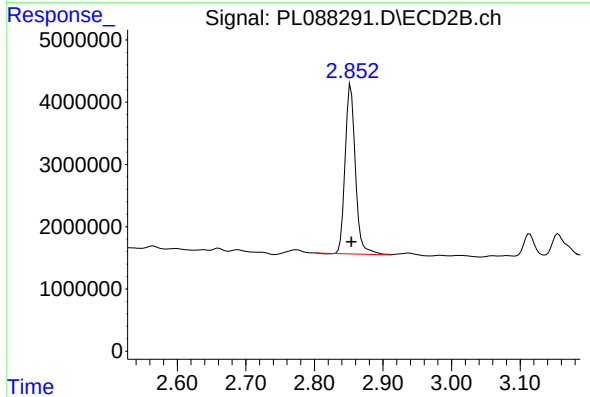


#1 Tetrachloro-m-xylene

R.T.: 2.853 min
Delta R.T.: 0.000 min
Response: 28306443
Conc: 20.18 ng/ml

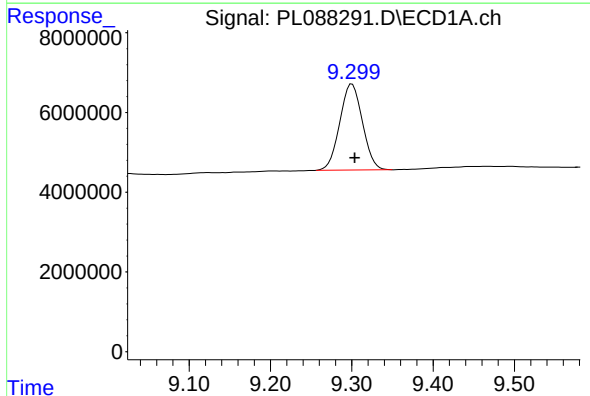

#28 Decachlorobiphenyl

R.T.: 9.300 min
Delta R.T.: -0.003 min
Response: 41730177
Conc: 21.67 ng/ml

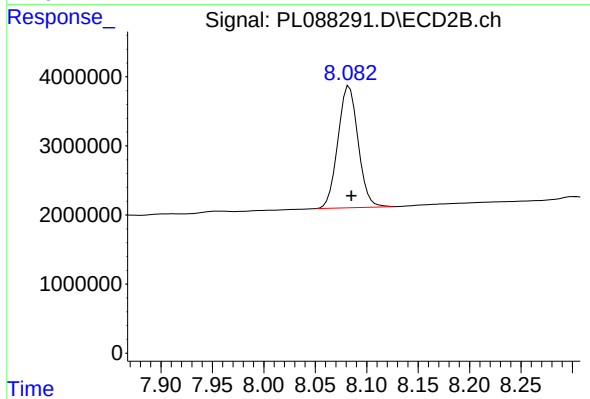

#28 Decachlorobiphenyl

R.T.: 8.083 min
Delta R.T.: -0.002 min
Response: 24122953
Conc: 18.95 ng/ml