

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022719\
 Data File : PL045145.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Feb 2019 12:12
 Operator : AJ\SJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 28 03:06:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.363	3.982	162.4E6	50493889	23.610	23.578
28)	SA Decachlor...	8.047	9.038	206.0E6	57857225	24.624	25.321
Target Compounds							
9)	A Endosulfan I	5.368	6.209	99063283	28896153	11.083	11.604
10)	B gamma-Chl...	5.259	6.087	108.8E6	30772517	11.113	11.470
12)	B 4,4'-DDE	5.484	6.317	191.9E6	53469923	21.859	22.890
13)	MA Dieldrin	5.609	6.466	225.4E6	60737307	23.580	23.636
19)	B Endosulfa...	6.515	7.240	184.5E6	52212940	22.704	23.211
20)	A Methoxychlor	6.776	7.564	529.4E6	142.6E6	120.544	116.192
21)	B Endrin ke...	6.999	7.709	185.0E6	48861404	20.080	20.544
25)	Chlordane-3	5.259	6.087	108.8E6	30772517	94.823	78.979



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022719\
Data File : PL045145.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Feb 2019 12:12
Operator : AJ\SJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 28 03:06:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

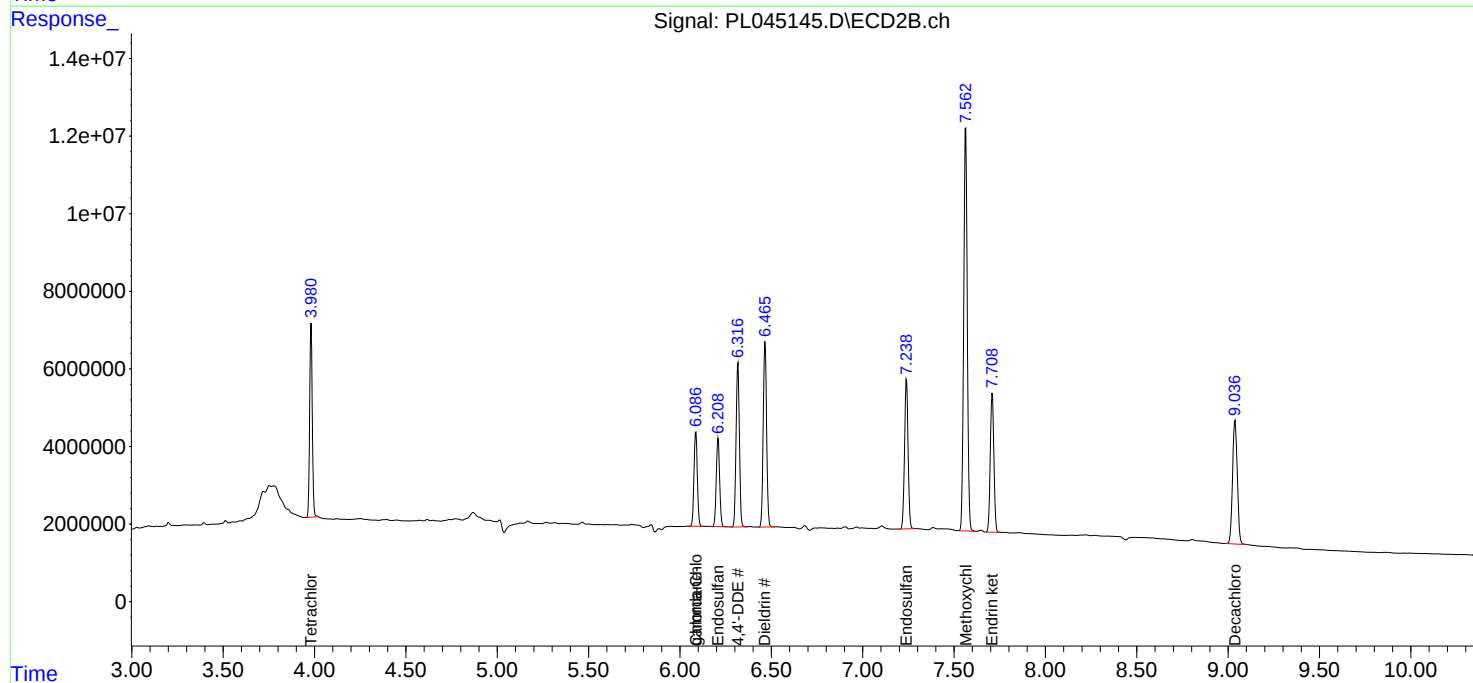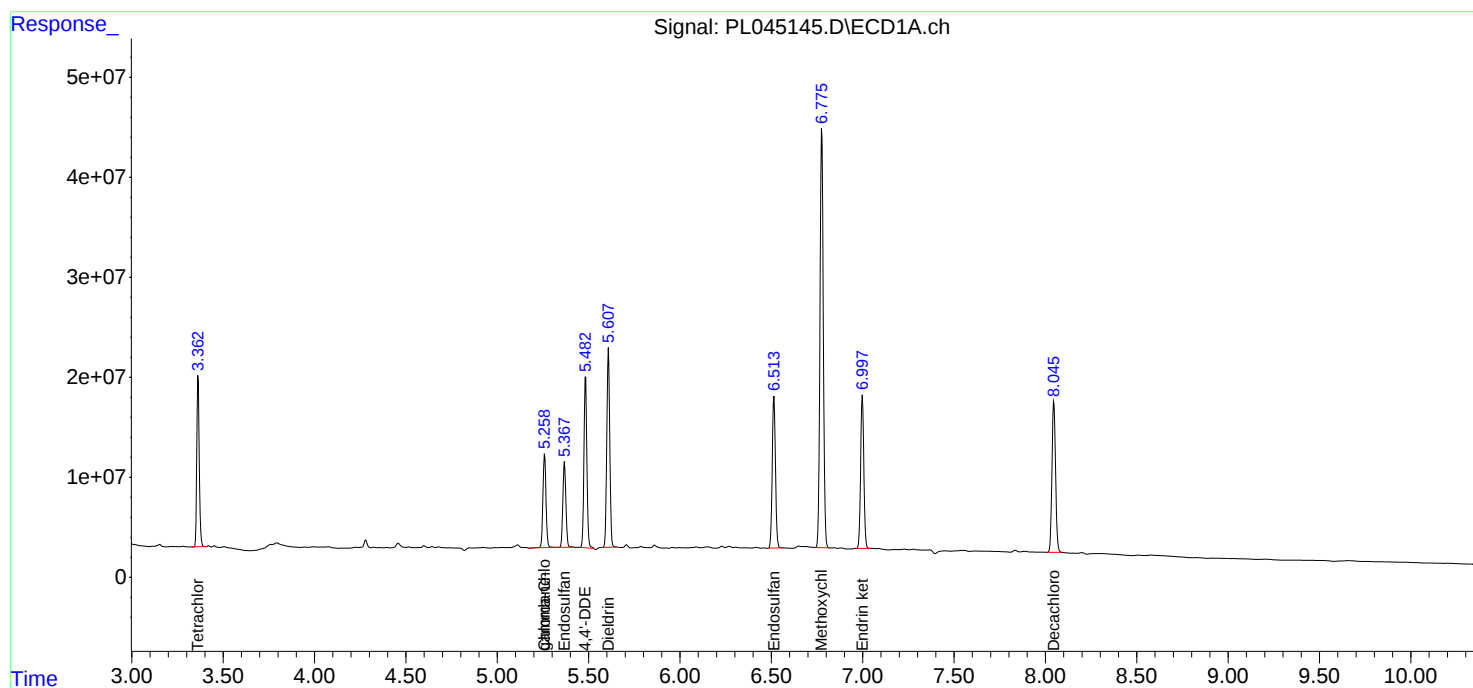


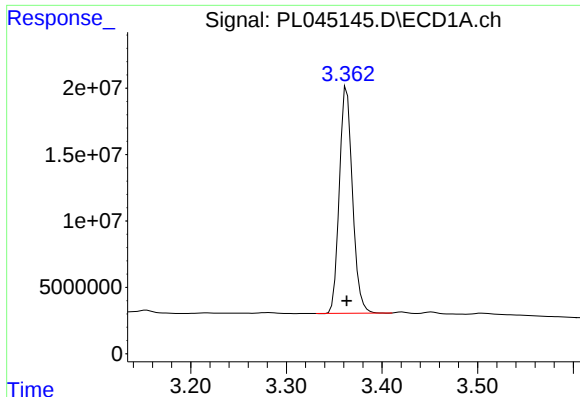

#1 Tetrachloro-m-xylene


R.T.: 3.363 min
Delta R.T.: 0.000 min
Response: 162421450
Conc: 23.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

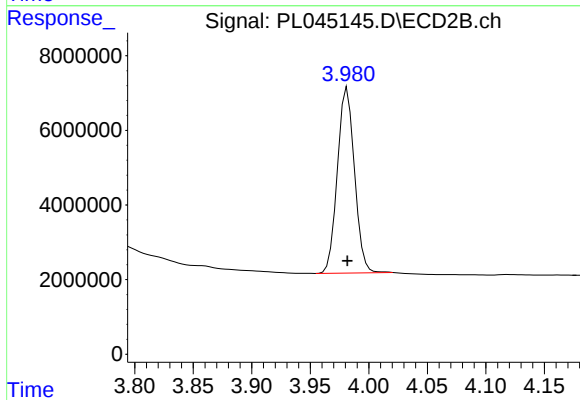


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 50493889
Conc: 23.58 ng/ml

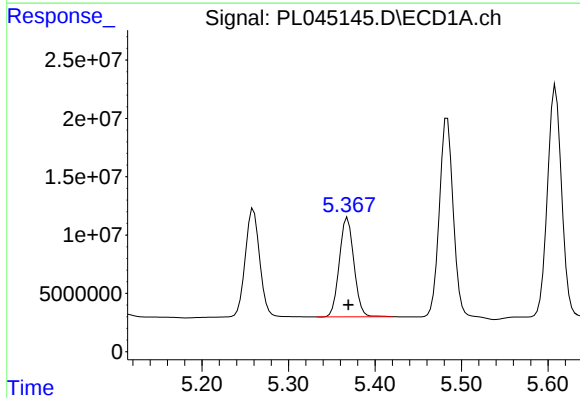


#9 Endosulfan I

R.T.: 5.368 min
Delta R.T.: 0.000 min
Response: 99063283
Conc: 11.08 ng/ml

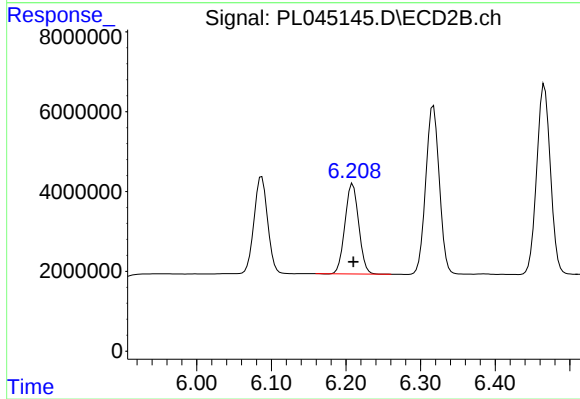

#9 Endosulfan I


R.T.: 6.209 min
Delta R.T.: 0.000 min
Response: 28896153
Conc: 11.60 ng/ml

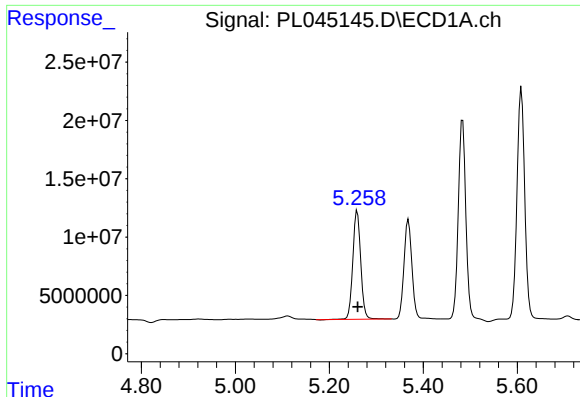

#10 gamma-Chlordane


R.T.: 5.259 min
Delta R.T.: -0.001 min
Response: 108764048
Conc: 11.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

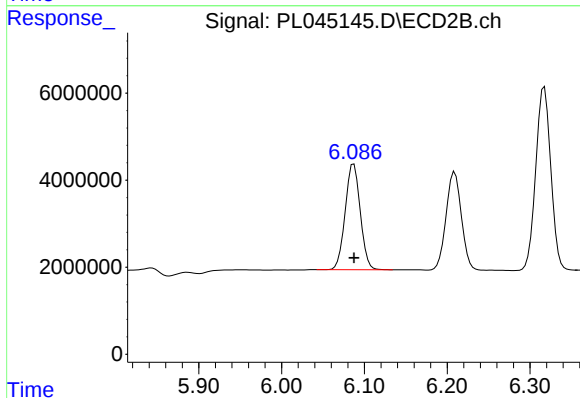


#10 gamma-Chlordane

R.T.: 6.087 min
Delta R.T.: 0.000 min
Response: 30772517
Conc: 11.47 ng/ml

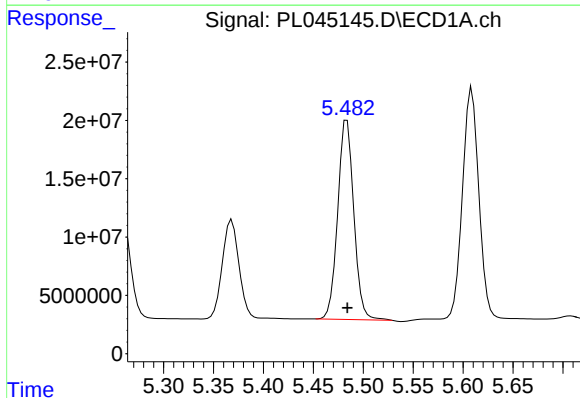


#12 4,4'-DDE

R.T.: 5.484 min
Delta R.T.: 0.000 min
Response: 191878631
Conc: 21.86 ng/ml

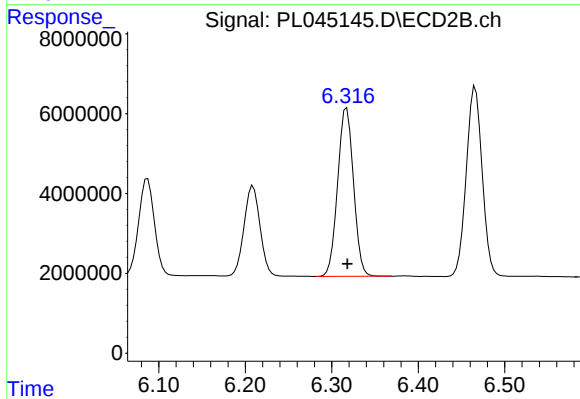

#12 4,4'-DDE


R.T.: 6.317 min
Delta R.T.: 0.000 min
Response: 53469923
Conc: 22.89 ng/ml

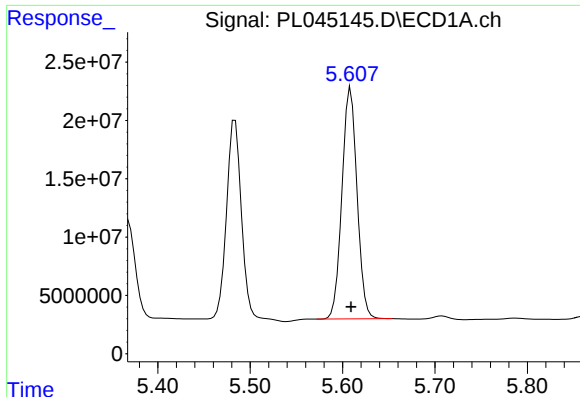

#13 Dieldrin


R.T.: 5.609 min
Delta R.T.: 0.000 min
Response: 225373982
Conc: 23.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

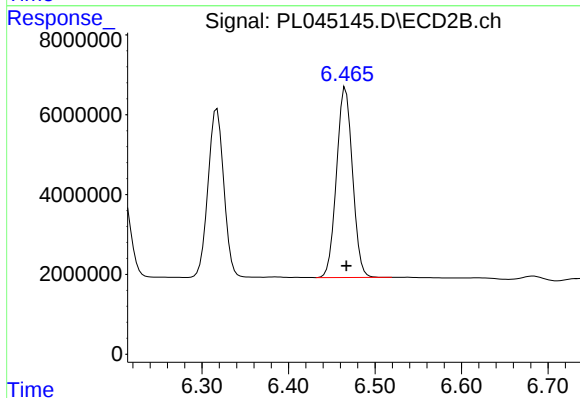


#13 Dieldrin

R.T.: 6.466 min
Delta R.T.: 0.000 min
Response: 60737307
Conc: 23.64 ng/ml

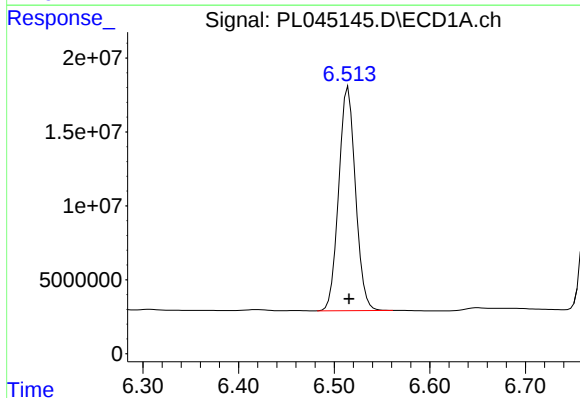


#19 Endosulfan Sulfate

R.T.: 6.515 min
Delta R.T.: 0.000 min
Response: 184539172
Conc: 22.70 ng/ml

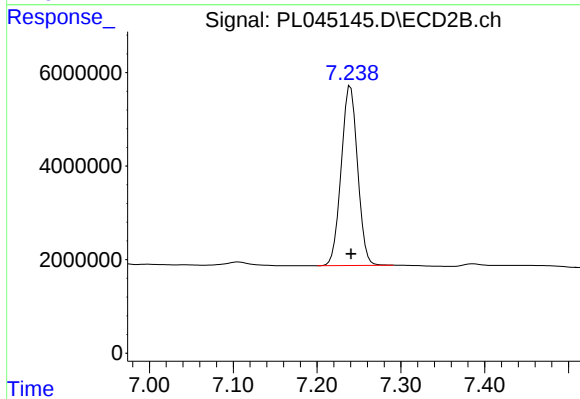

#19 Endosulfan Sulfate


R.T.: 7.240 min
Delta R.T.: 0.000 min
Response: 52212940
Conc: 23.21 ng/ml

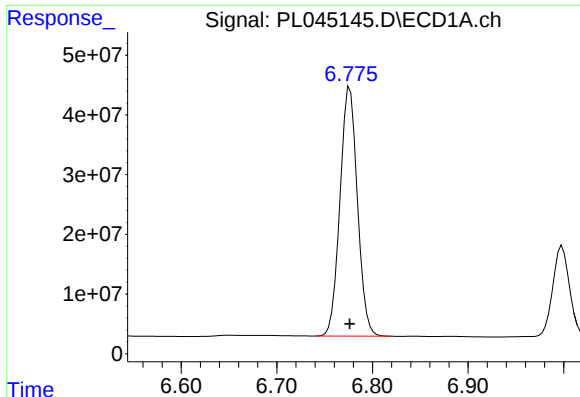

#20 Methoxychlor


R.T.: 6.776 min
Delta R.T.: 0.000 min
Response: 529396245
Conc: 120.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

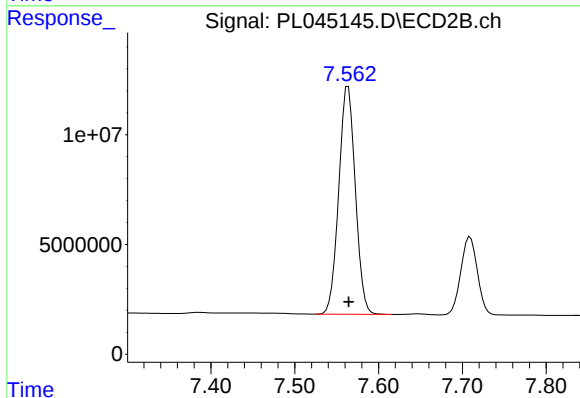


#20 Methoxychlor

R.T.: 7.564 min
Delta R.T.: 0.000 min
Response: 142616135
Conc: 116.19 ng/ml

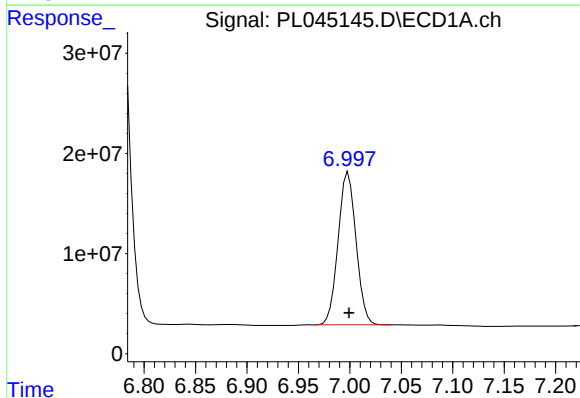


#21 Endrin ketone

R.T.: 6.999 min
Delta R.T.: 0.000 min
Response: 184993665
Conc: 20.08 ng/ml

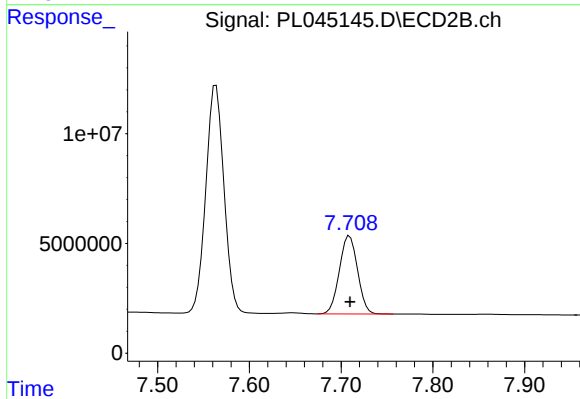

#21 Endrin ketone


R.T.: 7.709 min
Delta R.T.: 0.000 min
Response: 48861404
Conc: 20.54 ng/ml

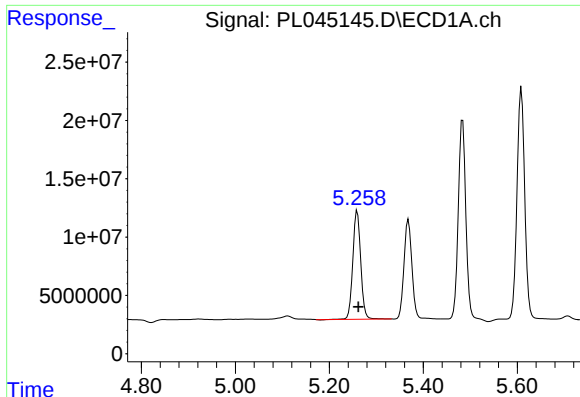

#25 Chlordane-3


R.T.: 5.259 min
Delta R.T.: -0.002 min
Response: 108764048
Conc: 94.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

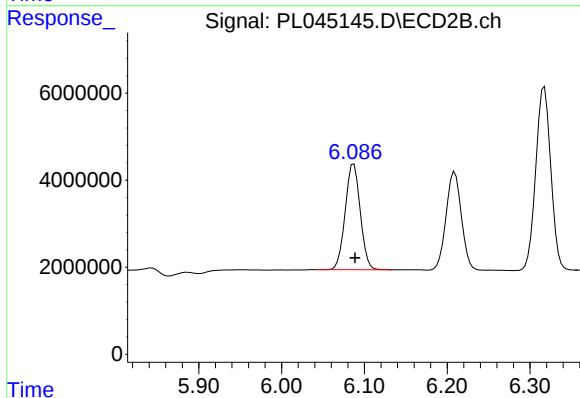


#25 Chlordane-3

R.T.: 6.087 min
Delta R.T.: -0.002 min
Response: 30772517
Conc: 78.98 ng/ml

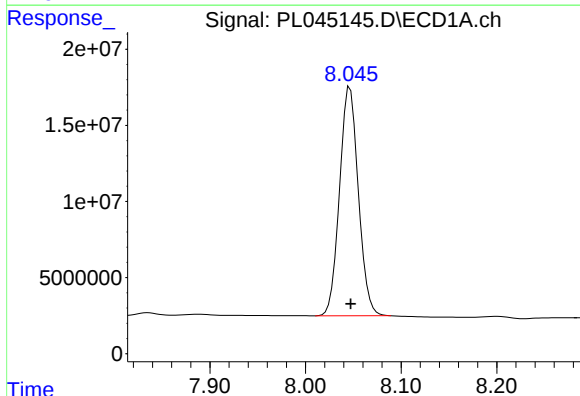

#28 Decachlorobiphenyl

R.T.: 8.047 min
Delta R.T.: 0.000 min
Response: 206043243
Conc: 24.62 ng/ml

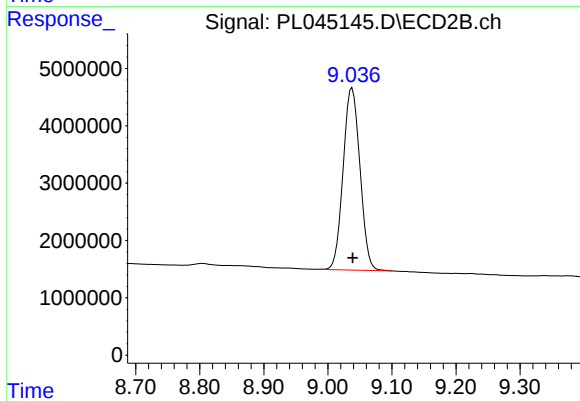

#28 Decachlorobiphenyl

R.T.: 9.038 min
Delta R.T.: -0.001 min
Response: 57857225
Conc: 25.32 ng/ml