

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022719\
 Data File : PL045151.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Feb 2019 14:12
 Operator : AJ\SJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 27 16:51:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 16:50:41 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.364	3.982	730.1E6	208.0E6	99.799	98.307
28)	SA Decachlor...	8.048	9.039	773.8E6	205.3E6	94.870	93.211
Target Compounds							
23)	Chlordane-1	4.211	4.975	349.9E6	109.1E6	1013.949	975.409
24)	Chlordane-2	4.703	5.442	370.4E6	111.4E6	965.913	937.558
25)	Chlordane-3	5.261	6.088	1210.2E6	394.1E6	1011.524	1005.869
26)	Chlordane-4	5.316	6.162	1096.2E6	464.8E6	1002.357	994.650
27)	Chlordane-5	6.142	6.966	365.1E6	90337719	1029.071	988.866



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022719\
Data File : PL045151.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Feb 2019 14:12
Operator : AJ\SJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 27 16:51:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 16:50:41 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

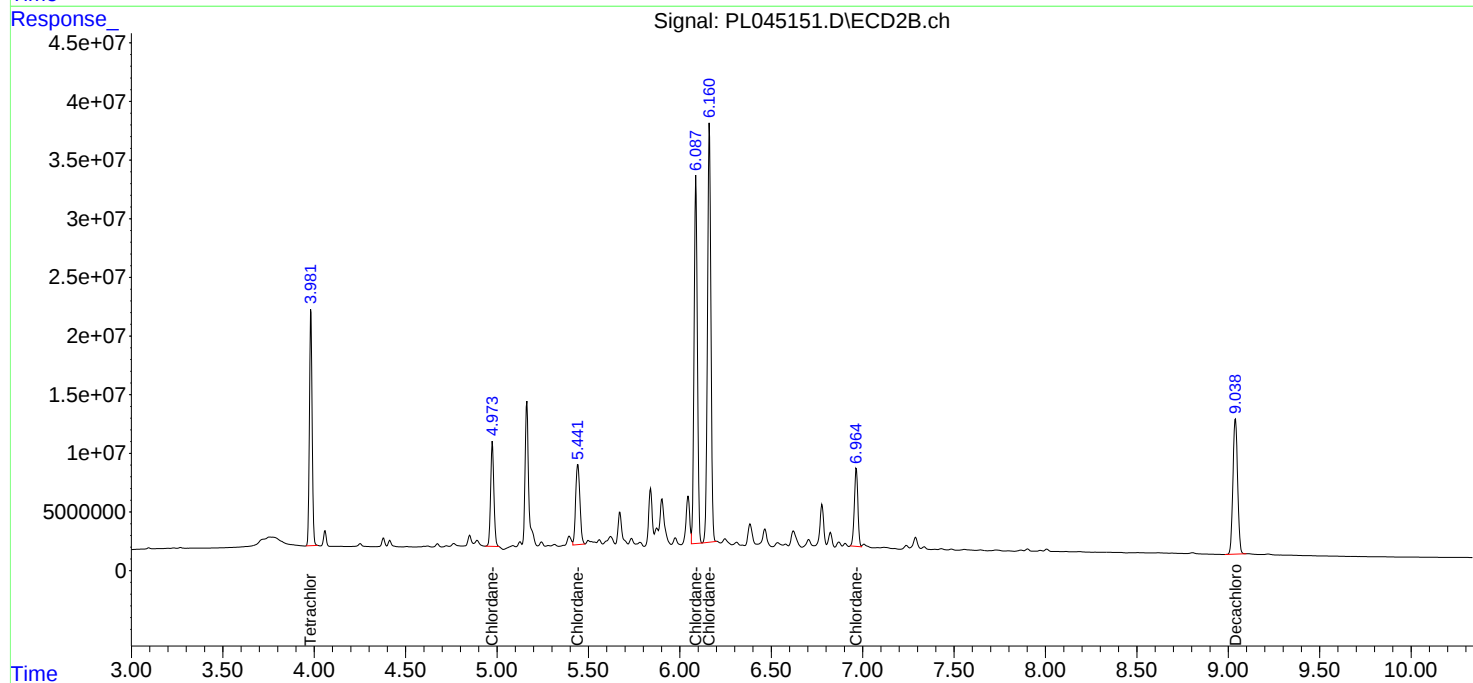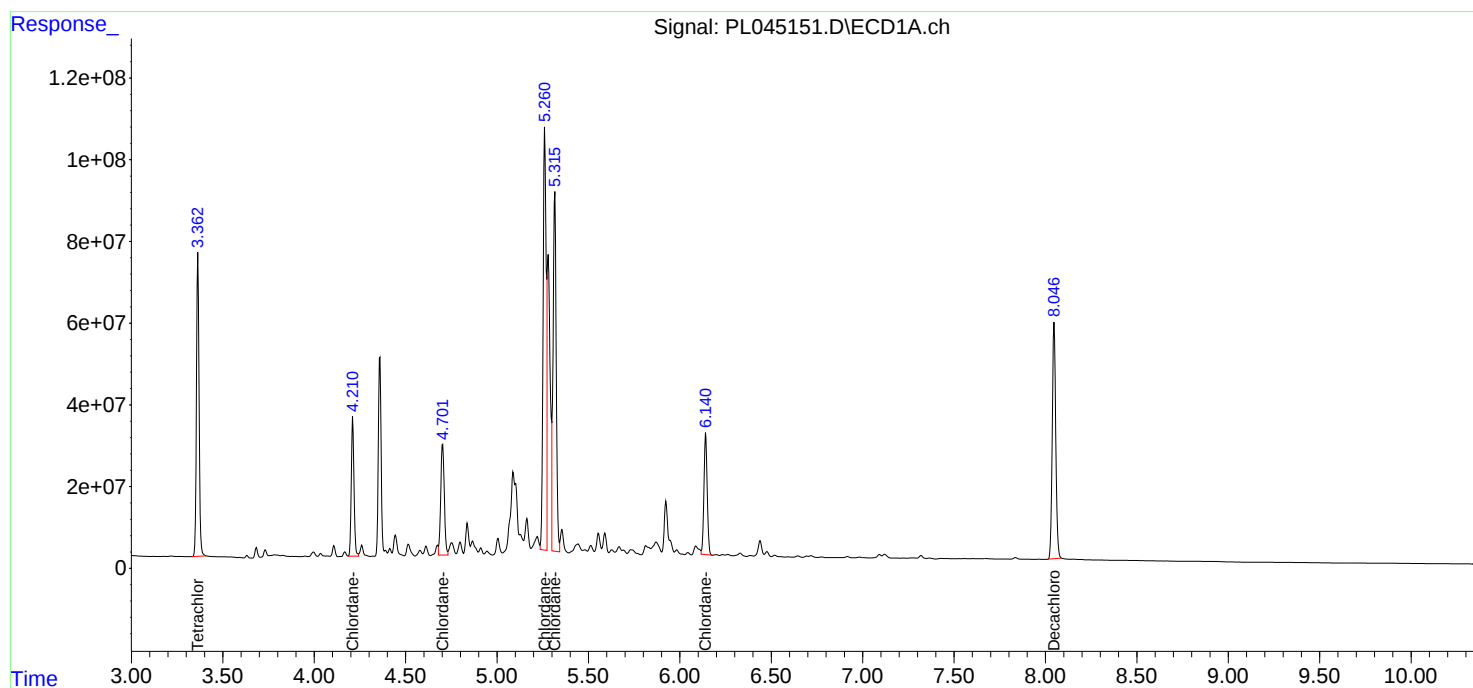


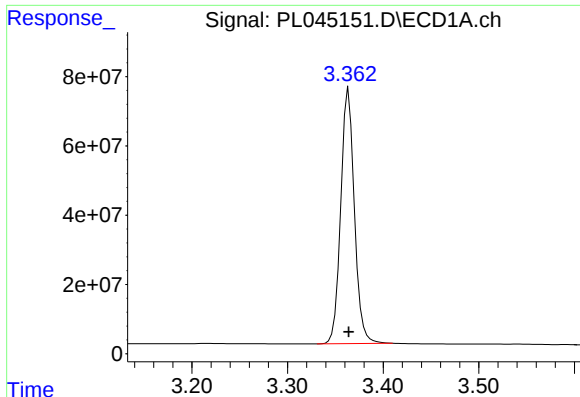

#1 Tetrachloro-m-xylene


R.T.: 3.364 min
Delta R.T.: 0.000 min
Response: 730116912
Conc: 99.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

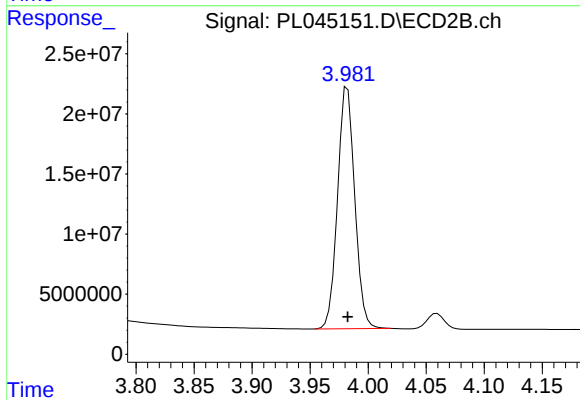


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 208034053
Conc: 98.31 ng/ml

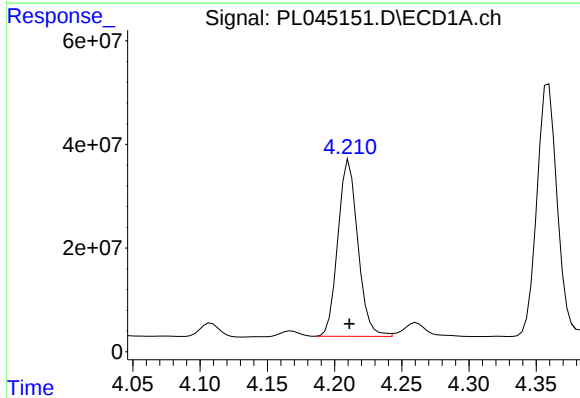


#23 Chlordane-1

R.T.: 4.211 min
Delta R.T.: 0.000 min
Response: 349858819
Conc: 1013.95 ng/ml

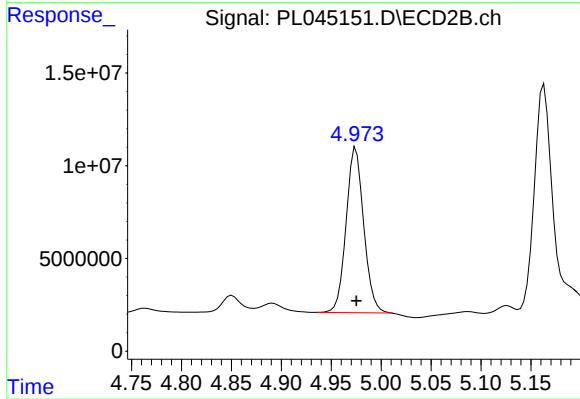

#23 Chlordane-1


R.T.: 4.975 min
Delta R.T.: 0.000 min
Response: 109075101
Conc: 975.41 ng/ml

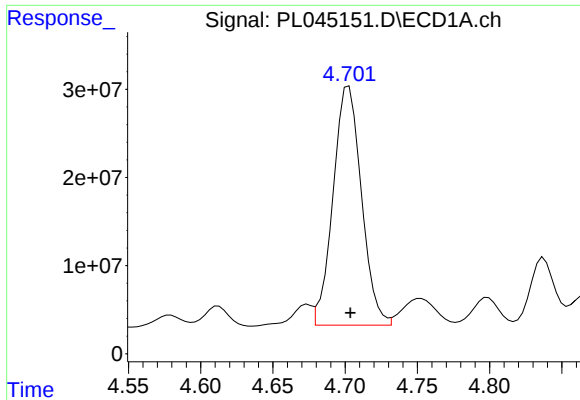

#24 Chlordane-2


R.T.: 4.703 min
Delta R.T.: -0.001 min
Response: 370378190
Conc: 965.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

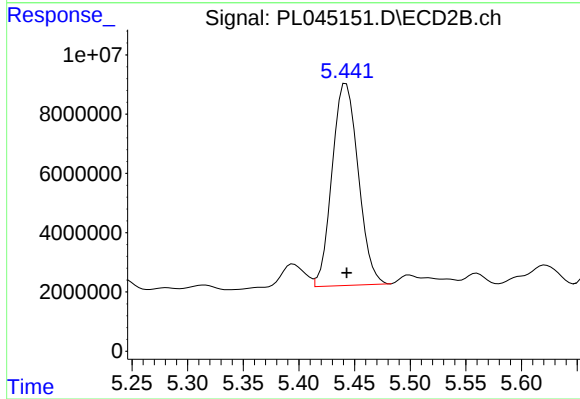


#24 Chlordane-2

R.T.: 5.442 min
Delta R.T.: 0.000 min
Response: 111398540
Conc: 937.56 ng/ml

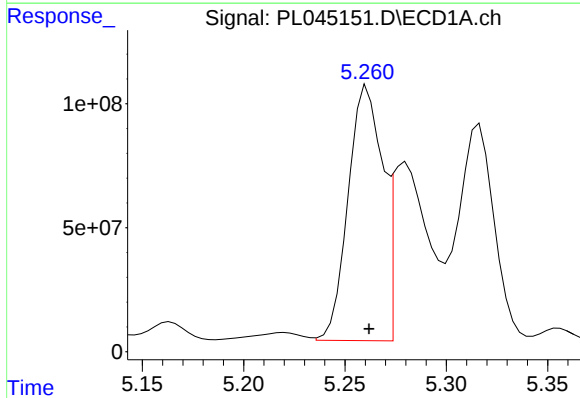


#25 Chlordane-3

R.T.: 5.261 min
Delta R.T.: 0.000 min
Response: 1210244892
Conc: 1011.52 ng/ml

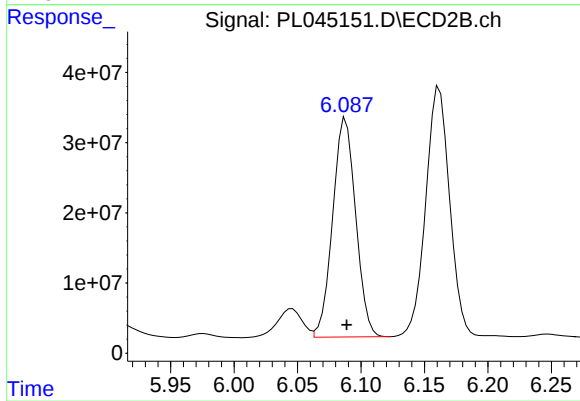

#25 Chlordane-3


R.T.: 6.088 min
Delta R.T.: 0.000 min
Response: 394100208
Conc: 1005.87 ng/ml

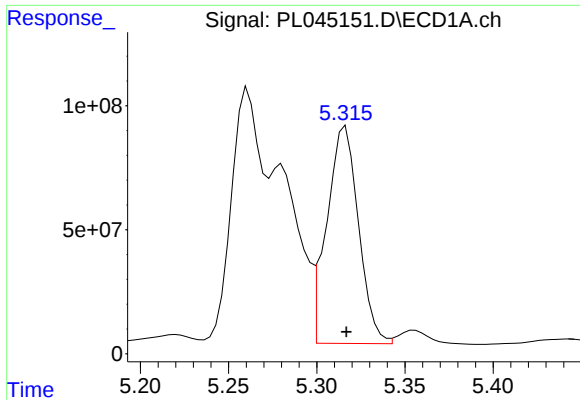

#26 Chlordane-4


R.T.: 5.316 min
Delta R.T.: 0.000 min
Response: 1096217266
Conc: 1002.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

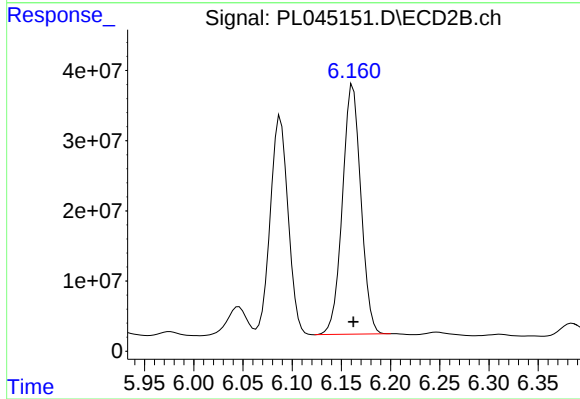


#26 Chlordane-4

R.T.: 6.162 min
Delta R.T.: 0.000 min
Response: 464803337
Conc: 994.65 ng/ml

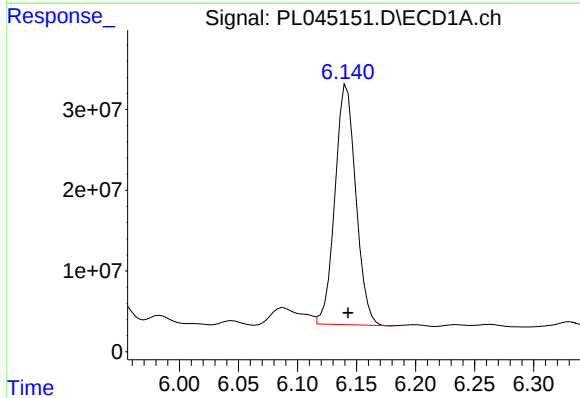


#27 Chlordane-5

R.T.: 6.142 min
Delta R.T.: -0.001 min
Response: 365146441
Conc: 1029.07 ng/ml

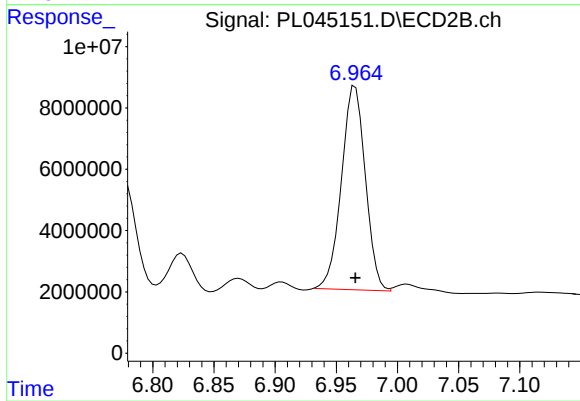

#27 Chlordane-5


R.T.: 6.966 min
Delta R.T.: 0.000 min
Response: 90337719
Conc: 988.87 ng/ml

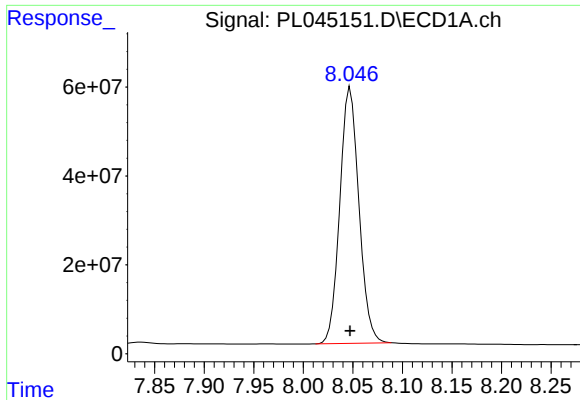

#28 Decachlorobiphenyl

R.T.: 8.048 min
Delta R.T.: 0.000 min
Response: 773783282
Conc: 94.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

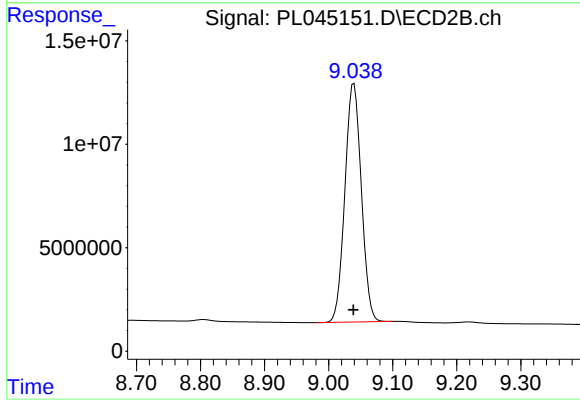

#28 Decachlorobiphenyl

R.T.: 9.039 min
Delta R.T.: 0.000 min
Response: 205302063
Conc: 93.21 ng/ml